

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100421\
 Data File : P0081757.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Oct 2021 21:12
 Operator : AJ\MA
 Sample : M4063-05
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SW-RR-01-(2.0)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 01:13:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 24 02:21:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.867	3.983	1813705	493663	20.339	18.530
2)	SA Decachlor...	10.875	9.326	1580603	489361	21.220	21.072

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100421\
Data File : P0081757.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Oct 2021 21:12
Operator : AJ\MA
Sample : M4063-05
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SW-RR-01-(2.0)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 01:13:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 24 02:21:54 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

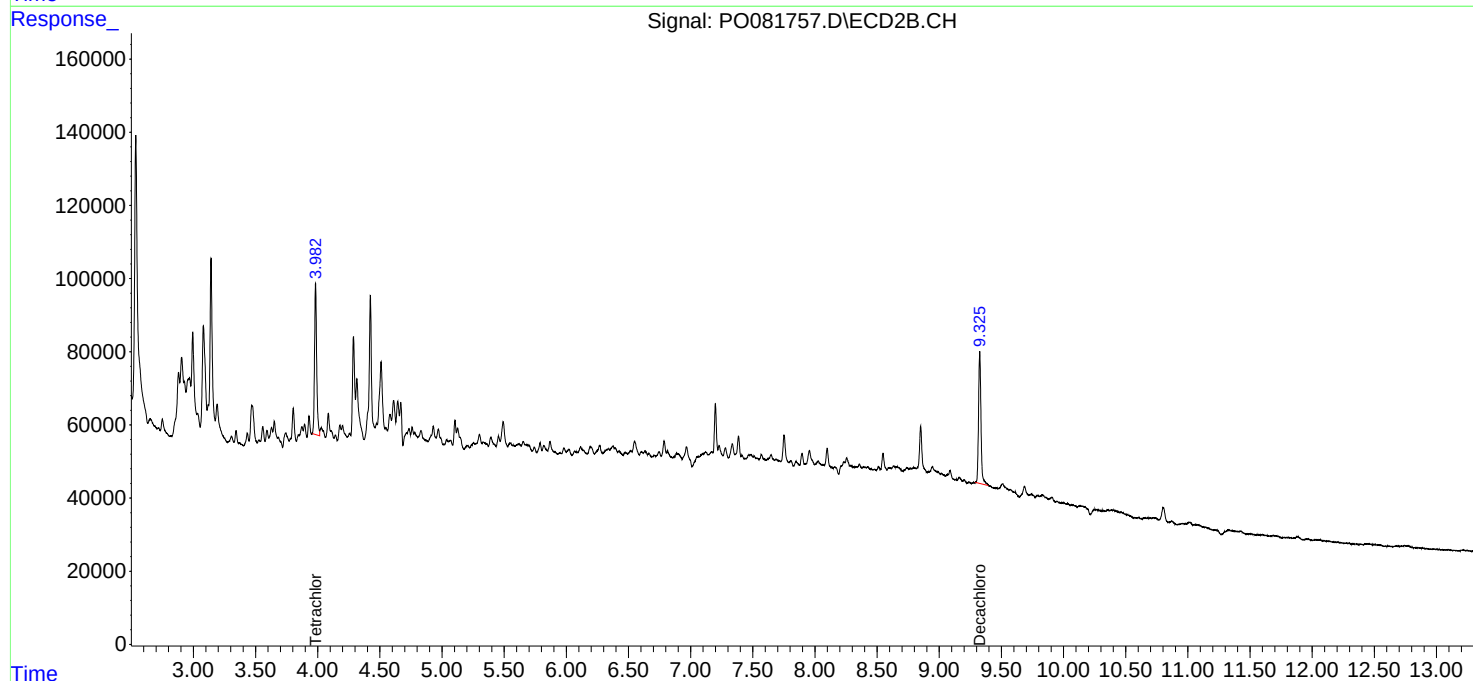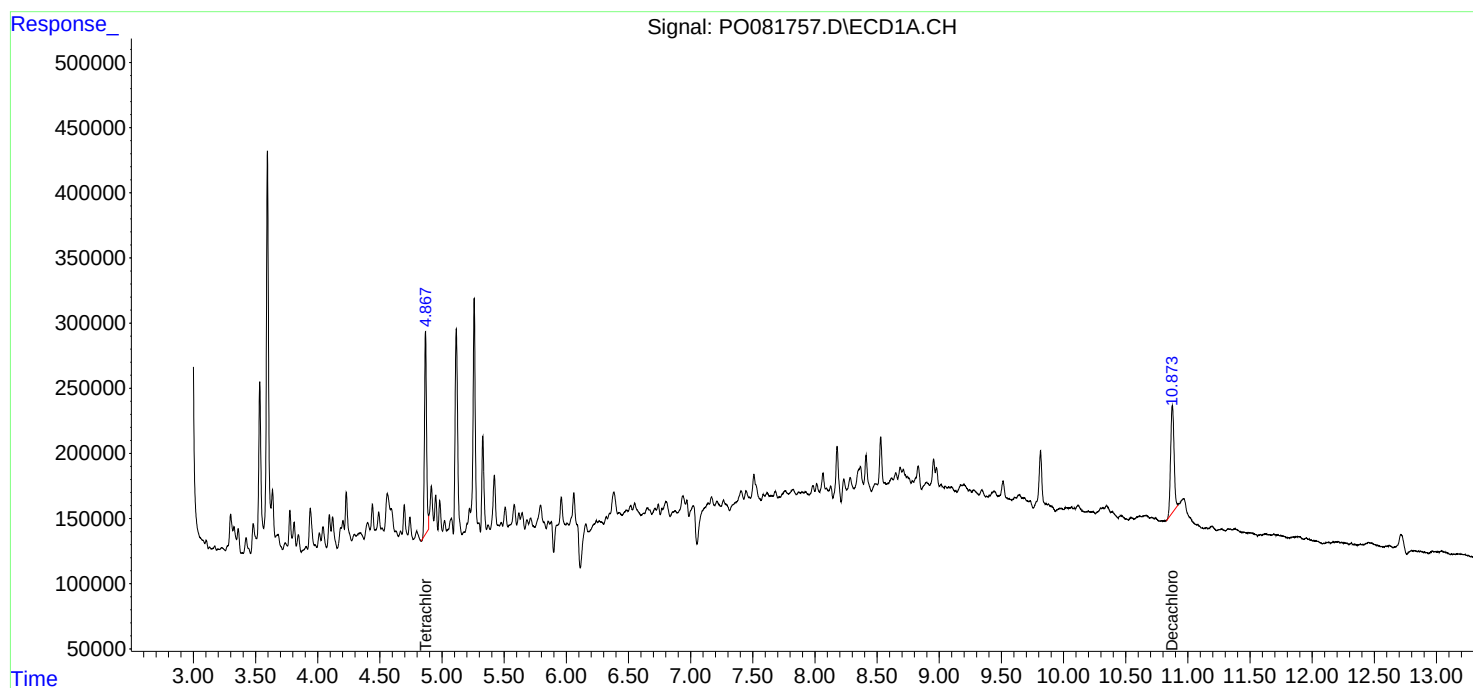


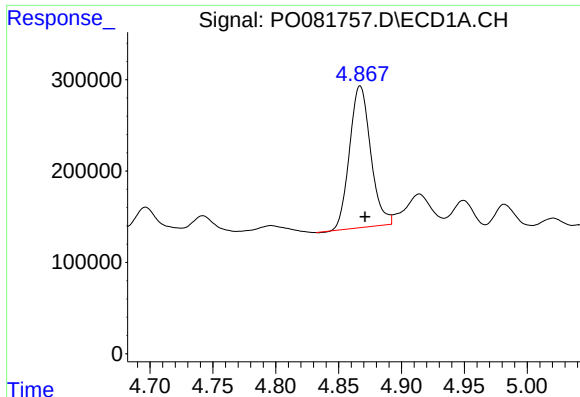

#1 Tetrachloro-m-xylene


R.T.: 4.867 min
Delta R.T.: -0.004 min
Response: 1813705
Conc: 20.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
SW-RR-01-(2.0)

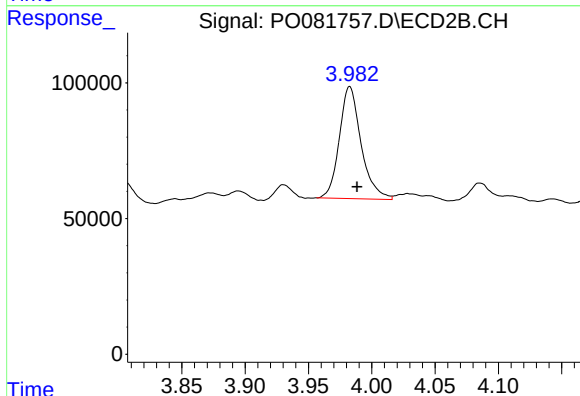


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: -0.006 min
Response: 493663
Conc: 18.53 ng/ml

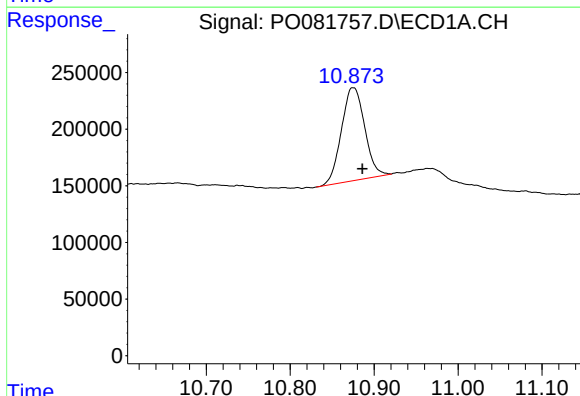

#2 Decachlorobiphenyl

R.T.: 10.875 min
Delta R.T.: -0.011 min
Response: 1580603
Conc: 21.22 ng/ml

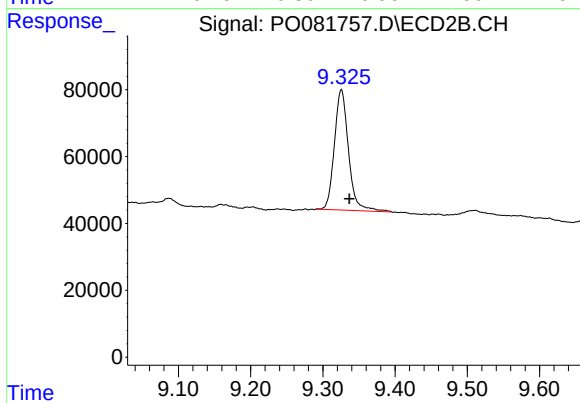

#2 Decachlorobiphenyl

R.T.: 9.326 min
Delta R.T.: -0.011 min
Response: 489361
Conc: 21.07 ng/ml