

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100423\
 Data File : PO098520.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2023 14:02
 Operator : YP/AJ
 Sample : 04697-12
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PIPE-WRAP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/05/2023
 Supervised By :Ankita Jodhani 10/05/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 14:56:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 28 01:18:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.482	3.634	27100241	13756436	14.113	17.662m#
2) SA Decachlor...	10.298	8.644	19182071	7904346	15.802	14.753

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100423\
Data File : PO098520.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2023 14:02
Operator : YP/AJ
Sample : 04697-12
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PIPE-WRAP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/05/2023
Supervised By :Ankita Jodhani 10/05/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 14:56:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092723.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 28 01:18:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

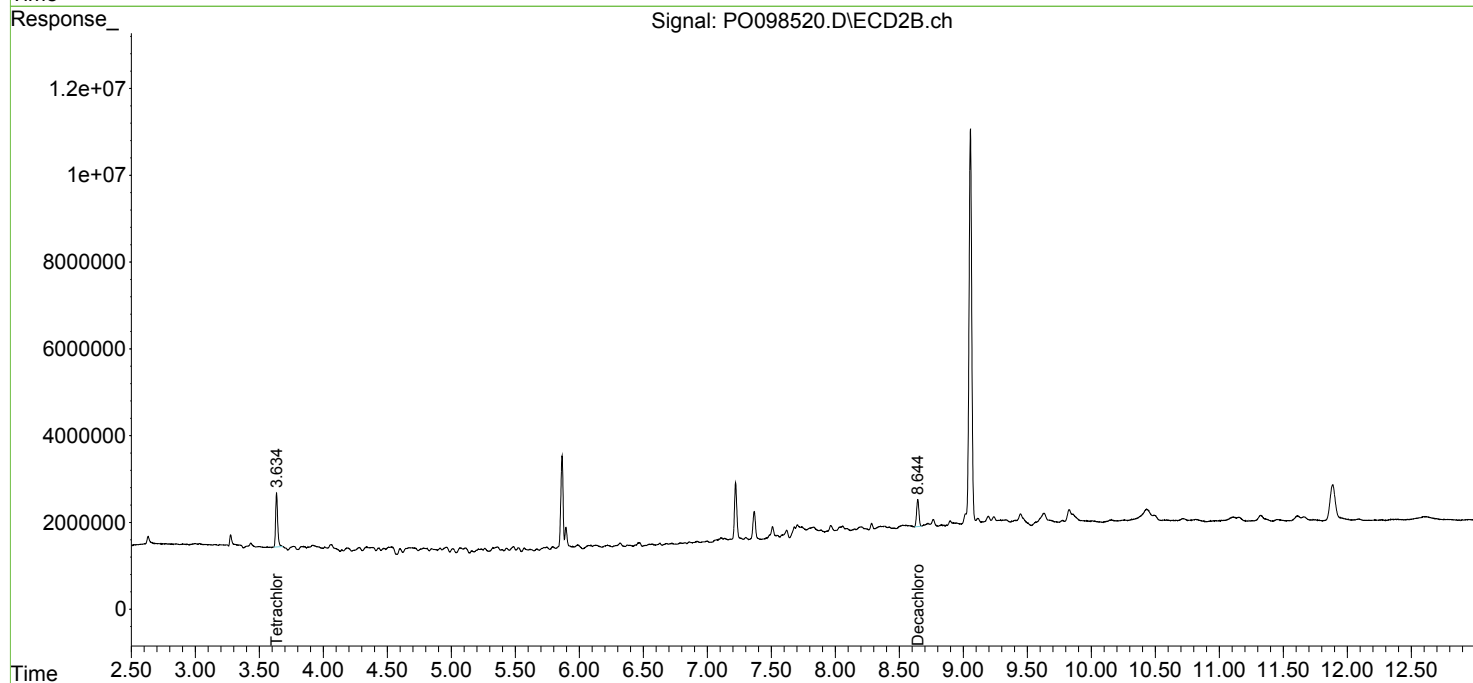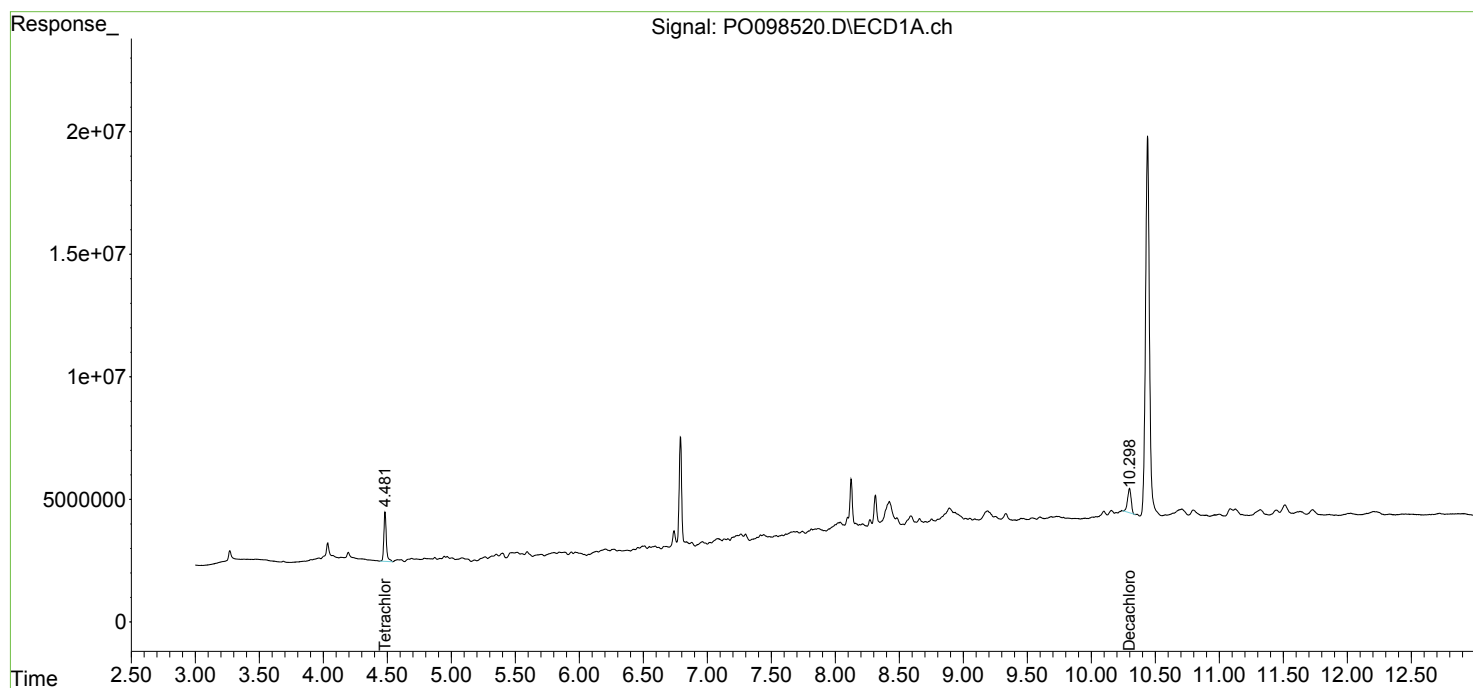

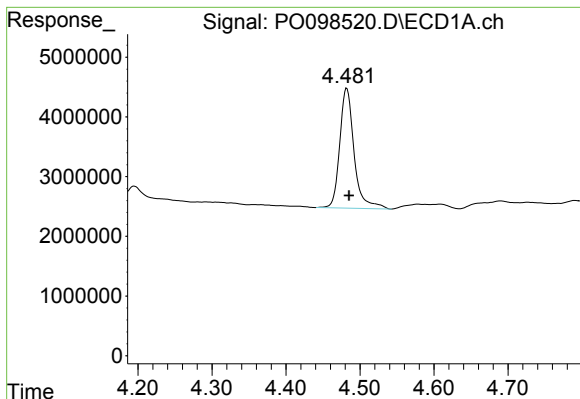


#1 Tetrachloro-m-xylene

R.T.: 4.482 min
Delta R.T.: -0.003 min
Response: 27100241
Conc: 14.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
PIPE-WRAP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/05/2023
Supervised By :Ankita Jodhani 10/05/2023

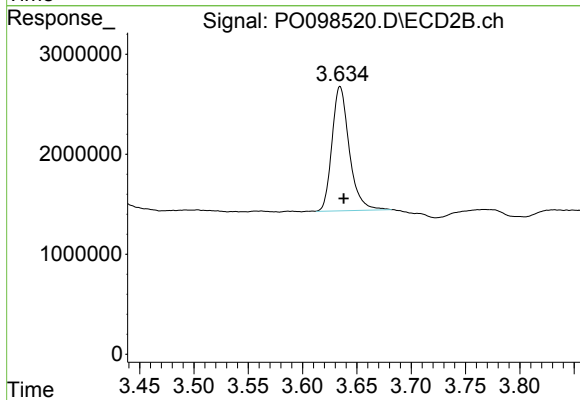


#1 Tetrachloro-m-xylene

R.T.: 3.634 min
Delta R.T.: -0.004 min
Response: 13756436
Conc: 17.66 ng/ml m

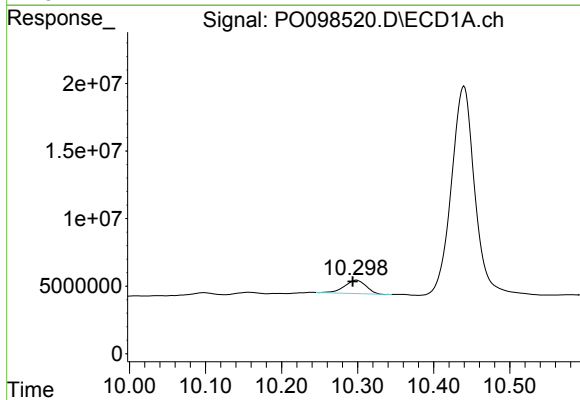

#2 Decachlorobiphenyl

R.T.: 10.298 min
Delta R.T.: 0.005 min
Response: 19182071
Conc: 15.80 ng/ml

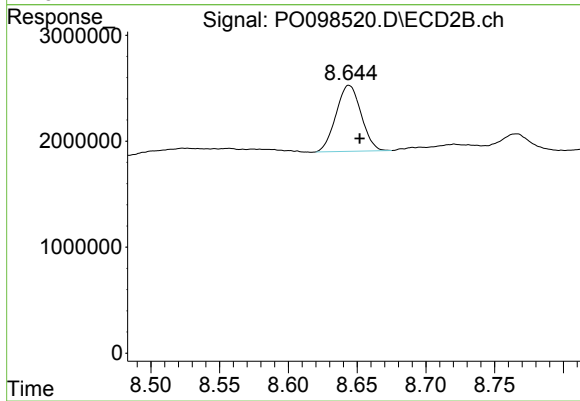

#2 Decachlorobiphenyl

R.T.: 8.644 min
Delta R.T.: -0.008 min
Response: 7904346
Conc: 14.75 ng/ml