

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100423\
 Data File : P0098524.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2023 15:10
 Operator : YP/AJ
 Sample : 04701-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CONC-WC-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/05/2023
 Supervised By :Ankita Jodhani 10/05/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 16:00:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 28 01:18:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.483	3.636	29174998	11461524	15.194	14.716
2) SA Decachlor...	10.299	8.642	28947646	12459496	23.848	23.255m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100423\
Data File : P0098524.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2023 15:10
Operator : YP/AJ
Sample : 04701-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CONC-WC-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/05/2023
Supervised By :Ankita Jodhani 10/05/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 16:00:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092723.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 28 01:18:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

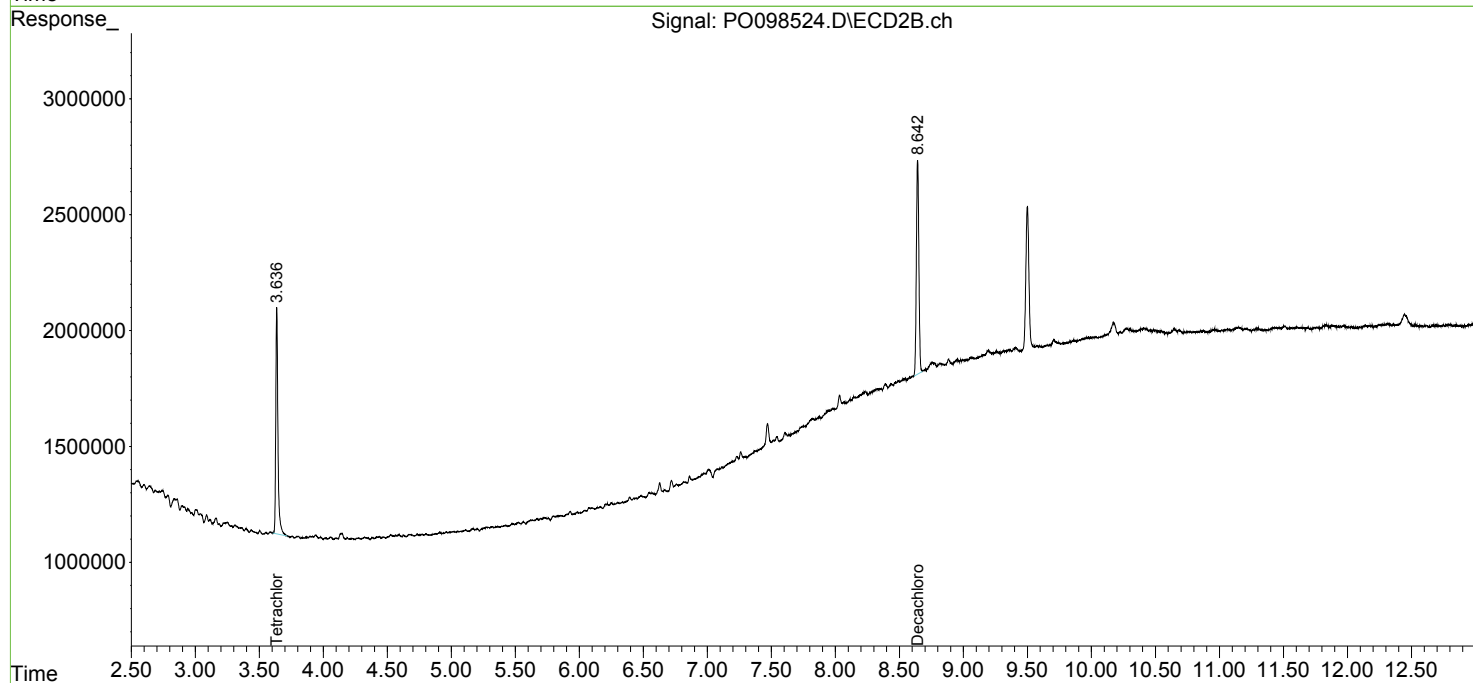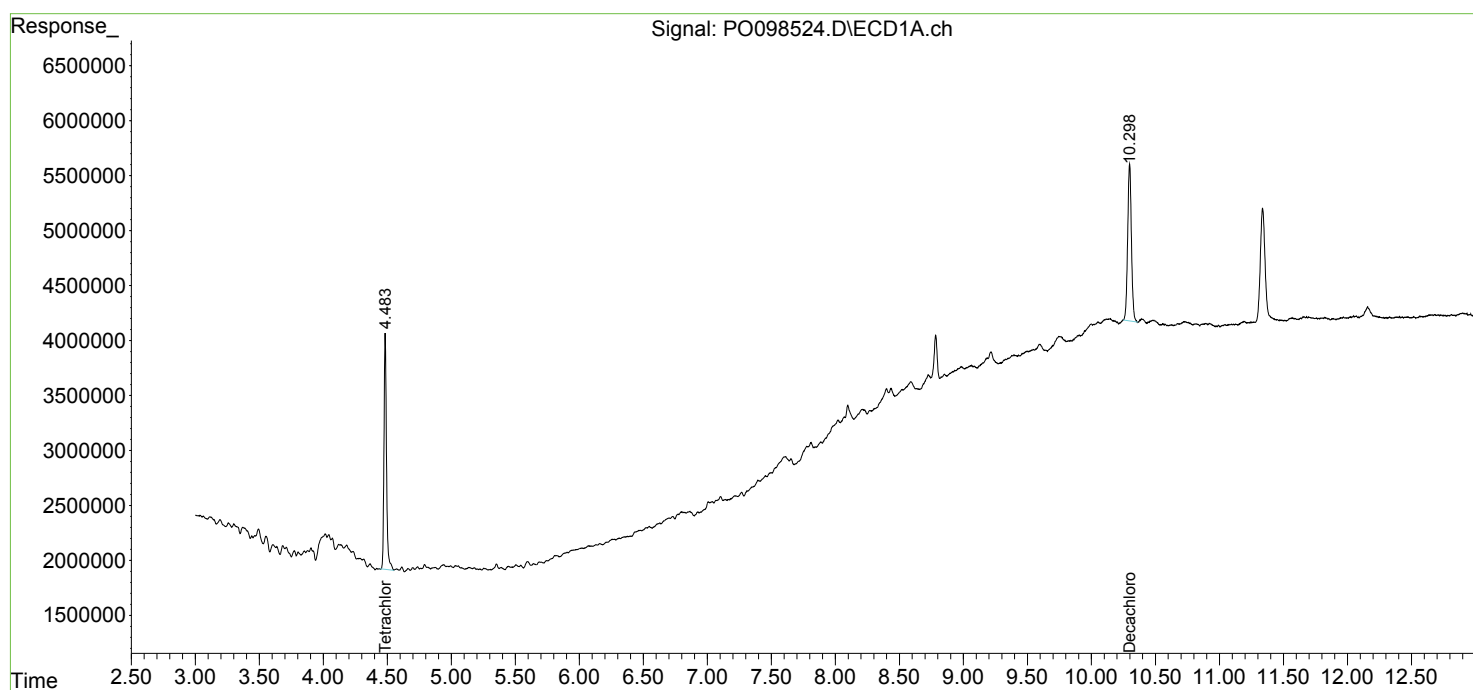

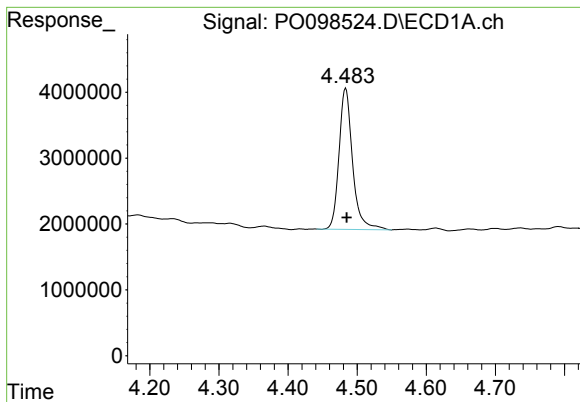


#1 Tetrachloro-m-xylene

R.T.: 4.483 min
Delta R.T.: -0.002 min
Response: 29174998
Conc: 15.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONC-WC-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/05/2023
Supervised By :Ankita Jodhani 10/05/2023

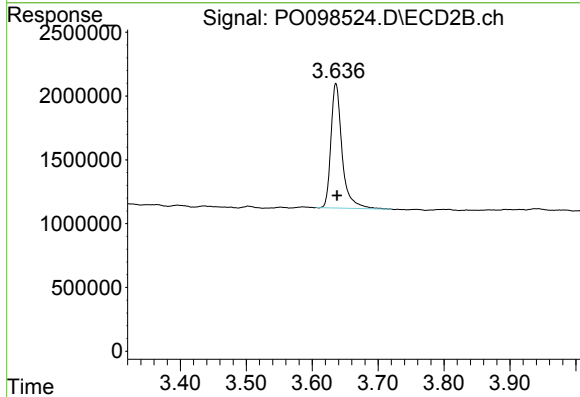


#1 Tetrachloro-m-xylene

R.T.: 3.636 min
Delta R.T.: -0.002 min
Response: 11461524
Conc: 14.72 ng/ml

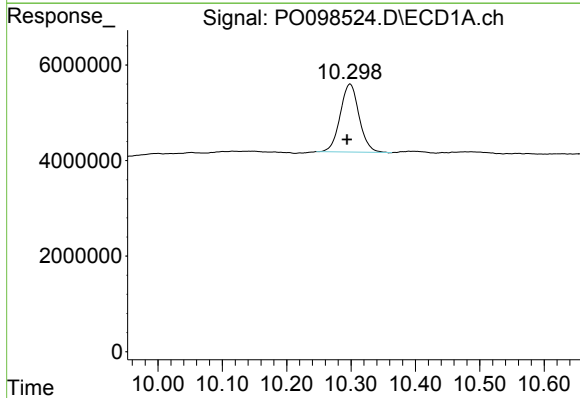

#2 Decachlorobiphenyl

R.T.: 10.299 min
Delta R.T.: 0.005 min
Response: 28947646
Conc: 23.85 ng/ml

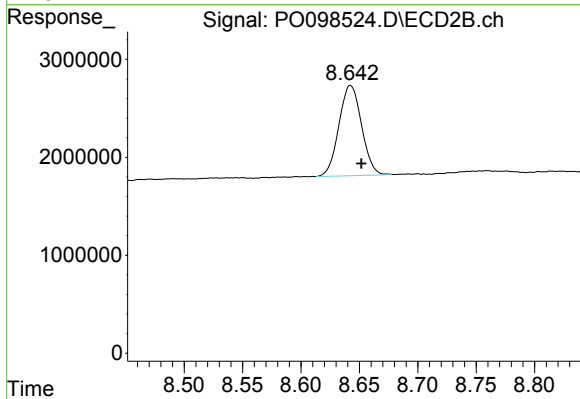

#2 Decachlorobiphenyl

R.T.: 8.642 min
Delta R.T.: -0.010 min
Response: 12459496
Conc: 23.26 ng/ml m