

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100423\
 Data File : PO098552.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2023 23:05
 Operator : YP/AJ
 Sample : 04726-02
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 K242-9B

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/05/2023
 Supervised By :Ankita Jodhani 10/05/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 02:20:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 28 01:18:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.481	3.635	33148223	15534775	17.263m	19.946
2) SA Decachlor...	10.294	8.640	20187766	9420247	16.631	17.583m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100423\
Data File : P0098552.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2023 23:05
Operator : YP/AJ
Sample : 04726-02
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
K242-9B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/05/2023
Supervised By :Ankita Jodhani 10/05/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 02:20:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092723.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 28 01:18:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

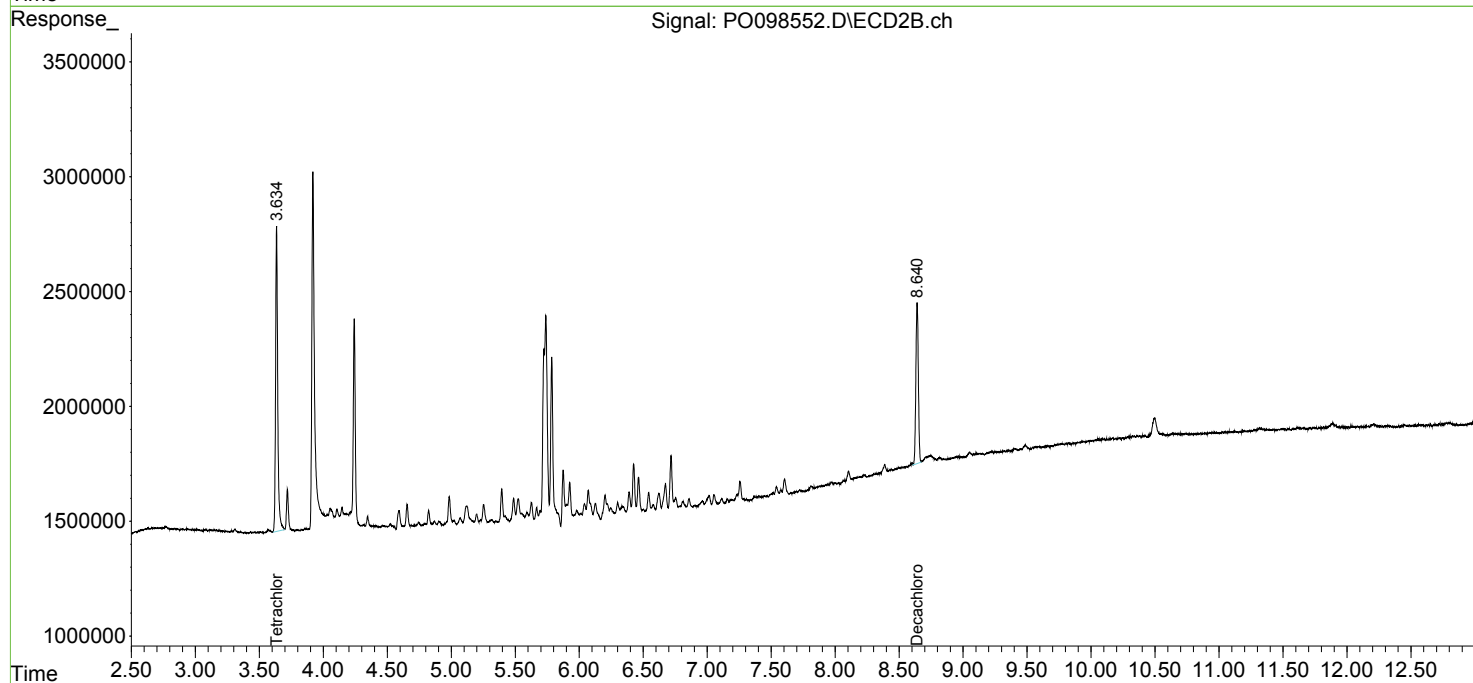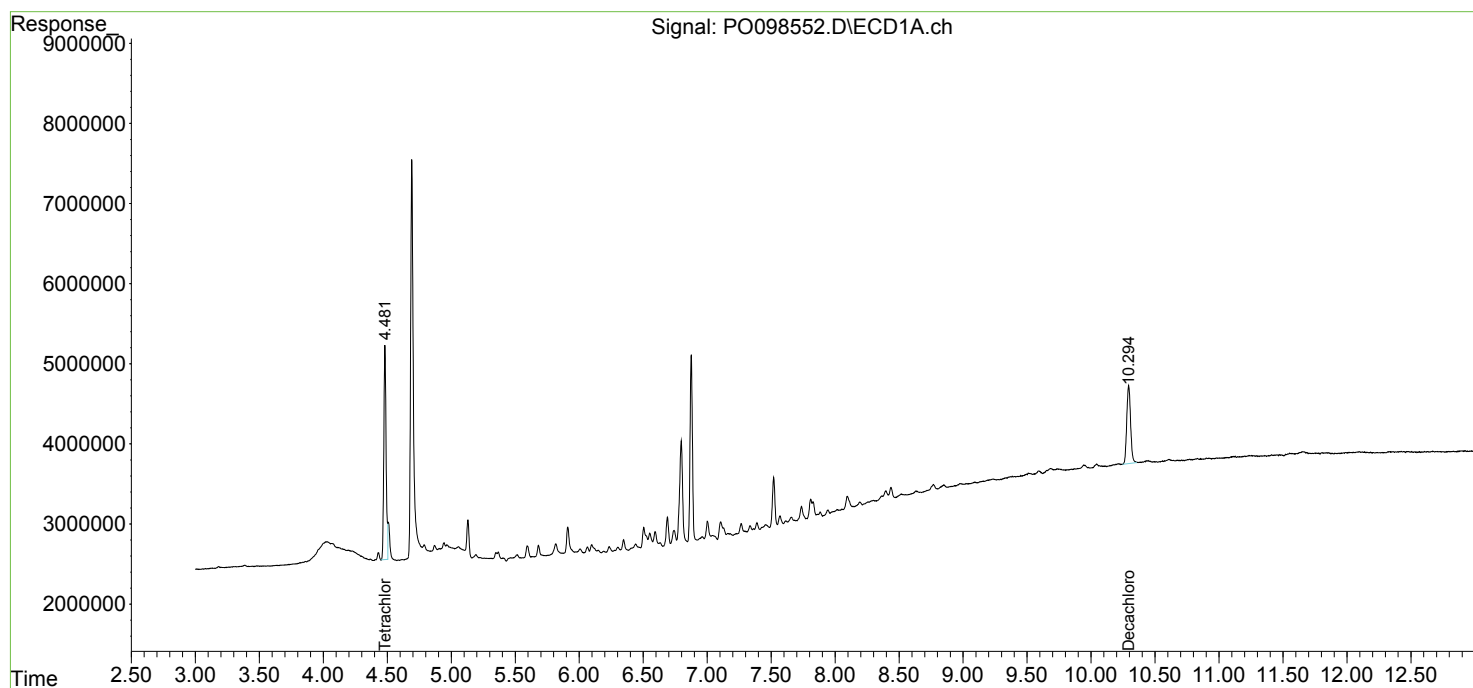

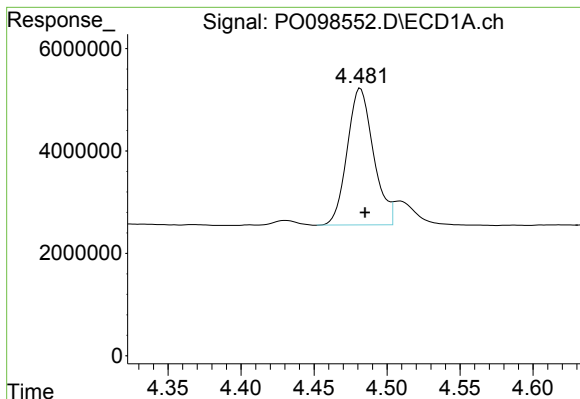


#1 Tetrachloro-m-xylene

R.T.: 4.481 min
Delta R.T.: -0.004 min
Response: 33148223
Conc: 17.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
K242-9B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/05/2023
Supervised By :Ankita Jodhani 10/05/2023

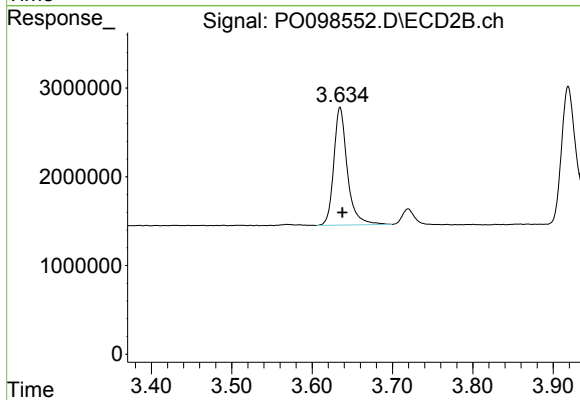


#1 Tetrachloro-m-xylene

R.T.: 3.635 min
Delta R.T.: -0.003 min
Response: 15534775
Conc: 19.95 ng/ml

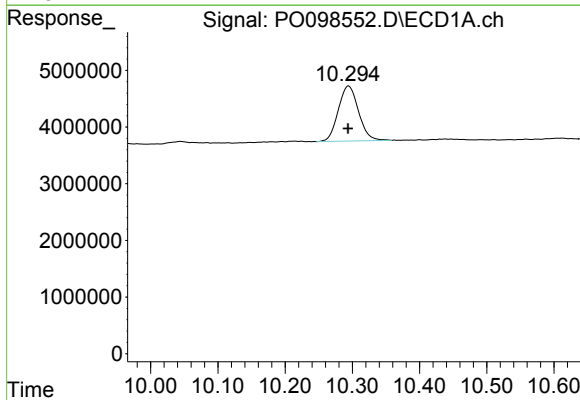

#2 Decachlorobiphenyl

R.T.: 10.294 min
Delta R.T.: 0.000 min
Response: 20187766
Conc: 16.63 ng/ml

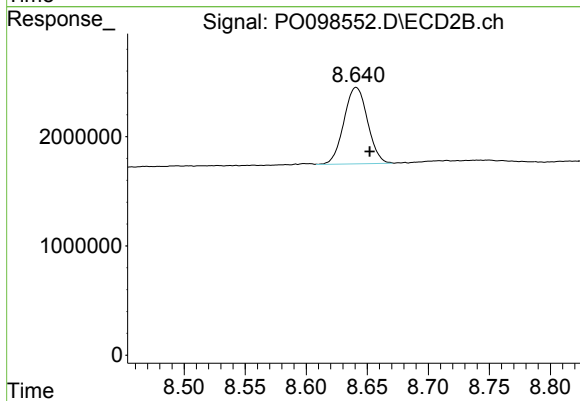

#2 Decachlorobiphenyl

R.T.: 8.640 min
Delta R.T.: -0.011 min
Response: 9420247
Conc: 17.58 ng/ml m