

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100518\
 Data File : PO049700.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Oct 2018 19:02
 Operator : SM/SJ
 Sample : J5223-03RE
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SSSI-1001-S-DH-01RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 22:54:21 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 02 05:32:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.386	3.515	5176013	5050771	14.658	14.850
2)	SA Decachlor...	10.096	8.441	3574563	2586642	7.544	8.466
Target Compounds							
7)	L1 AR-1016-5	0.000	5.032	0	463267	N.D.	42.860 #
15)	L3 AR-1232-5	0.000	5.032	0	463267	N.D.	115.771 #
20)	L4 AR-1242-5	6.416	0.000	330497	0	36.493	N.D. #
24)	L5 AR-1248-4	6.416	5.032	330497	463267	20.338	34.438 #
25)	L5 AR-1248-5	6.416	0.000	330497	0	21.404	N.D. #
26)	L6 AR-1254-1	6.416	0.000	330497	0	18.700	N.D. #
29)	L6 AR-1254-4	7.269	0.000	1026673	0	40.740	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100518\
Data File : PO049700.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Oct 2018 19:02
Operator : SM/SJ
Sample : J5223-03RE
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SSSI-1001-S-DH-01RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 22:54:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100118.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 02 05:32:25 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

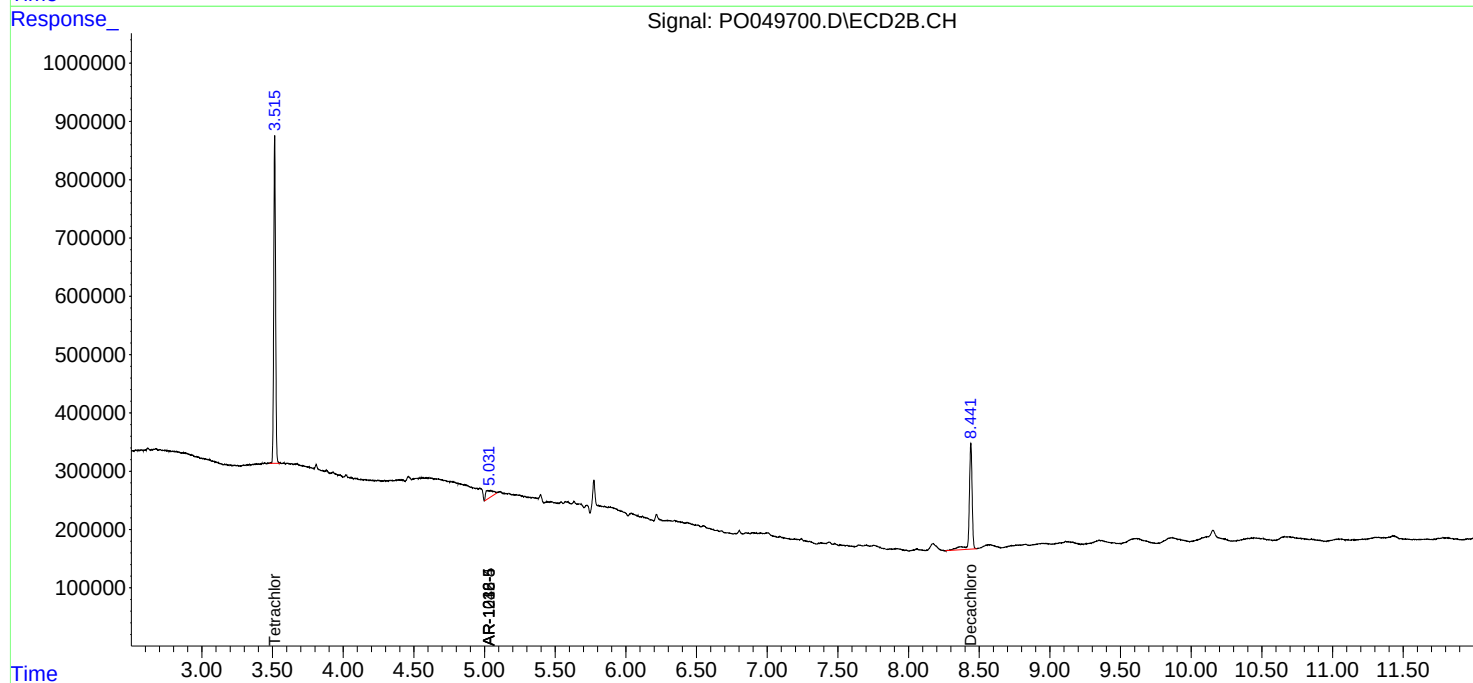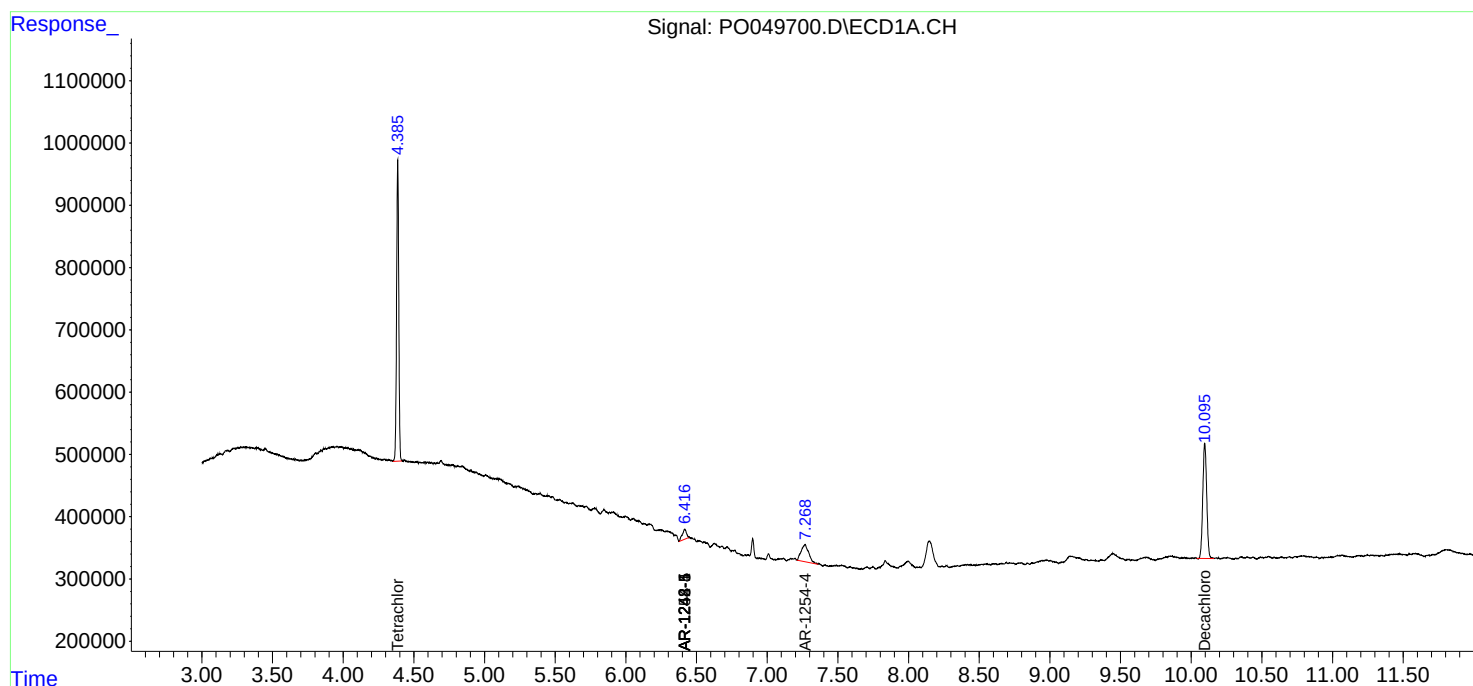


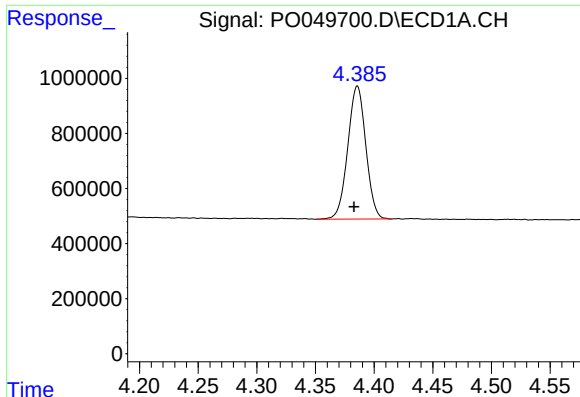

#1 Tetrachloro-m-xylene


R.T.: 4.386 min
Delta R.T.: 0.003 min
Response: 5176013
Conc: 14.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
SSSI-1001-S-DH-01RE

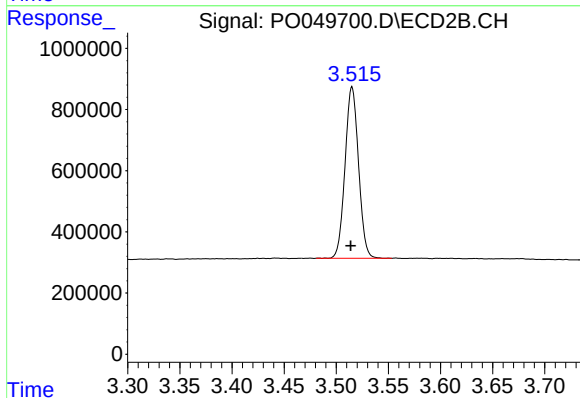


#1 Tetrachloro-m-xylene

R.T.: 3.515 min
Delta R.T.: 0.001 min
Response: 5050771
Conc: 14.85 ng/ml

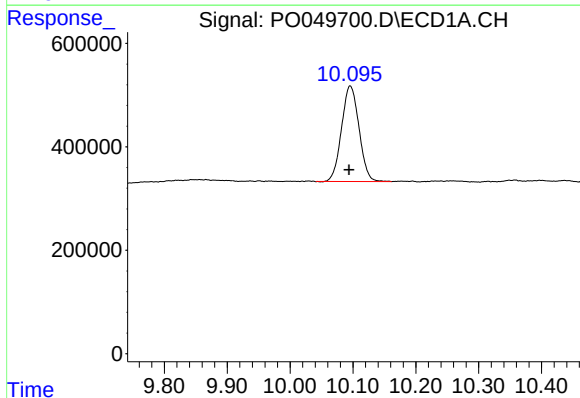


#2 Decachlorobiphenyl

R.T.: 10.096 min
Delta R.T.: 0.001 min
Response: 3574563
Conc: 7.54 ng/ml

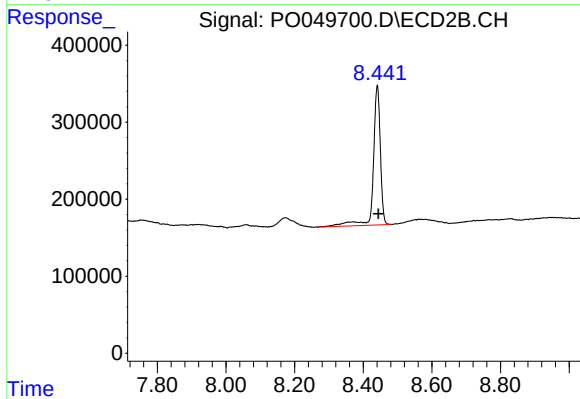

#2 Decachlorobiphenyl


R.T.: 8.441 min
Delta R.T.: -0.004 min
Response: 2586642
Conc: 8.47 ng/ml

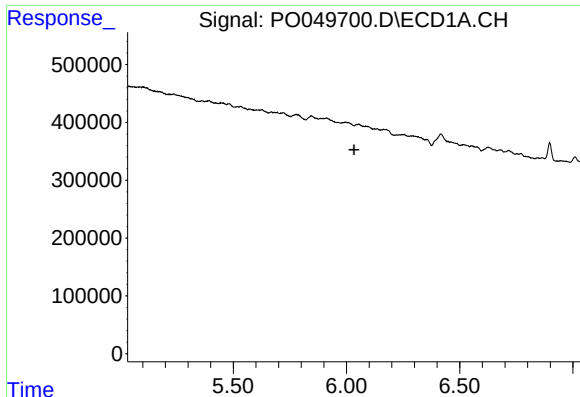

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T. : 6.033 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SSSI-1001-S-DH-01RE

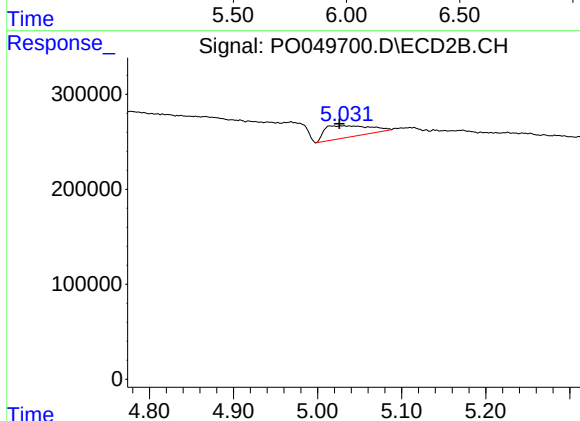


#7 AR-1016-5

R.T.: 5.032 min
Delta R.T.: 0.006 min
Response: 463267
Conc: 42.86 ng/ml

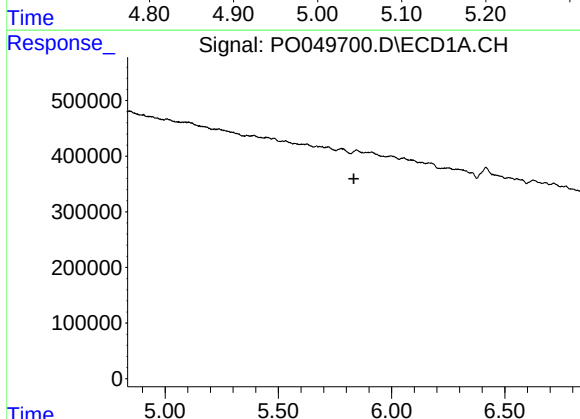


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 5.834 min
Response: 0
Conc: N.D.

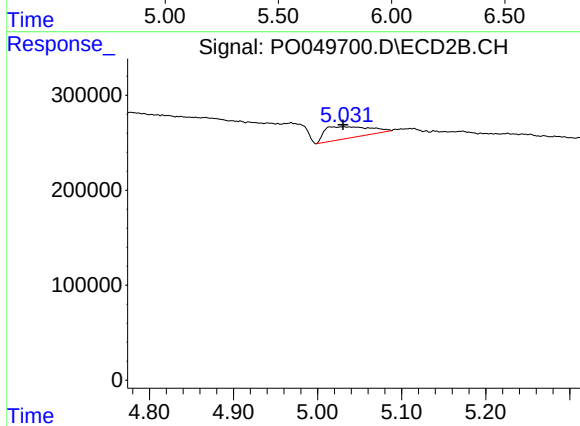

#15 AR-1232-5


R.T.: 5.032 min
Delta R.T.: 0.001 min
Response: 463267
Conc: 115.77 ng/ml

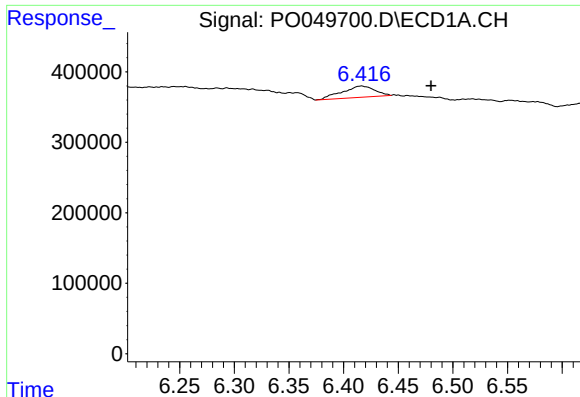

#20 AR-1242-5


R.T.: 6.416 min
Delta R.T.: -0.064 min
Response: 330497
Conc: 36.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
SSSI-1001-S-DH-01RE

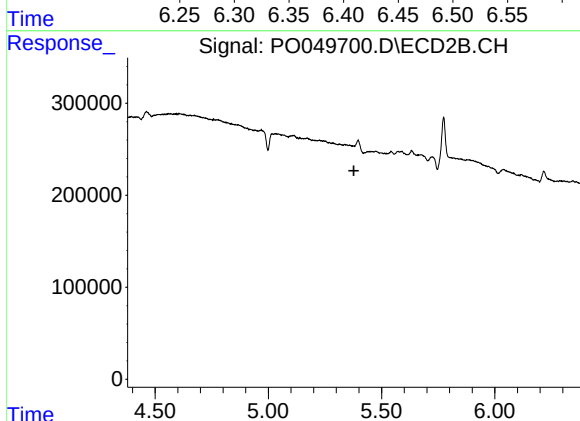


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 5.378 min
Response: 0
Conc: N.D.

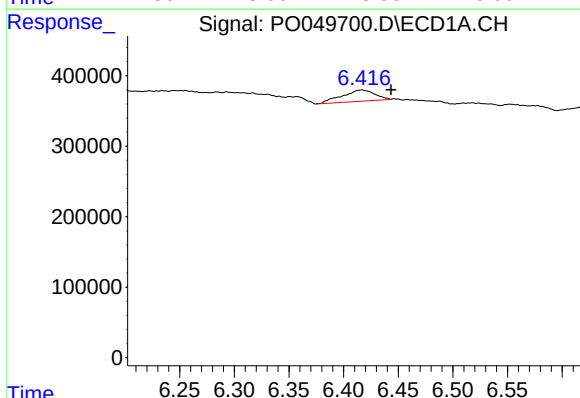


#24 AR-1248-4

R.T.: 6.416 min
Delta R.T.: -0.027 min
Response: 330497
Conc: 20.34 ng/ml

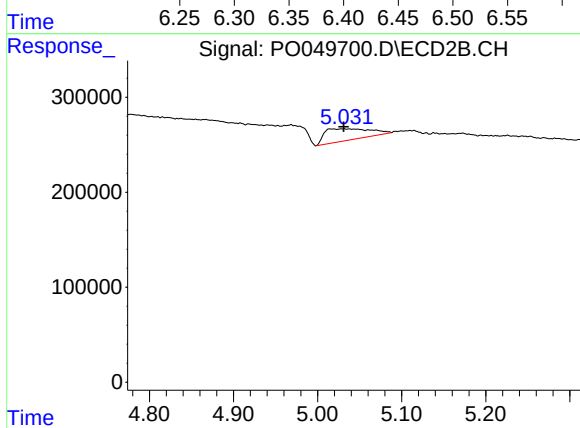

#24 AR-1248-4


R.T.: 5.032 min
Delta R.T.: 0.000 min
Response: 463267
Conc: 34.44 ng/ml

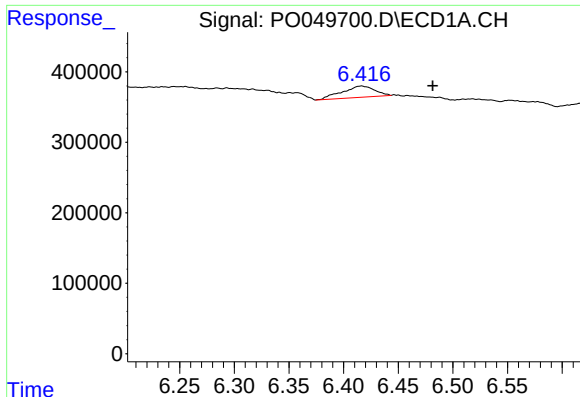

#25 AR-1248-5


R.T.: 6.416 min
Delta R.T.: -0.065 min
Response: 330497
Conc: 21.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
SSSI-1001-S-DH-01RE

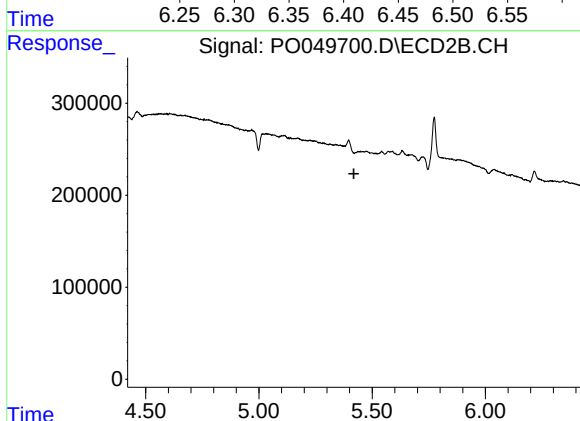


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.419 min
Response: 0
Conc: N.D.

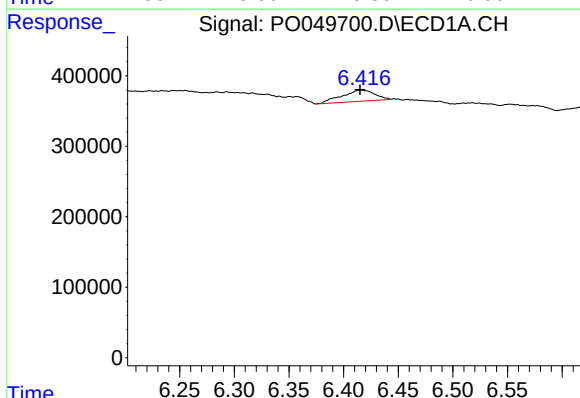


#26 AR-1254-1

R.T.: 6.416 min
Delta R.T.: 0.001 min
Response: 330497
Conc: 18.70 ng/ml

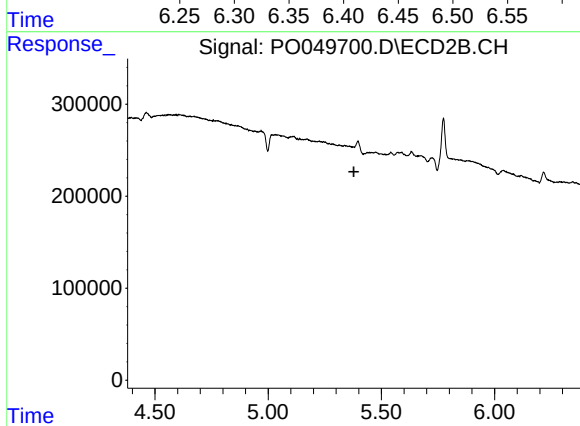

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.379 min
Response: 0
Conc: N.D.

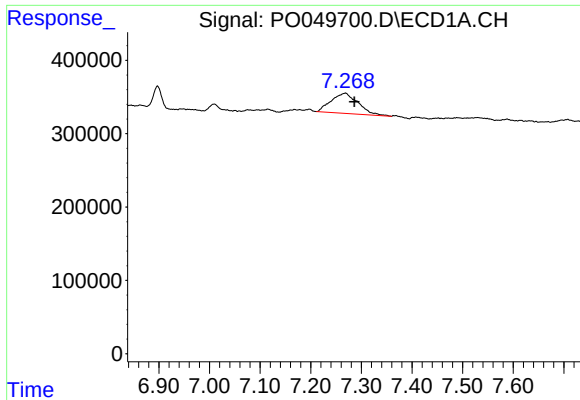

#29 AR-1254-4

R.T.: 7.269 min
Delta R.T.: -0.018 min
Response: 1026673
Conc: 40.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
SSSI-1001-S-DH-01RE

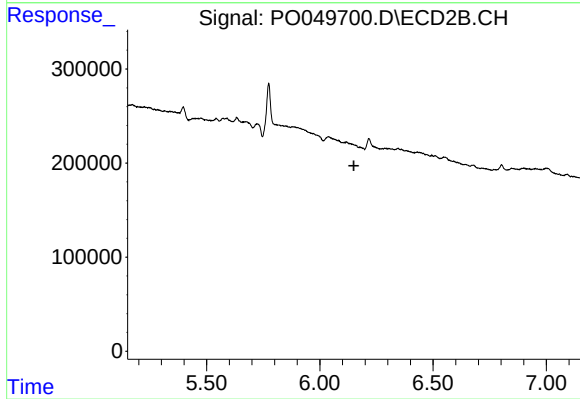

#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.151 min
Response: 0
Conc: N.D.