

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100518\
 Data File : P0049687.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Oct 2018 14:35
 Operator : SM/SJ
 Sample : J5192-03RE
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AU-05-100218-BRE

Manual Integrations
 APPROVED

Sohil
 10/9/2018 11:15:54 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 15:09:52 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 02 05:32:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.383	3.515	3148054	3446683	8.915m	10.134
2) SA Decachlor...	10.092	8.440	1893836	1125650	3.997m	3.684

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100518\
Data File : P0049687.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Oct 2018 14:35
Operator : SM/SJ
Sample : J5192-03RE
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AU-05-100218-BRE


Manual Integrations
APPROVED

Sohil
10/9/2018 11:15:54 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 15:09:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100118.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 02 05:32:25 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

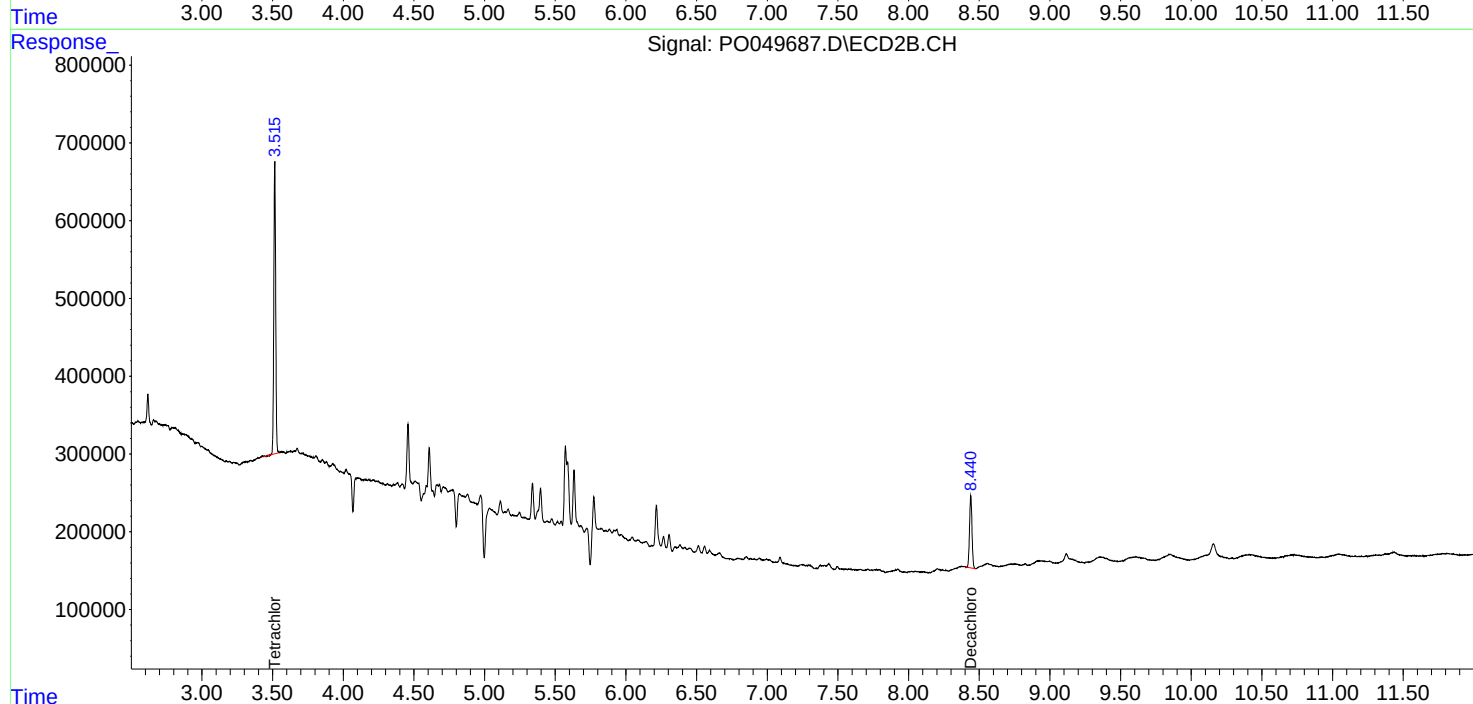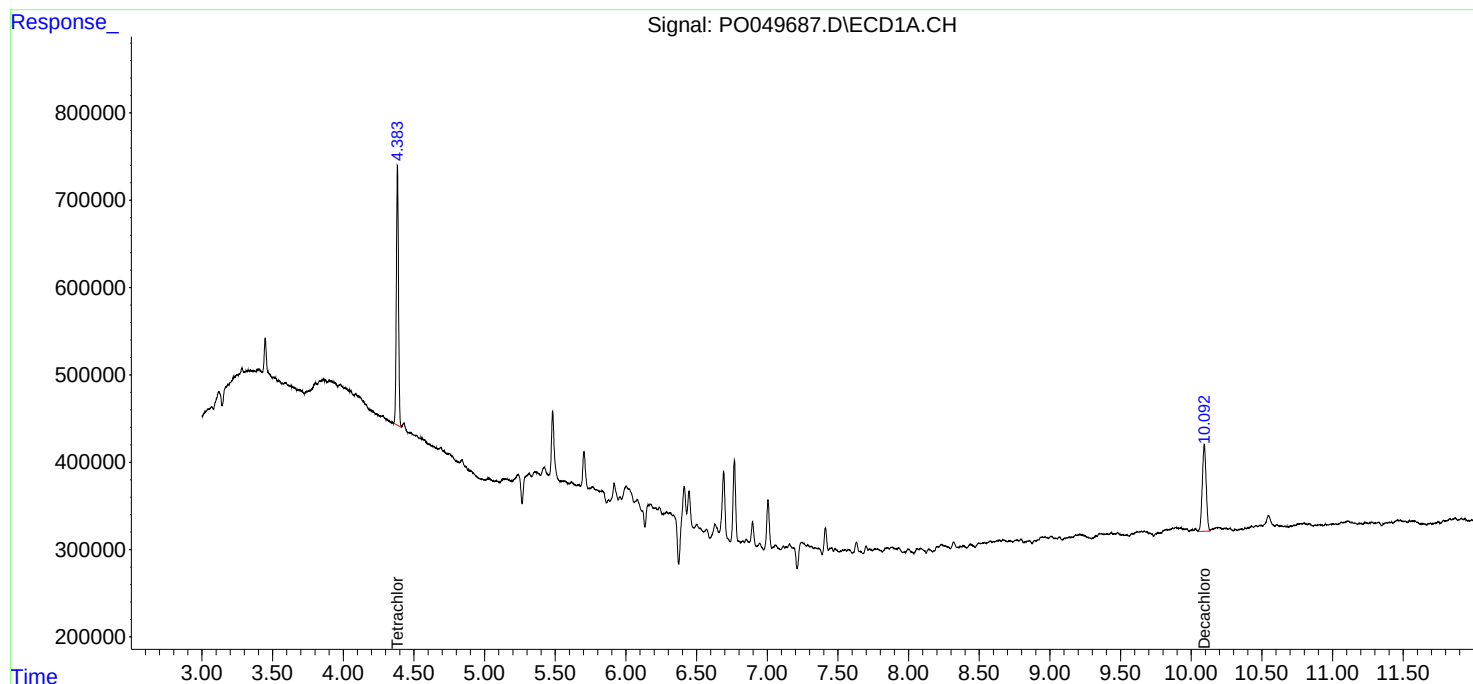

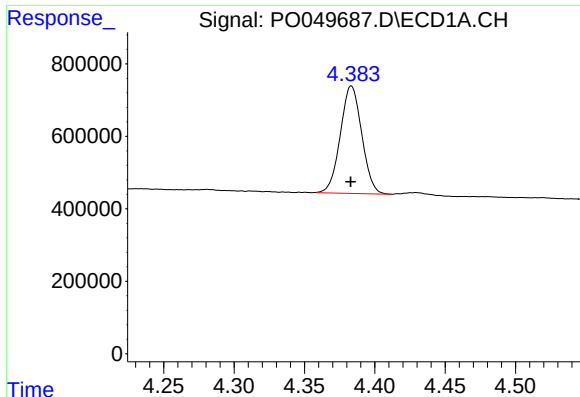


#1 Tetrachloro-m-xylene

R.T.: 4.383 min
Delta R.T.: 0.000 min
Response: 3148054
Conc: 8.91 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AU-05-100218-BRE


Manual Integrations
APPROVED

Sohil
10/9/2018 11:15:54 AM

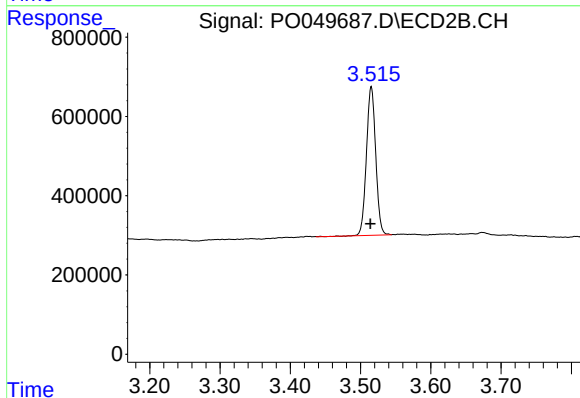


#1 Tetrachloro-m-xylene

R.T.: 3.515 min
Delta R.T.: 0.001 min
Response: 3446683
Conc: 10.13 ng/ml

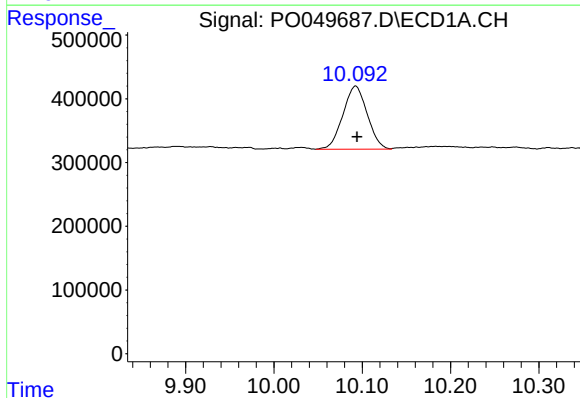

#2 Decachlorobiphenyl

R.T.: 10.092 min
Delta R.T.: -0.002 min
Response: 1893836
Conc: 4.00 ng/ml m

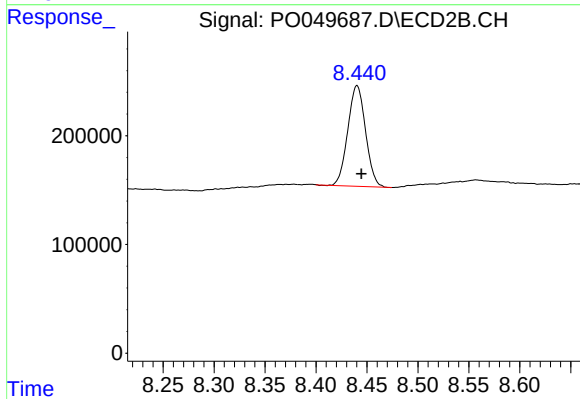

#2 Decachlorobiphenyl

R.T.: 8.440 min
Delta R.T.: -0.004 min
Response: 1125650
Conc: 3.68 ng/ml