

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100518\
 Data File : PO049714.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Oct 2018 22:45
 Operator : SM/SJ
 Sample : J5264-03
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 100318-SIDI-E-D-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 23:51:12 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 02 05:32:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.384	3.514	5968349	5487090	16.901	16.133
2)	SA Decachlor...	10.091	8.438	5315319	3701414	11.217	12.115

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100518\
Data File : PO049714.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Oct 2018 22:45
Operator : SM/SJ
Sample : J5264-03
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
100318-SIDI-E-D-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 23:51:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100118.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 02 05:32:25 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

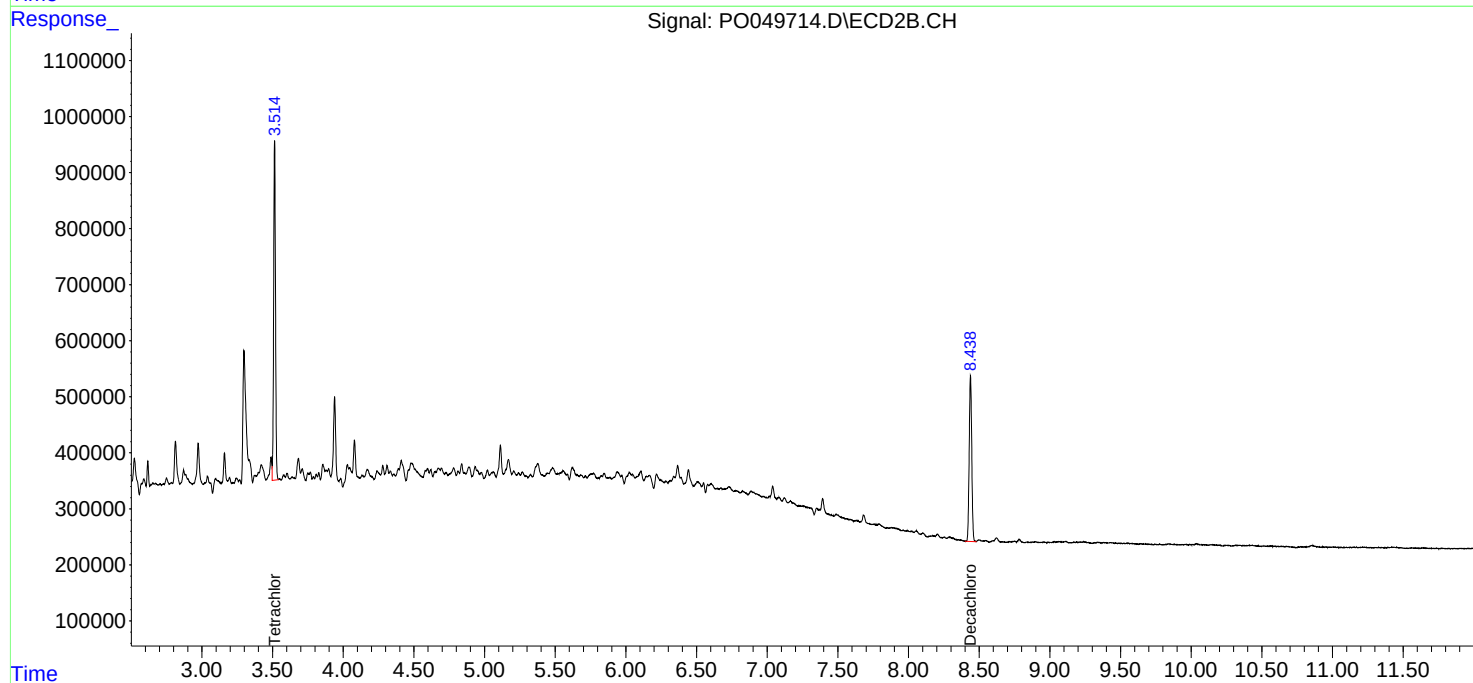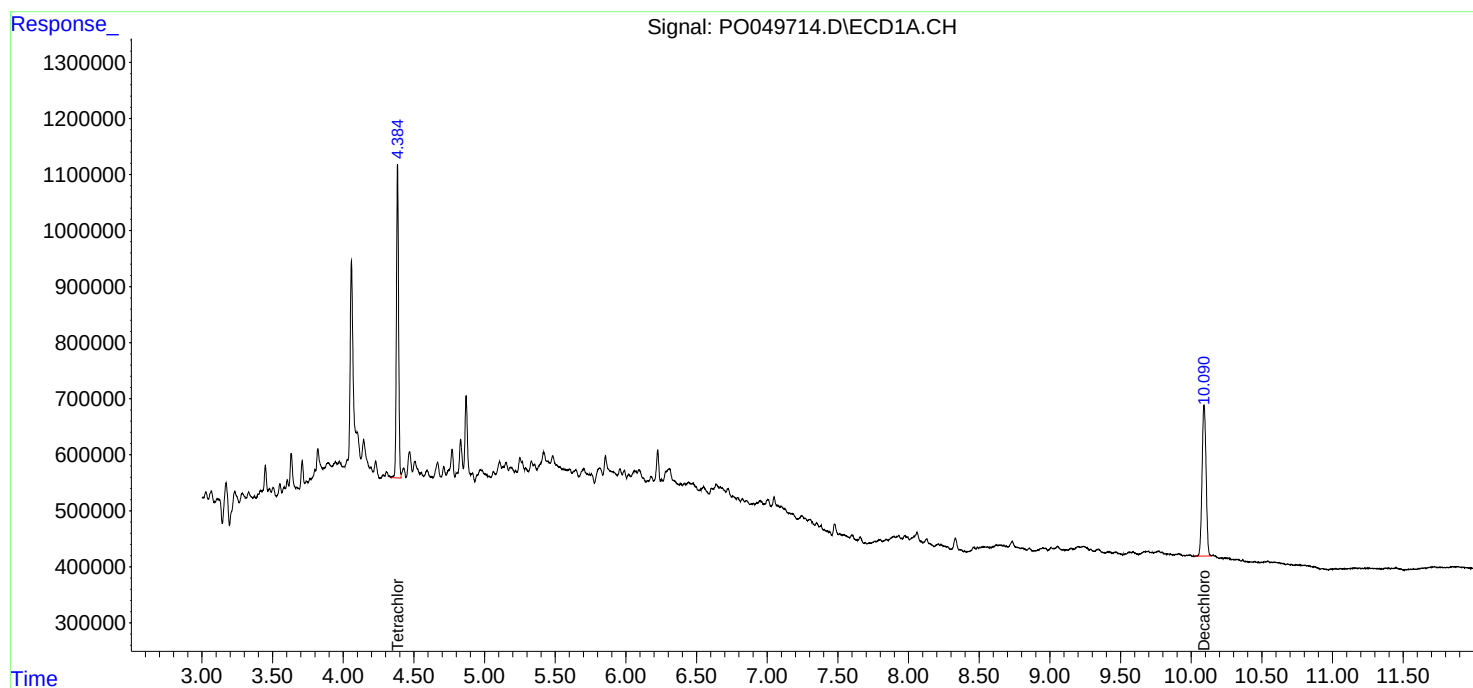


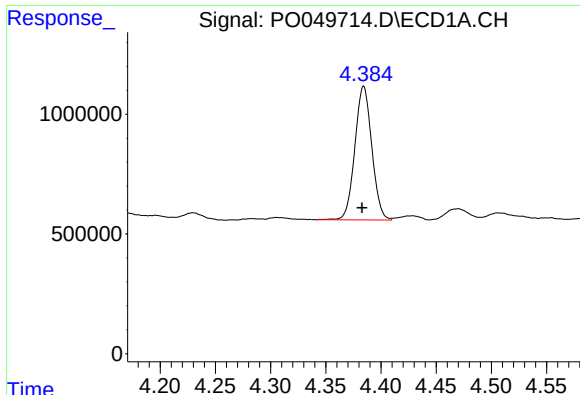

#1 Tetrachloro-m-xylene


R.T.: 4.384 min
Delta R.T.: 0.001 min
Response: 5968349
Conc: 16.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
100318-SIDI-E-D-S

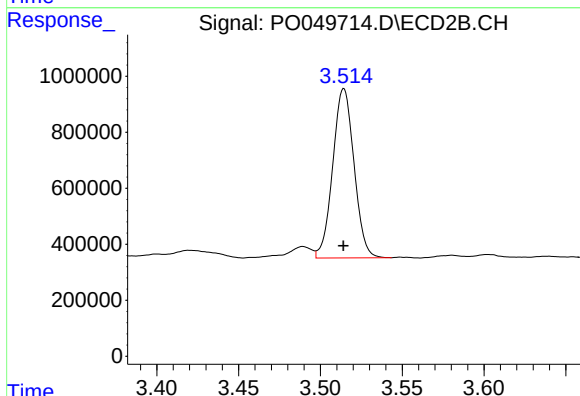


#1 Tetrachloro-m-xylene

R.T.: 3.514 min
Delta R.T.: 0.000 min
Response: 5487090
Conc: 16.13 ng/ml

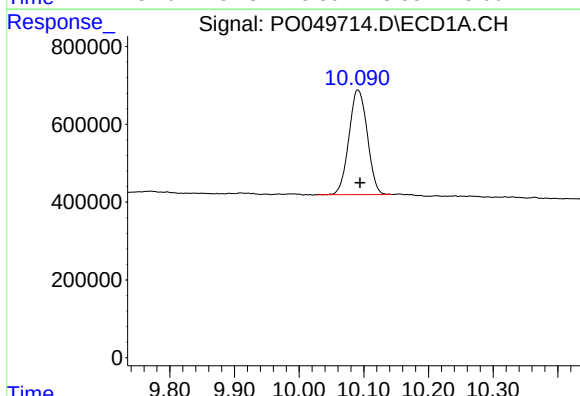

#2 Decachlorobiphenyl

R.T.: 10.091 min
Delta R.T.: -0.003 min
Response: 5315319
Conc: 11.22 ng/ml

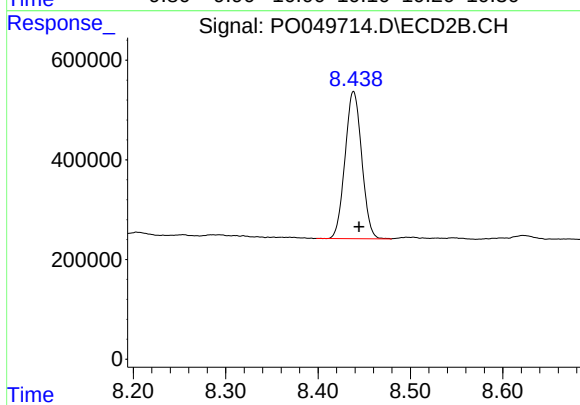

#2 Decachlorobiphenyl

R.T.: 8.438 min
Delta R.T.: -0.006 min
Response: 3701414
Conc: 12.11 ng/ml