

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100518\
Data File : PO049734.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Oct 2018 4:36
Operator : SM/SJ
Sample : J5264-07
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
100318-TIPC-E-D-M

Manual Integrations
APPROVED

Sonali
10/9/2018 11:17:47 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 04:49:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100118.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 02 05:32:25 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.385	3.514	5628828	5288561	15.940	15.549m
2) SA Decachlor...	10.092	8.439	4975170	3527551	10.499m	11.546

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100518\
Data File : PO049734.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Oct 2018 4:36
Operator : SM/SJ
Sample : J5264-07
Misc :
ALS Vial : 51 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
100318-TIPC-E-D-M


Manual Integrations
APPROVED

Sonni
10/9/2018 11:17:47 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 04:49:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100118.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 02 05:32:25 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

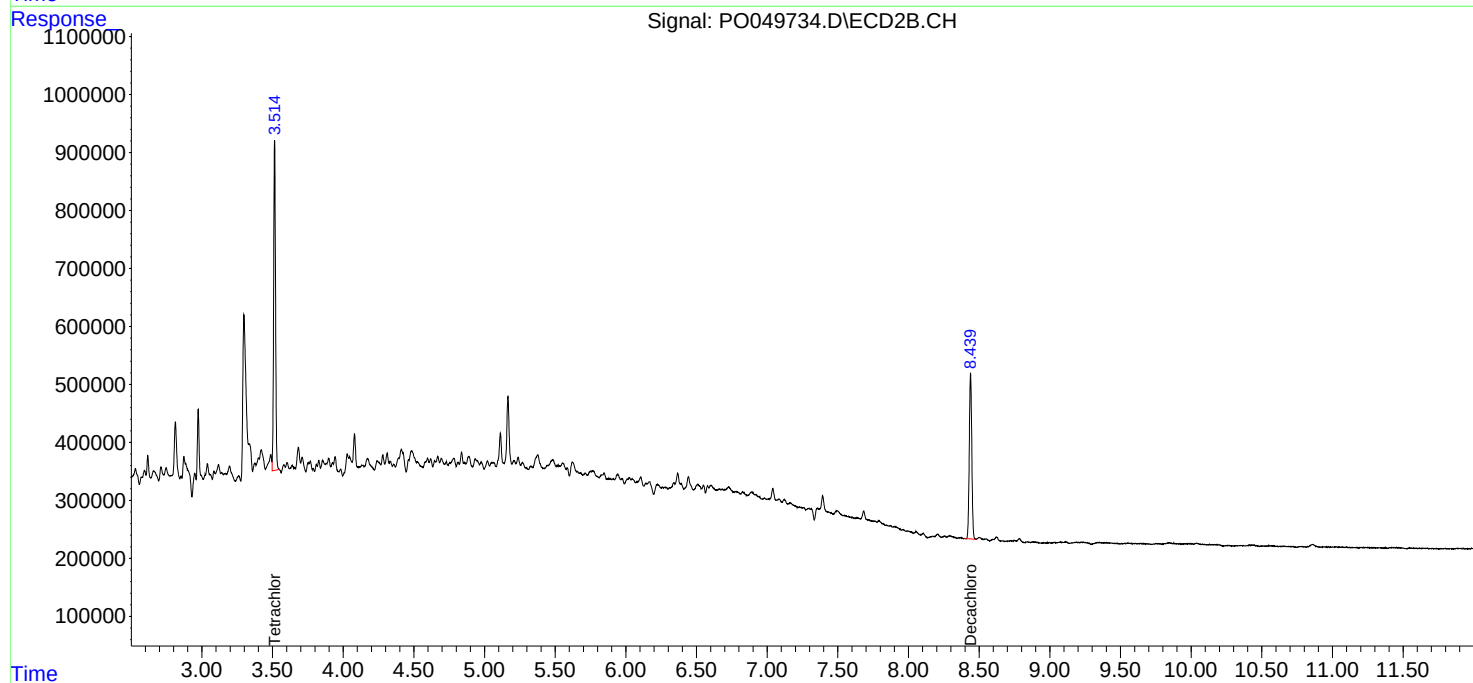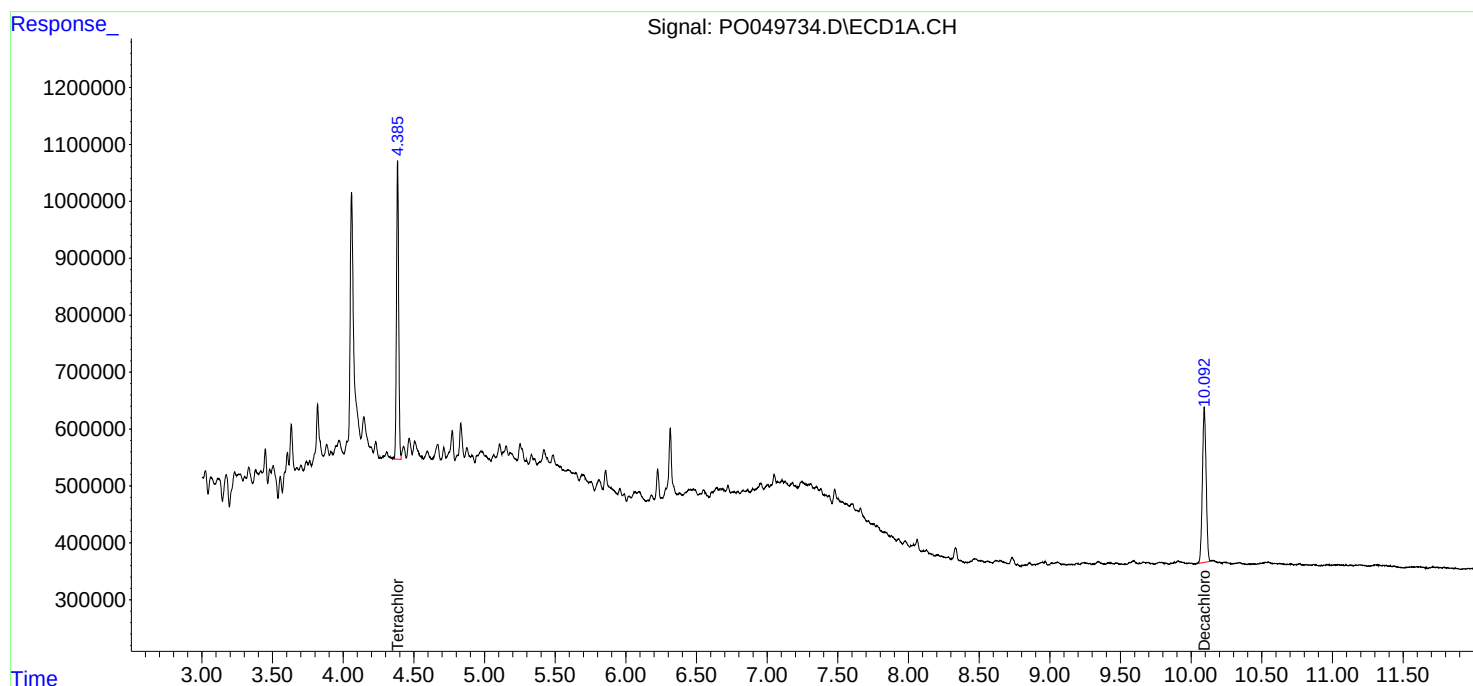

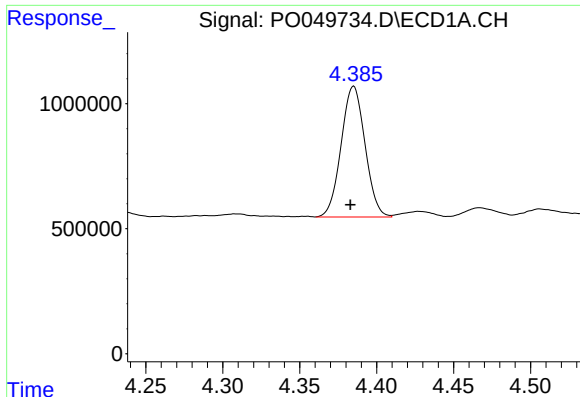


#1 Tetrachloro-m-xylene

R.T.: 4.385 min
Delta R.T.: 0.002 min
Response: 5628828
Conc: 15.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
100318-TIPC-E-D-M


Manual Integrations
APPROVED

Sonni
10/9/2018 11:17:47 AM

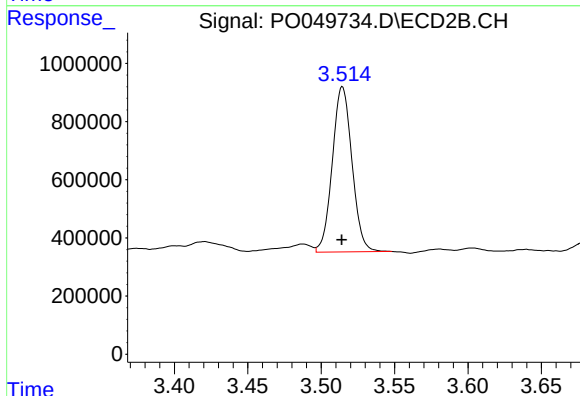


#1 Tetrachloro-m-xylene

R.T.: 3.514 min
Delta R.T.: 0.000 min
Response: 5288561
Conc: 15.55 ng/ml m

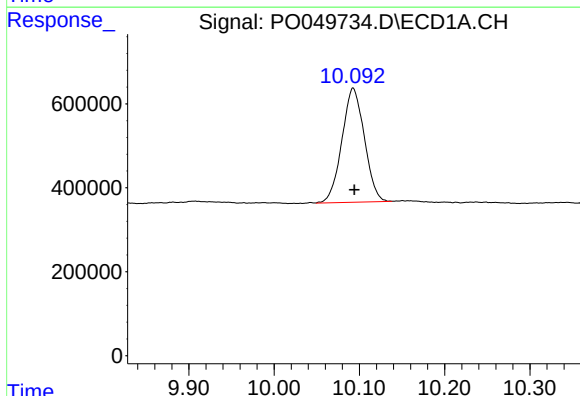

#2 Decachlorobiphenyl

R.T.: 10.092 min
Delta R.T.: -0.002 min
Response: 4975170
Conc: 10.50 ng/ml m

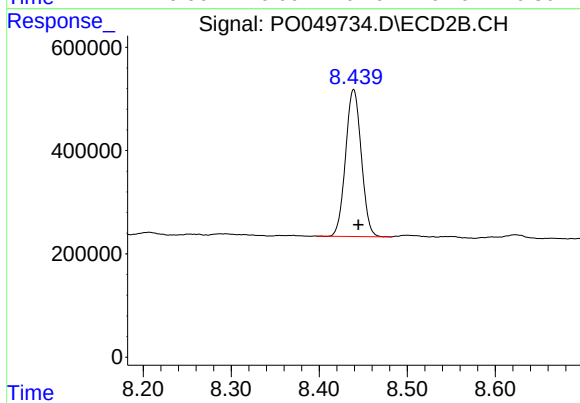

#2 Decachlorobiphenyl

R.T.: 8.439 min
Delta R.T.: -0.005 min
Response: 3527551
Conc: 11.55 ng/ml