

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100520\
 Data File : PO071973.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Oct 2020 13:02
 Operator : DD\AJ
 Sample : L4200-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB-2020-WS-000-01

Manual Integrations
 APPROVED

Ankita
 10/6/2020 12:16:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 01:05:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.327	3.511	1551798	806116	21.605	21.522
2) SA Decachlor...	9.936	8.684	1876624	1018503	17.044	17.906
Target Compounds						
26) L6 AR-1254-1	6.522	5.586	187456	148039	53.655	61.945
27) L6 AR-1254-2	6.749	5.747	311915	126948	56.655	59.350
28) L6 AR-1254-3	7.125	6.155	342616	225121	59.326	66.306
29) L6 AR-1254-4	7.420	6.396	382169	184259	65.598	75.884
30) L6 AR-1254-5	7.841	6.816	309254	174154	57.462m	53.224

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100520\
Data File : P0071973.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Oct 2020 13:02
Operator : DD\AJ
Sample : L4200-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB-2020-WS-000-01


Manual Integrations
APPROVED

Ankita
10/6/2020 12:16:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 01:05:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

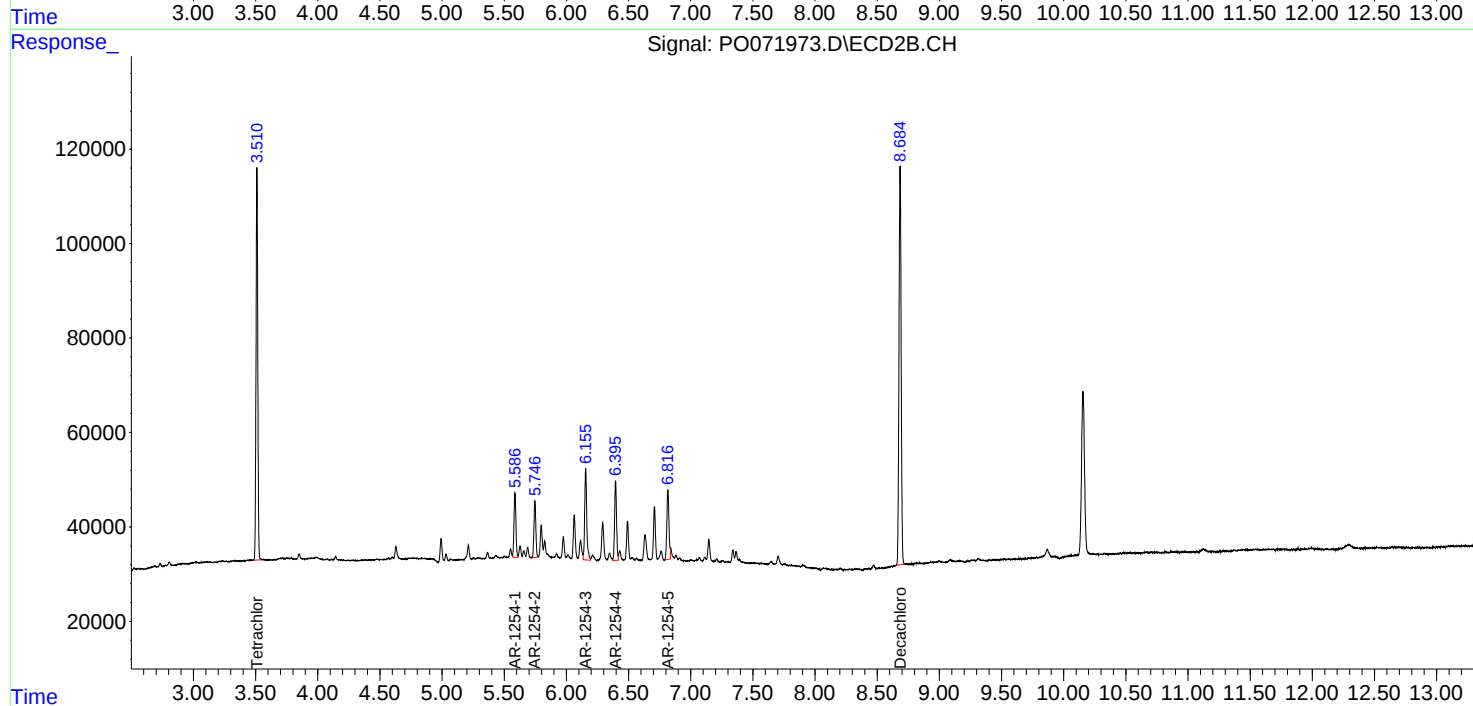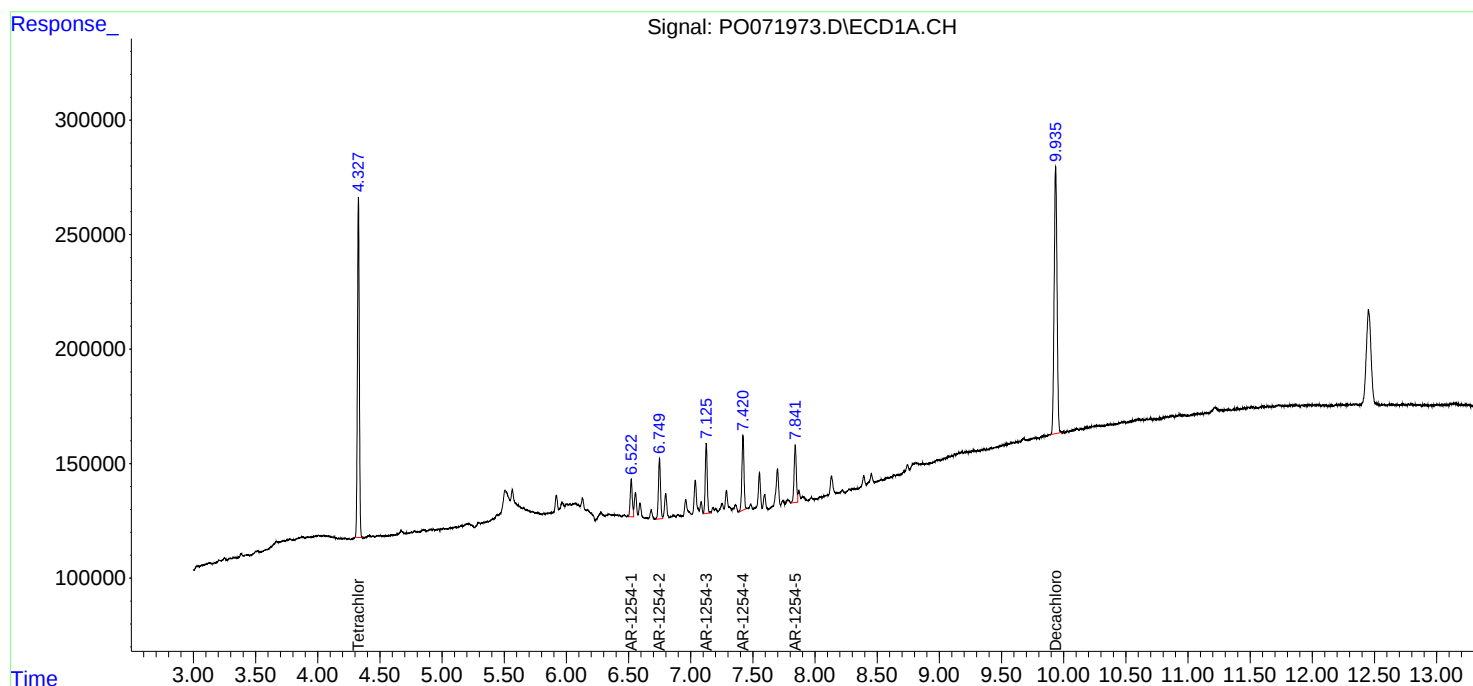

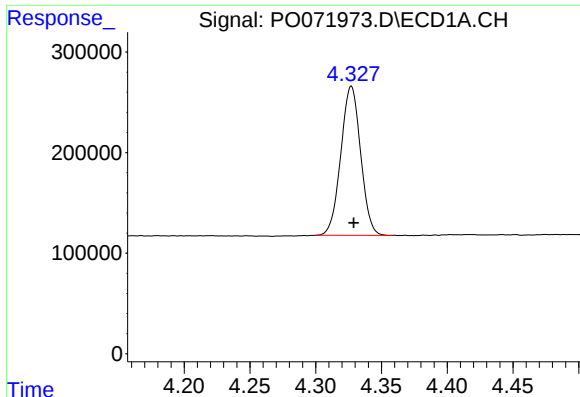


#1 Tetrachloro-m-xylene

R.T.: 4.327 min
Delta R.T.: -0.002 min
Response: 1551798
Conc: 21.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB-2020-WS-000-01


Manual Integrations
APPROVED

Ankita
10/6/2020 12:16:55 PM

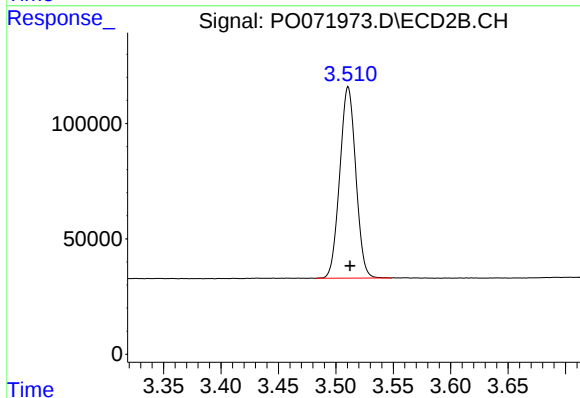


#1 Tetrachloro-m-xylene

R.T.: 3.511 min
Delta R.T.: -0.002 min
Response: 806116
Conc: 21.52 ng/ml

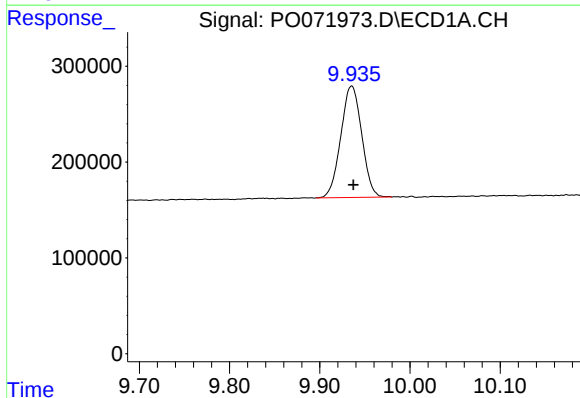


#2 Decachlorobiphenyl

R.T.: 9.936 min
Delta R.T.: -0.002 min
Response: 1876624
Conc: 17.04 ng/ml

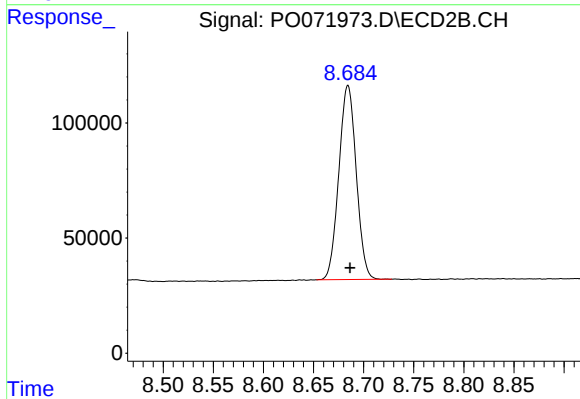

#2 Decachlorobiphenyl

R.T.: 8.684 min
Delta R.T.: -0.002 min
Response: 1018503
Conc: 17.91 ng/ml

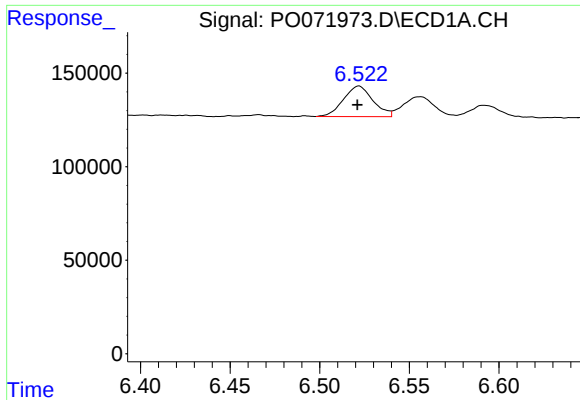


#26 AR-1254-1

R.T.: 6.522 min
Delta R.T.: 0.000 min
Response: 187456
Conc: 53.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB-2020-WS-000-01


Manual Integrations
APPROVED

Ankita
10/6/2020 12:16:55 PM

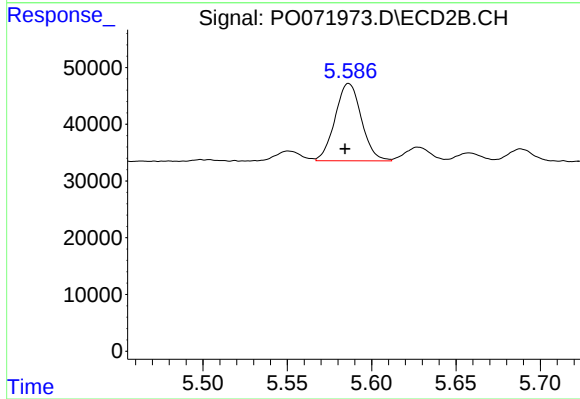


#26 AR-1254-1

R.T.: 5.586 min
Delta R.T.: 0.002 min
Response: 148039
Conc: 61.95 ng/ml

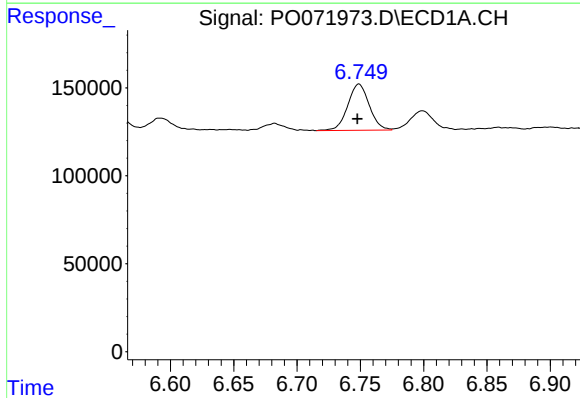


#27 AR-1254-2

R.T.: 6.749 min
Delta R.T.: 0.001 min
Response: 311915
Conc: 56.65 ng/ml

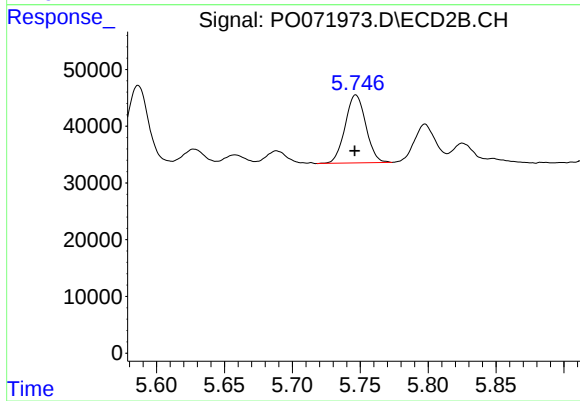

#27 AR-1254-2

R.T.: 5.747 min
Delta R.T.: 0.000 min
Response: 126948
Conc: 59.35 ng/ml

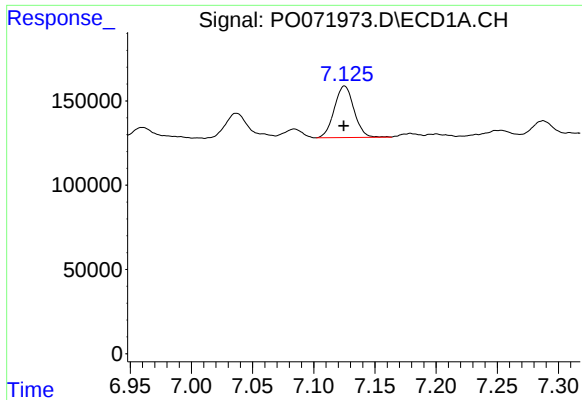


#28 AR-1254-3

R.T.: 7.125 min
Delta R.T.: 0.000 min
Response: 342616
Conc: 59.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB-2020-WS-000-01


Manual Integrations
APPROVED

Ankita
10/6/2020 12:16:55 PM

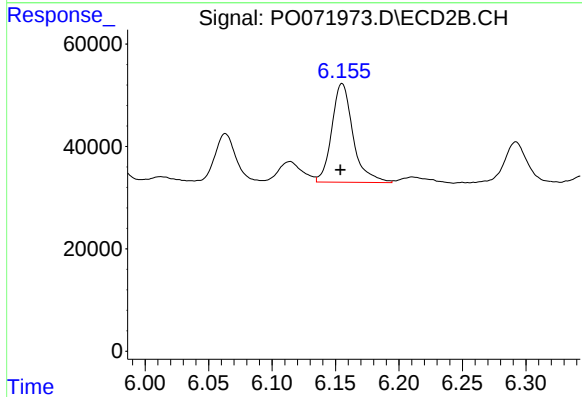


#28 AR-1254-3

R.T.: 6.155 min
Delta R.T.: 0.001 min
Response: 225121
Conc: 66.31 ng/ml

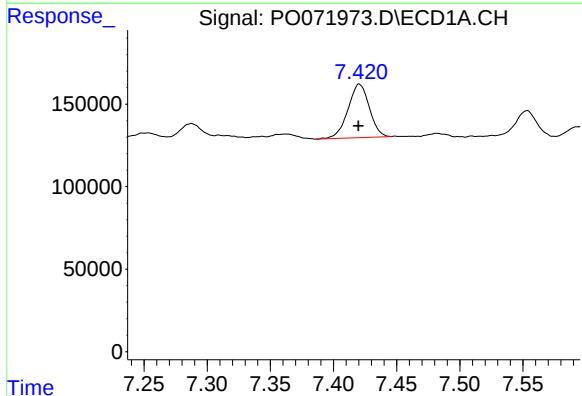


#29 AR-1254-4

R.T.: 7.420 min
Delta R.T.: 0.000 min
Response: 382169
Conc: 65.60 ng/ml

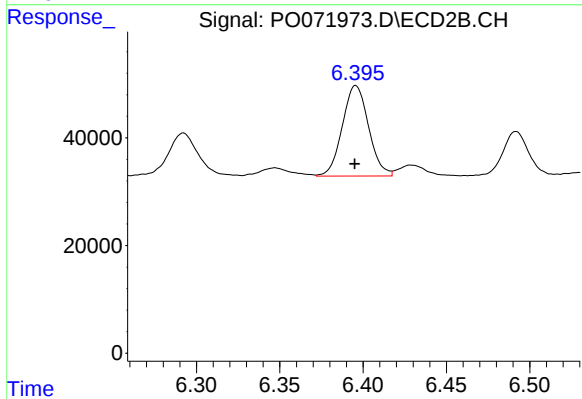

#29 AR-1254-4

R.T.: 6.396 min
Delta R.T.: 0.000 min
Response: 184259
Conc: 75.88 ng/ml

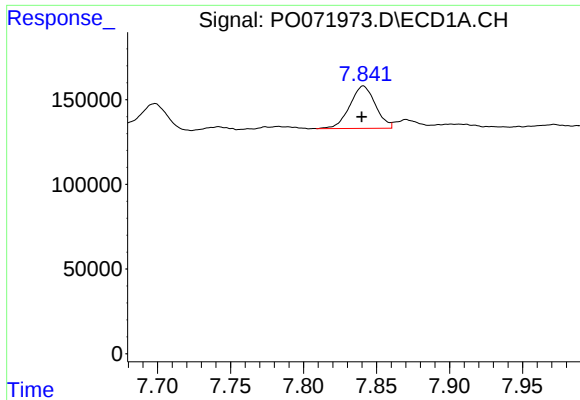


#30 AR-1254-5

R.T.: 7.841 min
Delta R.T.: 0.000 min
Response: 309254
Conc: 57.46 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PB-2020-WS-000-01

Manual Integrations
APPROVED

Ankita
10/6/2020 12:16:55 PM

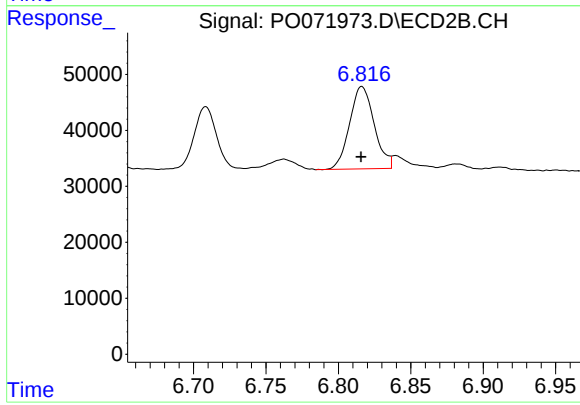

#30 AR-1254-5

R.T.: 6.816 min
Delta R.T.: 0.000 min
Response: 174154
Conc: 53.22 ng/ml