

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100520\
 Data File : PO072012.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Oct 2020 00:09
 Operator : DD\AJ
 Sample : L4260-11
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PAV-B23-100220-0-10

Manual Integrations
 APPROVED

Ankita
 10/6/2020 12:17:16 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 01:21:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.326	3.510	1979922	943441	27.566m	25.188
2) SA Decachlor...	9.934	8.683	2114326	981204	19.202	17.251

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100520\
Data File : PO072012.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Oct 2020 00:09
Operator : DD\AJ
Sample : L4260-11
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PAV-B23-100220-0-10


Manual Integrations
APPROVED

Ankita
10/6/2020 12:17:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 01:21:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

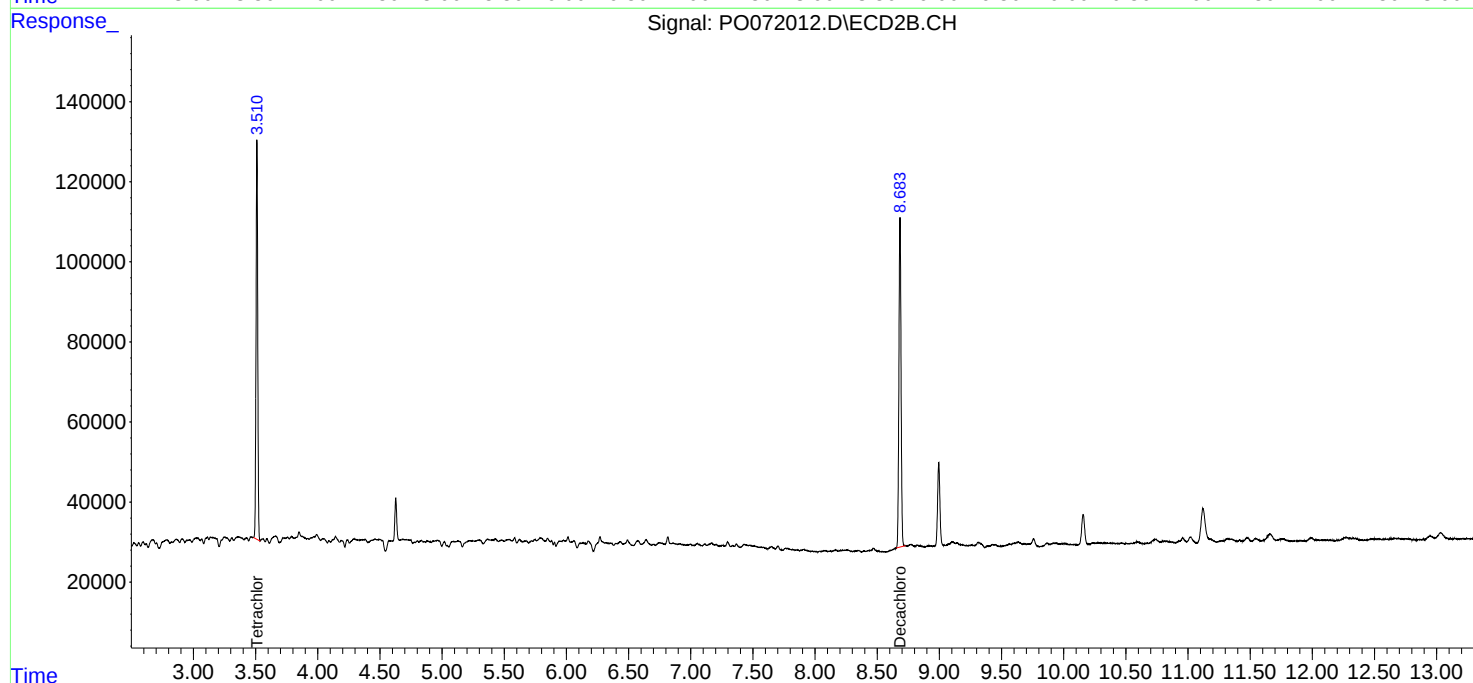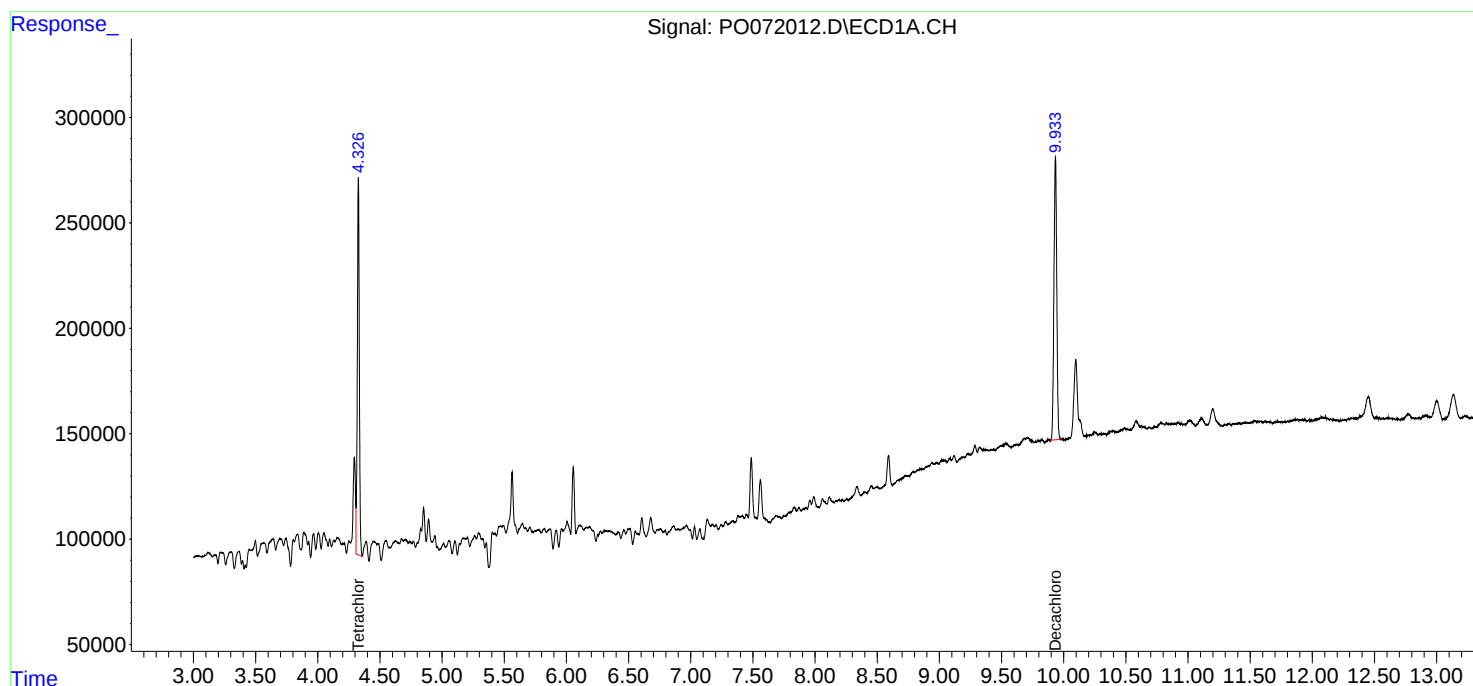

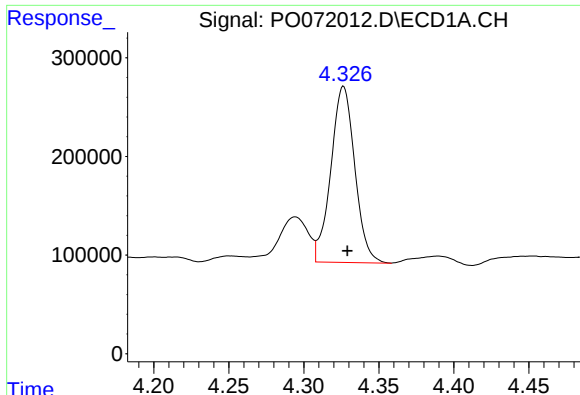

#1 Tetrachloro-m-xylene

R.T.: 4.326 min

Delta R.T.: -0.003 min


Response: 1979922

Conc: 27.57 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PAV-B23-100220-0-10

Manual Integrations
APPROVED

Ankita
10/6/2020 12:17:16 PM

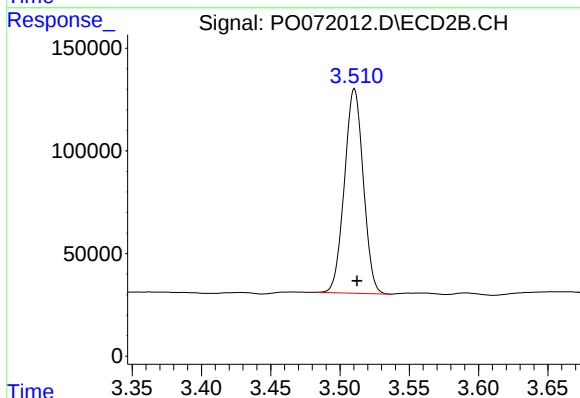


#1 Tetrachloro-m-xylene

R.T.: 3.510 min

Delta R.T.: -0.002 min

Response: 943441

Conc: 25.19 ng/ml

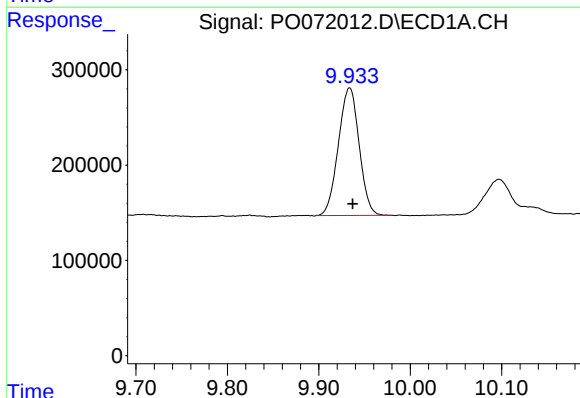


#2 Decachlorobiphenyl

R.T.: 9.934 min

Delta R.T.: -0.003 min

Response: 2114326

Conc: 19.20 ng/ml

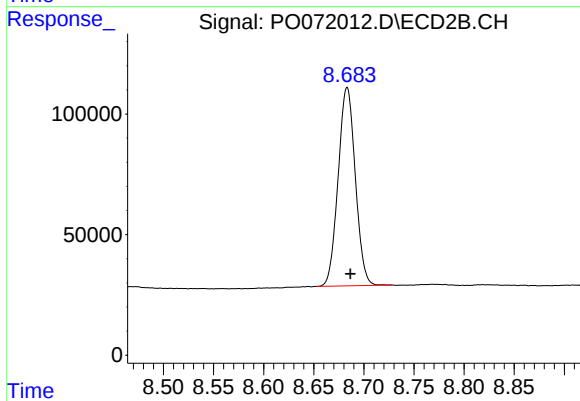

#2 Decachlorobiphenyl

R.T.: 8.683 min

Delta R.T.: -0.003 min

Response: 981204

Conc: 17.25 ng/ml