

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100520\
 Data File : PO072015.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Oct 2020 1:00
 Operator : DD\AJ
 Sample : L4247-11
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 B-18(0-1)

Manual Integrations
 APPROVED

Ankita
 10/6/2020 12:17:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 05:48:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.329	3.513	1719924	823967	23.946m	21.998
2) SA Decachlor...	9.935	8.685	1940217	895319	17.621	15.741

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100520\
Data File : PO072015.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Oct 2020 1:00
Operator : DD\AJ
Sample : L4247-11
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
B-18(0-1)


Manual Integrations
APPROVED

Ankita
10/6/2020 12:17:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 05:48:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

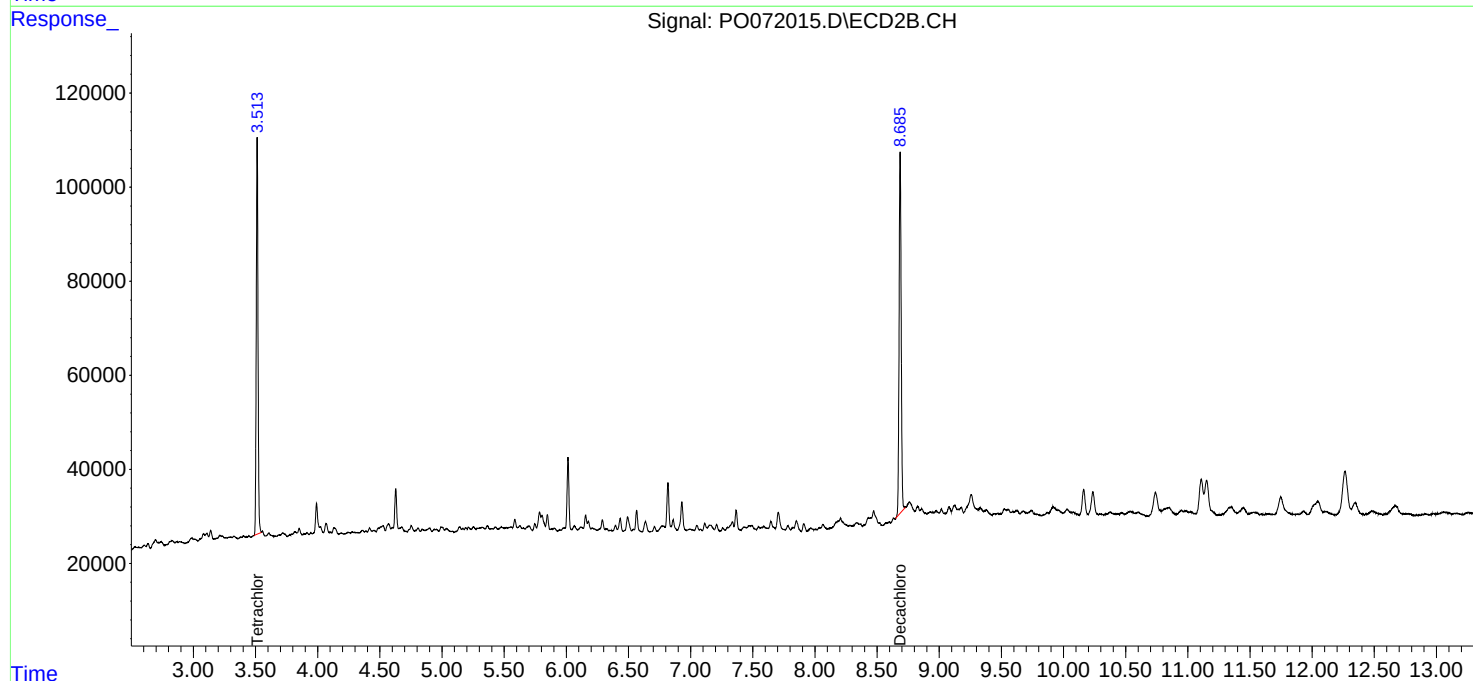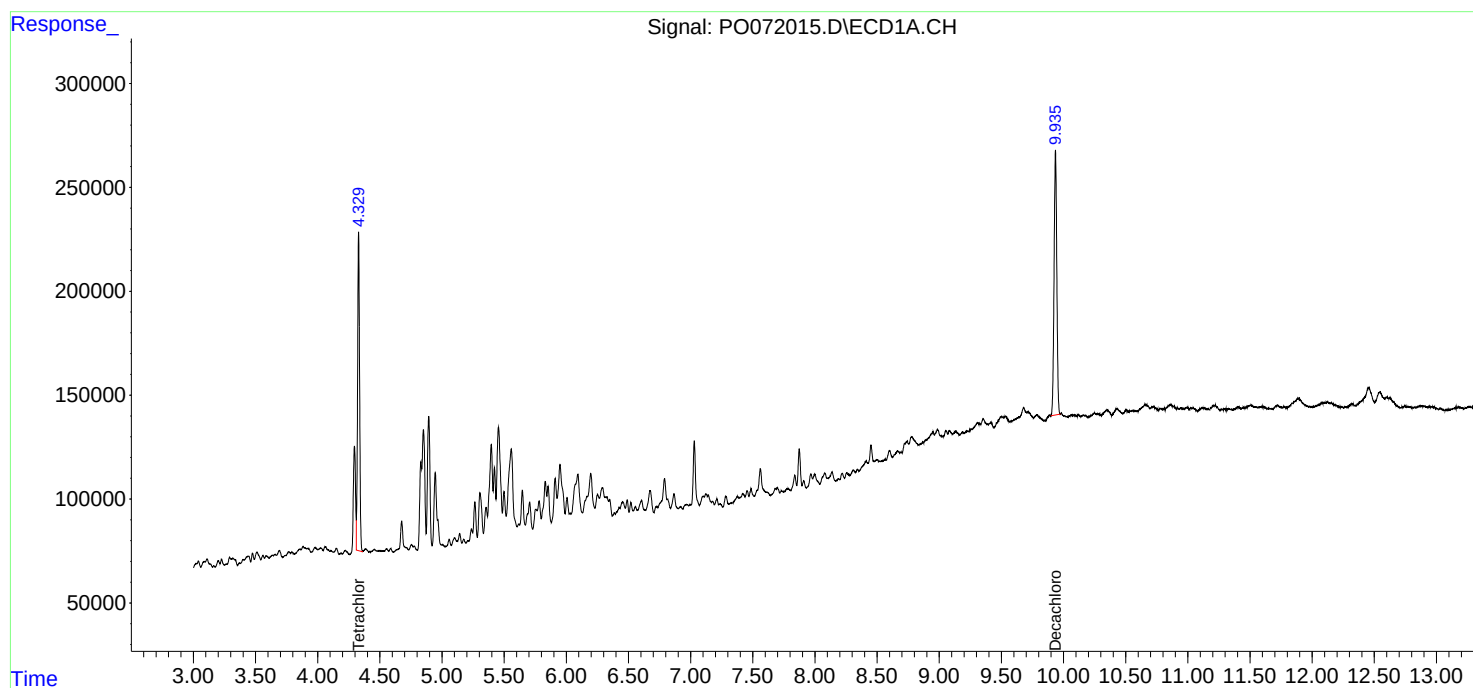

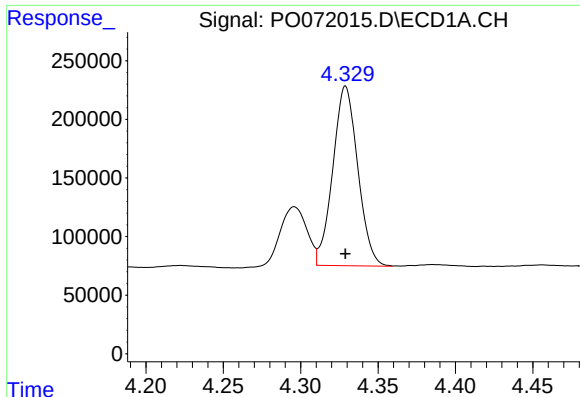


#1 Tetrachloro-m-xylene

R.T.: 4.329 min
Delta R.T.: 0.000 min
Response: 1719924
Conc: 23.95 ng/ml m

Instrument :
ECD_O
ClientSampleId :
B-18(0-1)


Manual Integrations
APPROVED

Ankita
10/6/2020 12:17:47 PM

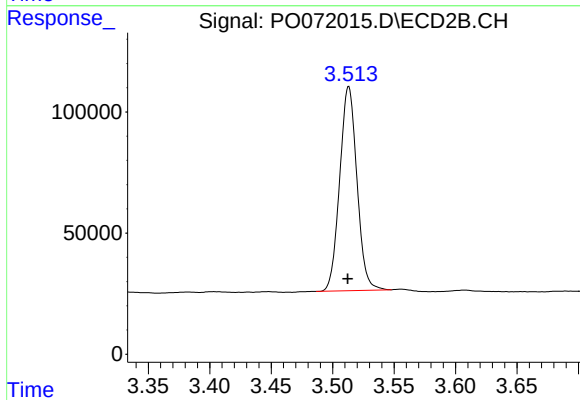


#1 Tetrachloro-m-xylene

R.T.: 3.513 min
Delta R.T.: 0.000 min
Response: 823967
Conc: 22.00 ng/ml

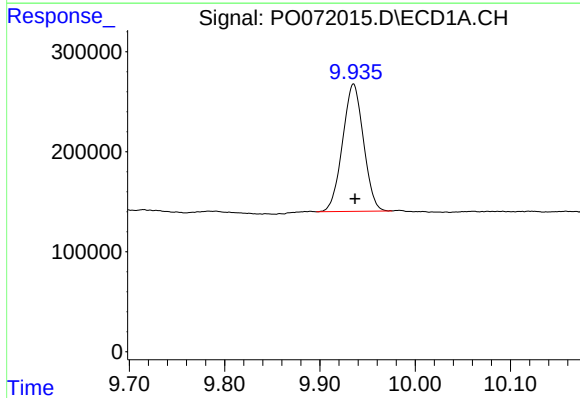

#2 Decachlorobiphenyl

R.T.: 9.935 min
Delta R.T.: -0.002 min
Response: 1940217
Conc: 17.62 ng/ml

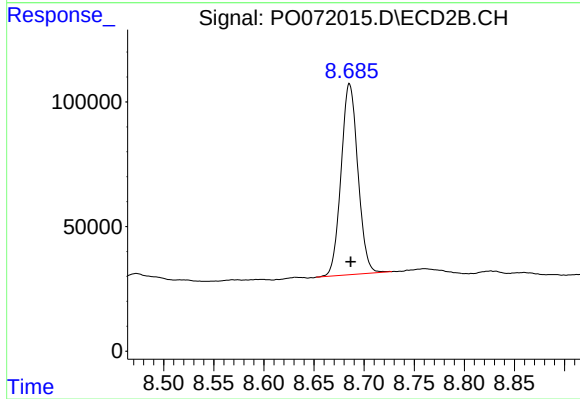

#2 Decachlorobiphenyl

R.T.: 8.685 min
Delta R.T.: -0.001 min
Response: 895319
Conc: 15.74 ng/ml