

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100520\
 Data File : PO072016.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Oct 2020 1:17
 Operator : DD\AJ
 Sample : L4219-01
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CL-01-100120

Manual Integrations
 APPROVED

Ankita
 10/6/2020 12:17:32 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 05:48:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.326	3.511	1680239	941649	23.393m	25.140
2)	SA Decachlor...	9.933	8.684	1701089	812883	15.449	14.291
Target Compounds							
26)	L6 AR-1254-1	6.520	5.585	610812	461682	174.830	193.185
27)	L6 AR-1254-2	6.748	5.746	996082	411252	180.924	192.267
28)	L6 AR-1254-3	7.124	6.155	1119134	642856	193.784	189.345
29)	L6 AR-1254-4	7.419	6.396	1115036	504479	191.391	207.761
30)	L6 AR-1254-5	7.840	6.817	1077503	637957	200.210	194.968

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100520\
Data File : PO072016.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Oct 2020 1:17
Operator : DD\AJ
Sample : L4219-01
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
CL-01-100120


Manual Integrations
APPROVED

Ankita
10/6/2020 12:17:32 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 05:48:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

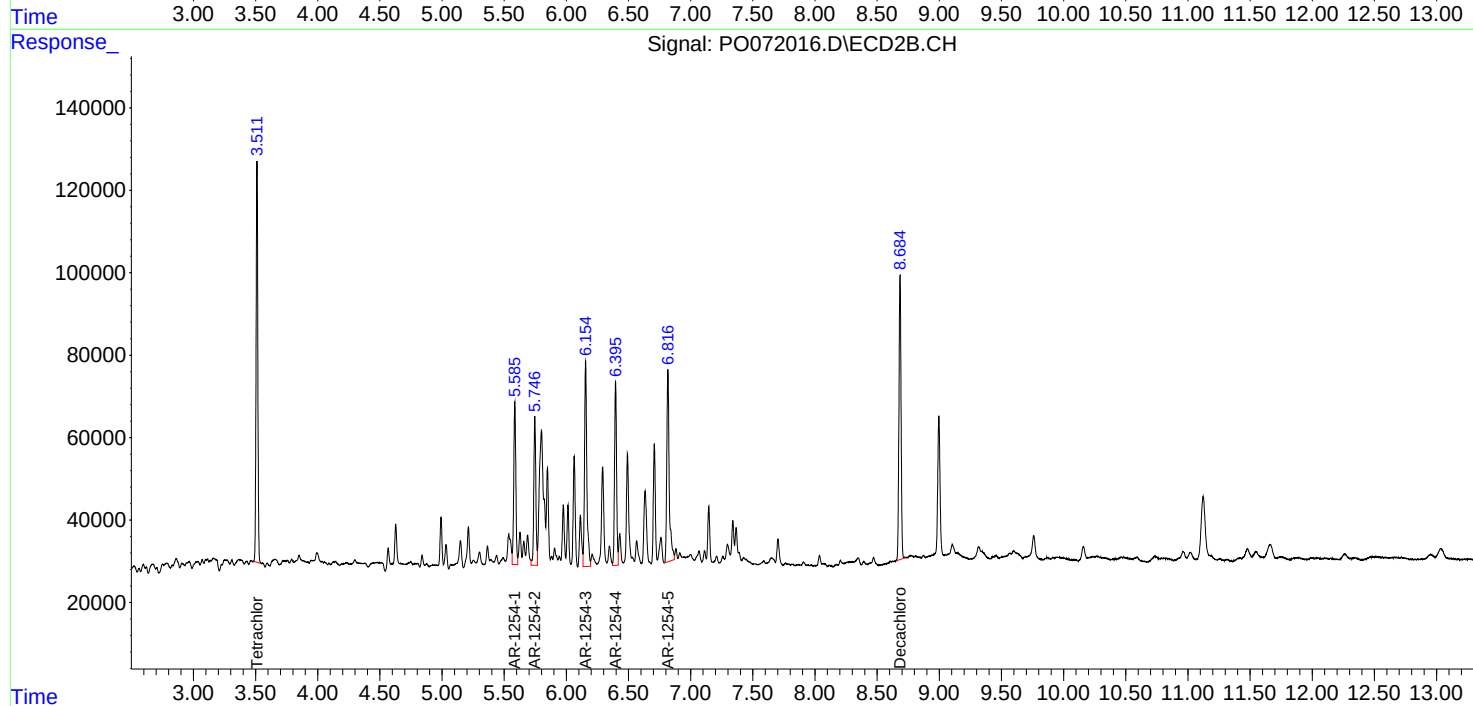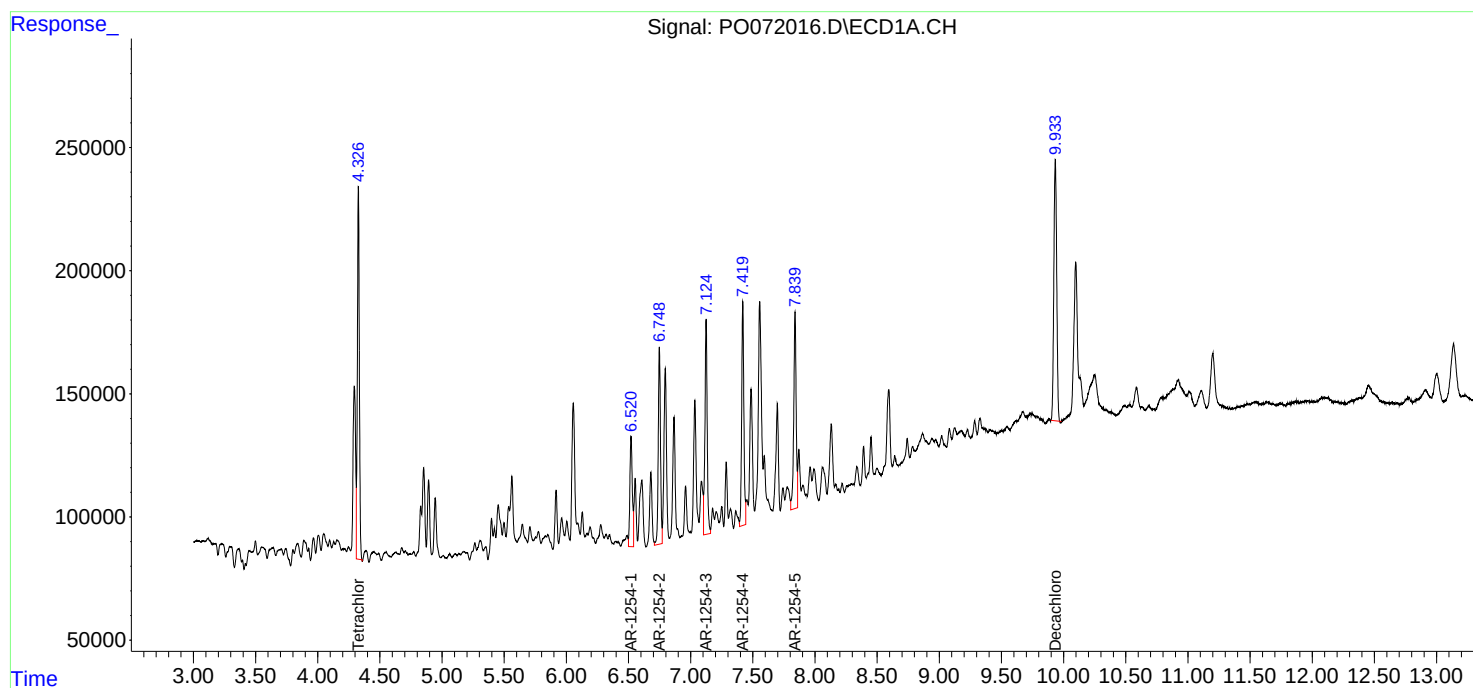

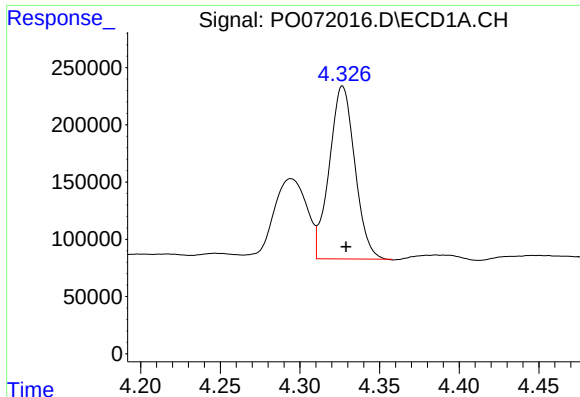

#1 Tetrachloro-m-xylene

R.T.: 4.326 min

Delta R.T.: -0.003 min


Response: 1680239

Conc: 23.39 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CL-01-100120

Manual Integrations
APPROVED

Ankita
10/6/2020 12:17:32 PM

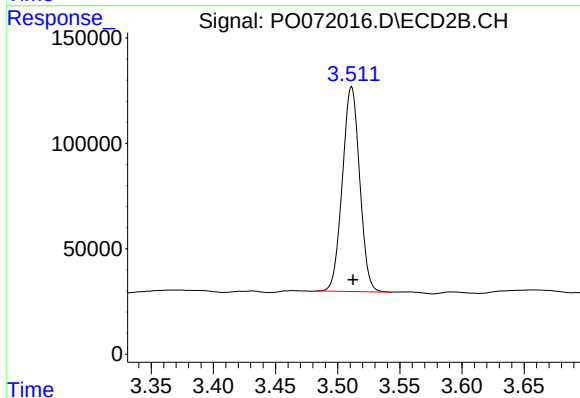


#1 Tetrachloro-m-xylene

R.T.: 3.511 min

Delta R.T.: -0.001 min

Response: 941649

Conc: 25.14 ng/ml

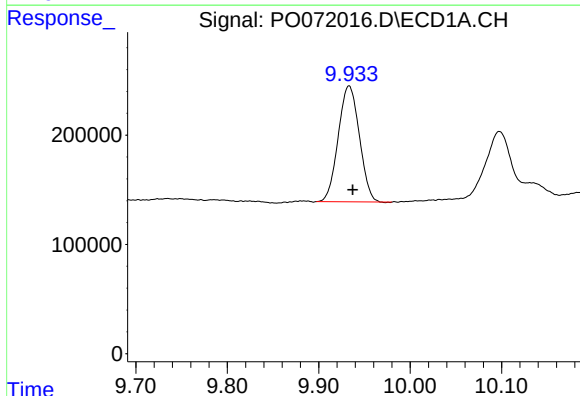


#2 Decachlorobiphenyl

R.T.: 9.933 min

Delta R.T.: -0.004 min

Response: 1701089

Conc: 15.45 ng/ml

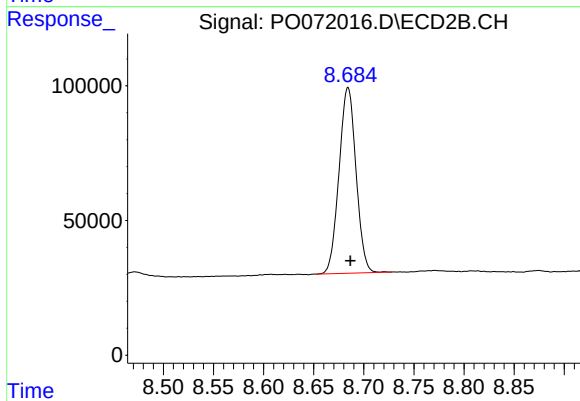


#2 Decachlorobiphenyl

R.T.: 8.684 min

Delta R.T.: -0.002 min

Response: 812883

Conc: 14.29 ng/ml

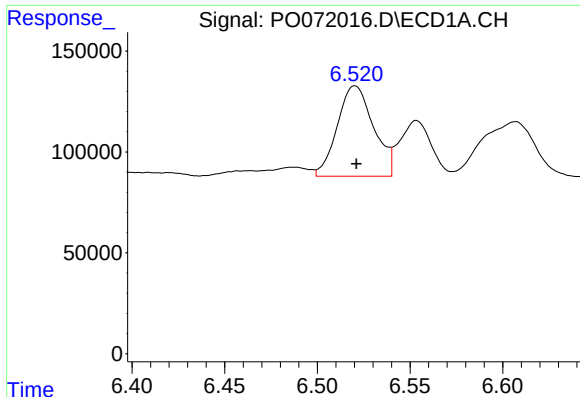


#26 AR-1254-1

R.T.: 6.520 min
Delta R.T.: 0.000 min
Response: 610812
Conc: 174.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
CL-01-100120


Manual Integrations
APPROVED

Ankita
10/6/2020 12:17:32 PM

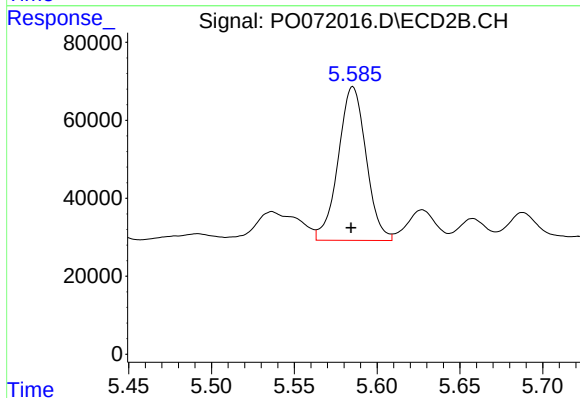


#26 AR-1254-1

R.T.: 5.585 min
Delta R.T.: 0.001 min
Response: 461682
Conc: 193.19 ng/ml

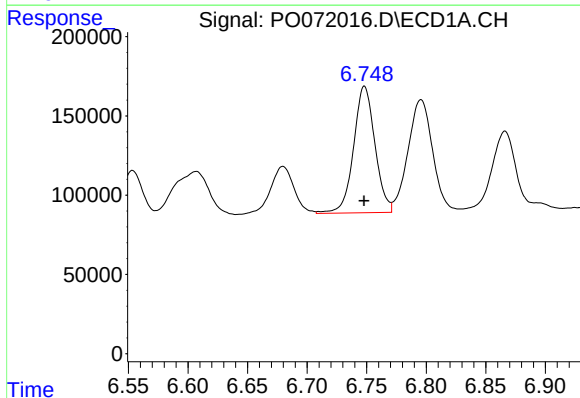


#27 AR-1254-2

R.T.: 6.748 min
Delta R.T.: 0.000 min
Response: 996082
Conc: 180.92 ng/ml

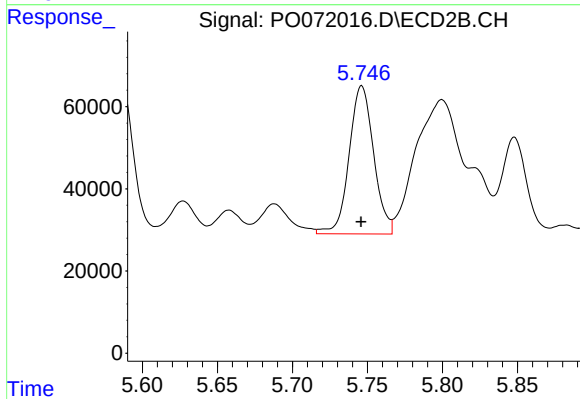

#27 AR-1254-2

R.T.: 5.746 min
Delta R.T.: 0.000 min
Response: 411252
Conc: 192.27 ng/ml

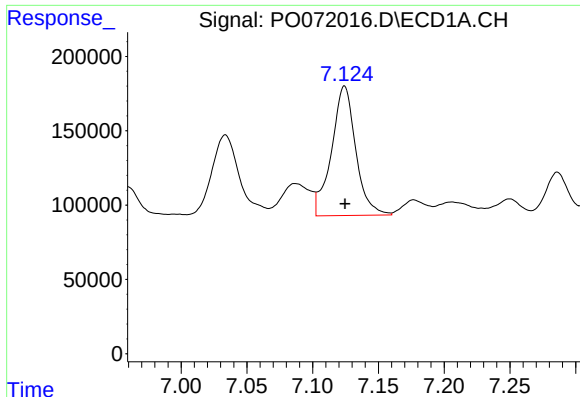


#28 AR-1254-3

R.T.: 7.124 min
Delta R.T.: 0.000 min
Response: 1119134
Conc: 193.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
CL-01-100120


Manual Integrations
APPROVED

Ankita
10/6/2020 12:17:32 PM

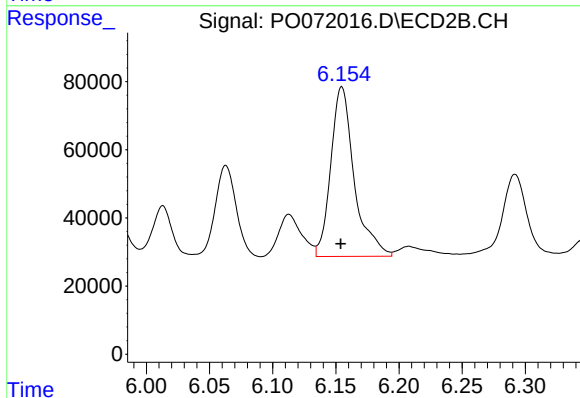


#28 AR-1254-3

R.T.: 6.155 min
Delta R.T.: 0.000 min
Response: 642856
Conc: 189.35 ng/ml

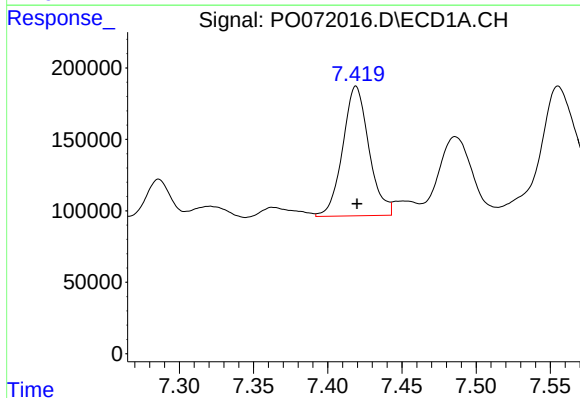


#29 AR-1254-4

R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 1115036
Conc: 191.39 ng/ml

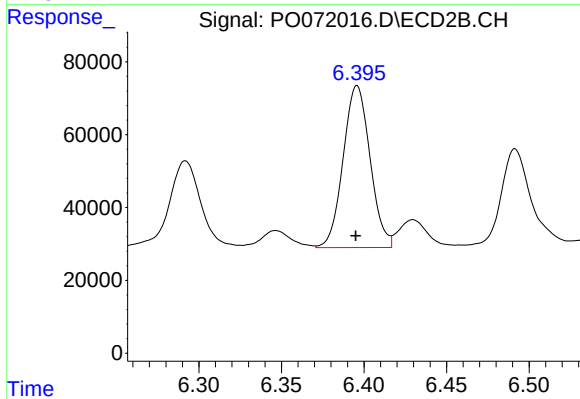

#29 AR-1254-4

R.T.: 6.396 min
Delta R.T.: 0.000 min
Response: 504479
Conc: 207.76 ng/ml

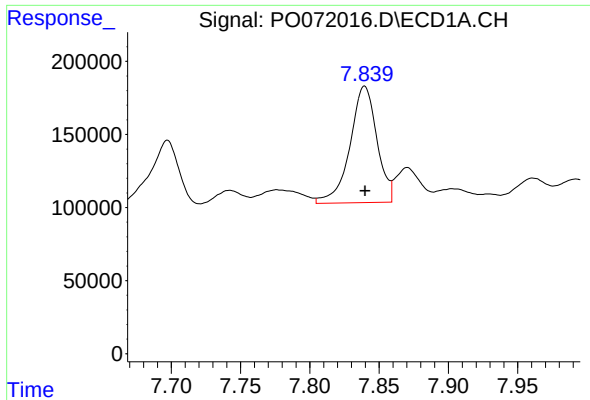


#30 AR-1254-5

R.T.: 7.840 min
Delta R.T.: 0.000 min
Response: 1077503
Conc: 200.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
CL-01-100120

Manual Integrations
APPROVED

Ankita
10/6/2020 12:17:32 PM

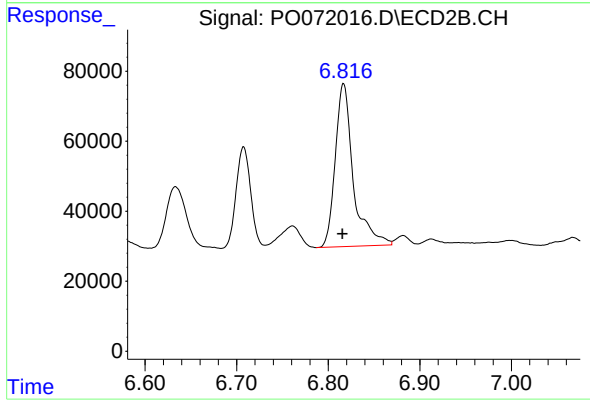

#30 AR-1254-5

R.T.: 6.817 min
Delta R.T.: 0.001 min
Response: 637957
Conc: 194.97 ng/ml