

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100520\
 Data File : PO072020.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Oct 2020 2:25
 Operator : DD\AJ
 Sample : L4246-01
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 108885

Manual Integrations
 APPROVED

Ankita
 10/6/2020 12:17:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 05:50:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.344f	3.540f	2246294	829775	31.274m	22.153 #
2) SA Decachlor...	9.935	8.687	1904958	828321	17.301	14.563

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100520\
Data File : PO072020.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Oct 2020 2:25
Operator : DD\AJ
Sample : L4246-01
Misc :
ALS Vial : 49 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
108885


Manual Integrations
APPROVED

Ankita
10/6/2020 12:17:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 05:50:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

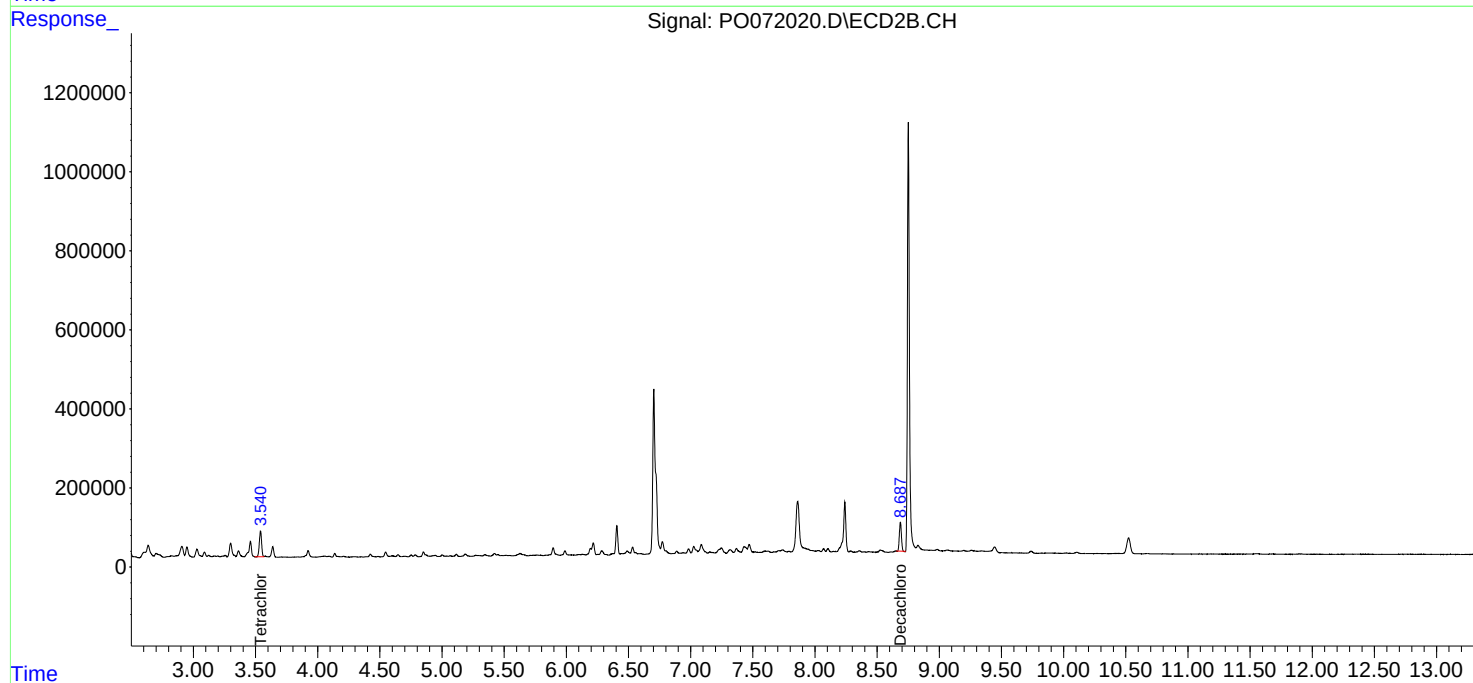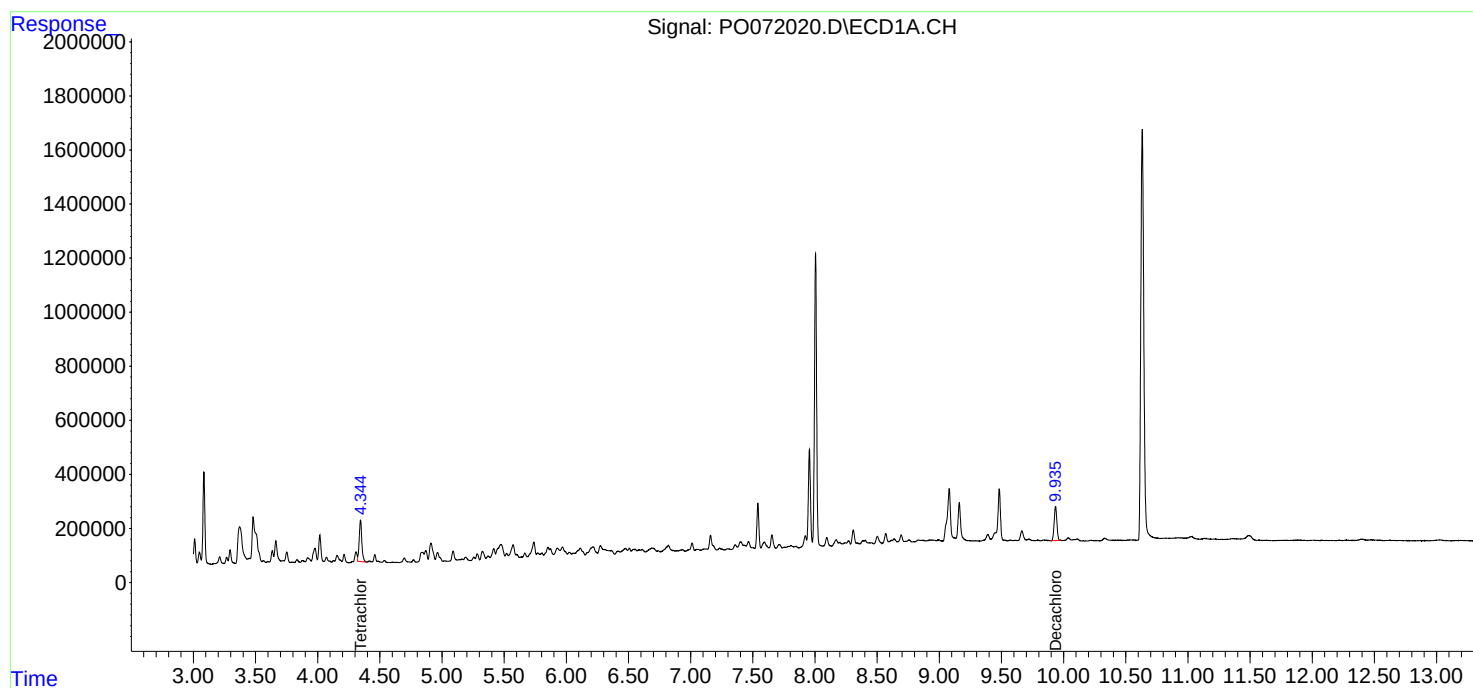

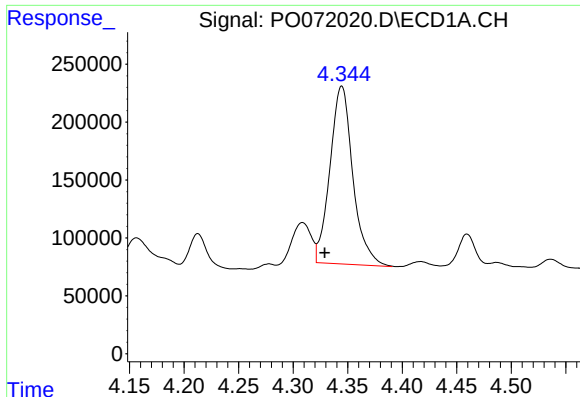

#1 Tetrachloro-m-xylene

R.T.: 4.344 min

Delta R.T.: 0.015 min


Response: 2246294

Conc: 31.27 ng/ml m

Instrument :
ECD_O
ClientSampleId :
108885

Manual Integrations
APPROVED

Ankita
10/6/2020 12:17:39 PM

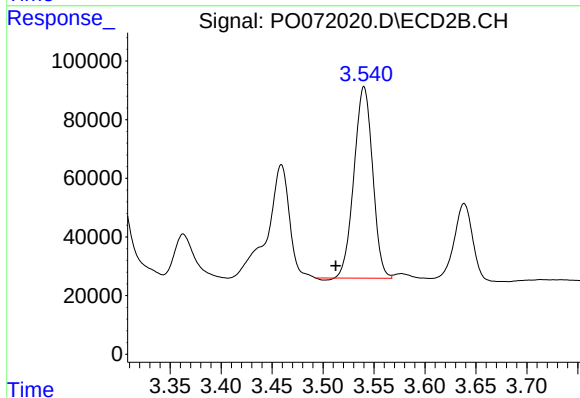


#1 Tetrachloro-m-xylene

R.T.: 3.540 min

Delta R.T.: 0.028 min

Response: 829775

Conc: 22.15 ng/ml

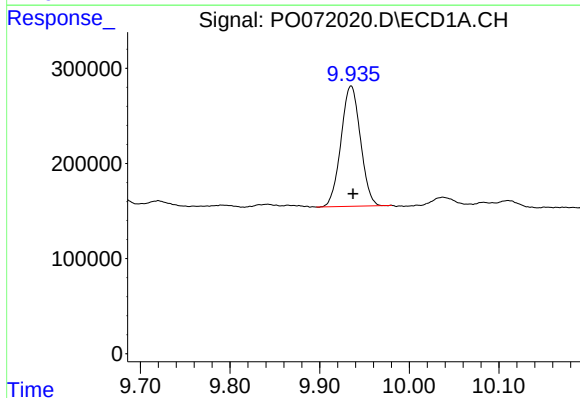


#2 Decachlorobiphenyl

R.T.: 9.935 min

Delta R.T.: -0.002 min

Response: 1904958

Conc: 17.30 ng/ml

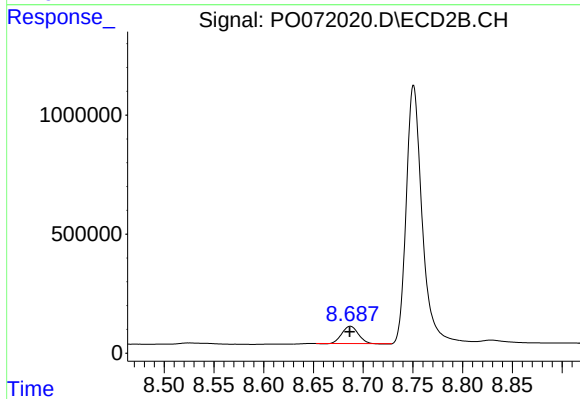

#2 Decachlorobiphenyl

R.T.: 8.687 min

Delta R.T.: 0.000 min

Response: 828321

Conc: 14.56 ng/ml