

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100521\
 Data File : P0081765.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Oct 2021 10:58
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 23:09:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 24 02:21:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.871	3.982	1946945	541482	21.833	20.324
2)	SA Decachlor...	10.878	9.326	1761758	527434	23.652	22.712
Target Compounds							
8)	L2 AR-1221-1	5.118	0.000	59551	0	54.420	N.D. #
9)	L2 AR-1221-2	5.225	0.000	23644	0	29.988	N.D. #
10)	L2 AR-1221-3	0.000	4.424	0	11622	N.D.	14.978 #
11)	L3 AR-1232-1	0.000	4.424	0	11622	N.D.	19.383 #
24)	L5 AR-1248-4	7.116f	0.000	21225	0	6.163	N.D. #
26)	L6 AR-1254-1	7.116	0.000	21225	0	5.920	N.D. #
28)	L6 AR-1254-3	7.740f	0.000	46645	0	8.267	N.D. #
33)	L7 AR-1260-3	0.000	7.199f	0	22252	N.D.	13.382 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100521\
Data File : P0081765.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Oct 2021 10:58
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 23:09:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 24 02:21:54 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

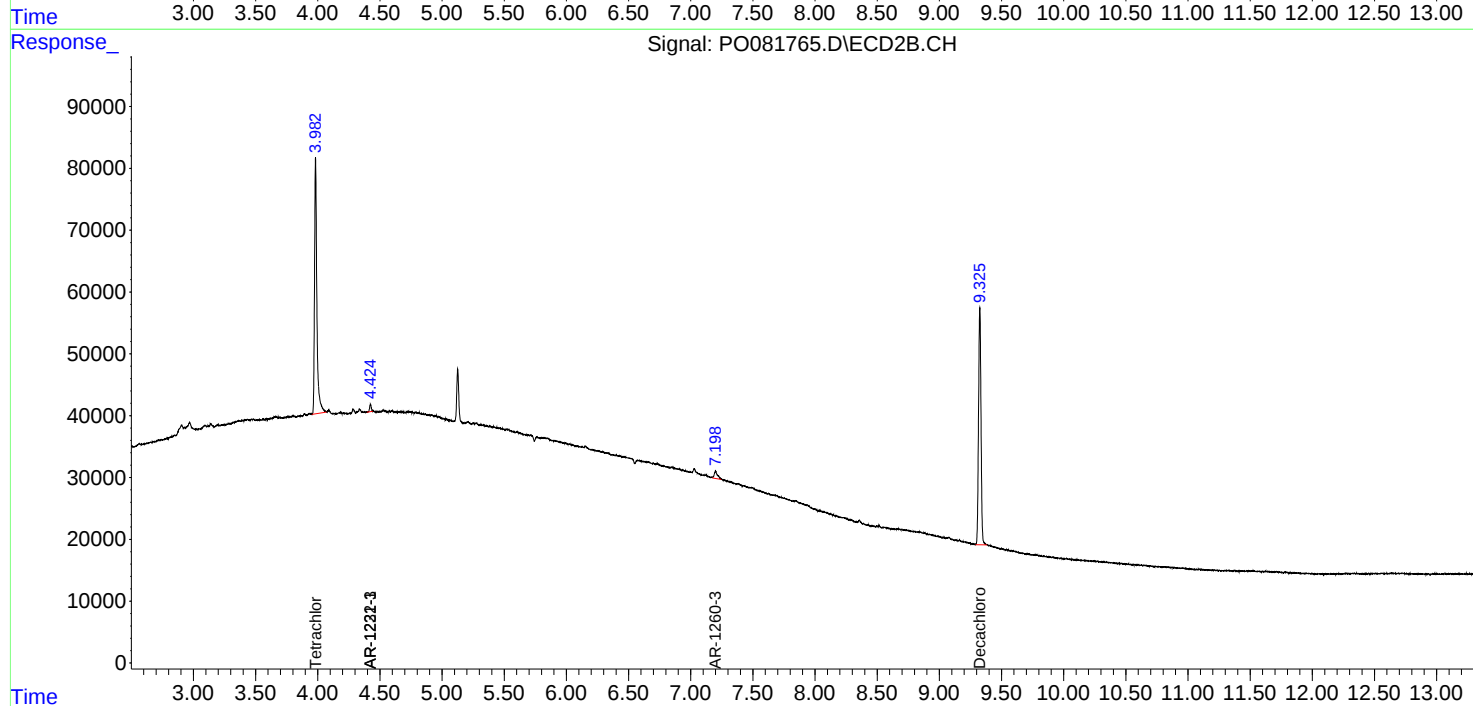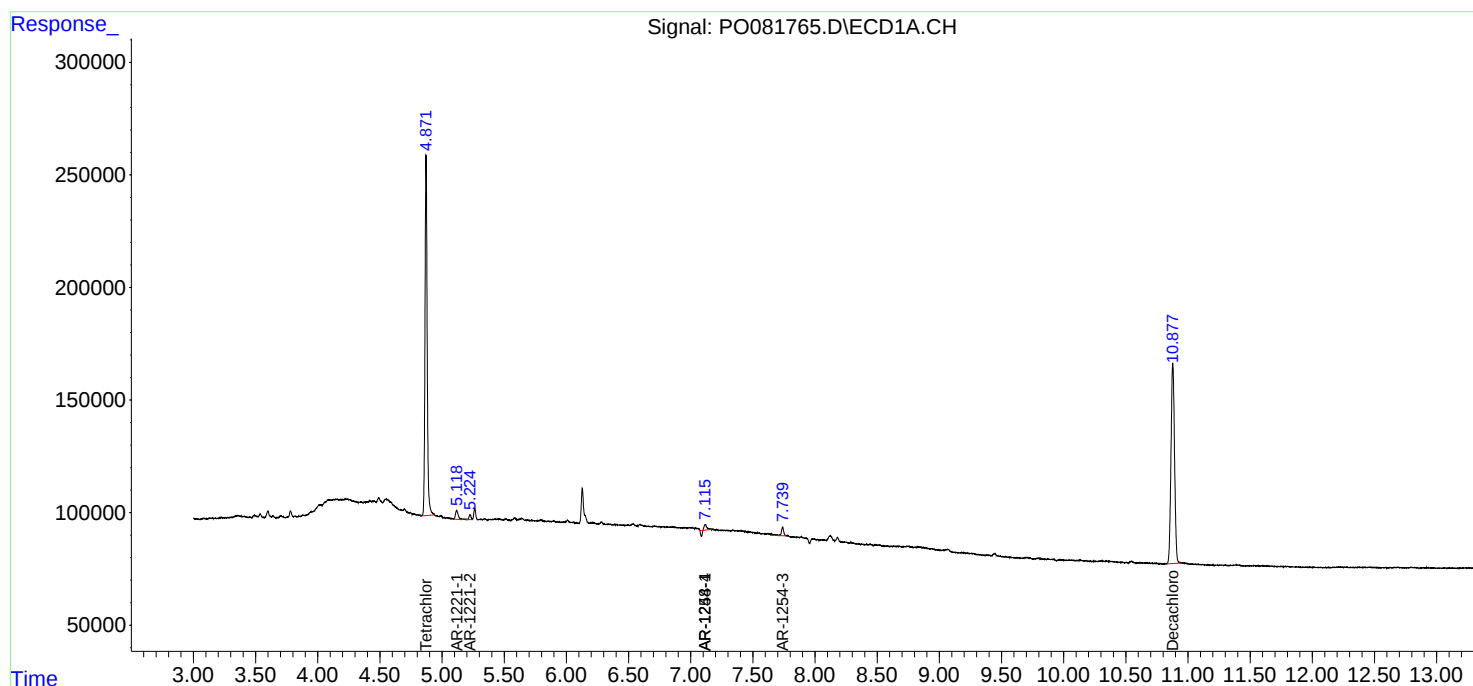


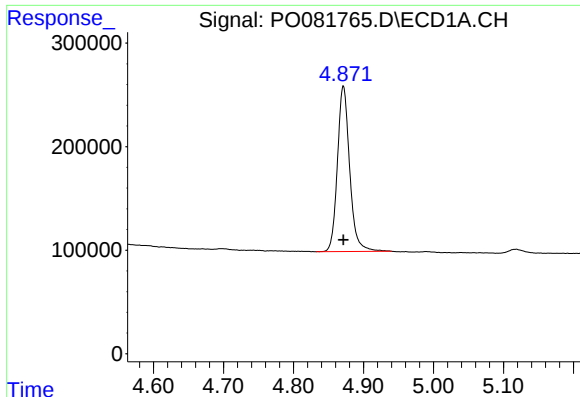

#1 Tetrachloro-m-xylene


R.T.: 4.871 min
Delta R.T.: 0.000 min
Response: 1946945
Conc: 21.83 ng/ml

Instrument :
ECD_O
ClientSampleId :

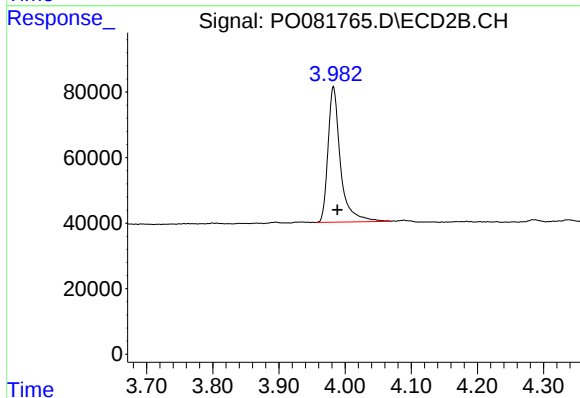


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: -0.006 min
Response: 541482
Conc: 20.32 ng/ml

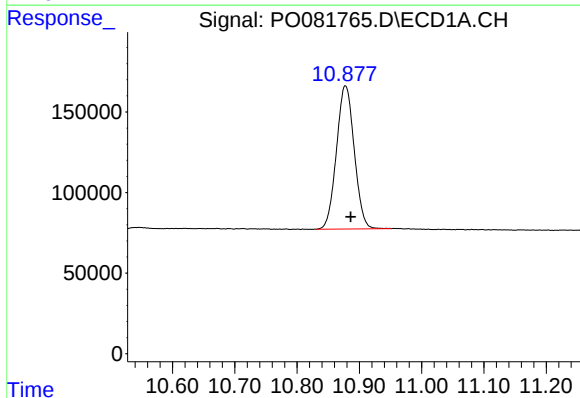


#2 Decachlorobiphenyl

R.T.: 10.878 min
Delta R.T.: -0.009 min
Response: 1761758
Conc: 23.65 ng/ml

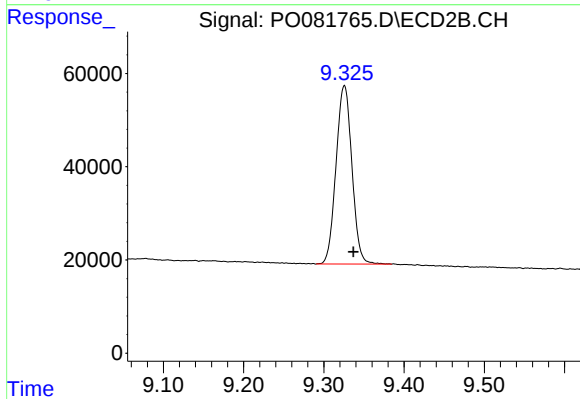

#2 Decachlorobiphenyl


R.T.: 9.326 min
Delta R.T.: -0.011 min
Response: 527434
Conc: 22.71 ng/ml

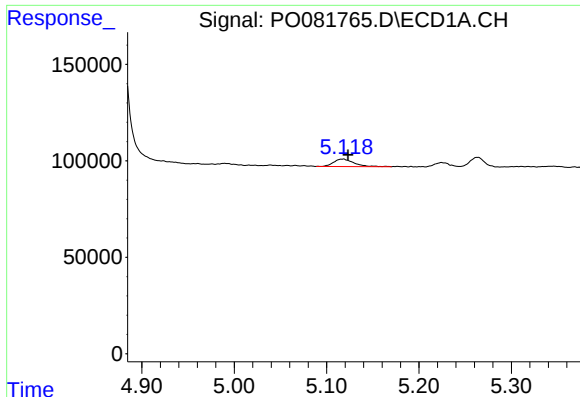

#8 AR-1221-1


R.T.: 5.118 min
Delta R.T.: -0.005 min
Response: 59551
Conc: 54.42 ng/ml

Instrument :
ECD_O
ClientSampleId :

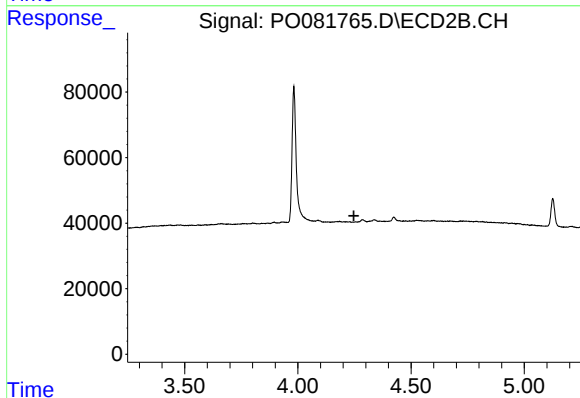


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.248 min
Response: 0
Conc: N.D.

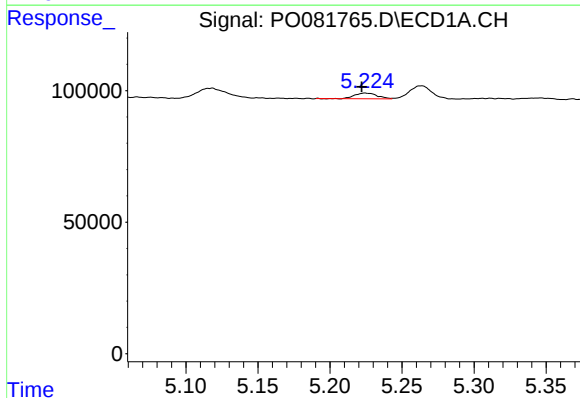


#9 AR-1221-2

R.T.: 5.225 min
Delta R.T.: 0.002 min
Response: 23644
Conc: 29.99 ng/ml

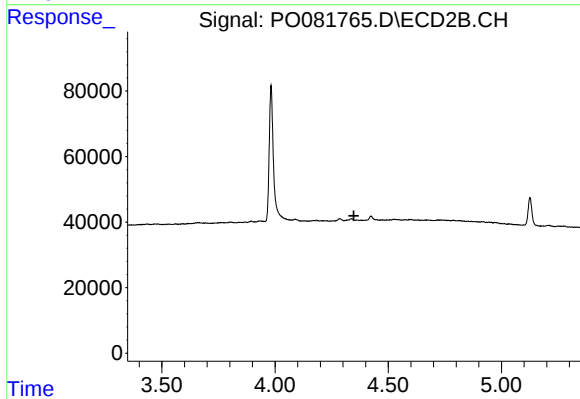

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.348 min
Response: 0
Conc: N.D.

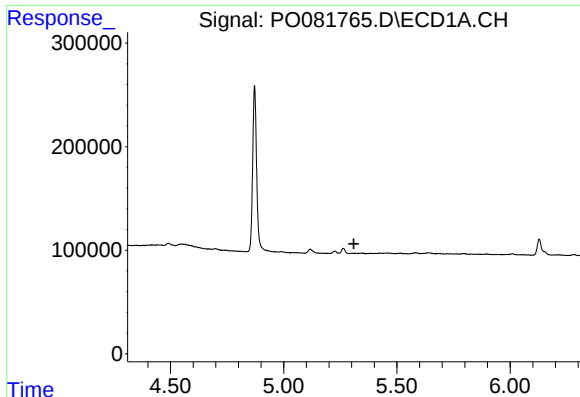

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 5.310 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

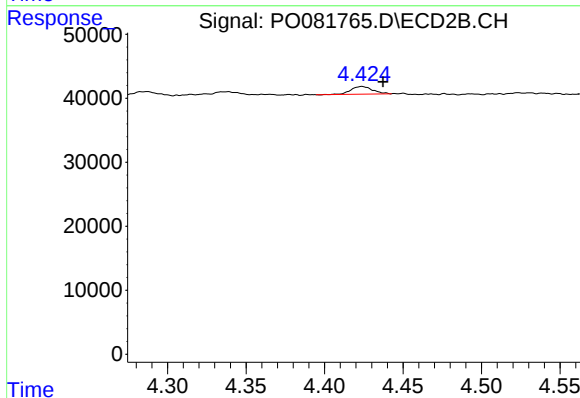


#10 AR-1221-3

R.T.: 4.424 min
Delta R.T.: -0.013 min
Response: 11622
Conc: 14.98 ng/ml

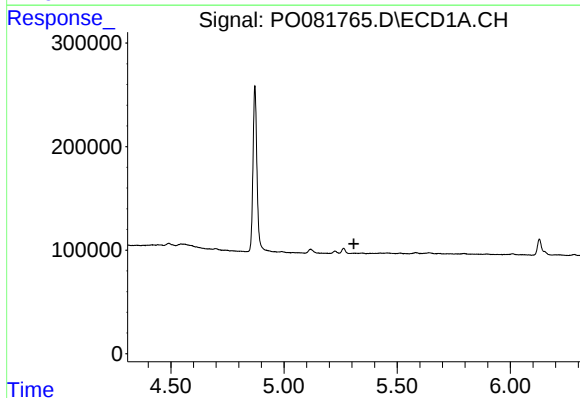


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T.: 5.309 min
Response: 0
Conc: N.D.

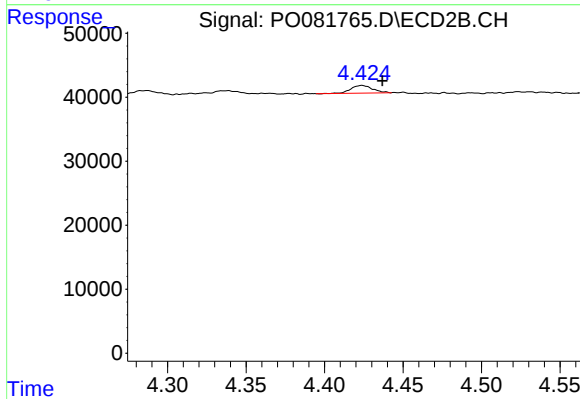

#11 AR-1232-1


R.T.: 4.424 min
Delta R.T.: -0.013 min
Response: 11622
Conc: 19.38 ng/ml

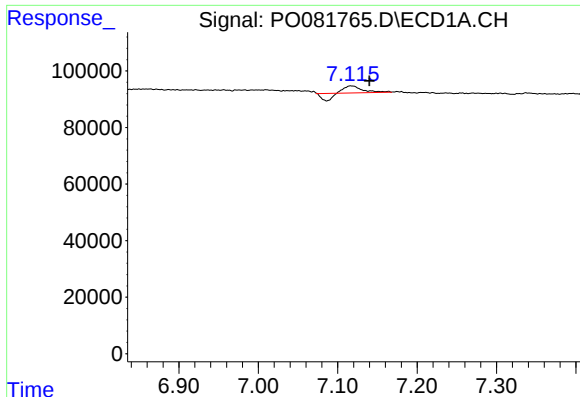

#24 AR-1248-4


R.T.: 7.116 min
Delta R.T.: -0.024 min
Response: 21225
Conc: 6.16 ng/ml

Instrument :
ECD_O
ClientSampleId :

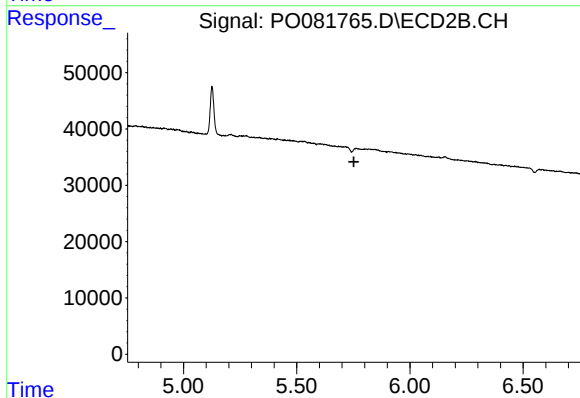


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.753 min
Response: 0
Conc: N.D.

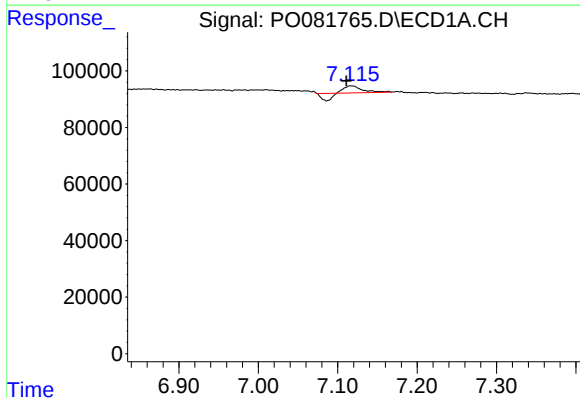


#26 AR-1254-1

R.T.: 7.116 min
Delta R.T.: 0.006 min
Response: 21225
Conc: 5.92 ng/ml

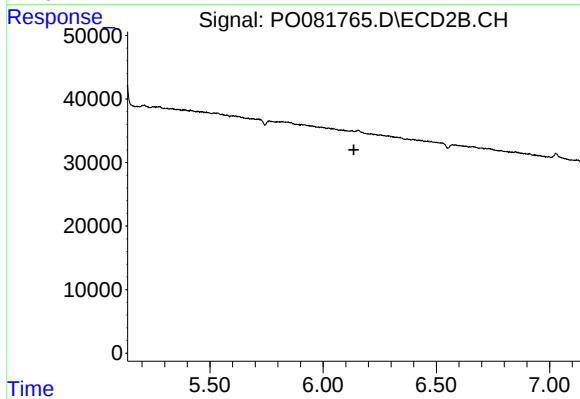

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.136 min
Response: 0
Conc: N.D.

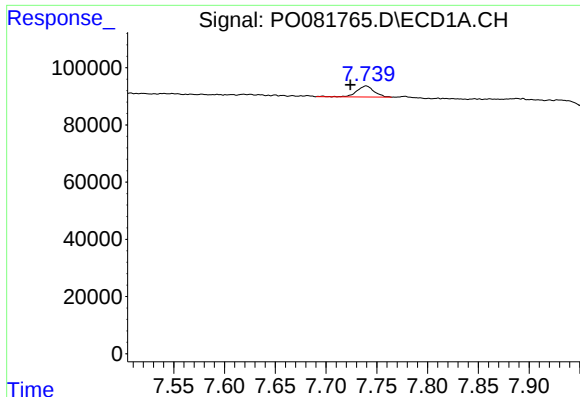

#28 AR-1254-3


R.T.: 7.740 min
Delta R.T.: 0.016 min
Response: 46645
Conc: 8.27 ng/ml

Instrument :
ECD_O
ClientSampleId :

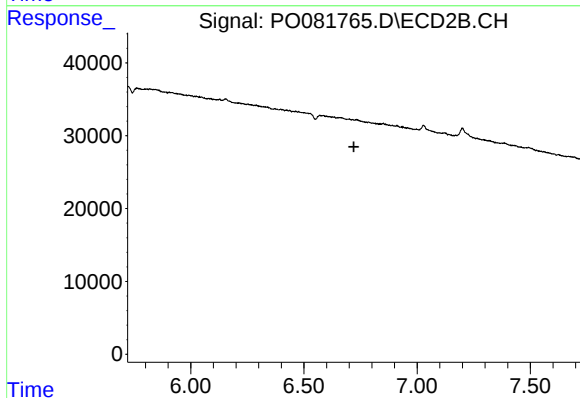


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.721 min
Response: 0
Conc: N.D.

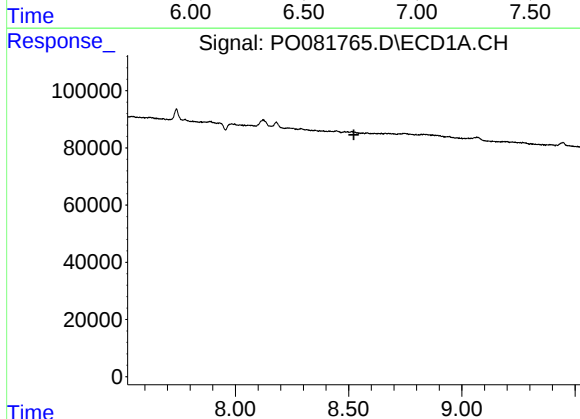

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.523 min
Response: 0
Conc: N.D.

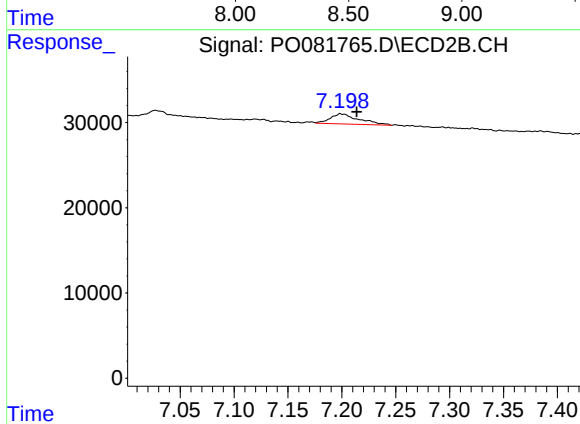

#33 AR-1260-3

R.T.: 7.199 min
Delta R.T.: -0.015 min
Response: 22252
Conc: 13.38 ng/ml