

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100521\
 Data File : P0081766.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Oct 2021 12:51
 Operator : AJ\MA
 Sample : PB139621BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB139621BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 23:09:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 24 02:21:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.878	3.980	2256810	618871	25.307	23.229
2)	SA Decachlor...	10.885	9.327	1994891	594856	26.782	25.615

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100521\
Data File : PO081766.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Oct 2021 12:51
Operator : AJ\MA
Sample : PB139621BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB139621BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 23:09:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 24 02:21:54 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

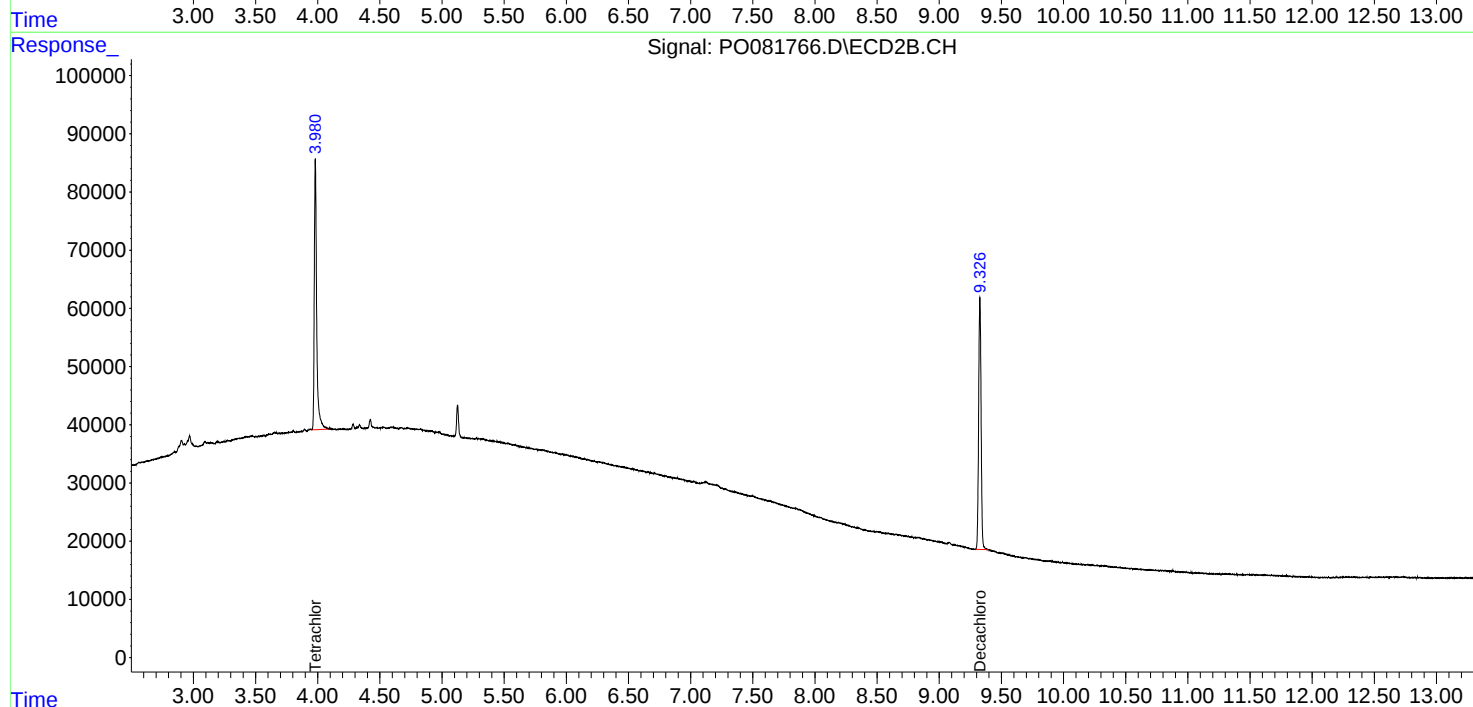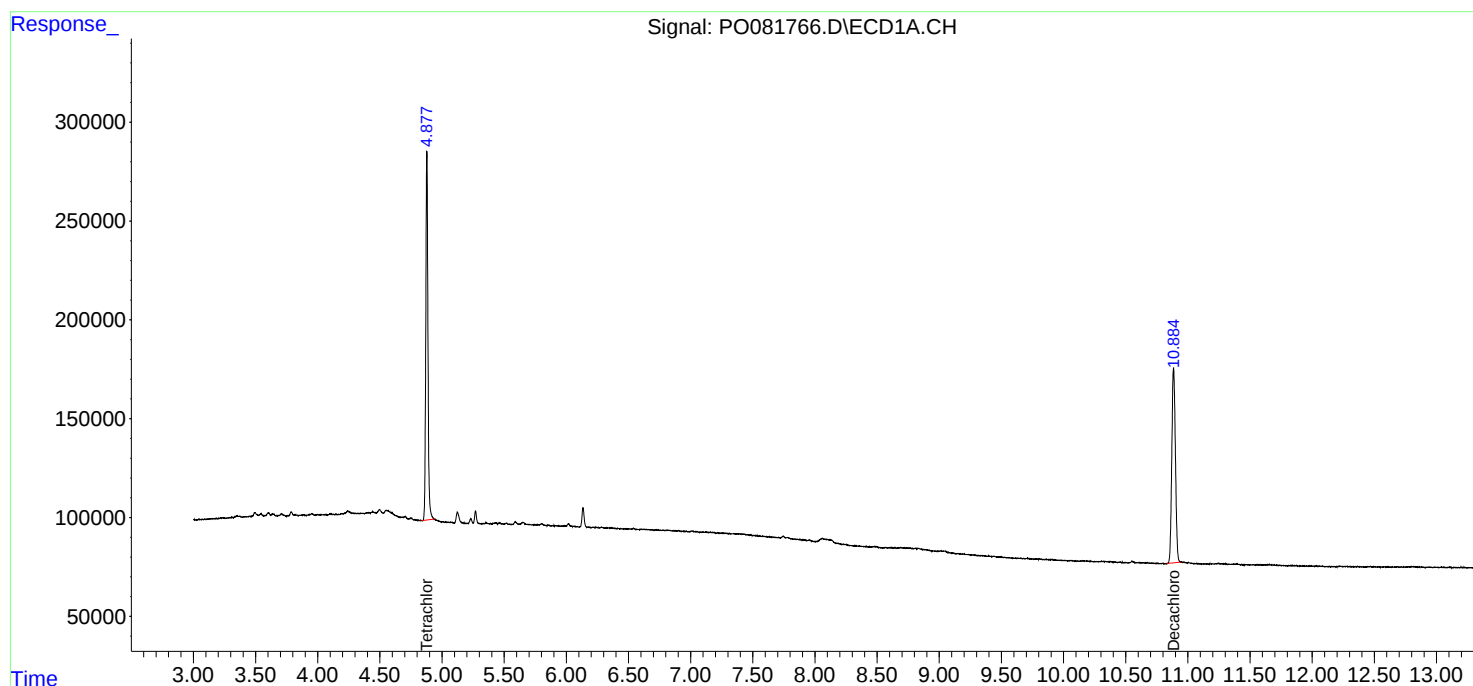


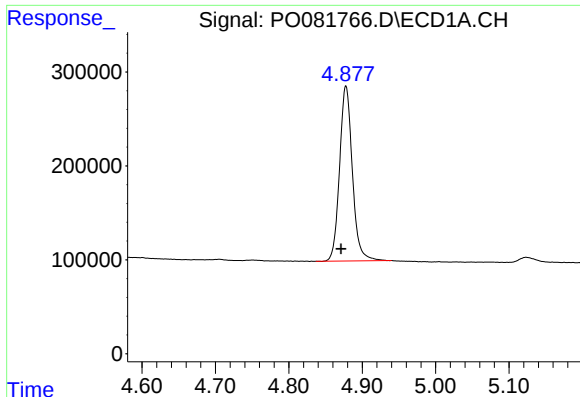

#1 Tetrachloro-m-xylene


R.T.: 4.878 min
Delta R.T.: 0.007 min
Response: 2256810
Conc: 25.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB139621BL

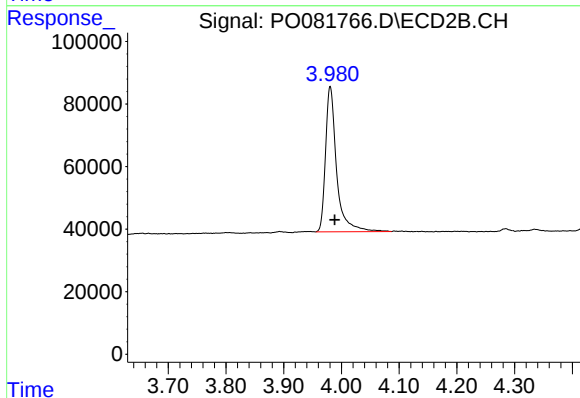


#1 Tetrachloro-m-xylene

R.T.: 3.980 min
Delta R.T.: -0.008 min
Response: 618871
Conc: 23.23 ng/ml

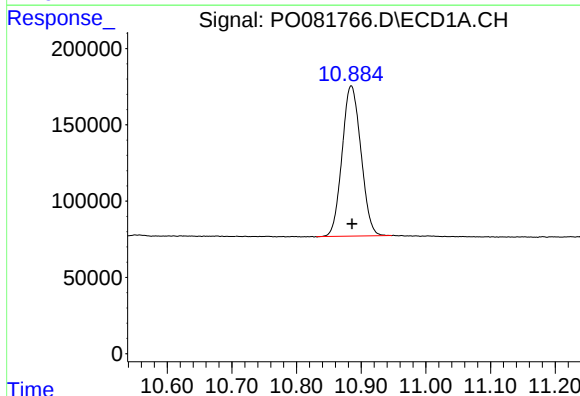

#2 Decachlorobiphenyl

R.T.: 10.885 min
Delta R.T.: -0.001 min
Response: 1994891
Conc: 26.78 ng/ml

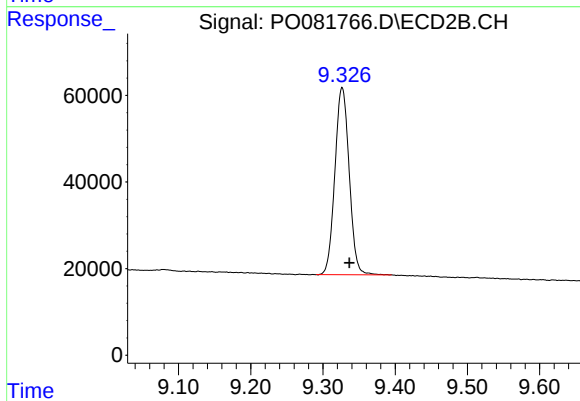

#2 Decachlorobiphenyl

R.T.: 9.327 min
Delta R.T.: -0.010 min
Response: 594856
Conc: 25.62 ng/ml