

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100521\
 Data File : P0081768.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Oct 2021 13:25
 Operator : AJ\MA
 Sample : M4041-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 N-1

Manual Integrations
 APPROVED

mohammad
 10/7/2021 8:34:19 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 23:10:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 24 02:21:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.866	3.980	1535178	769294	17.215m	28.875m#
2) SA Decachlor...	10.875	9.325	1908184	1862980	25.617	80.222m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO100521\
Data File : P0081768.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Oct 2021 13:25
Operator : AJ\MA
Sample : M4041-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
N-1


Manual Integrations
APPROVED

mohammad
10/7/2021 8:34:19 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 23:10:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0092321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 24 02:21:54 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

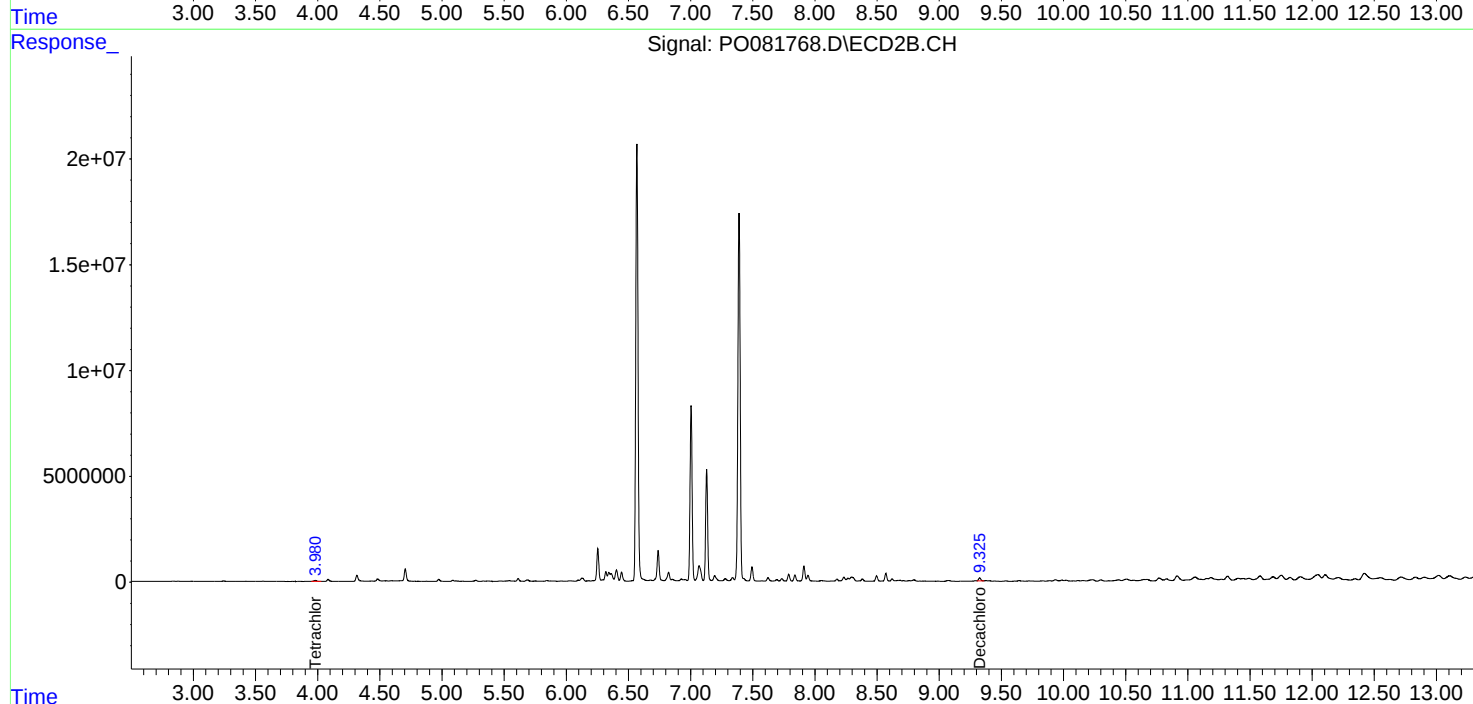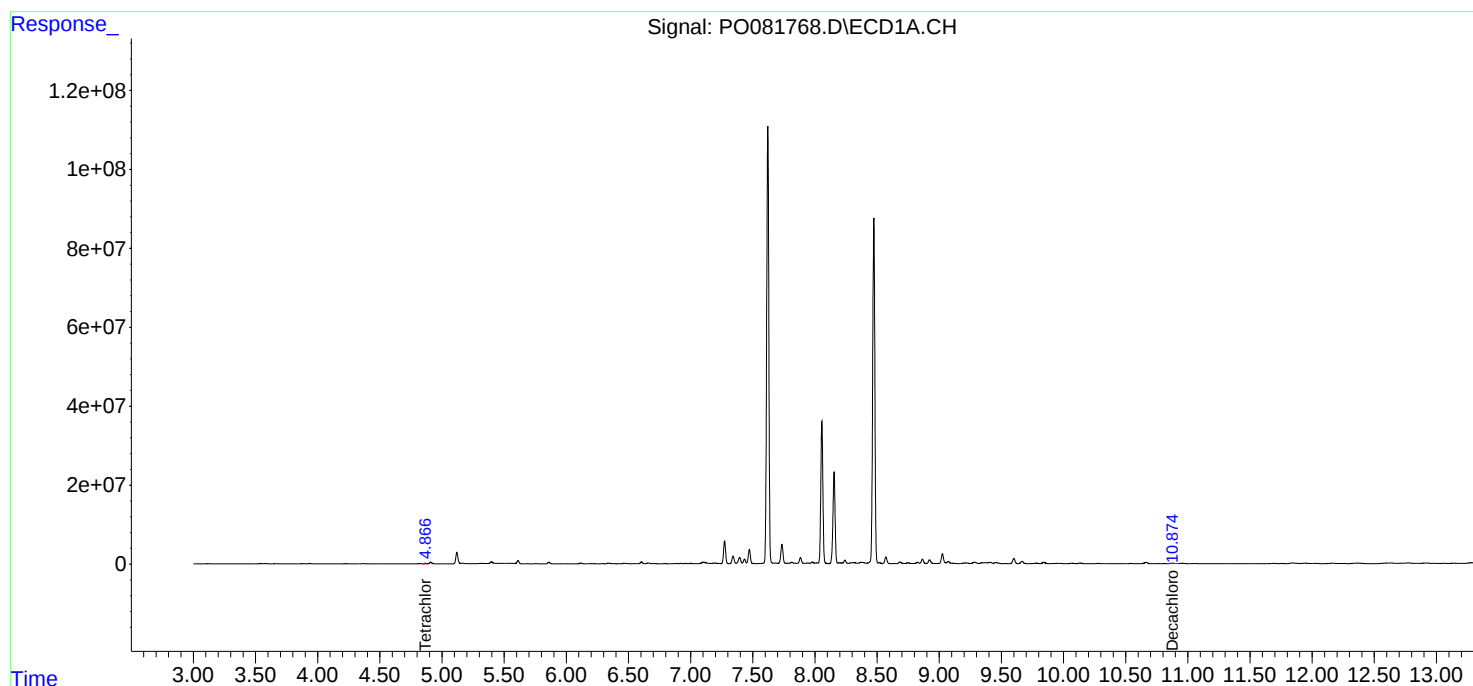

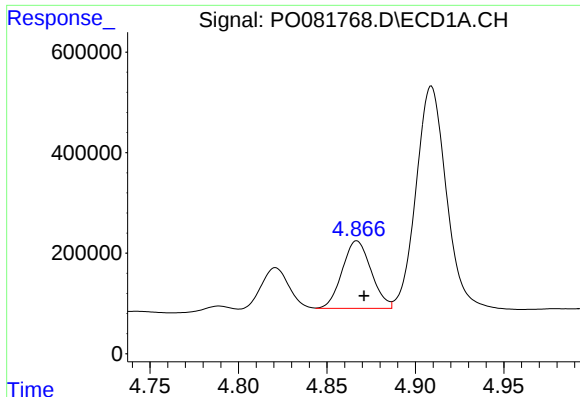


#1 Tetrachloro-m-xylene

R.T.: 4.866 min
Delta R.T.: -0.005 min
Response: 1535178
Conc: 17.22 ng/ml m

Instrument :
ECD_O
ClientSampleId :
N-1


Manual Integrations
APPROVED

mohammad
10/7/2021 8:34:19 AM

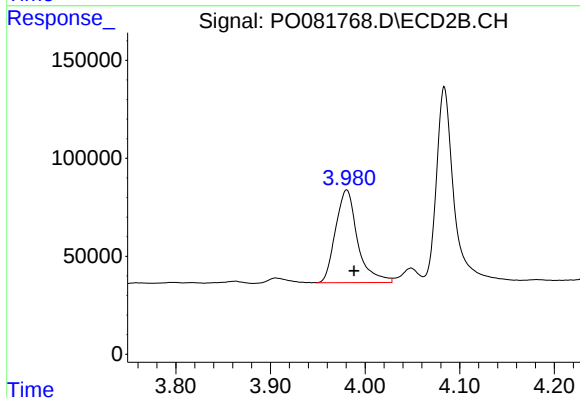


#1 Tetrachloro-m-xylene

R.T.: 3.980 min
Delta R.T.: -0.008 min
Response: 769294
Conc: 28.88 ng/ml m

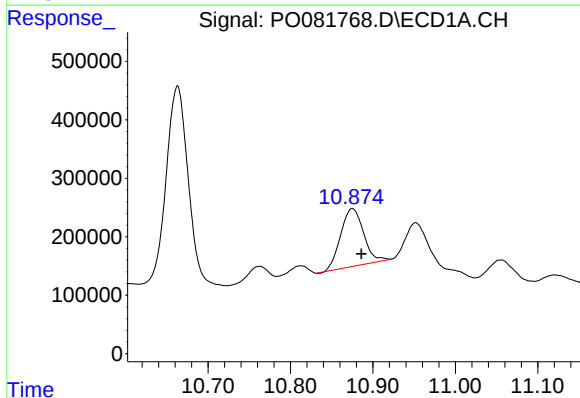

#2 Decachlorobiphenyl

R.T.: 10.875 min
Delta R.T.: -0.011 min
Response: 1908184
Conc: 25.62 ng/ml

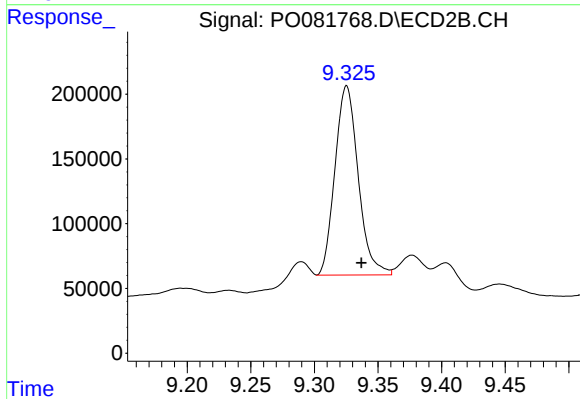

#2 Decachlorobiphenyl

R.T.: 9.325 min
Delta R.T.: -0.012 min
Response: 1862980
Conc: 80.22 ng/ml m