

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100521\
 Data File : P0081772.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Oct 2021 14:34
 Operator : AJ\MA
 Sample : M4047-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 149-ENV-1-GRAB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 23:11:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 24 02:21:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.867	3.982	2325897	662899	26.082	24.882
2) SA Decachlor...	10.872	9.324	1428944	447428	19.184	19.267

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100521\
Data File : PO081772.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Oct 2021 14:34
Operator : AJ\MA
Sample : M4047-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
149-ENV-1-GRAB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 23:11:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 24 02:21:54 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

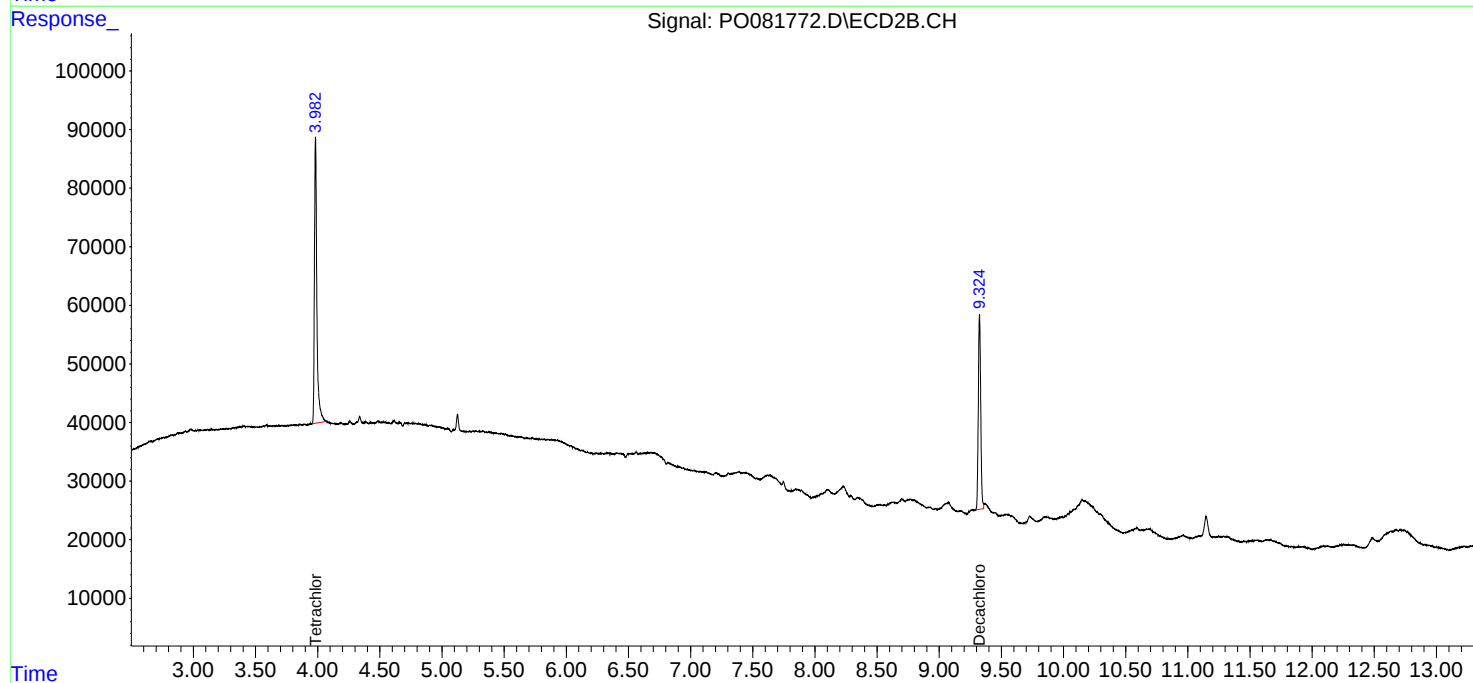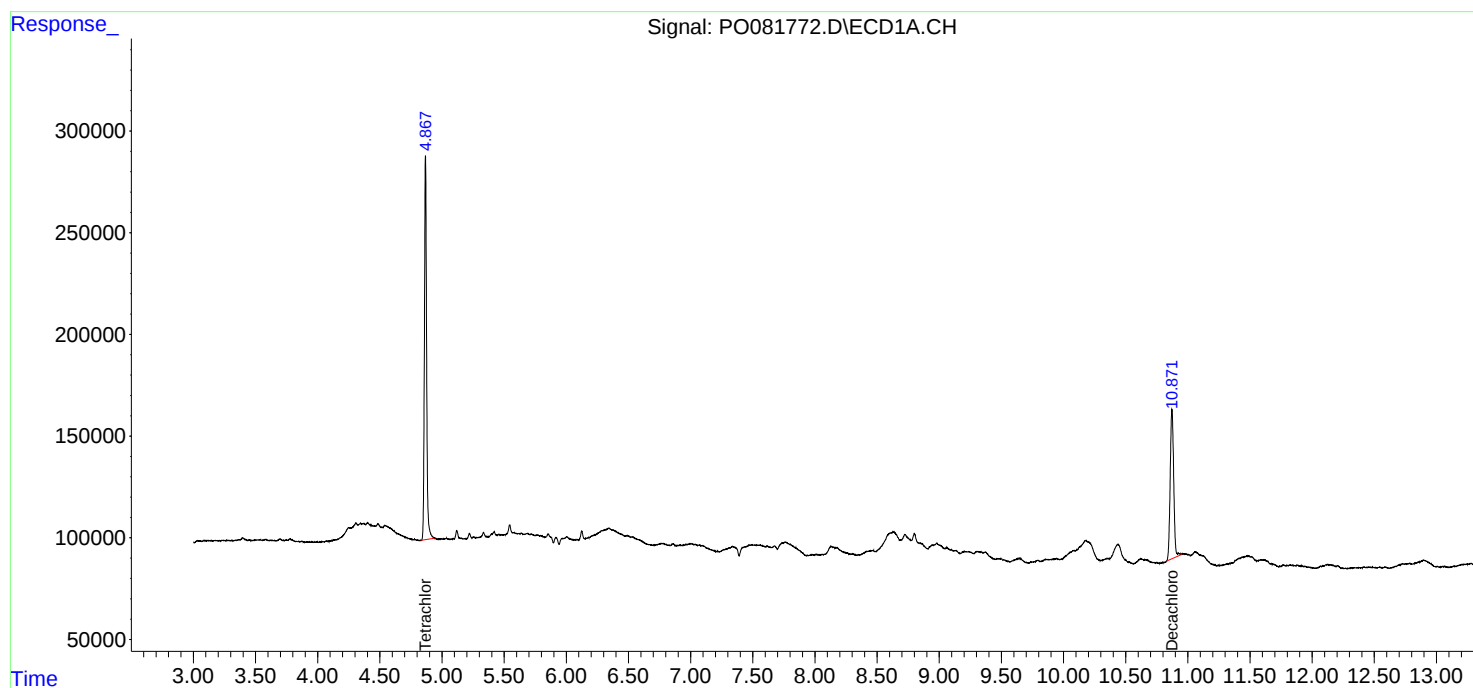


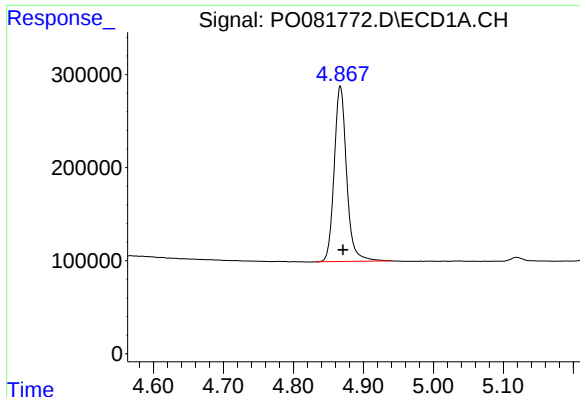

#1 Tetrachloro-m-xylene


R.T.: 4.867 min
Delta R.T.: -0.004 min
Response: 2325897
Conc: 26.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
149-ENV-1-GRAB

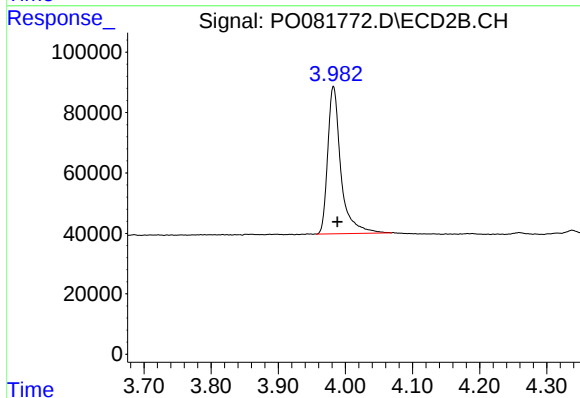


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: -0.006 min
Response: 662899
Conc: 24.88 ng/ml

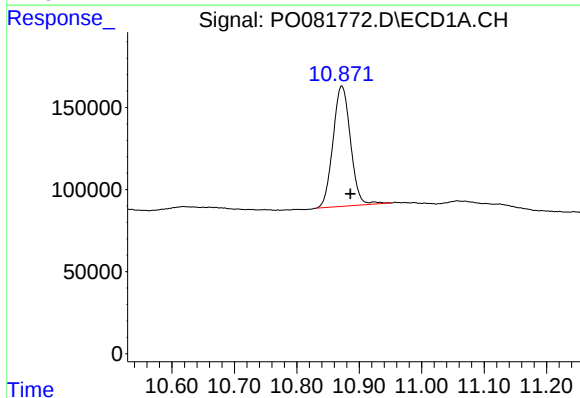

#2 Decachlorobiphenyl

R.T.: 10.872 min
Delta R.T.: -0.014 min
Response: 1428944
Conc: 19.18 ng/ml

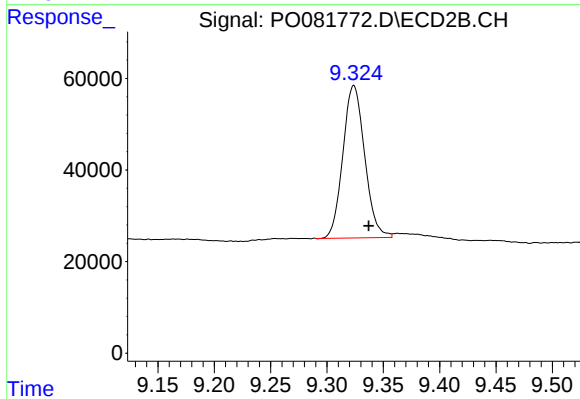

#2 Decachlorobiphenyl

R.T.: 9.324 min
Delta R.T.: -0.013 min
Response: 447428
Conc: 19.27 ng/ml