

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100522\
 Data File : PO089762.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2022 02:51
 Operator : YP/AJ
 Sample : N4962-09 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KZA317K-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/06/2022
 Supervised By :Ankita Jodhani 10/06/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 03:48:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 05 06:04:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.333	3.559	4779047	1399733	1.838m	1.550m
2) SA Decachlor...	10.095	8.592	2983708	1033316	2.776	1.300 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100522\
Data File : PO089762.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2022 02:51
Operator : YP/AJ
Sample : N4962-09 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KZA317K-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/06/2022
Supervised By :Ankita Jodhani 10/06/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 03:48:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100422.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 05 06:04:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

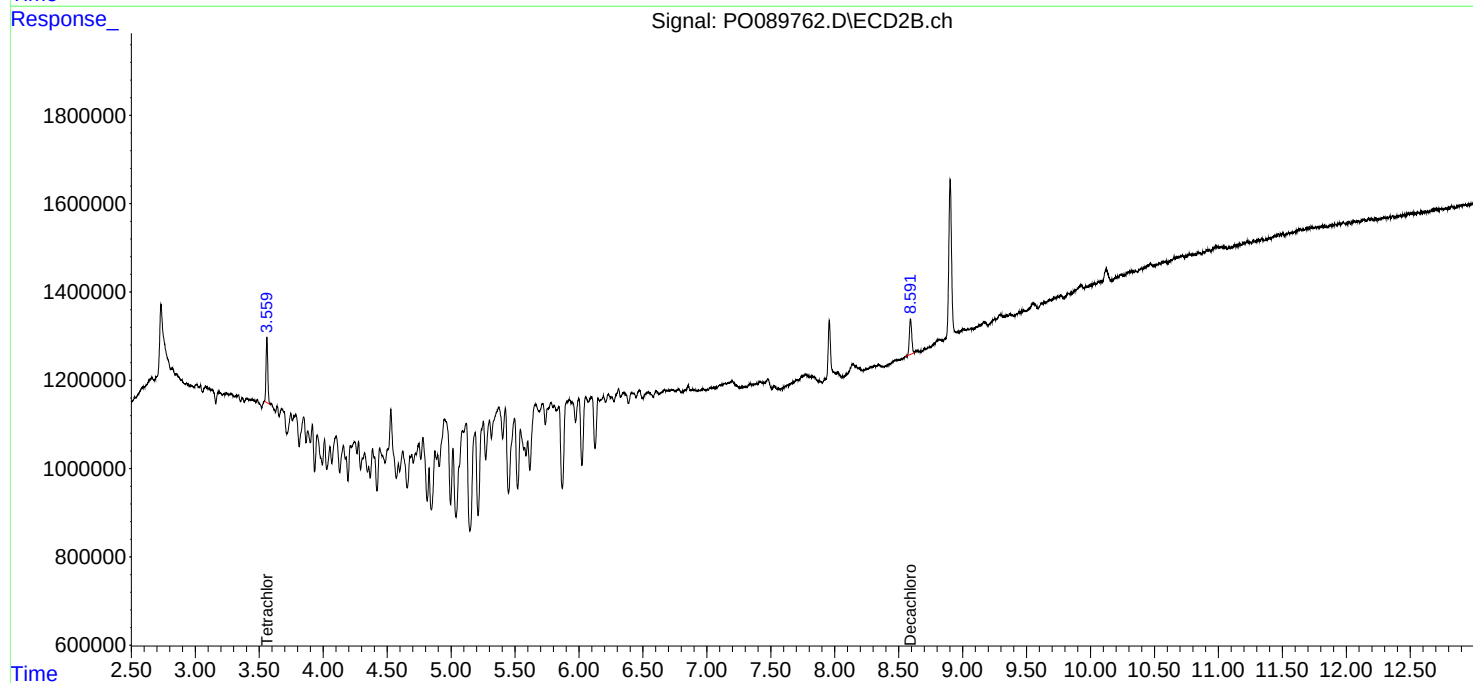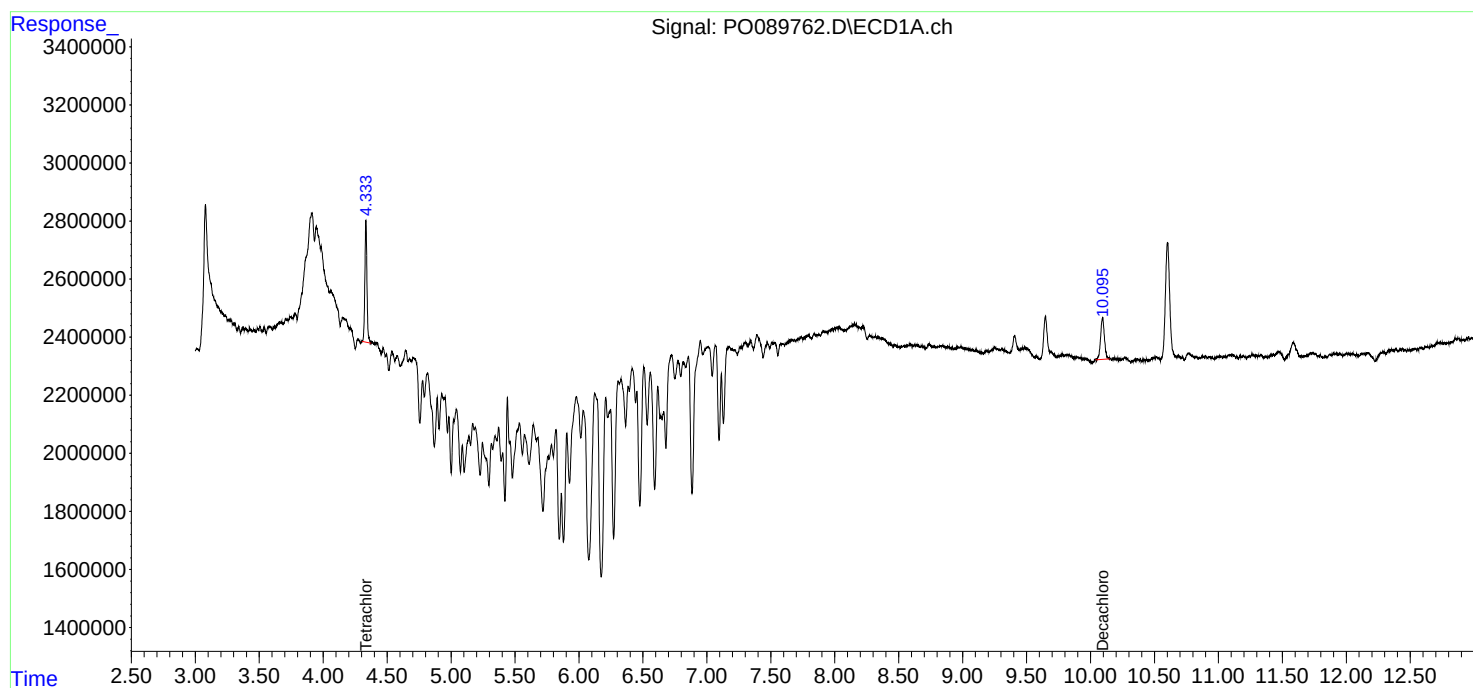

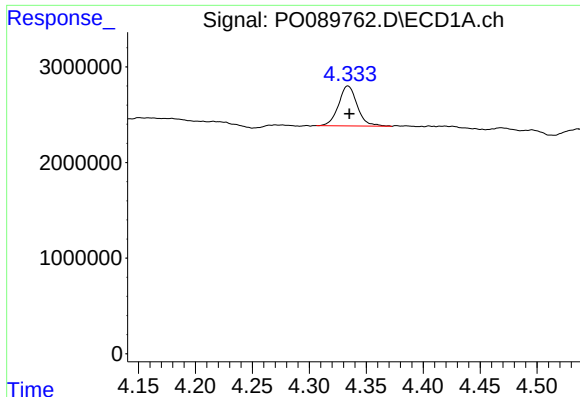


#1 Tetrachloro-m-xylene

R.T.: 4.333 min
Delta R.T.: -0.002 min
Response: 4779047
Conc: 1.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
KZA317K-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/06/2022
Supervised By :Ankita Jodhani 10/06/2022

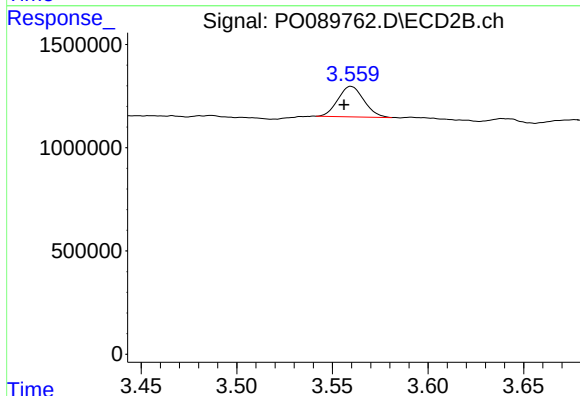


#1 Tetrachloro-m-xylene

R.T.: 3.559 min
Delta R.T.: 0.003 min
Response: 1399733
Conc: 1.55 ng/ml m

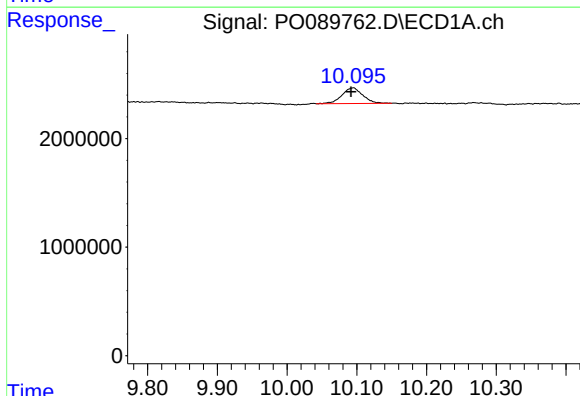

#2 Decachlorobiphenyl

R.T.: 10.095 min
Delta R.T.: 0.003 min
Response: 2983708
Conc: 2.78 ng/ml

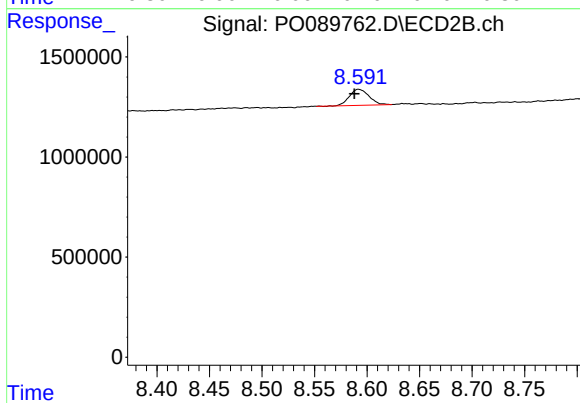

#2 Decachlorobiphenyl

R.T.: 8.592 min
Delta R.T.: 0.004 min
Response: 1033316
Conc: 1.30 ng/ml