

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100719\
Data File : P0061738.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Oct 2019 13:54
Operator : HP/AJ
Sample : K5146-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CL-01-100419

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 14:09:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.358	3.519	951354	747237	23.196	23.106
2)	SA Decachlor...	10.016	8.381	845290	555117	18.151	17.146

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100719\
Data File : PO061738.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Oct 2019 13:54
Operator : HP/AJ
Sample : K5146-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CL-01-100419

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 14:09:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

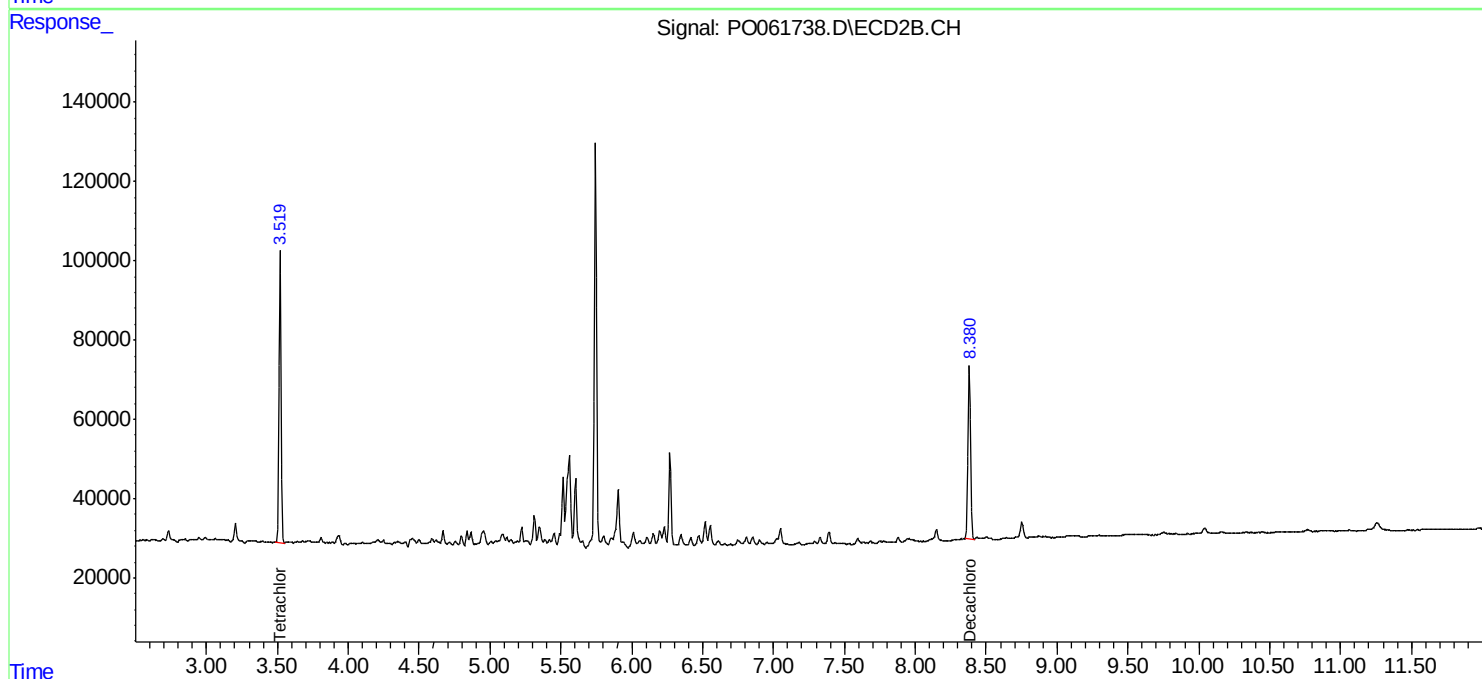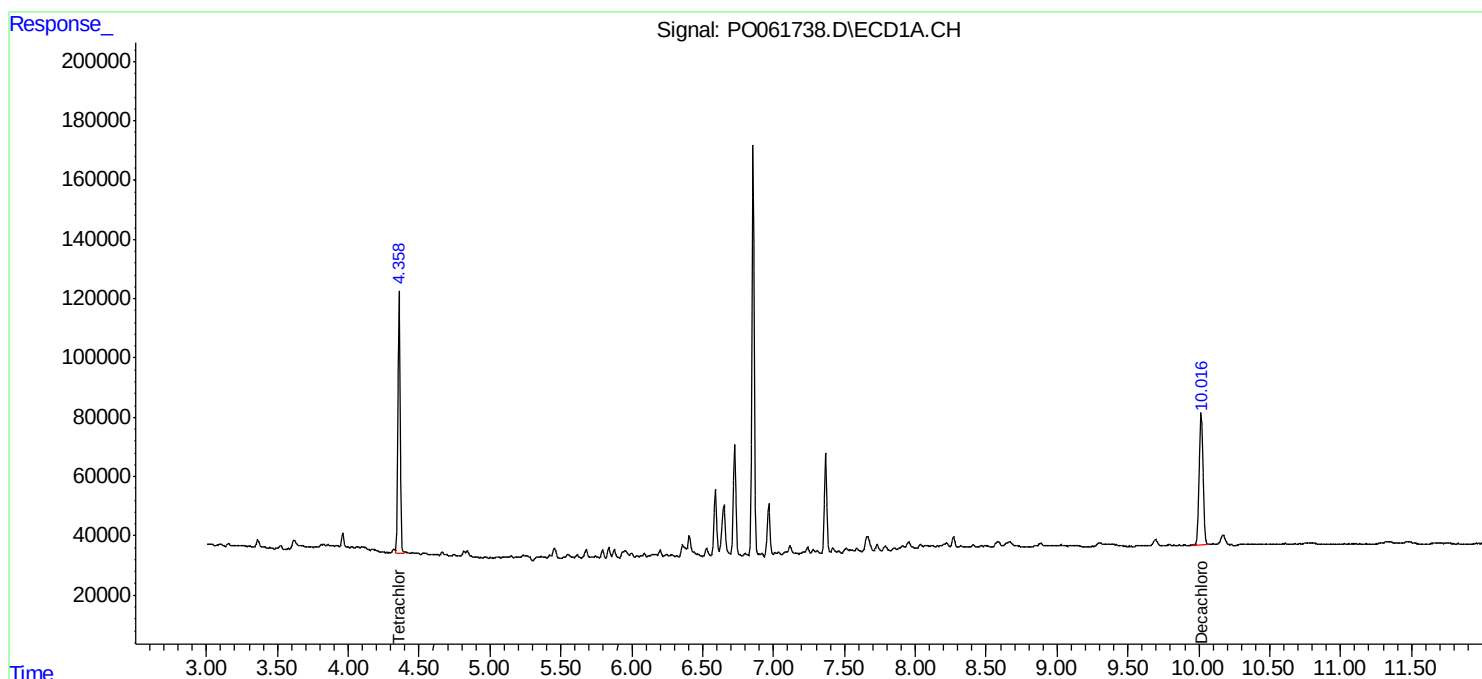


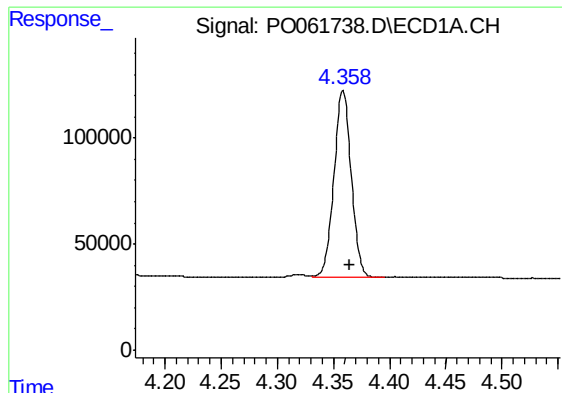

#1 Tetrachloro-m-xylene


R.T.: 4.358 min
Delta R.T.: -0.007 min
Response: 951354
Conc: 23.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
CL-01-100419

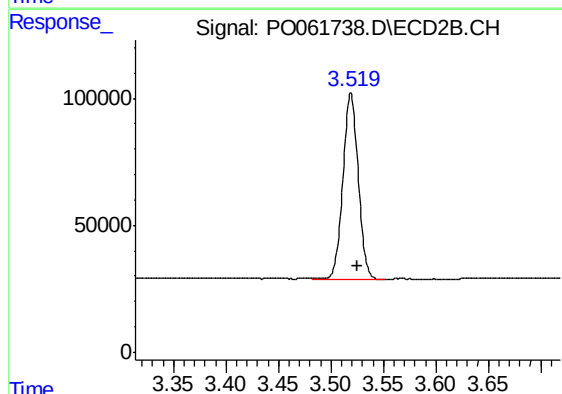


#1 Tetrachloro-m-xylene

R.T.: 3.519 min
Delta R.T.: -0.006 min
Response: 747237
Conc: 23.11 ng/ml

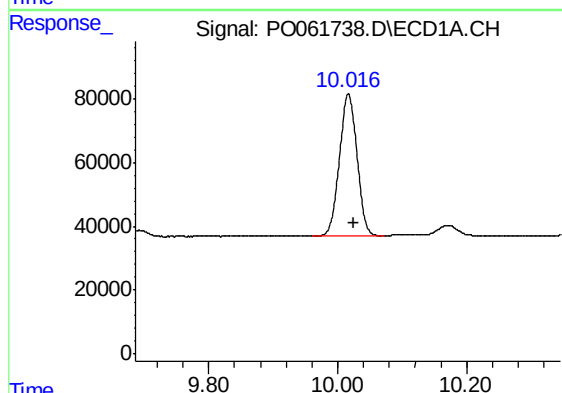

#2 Decachlorobiphenyl

R.T.: 10.016 min
Delta R.T.: -0.008 min
Response: 845290
Conc: 18.15 ng/ml

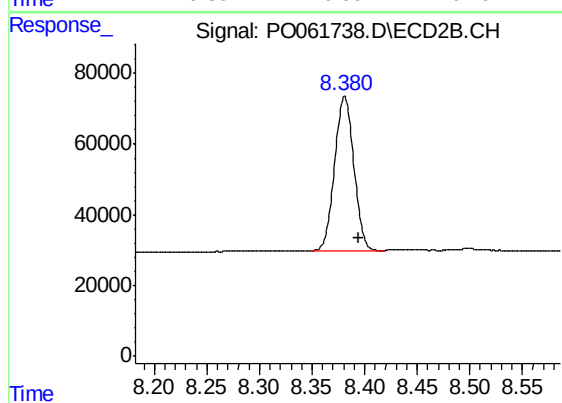

#2 Decachlorobiphenyl

R.T.: 8.381 min
Delta R.T.: -0.013 min
Response: 555117
Conc: 17.15 ng/ml