

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100719\
Data File : P0061756.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Oct 2019 19:39
Operator : HP/AJ
Sample : K5215-11
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
13933

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 02:51:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.360	3.521	986410	833991	24.050	25.789
2)	SA Decachlor...	10.030	8.393	676222	401170	14.520	12.391

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100719\
Data File : PO061756.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Oct 2019 19:39
Operator : HP/AJ
Sample : K5215-11
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
13933

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 02:51:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

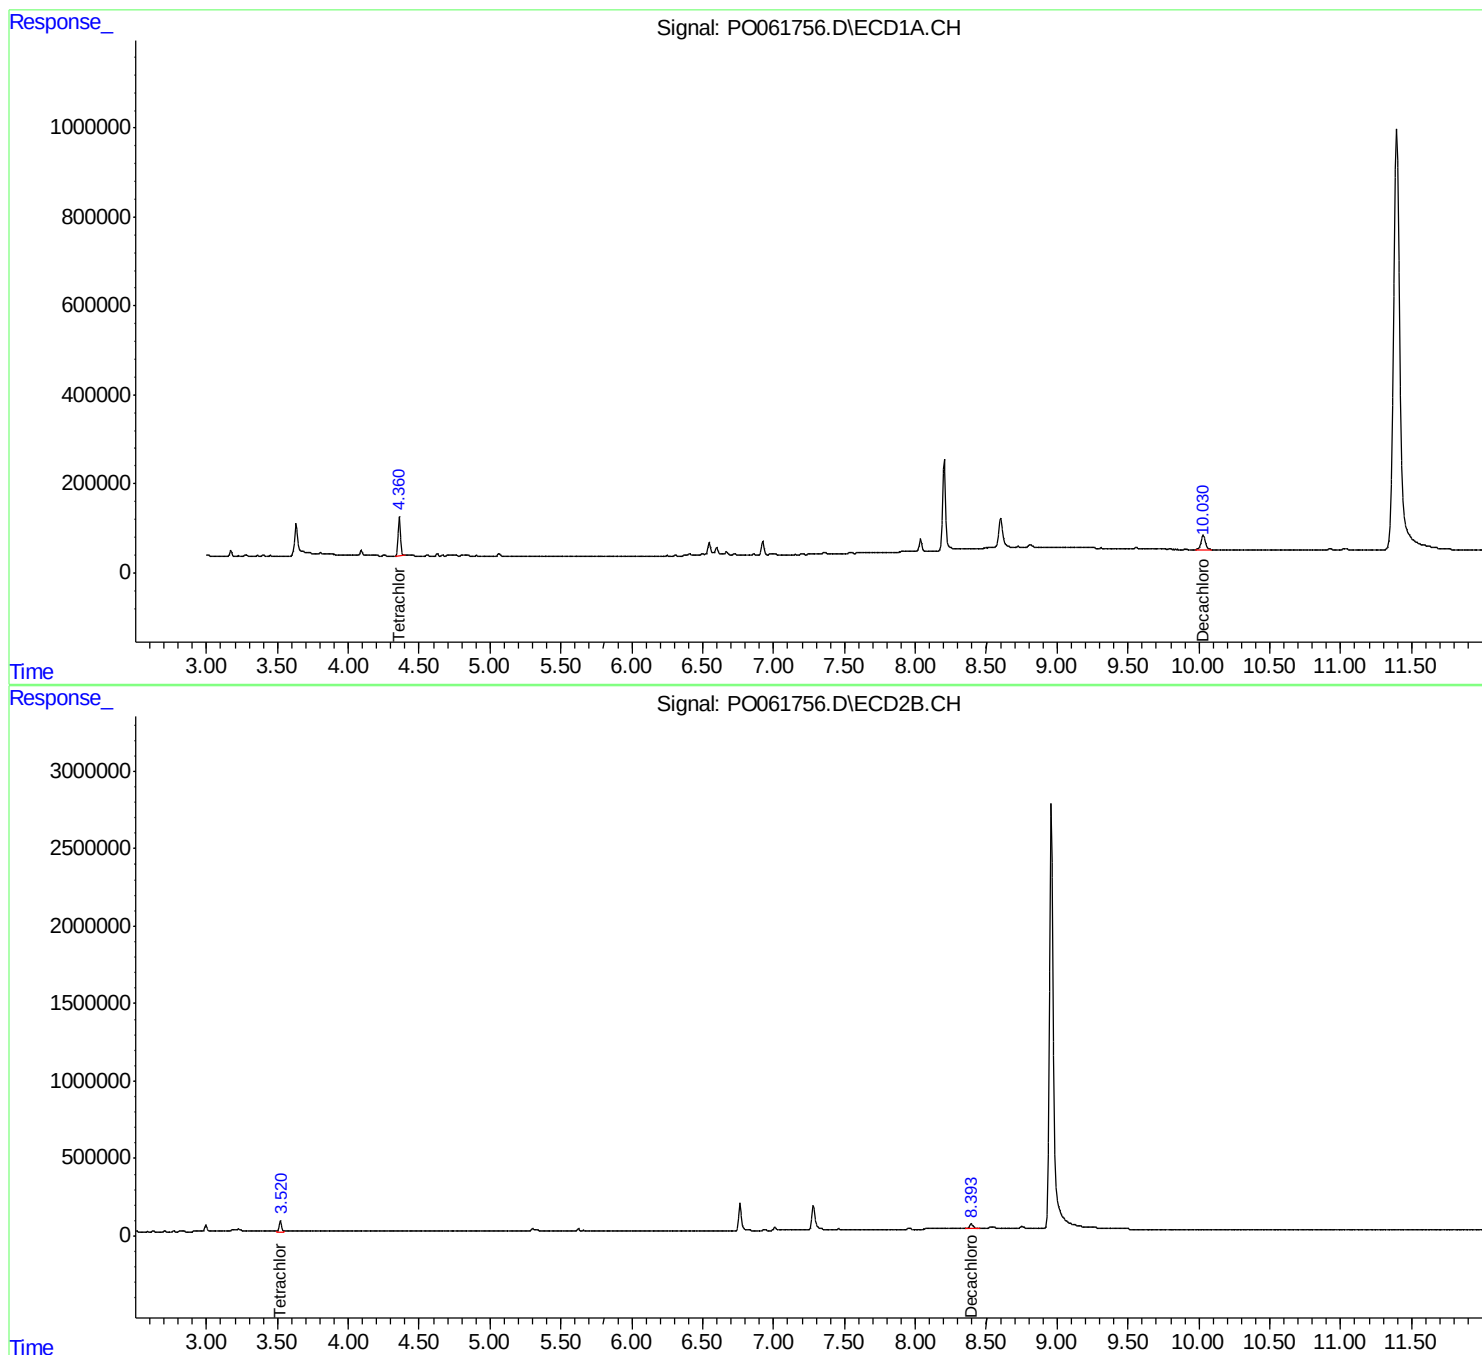


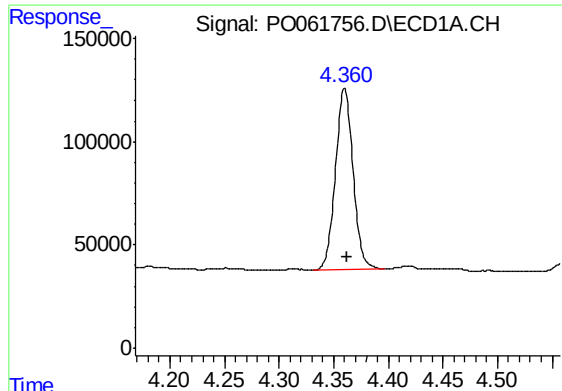

#1 Tetrachloro-m-xylene


R.T.: 4.360 min
Delta R.T.: -0.003 min
Response: 986410
Conc: 24.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
13933

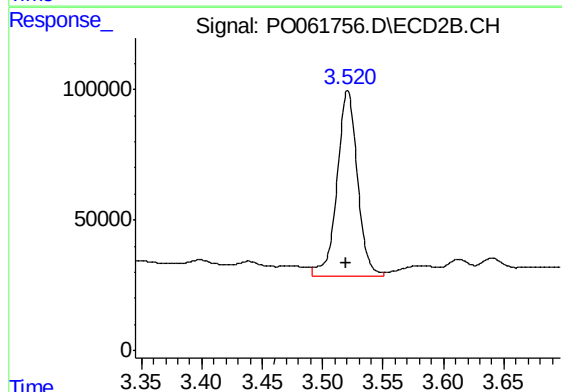


#1 Tetrachloro-m-xylene

R.T.: 3.521 min
Delta R.T.: 0.002 min
Response: 833991
Conc: 25.79 ng/ml

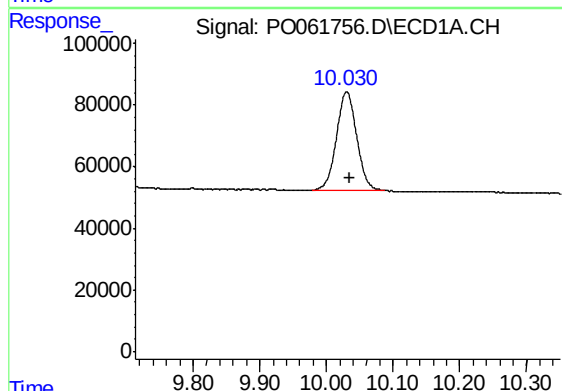

#2 Decachlorobiphenyl

R.T.: 10.030 min
Delta R.T.: -0.006 min
Response: 676222
Conc: 14.52 ng/ml

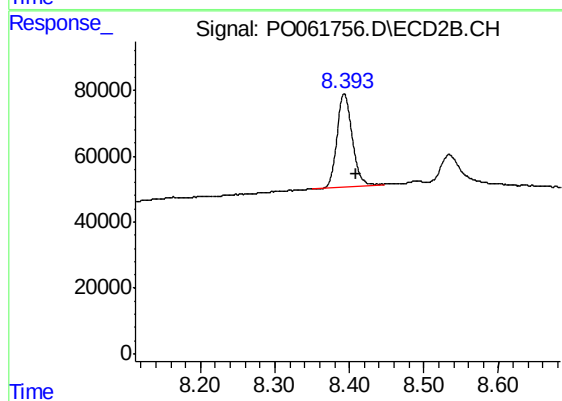

#2 Decachlorobiphenyl

R.T.: 8.393 min
Delta R.T.: -0.016 min
Response: 401170
Conc: 12.39 ng/ml