

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100719\
Data File : P0061760.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Oct 2019 20:44
Operator : HP/AJ
Sample : K5231-04
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
20190766-SS-COMPOSITE-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 02:54:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.359	3.519	1023053	764244	24.944	23.632
2)	SA Decachlor...	10.019	8.382	567079	381026	12.177	11.769

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100719\
Data File : PO061760.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Oct 2019 20:44
Operator : HP/AJ
Sample : K5231-04
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
20190766-SS-COMPOSITE-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 02:54:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

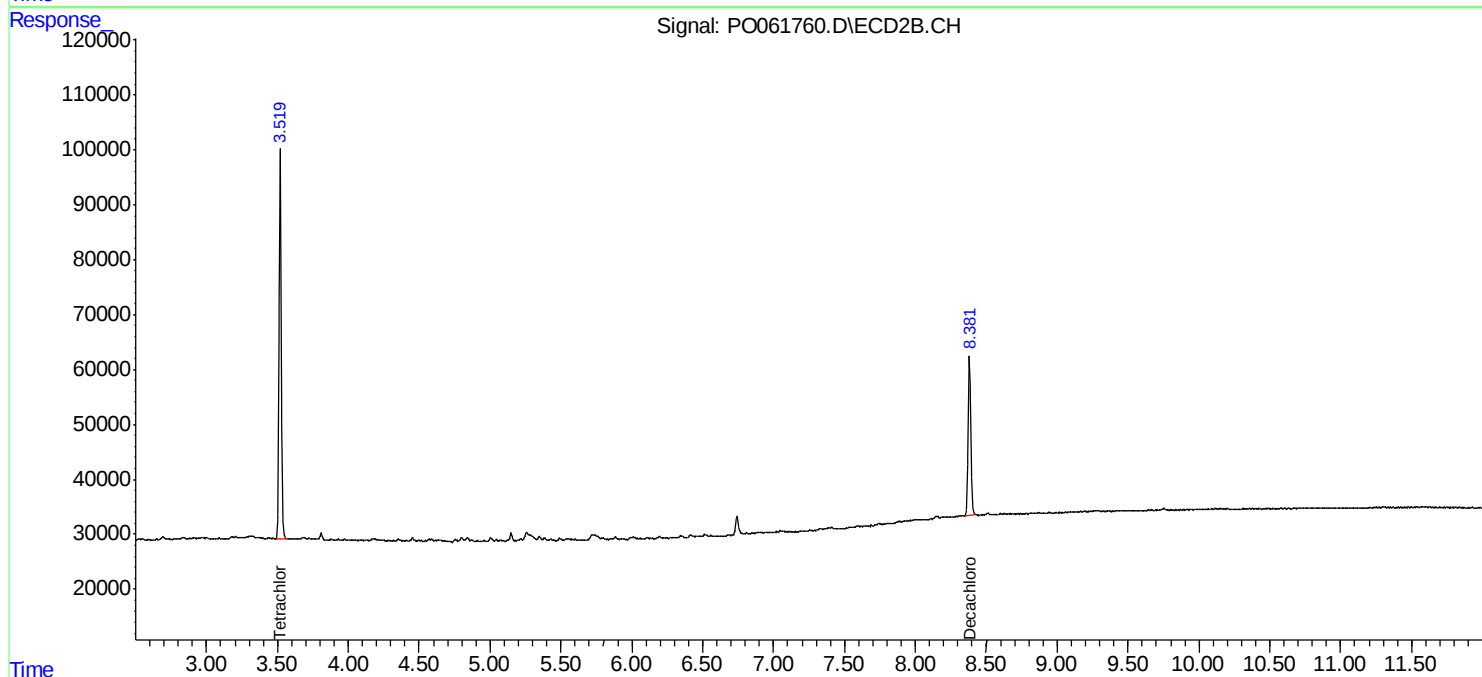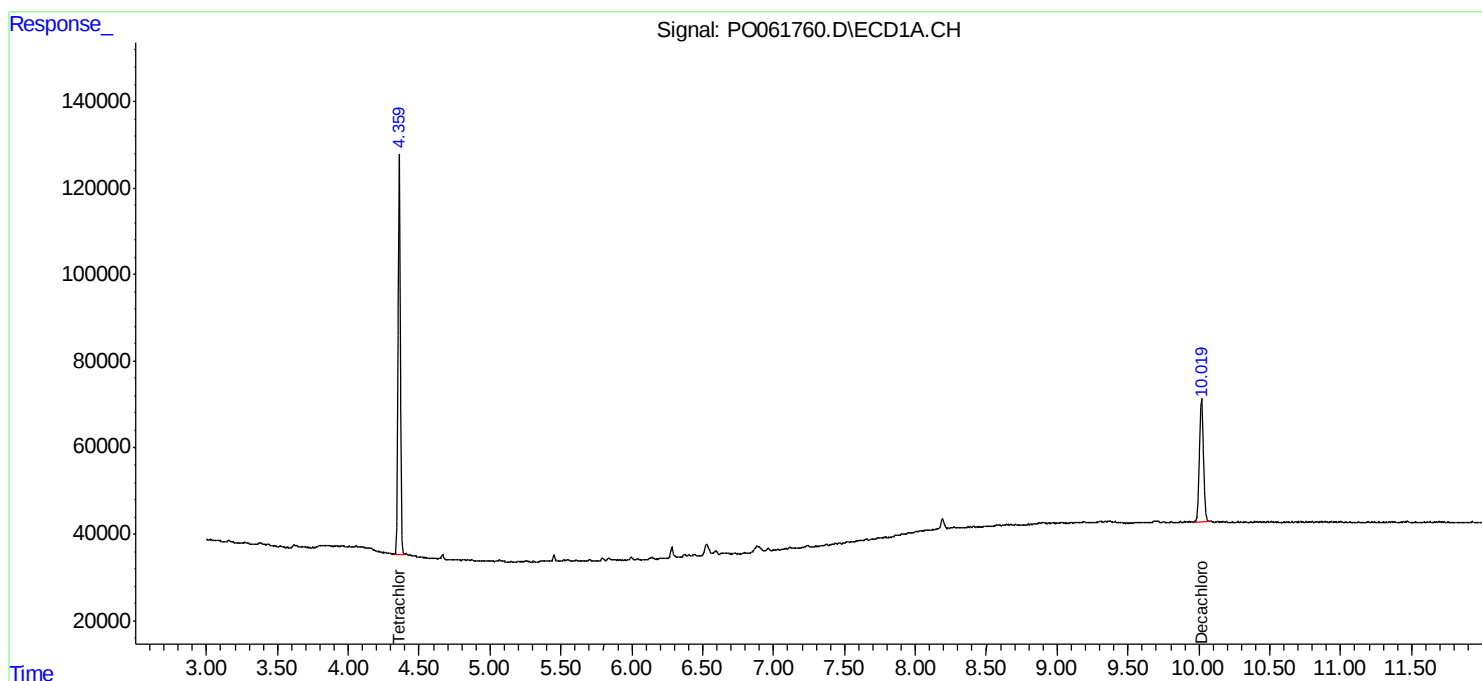


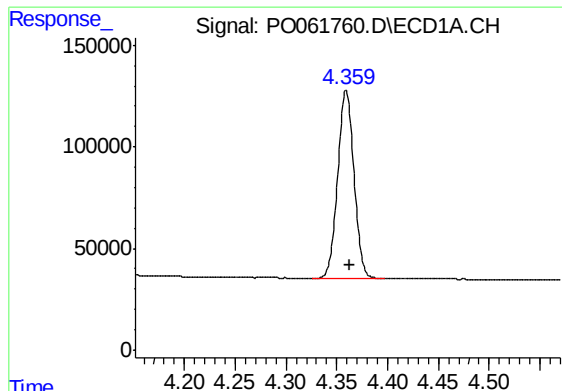

#1 Tetrachloro-m-xylene


R.T.: 4.359 min
Delta R.T.: -0.004 min
Response: 1023053
Conc: 24.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
20190766-SS-COMPOSITE-6

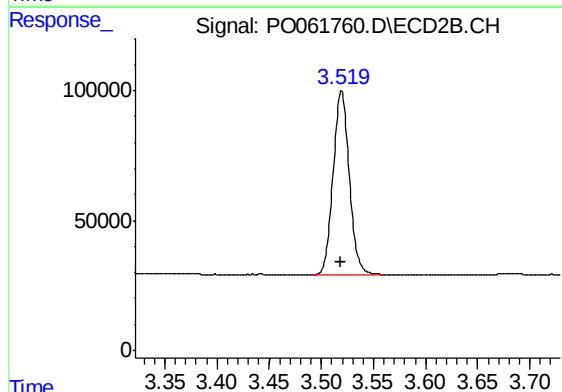


#1 Tetrachloro-m-xylene

R.T.: 3.519 min
Delta R.T.: 0.000 min
Response: 764244
Conc: 23.63 ng/ml

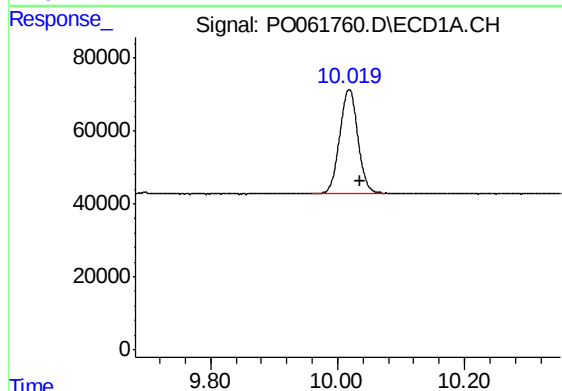

#2 Decachlorobiphenyl

R.T.: 10.019 min
Delta R.T.: -0.017 min
Response: 567079
Conc: 12.18 ng/ml

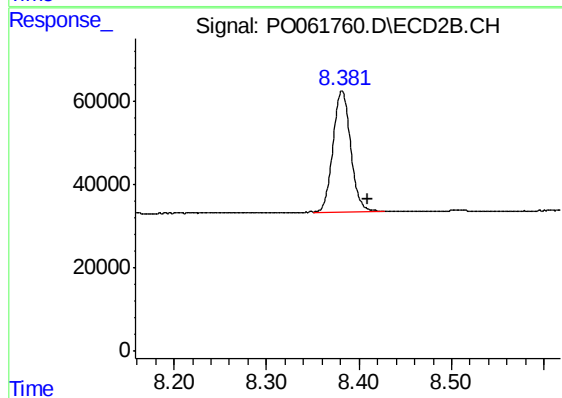

#2 Decachlorobiphenyl

R.T.: 8.382 min
Delta R.T.: -0.027 min
Response: 381026
Conc: 11.77 ng/ml