

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100719\
 Data File : P0061766.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Oct 2019 00:34
 Operator : HP/AJ
 Sample : K5212-02 10X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MLV01-PADS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 08 02:58:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.361	3.520	66891	91170	1.631	2.819 #
2)	SA Decachlor...	10.021	8.385	65312	46613	1.402	1.440

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100719\
Data File : PO061766.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Oct 2019 00:34
Operator : HP/AJ
Sample : K5212-02 10X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MLV01-PADS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 02:58:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

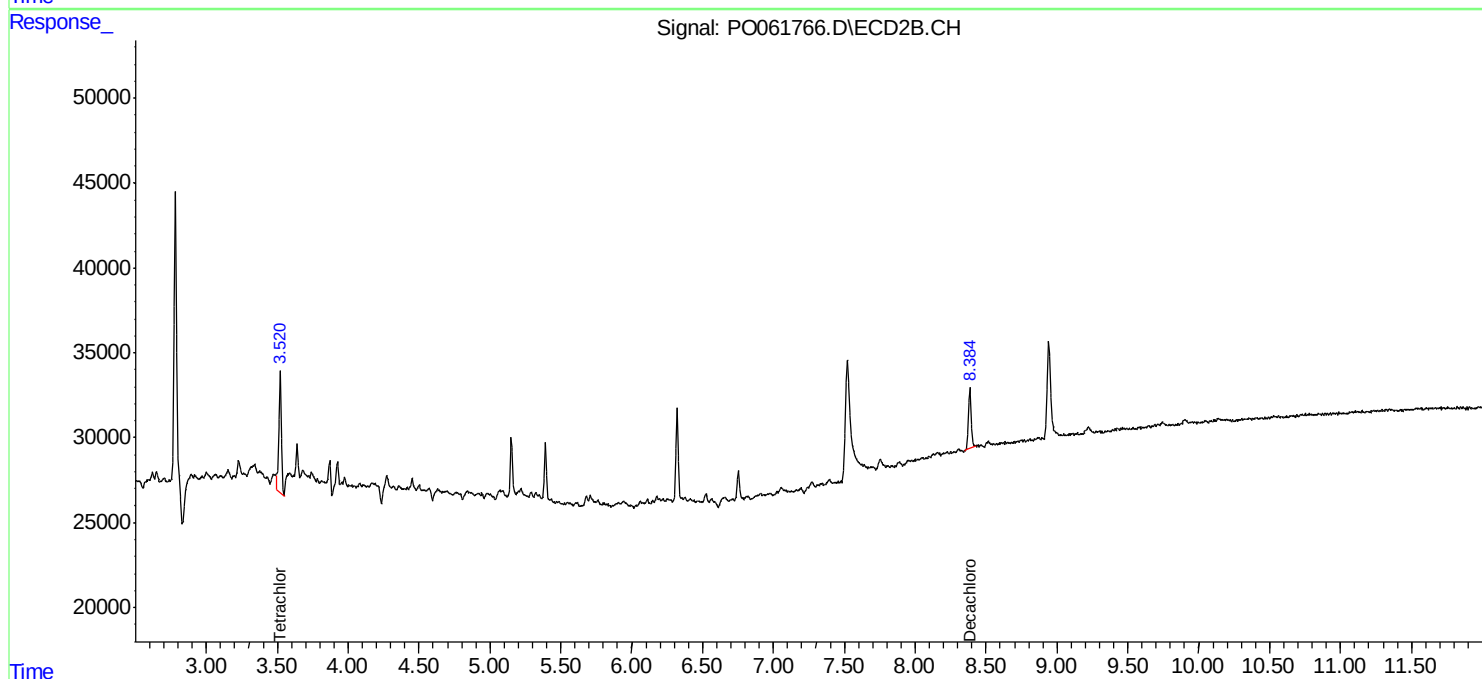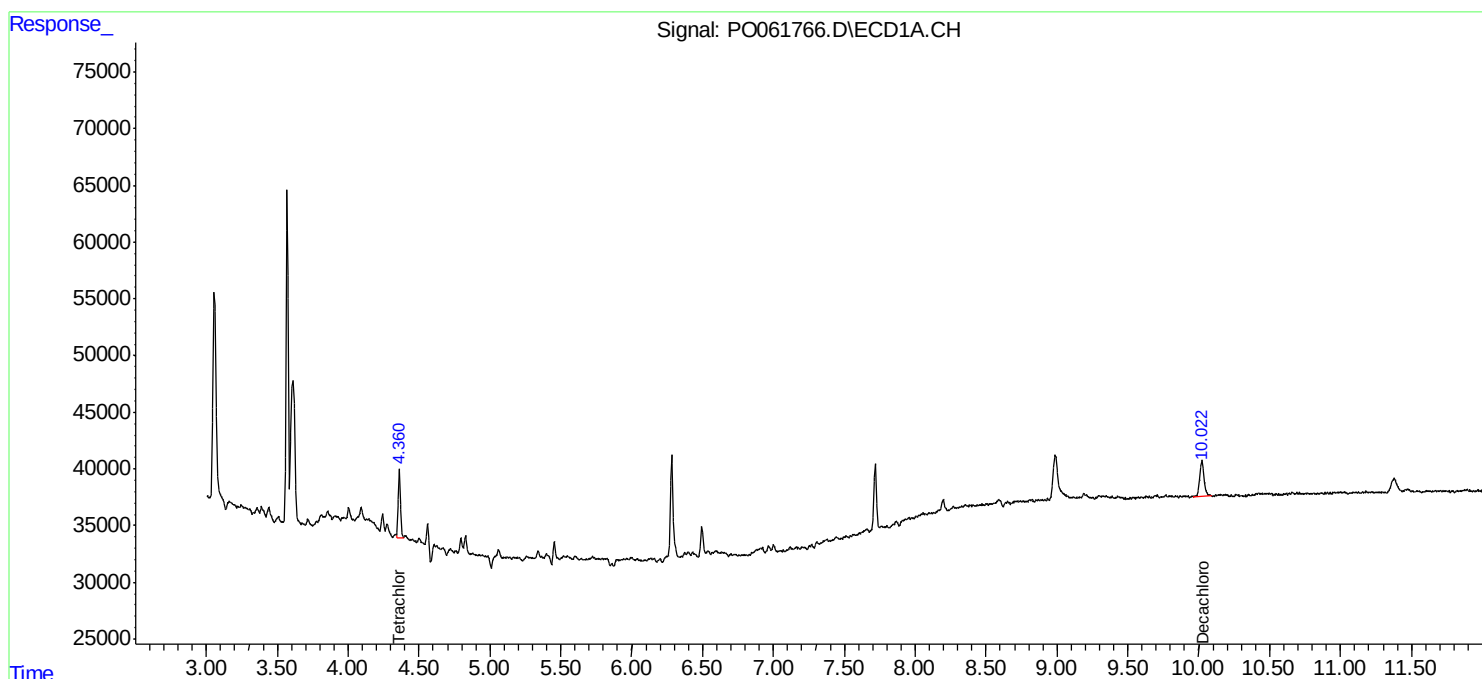


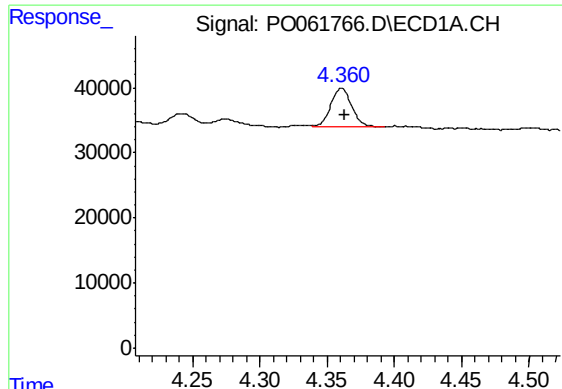

#1 Tetrachloro-m-xylene


R.T.: 4.361 min
Delta R.T.: -0.002 min
Response: 66891
Conc: 1.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
MLV01-PADS

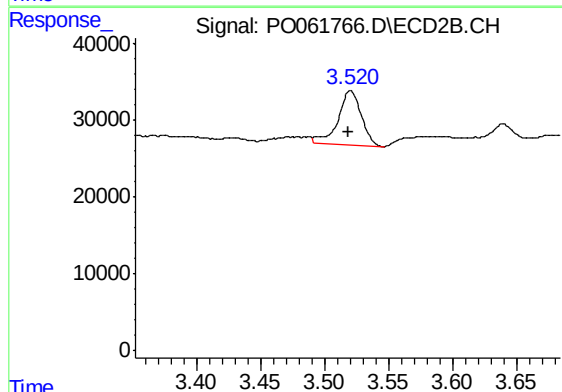


#1 Tetrachloro-m-xylene

R.T.: 3.520 min
Delta R.T.: 0.001 min
Response: 91170
Conc: 2.82 ng/ml

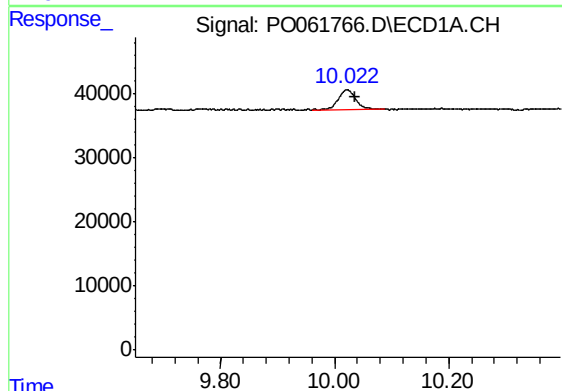

#2 Decachlorobiphenyl

R.T.: 10.021 min
Delta R.T.: -0.015 min
Response: 65312
Conc: 1.40 ng/ml

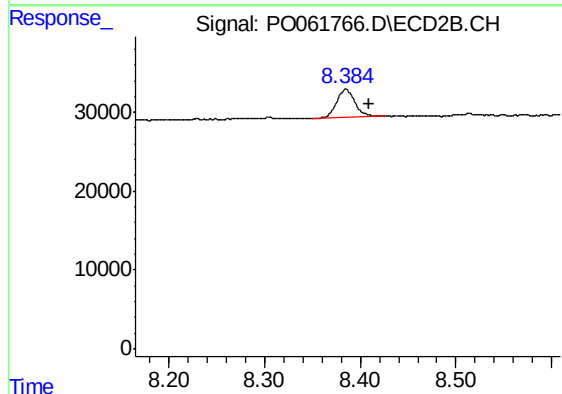

#2 Decachlorobiphenyl

R.T.: 8.385 min
Delta R.T.: -0.024 min
Response: 46613
Conc: 1.44 ng/ml