

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100719\
 Data File : P0061767.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Oct 2019 00:50
 Operator : HP/AJ
 Sample : K5215-12 10X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 30473

Manual Integrations
 APPROVED

Ankita
 10/9/2019 8:08:31 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 08 02:58:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.360	3.522	127310	87106	3.104	2.694
2)	SA Decachlor...	10.014	8.380	116382	89851	2.499m	2.775

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100719\
Data File : PO061767.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Oct 2019 00:50
Operator : HP/AJ
Sample : K5215-12 10X
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
30473


Manual Integrations
APPROVED

Ankita
10/9/2019 8:08:31 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 02:58:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

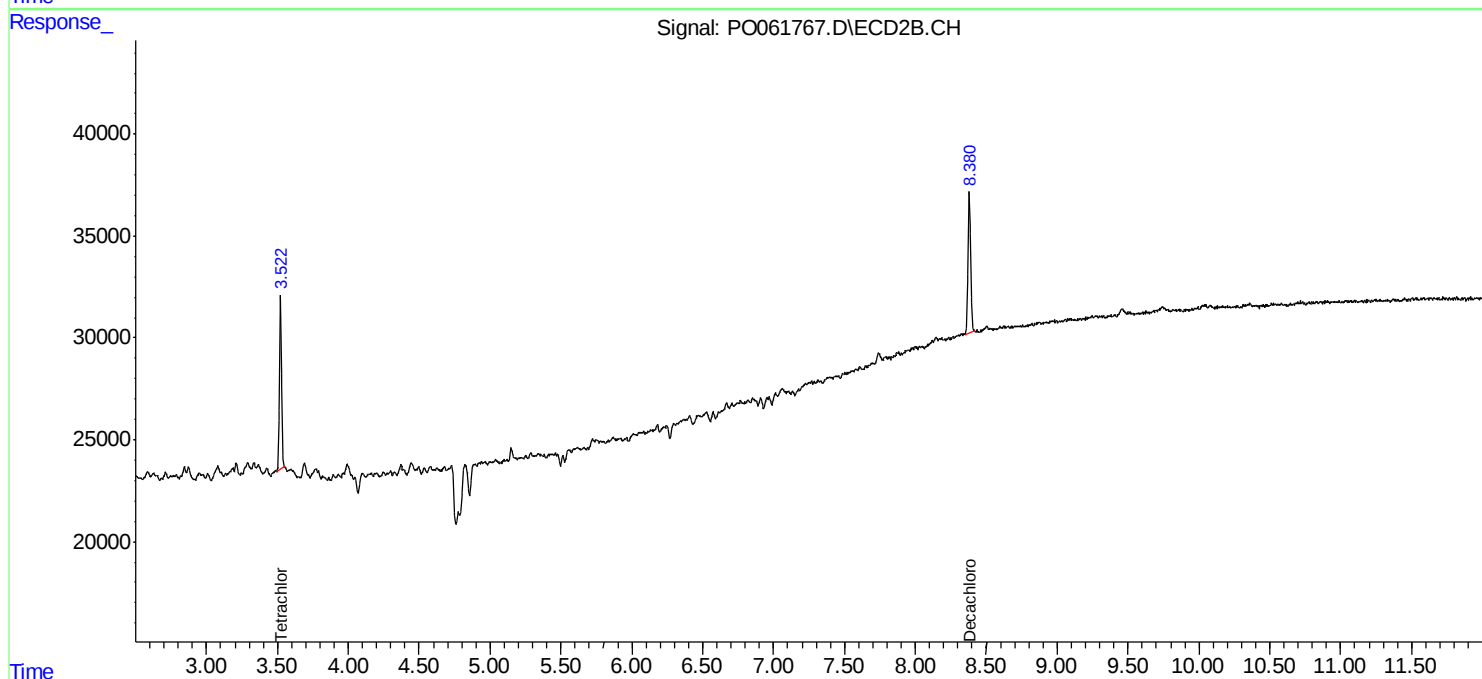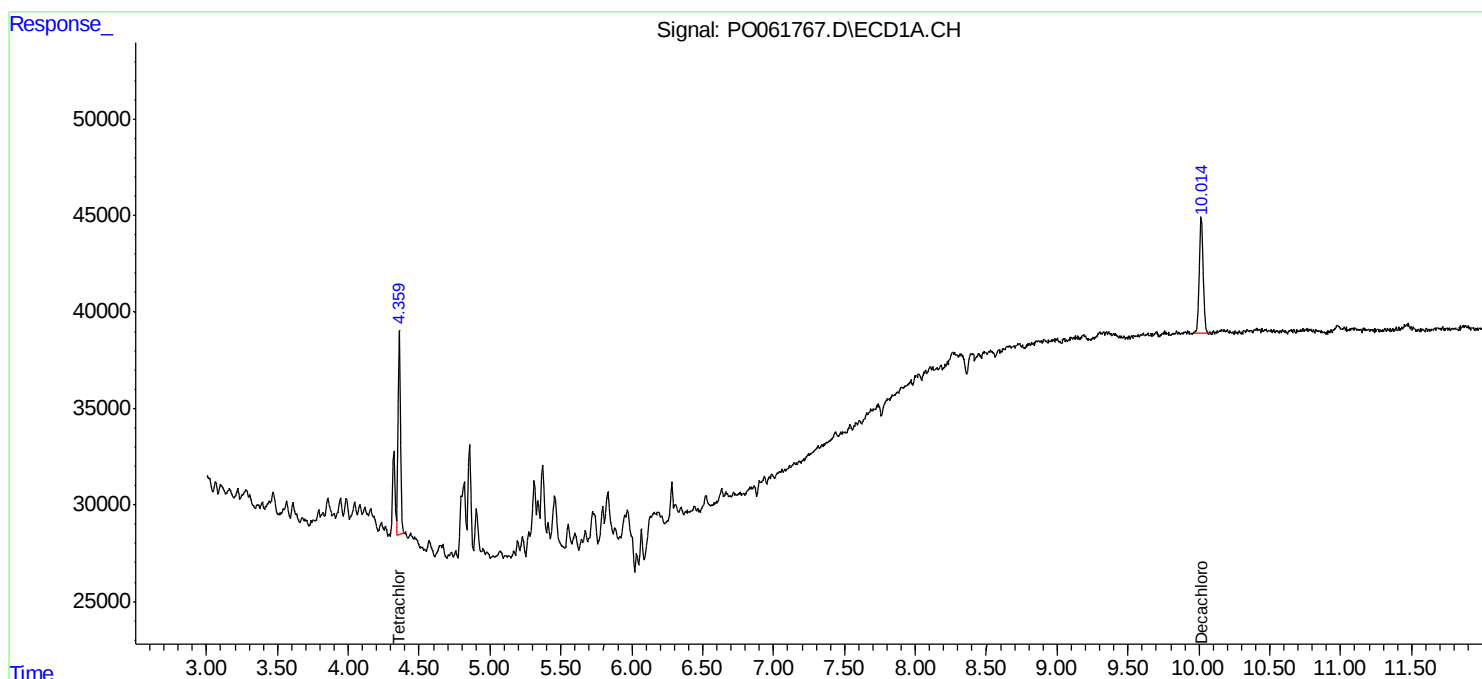

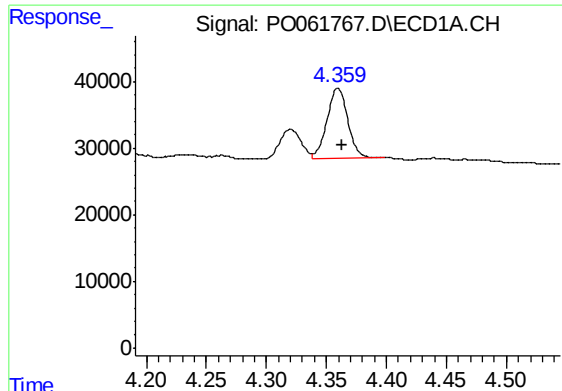


#1 Tetrachloro-m-xylene

R.T.: 4.360 min
Delta R.T.: -0.003 min
Response: 127310
Conc: 3.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
30473


Manual Integrations
APPROVED

Ankita
10/9/2019 8:08:31 AM

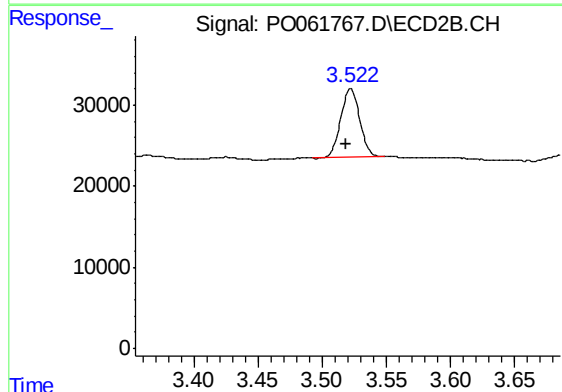


#1 Tetrachloro-m-xylene

R.T.: 3.522 min
Delta R.T.: 0.003 min
Response: 87106
Conc: 2.69 ng/ml

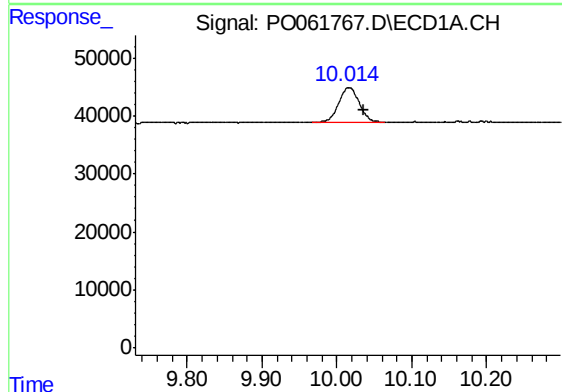

#2 Decachlorobiphenyl

R.T.: 10.014 min
Delta R.T.: -0.022 min
Response: 116382
Conc: 2.50 ng/ml m

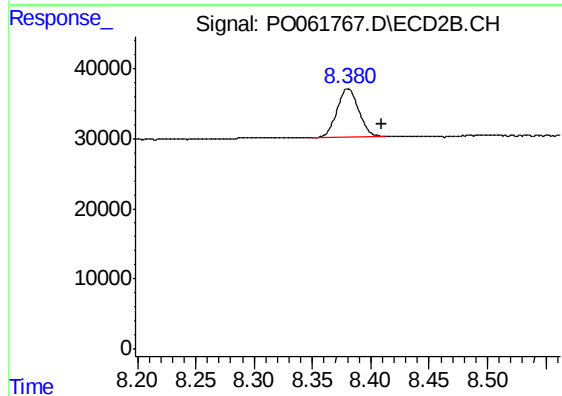

#2 Decachlorobiphenyl

R.T.: 8.380 min
Delta R.T.: -0.029 min
Response: 89851
Conc: 2.78 ng/ml