

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100720\
 Data File : PO072094.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Oct 2020 14:37
 Operator : DD\AJ
 Sample : L4224-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OR-02-100620

Manual Integrations
 APPROVED

Ankita
 10/8/2020 11:17:52 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 17:09:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.326	3.512	1770538	995493	24.650m	26.578
2) SA Decachlor...	9.935	8.687	1727590	837393	15.690	14.722
Target Compounds						
26) L6 AR-1254-1	6.520	5.585	544663	380463	155.896	159.200
27) L6 AR-1254-2	6.748	5.747	918581	407895	166.847	190.697
28) L6 AR-1254-3	7.125	6.156	1202067	737344	208.144	217.175
29) L6 AR-1254-4	7.420	6.397	819388	371166	140.644	152.858
30) L6 AR-1254-5	7.841	6.818	1334451	869988	247.954	265.880

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100720\
Data File : PO072094.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Oct 2020 14:37
Operator : DD\AJ
Sample : L4224-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OR-02-100620


Manual Integrations
APPROVED

Ankita
10/8/2020 11:17:52 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 17:09:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

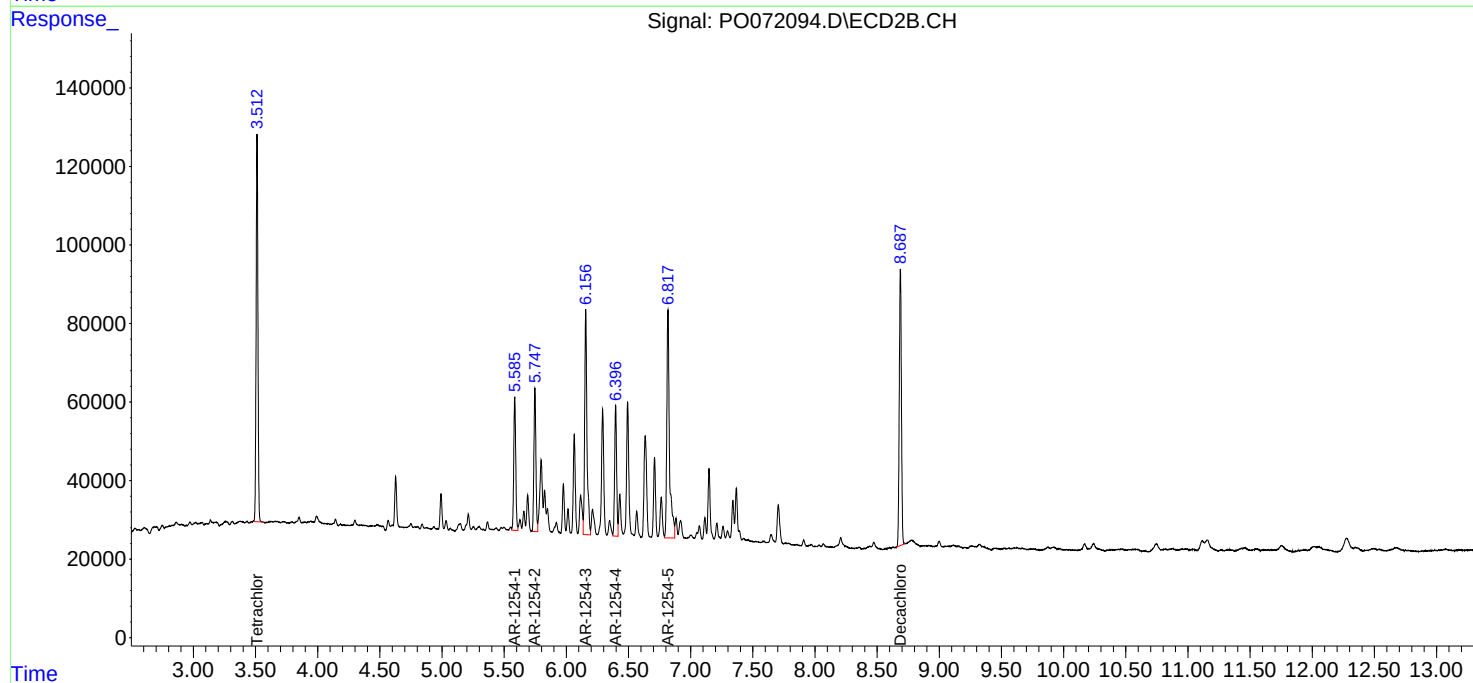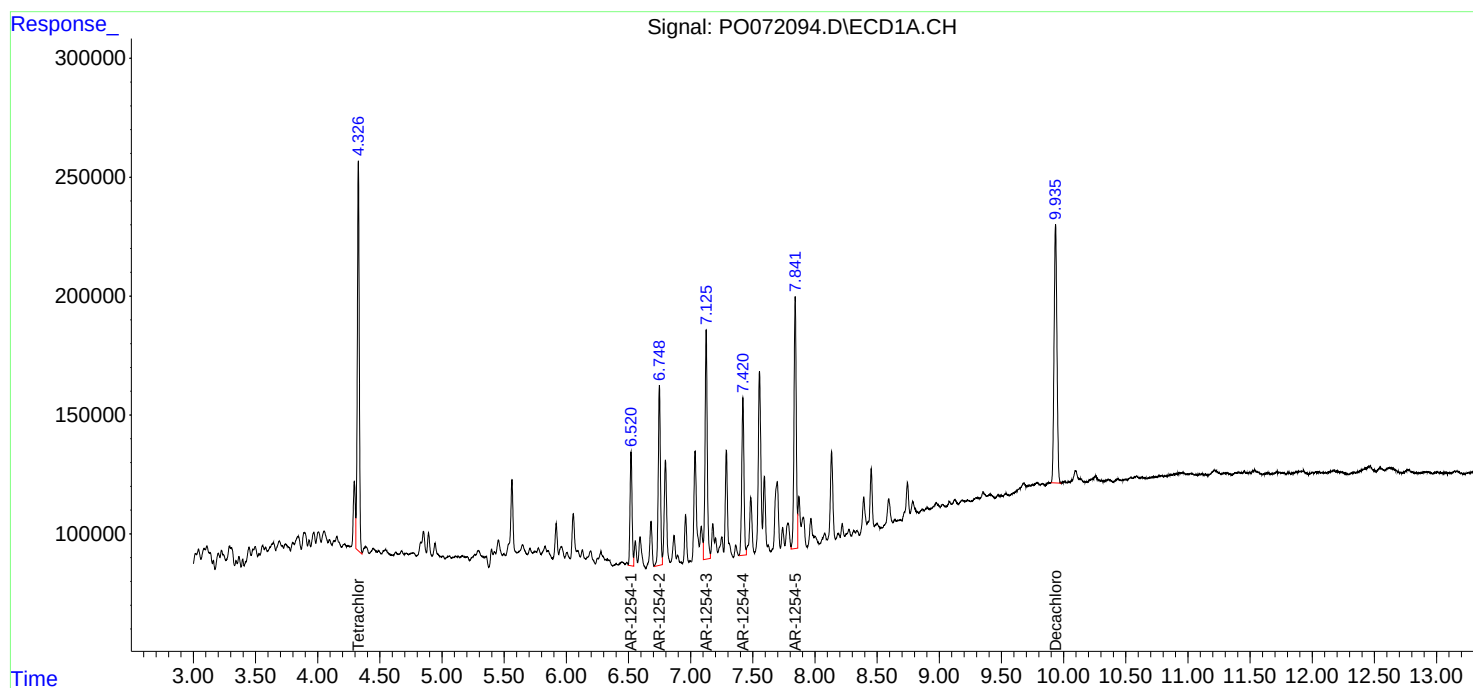

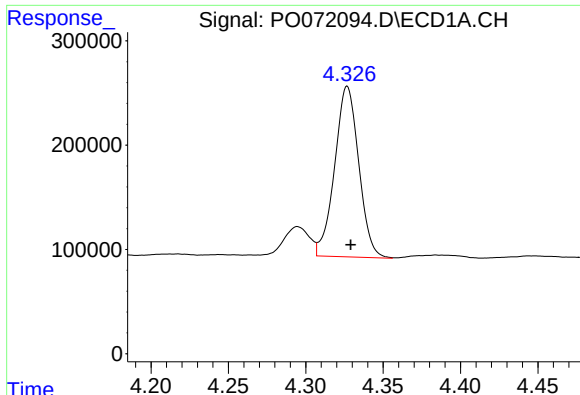


#1 Tetrachloro-m-xylene

R.T.: 4.326 min
Delta R.T.: -0.003 min
Response: 1770538
Conc: 24.65 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OR-02-100620


Manual Integrations
APPROVED

Ankita
10/8/2020 11:17:52 AM

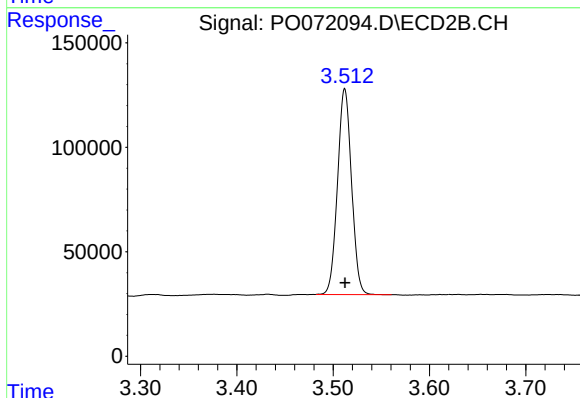


#1 Tetrachloro-m-xylene

R.T.: 3.512 min
Delta R.T.: 0.000 min
Response: 995493
Conc: 26.58 ng/ml

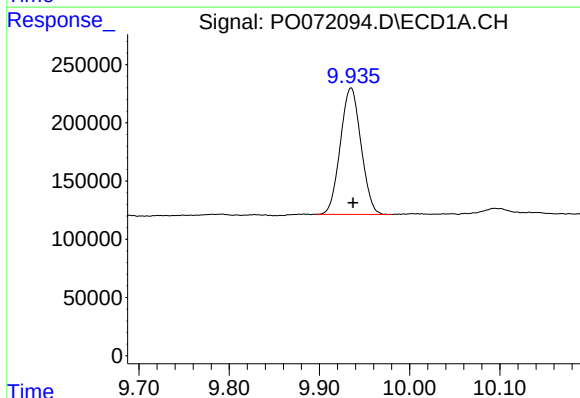


#2 Decachlorobiphenyl

R.T.: 9.935 min
Delta R.T.: -0.002 min
Response: 1727590
Conc: 15.69 ng/ml

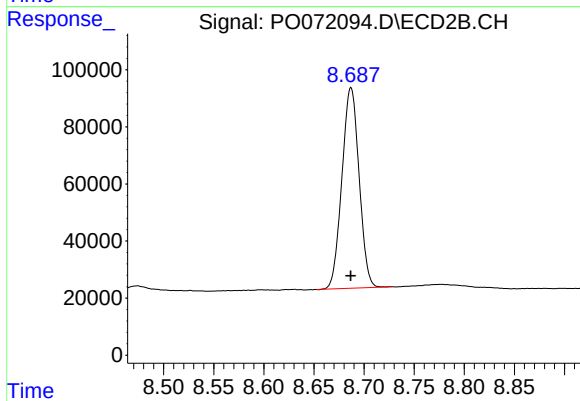

#2 Decachlorobiphenyl

R.T.: 8.687 min
Delta R.T.: 0.000 min
Response: 837393
Conc: 14.72 ng/ml

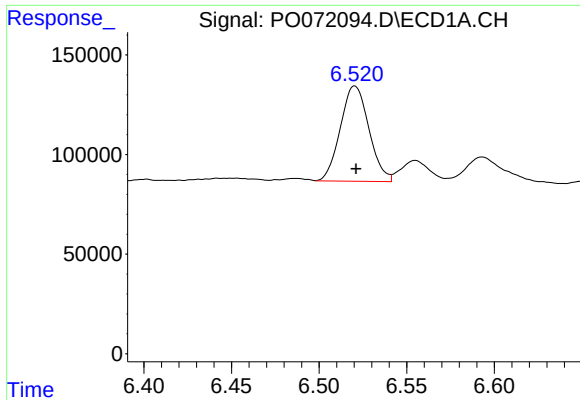


#26 AR-1254-1

R.T.: 6.520 min
Delta R.T.: 0.000 min
Response: 544663
Conc: 155.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
OR-02-100620


Manual Integrations
APPROVED

Ankita
10/8/2020 11:17:52 AM

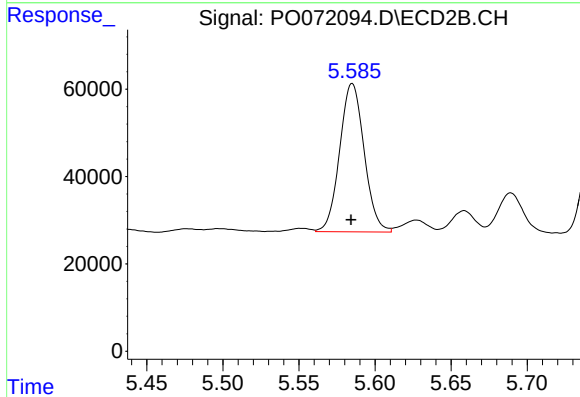


#26 AR-1254-1

R.T.: 5.585 min
Delta R.T.: 0.000 min
Response: 380463
Conc: 159.20 ng/ml

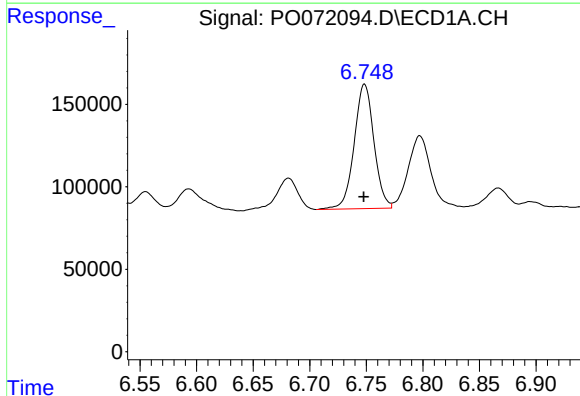


#27 AR-1254-2

R.T.: 6.748 min
Delta R.T.: 0.000 min
Response: 918581
Conc: 166.85 ng/ml

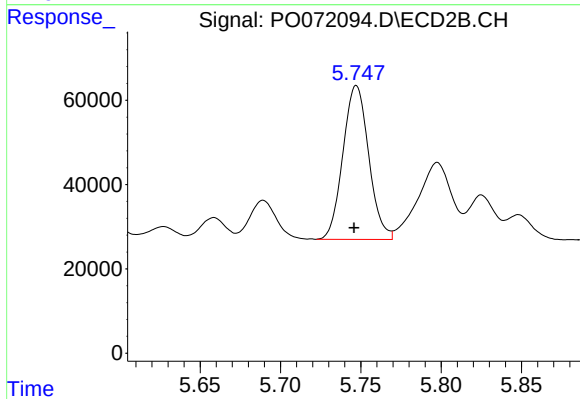

#27 AR-1254-2

R.T.: 5.747 min
Delta R.T.: 0.001 min
Response: 407895
Conc: 190.70 ng/ml

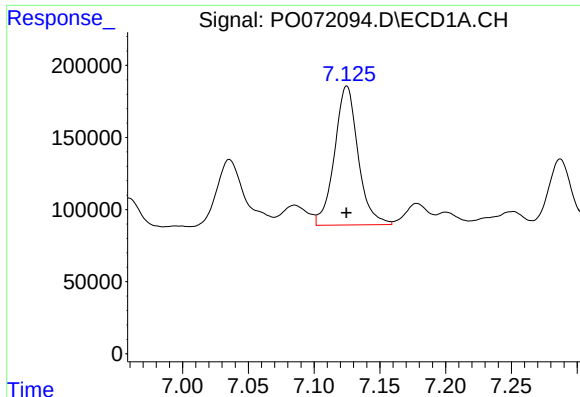


#28 AR-1254-3

R.T.: 7.125 min
Delta R.T.: 0.000 min
Response: 1202067
Conc: 208.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
OR-02-100620


Manual Integrations
APPROVED

Ankita
10/8/2020 11:17:52 AM

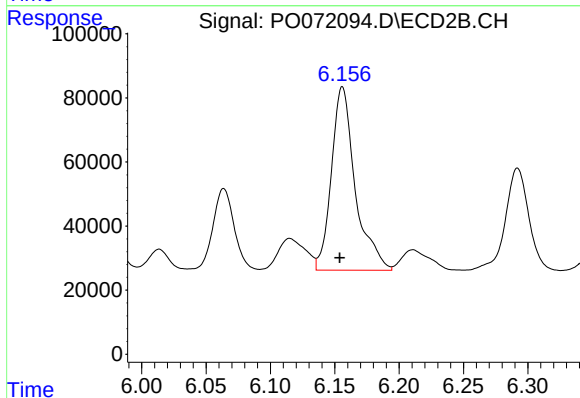


#28 AR-1254-3

R.T.: 6.156 min
Delta R.T.: 0.002 min
Response: 737344
Conc: 217.18 ng/ml

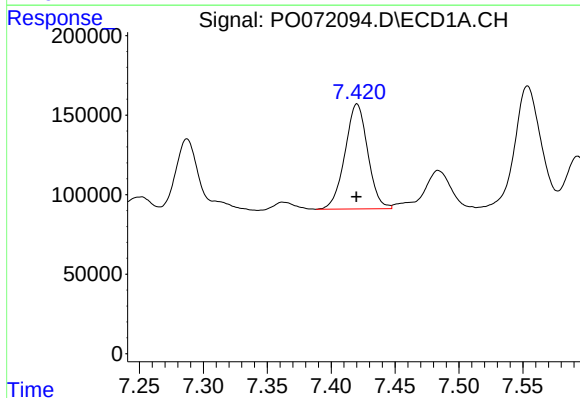


#29 AR-1254-4

R.T.: 7.420 min
Delta R.T.: 0.000 min
Response: 819388
Conc: 140.64 ng/ml

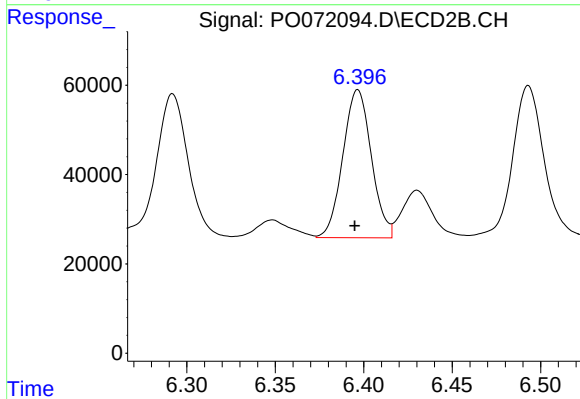

#29 AR-1254-4

R.T.: 6.397 min
Delta R.T.: 0.002 min
Response: 371166
Conc: 152.86 ng/ml

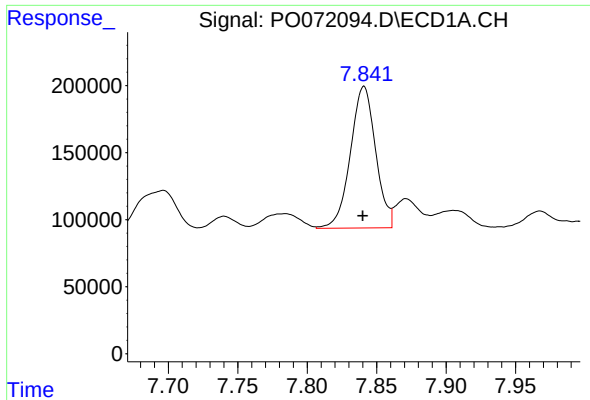


#30 AR-1254-5

R.T.: 7.841 min
Delta R.T.: 0.000 min
Response: 1334451
Conc: 247.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
OR-02-100620

Manual Integrations
APPROVED

Ankita
10/8/2020 11:17:52 AM

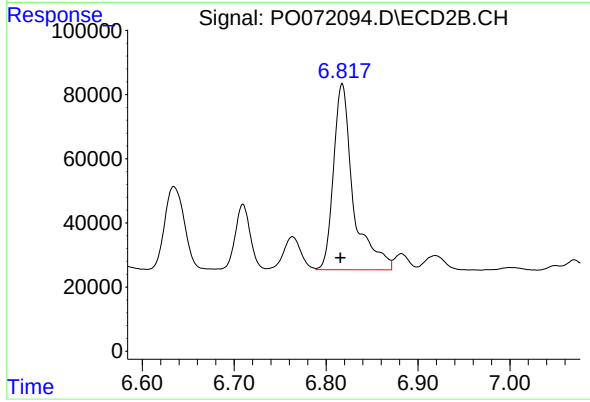

#30 AR-1254-5

R.T.: 6.818 min
Delta R.T.: 0.002 min
Response: 869988
Conc: 265.88 ng/ml