

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100721\
 Data File : PO081889.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Oct 2021 3:24
 Operator : AJ\MA
 Sample : M4111-07
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 08 04:41:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 07 09:43:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.991	3.979	1942058	599589	23.403	23.695
2)	SA Decachlor...	11.112	9.309	1360133	557720	22.931	23.609
Target Compounds							
8)	L2 AR-1221-1	5.241	0.000	28264	0	29.596	N.D. #
9)	L2 AR-1221-2	5.344	0.000	22729	0	35.205	N.D. #
30)	L6 AR-1254-5	8.572	0.000	2350	0	0.720	N.D. #
32)	L7 AR-1260-2	8.263f	0.000	20771	0	5.624	N.D. #
33)	L7 AR-1260-3	8.682f	0.000	25653	0	10.376	N.D. #
35)	L7 AR-1260-5	9.231	0.000	2348	0	0.402	N.D. #
36)	L8 AR-1262-1	8.682f	0.000	25653	0	6.525	N.D. #
37)	L8 AR-1262-2	9.231	0.000	2348	0	0.340	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100721\
Data File : PO081889.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Oct 2021 3:24
Operator : AJ\MA
Sample : M4111-07
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 04:41:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 07 09:43:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

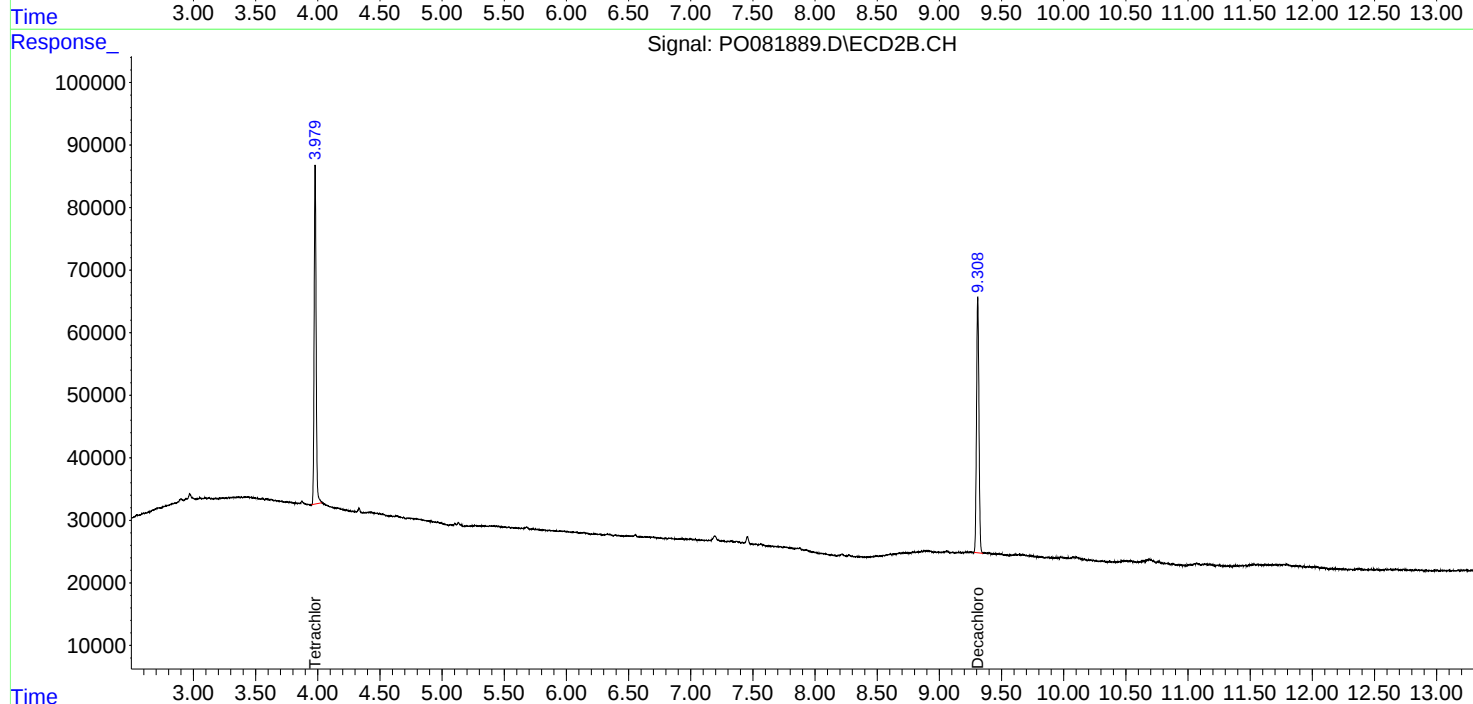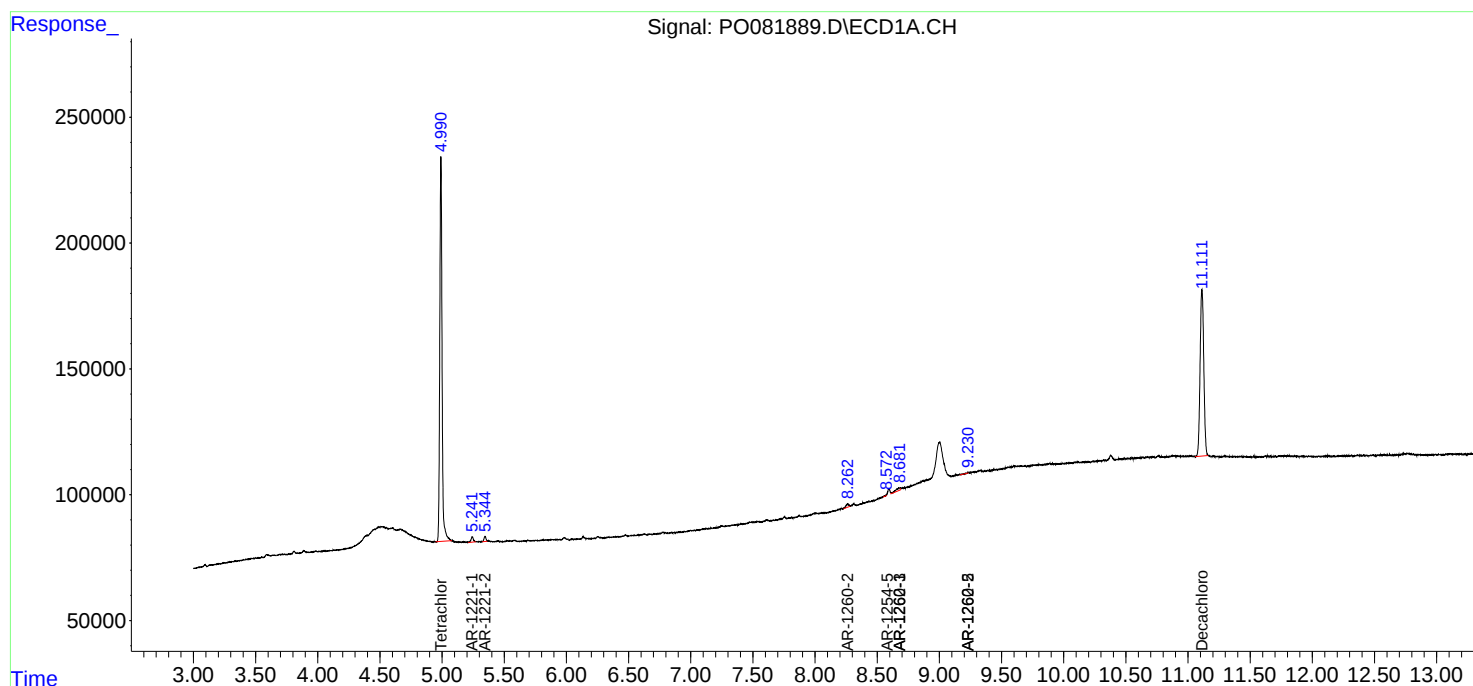


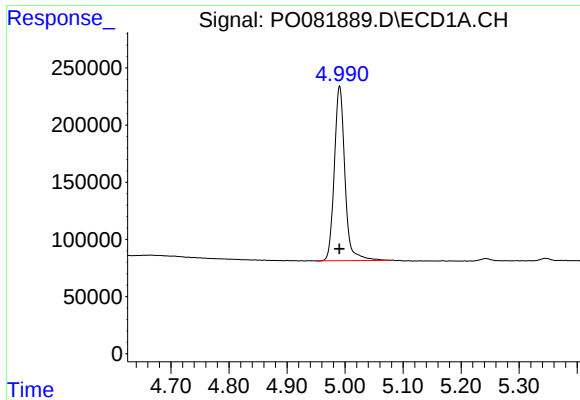

#1 Tetrachloro-m-xylene


R.T.: 4.991 min
Delta R.T.: 0.000 min
Response: 1942058
Conc: 23.40 ng/ml

Instrument :
ECD_O
ClientSampleId :

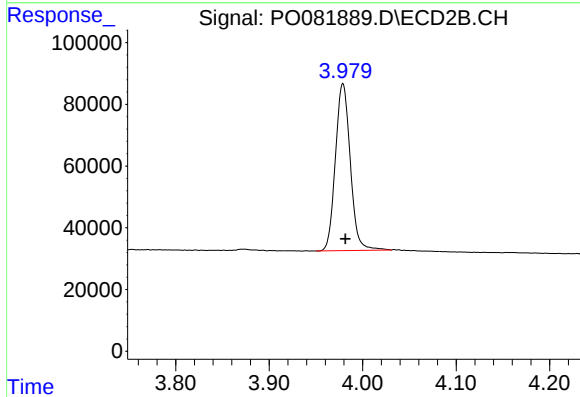


#1 Tetrachloro-m-xylene

R.T.: 3.979 min
Delta R.T.: -0.002 min
Response: 599589
Conc: 23.70 ng/ml

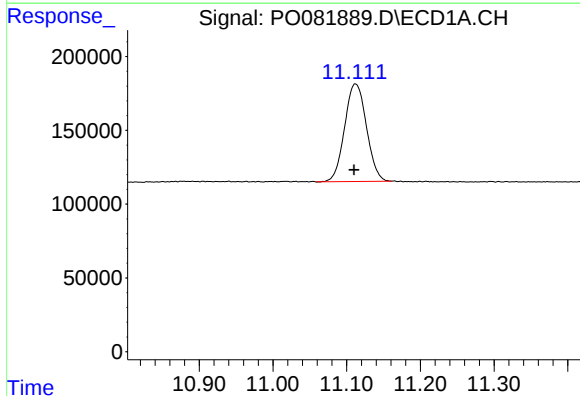


#2 Decachlorobiphenyl

R.T.: 11.112 min
Delta R.T.: 0.002 min
Response: 1360133
Conc: 22.93 ng/ml

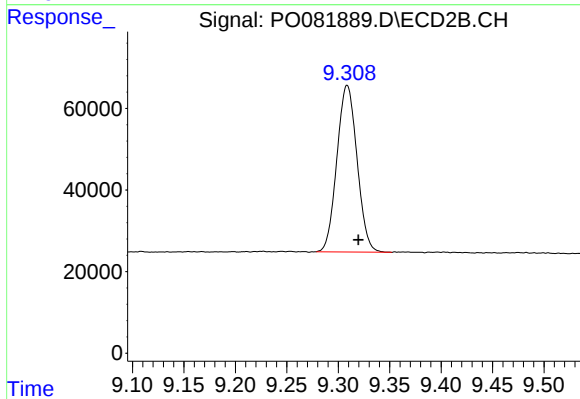

#2 Decachlorobiphenyl


R.T.: 9.309 min
Delta R.T.: -0.011 min
Response: 557720
Conc: 23.61 ng/ml

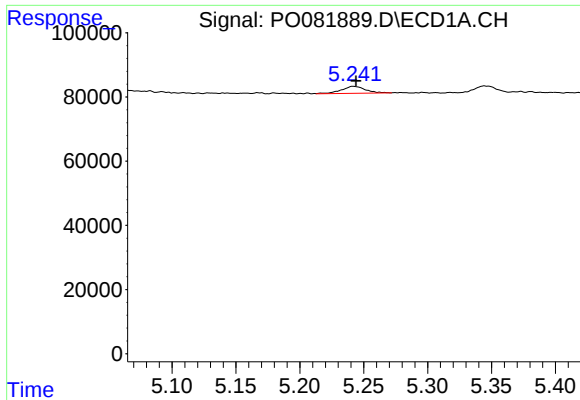

#8 AR-1221-1


R.T.: 5.241 min
Delta R.T.: -0.002 min
Response: 28264
Conc: 29.60 ng/ml

Instrument :
ECD_O
ClientSampleId :

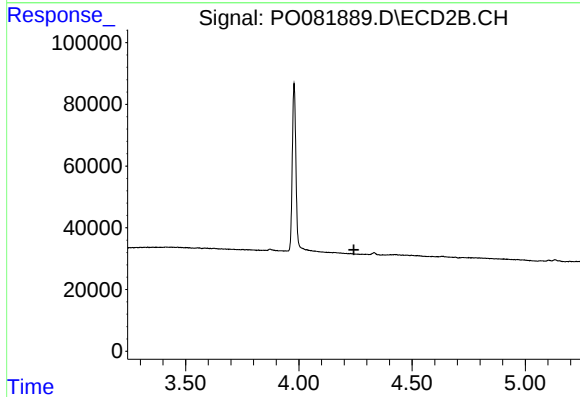


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.243 min
Response: 0
Conc: N.D.

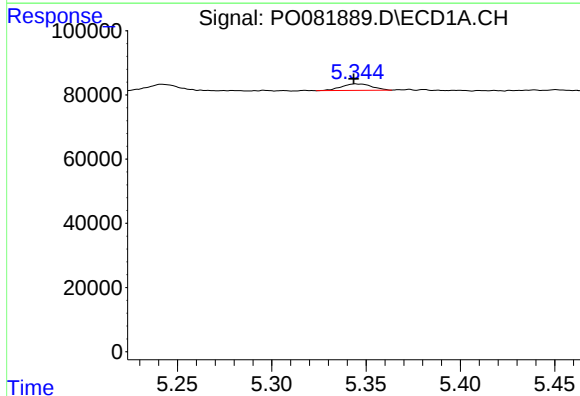


#9 AR-1221-2

R.T.: 5.344 min
Delta R.T.: 0.000 min
Response: 22729
Conc: 35.20 ng/ml

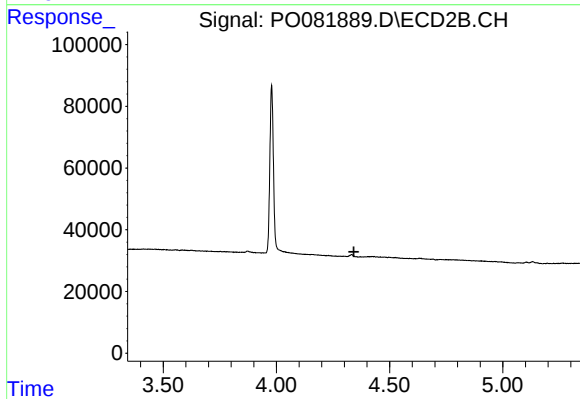

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.342 min
Response: 0
Conc: N.D.

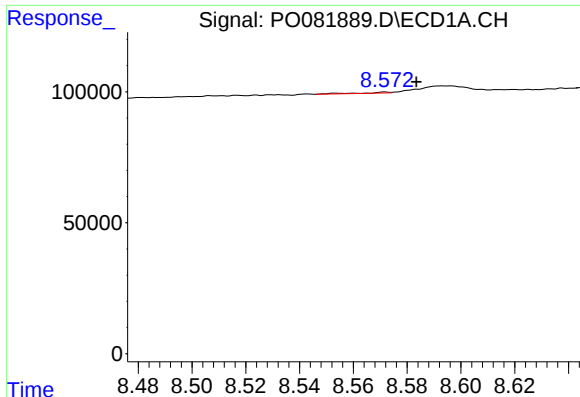

#30 AR-1254-5


R.T.: 8.572 min
Delta R.T.: -0.012 min
Response: 2350
Conc: 0.72 ng/ml

Instrument :
ECD_O
ClientSampleId :

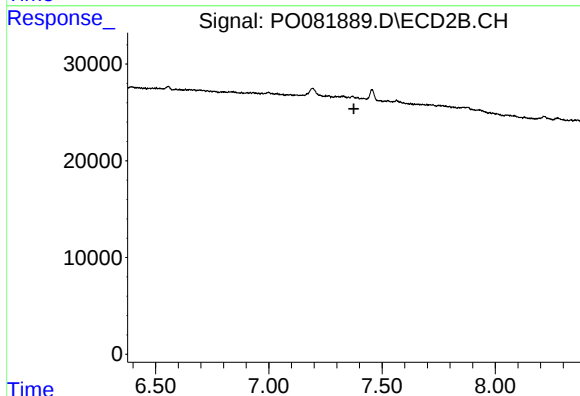


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.375 min
Response: 0
Conc: N.D.

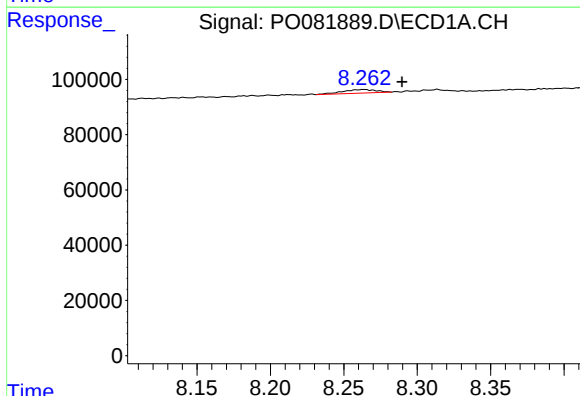


#32 AR-1260-2

R.T.: 8.263 min
Delta R.T.: -0.026 min
Response: 20771
Conc: 5.62 ng/ml

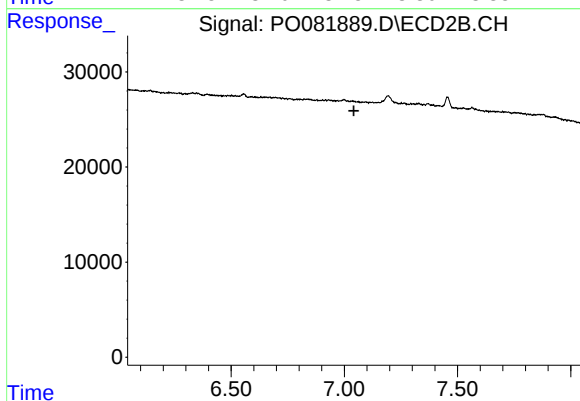

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.042 min
Response: 0
Conc: N.D.

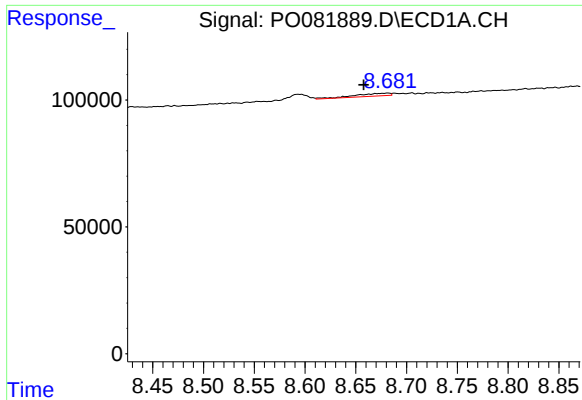

#33 AR-1260-3


R.T.: 8.682 min
Delta R.T.: 0.024 min
Response: 25653
Conc: 10.38 ng/ml

Instrument :
ECD_O
ClientSampleId :

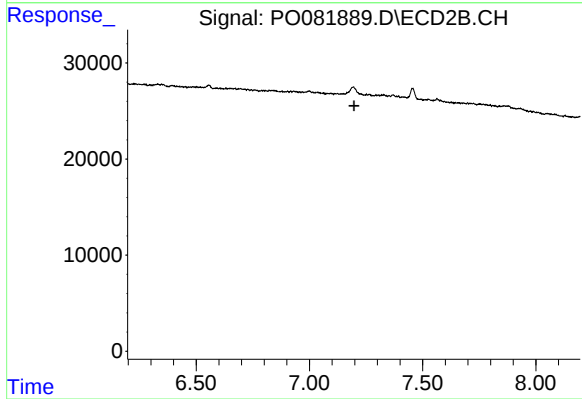


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.197 min
Response: 0
Conc: N.D.

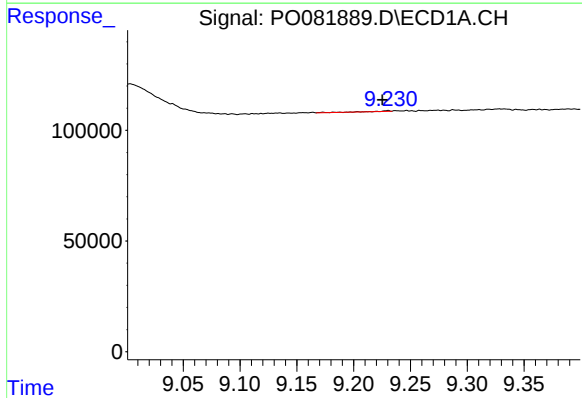


#35 AR-1260-5

R.T.: 9.231 min
Delta R.T.: 0.005 min
Response: 2348
Conc: 0.40 ng/ml

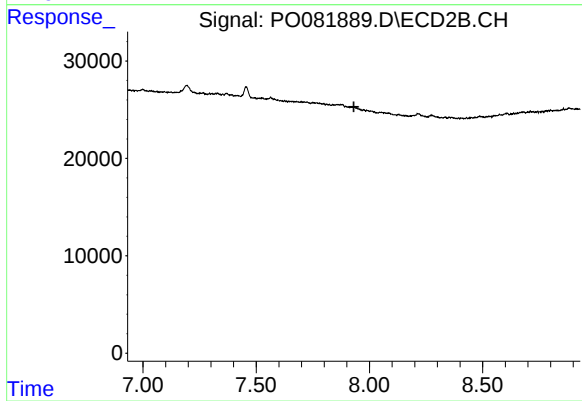

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.932 min
Response: 0
Conc: N.D.

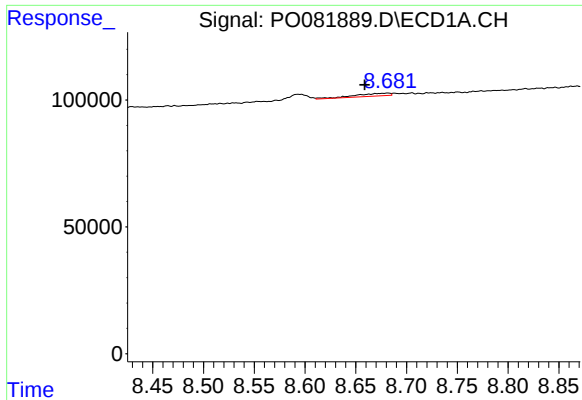

#36 AR-1262-1


R.T.: 8.682 min
Delta R.T.: 0.023 min
Response: 25653
Conc: 6.52 ng/ml

Instrument :
ECD_O
ClientSampleId :

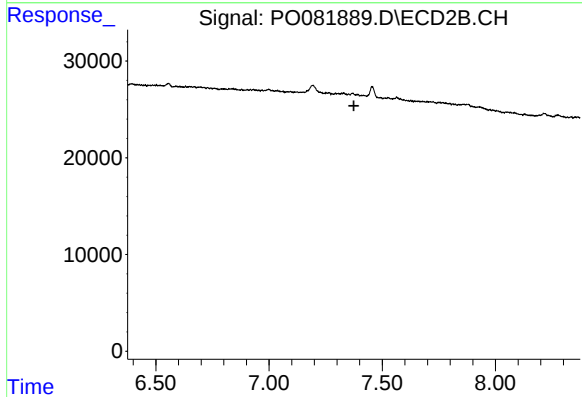


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.375 min
Response: 0
Conc: N.D.

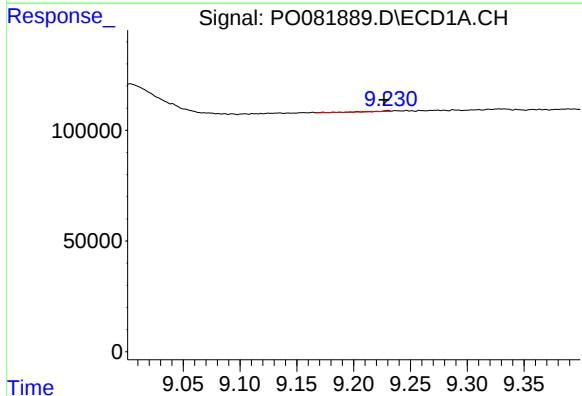

#37 AR-1262-2

R.T.: 9.231 min
Delta R.T.: 0.004 min
Response: 2348
Conc: 0.34 ng/ml

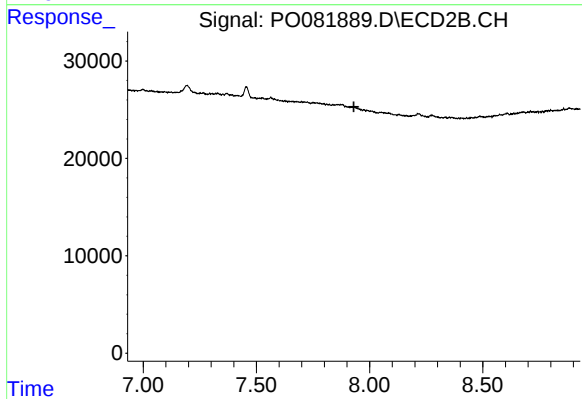

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.930 min
Response: 0
Conc: N.D.