

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100721\
 Data File : PO081896.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Oct 2021 5:25
 Operator : AJ\MA
 Sample : M4112-07
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 08 06:34:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 07 09:43:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.989	3.977	1818709	558311	21.917	22.064
2)	SA Decachlor...	11.110	9.307	1333065	523853	22.475	22.175
Target Compounds							
8)	L2 AR-1221-1	5.240	0.000	18677	0	19.557	N.D. #
9)	L2 AR-1221-2	5.344	0.000	21755	0	33.696	N.D. #
24)	L5 AR-1248-4	7.242f	0.000	12305	0	4.702	N.D. #
26)	L6 AR-1254-1	7.242	0.000	12305	0	4.498	N.D. #
28)	L6 AR-1254-3	7.873f	0.000	36723	0	9.000	N.D. #
32)	L7 AR-1260-2	8.315f	0.000	28886	0	7.822	N.D. #
34)	L7 AR-1260-4	8.912f	0.000	33705	0	11.289	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100721\
Data File : P0081896.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Oct 2021 5:25
Operator : AJ\MA
Sample : M4112-07
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 06:34:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 07 09:43:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

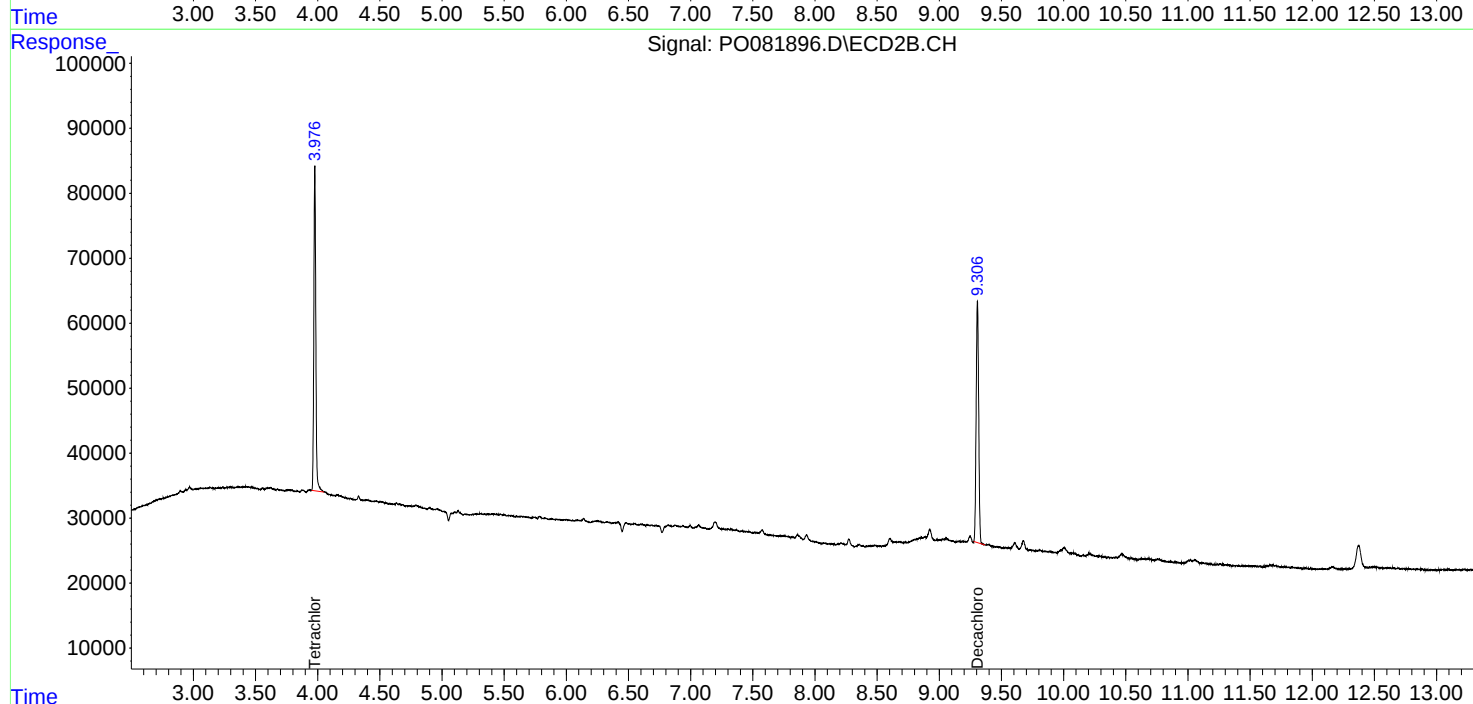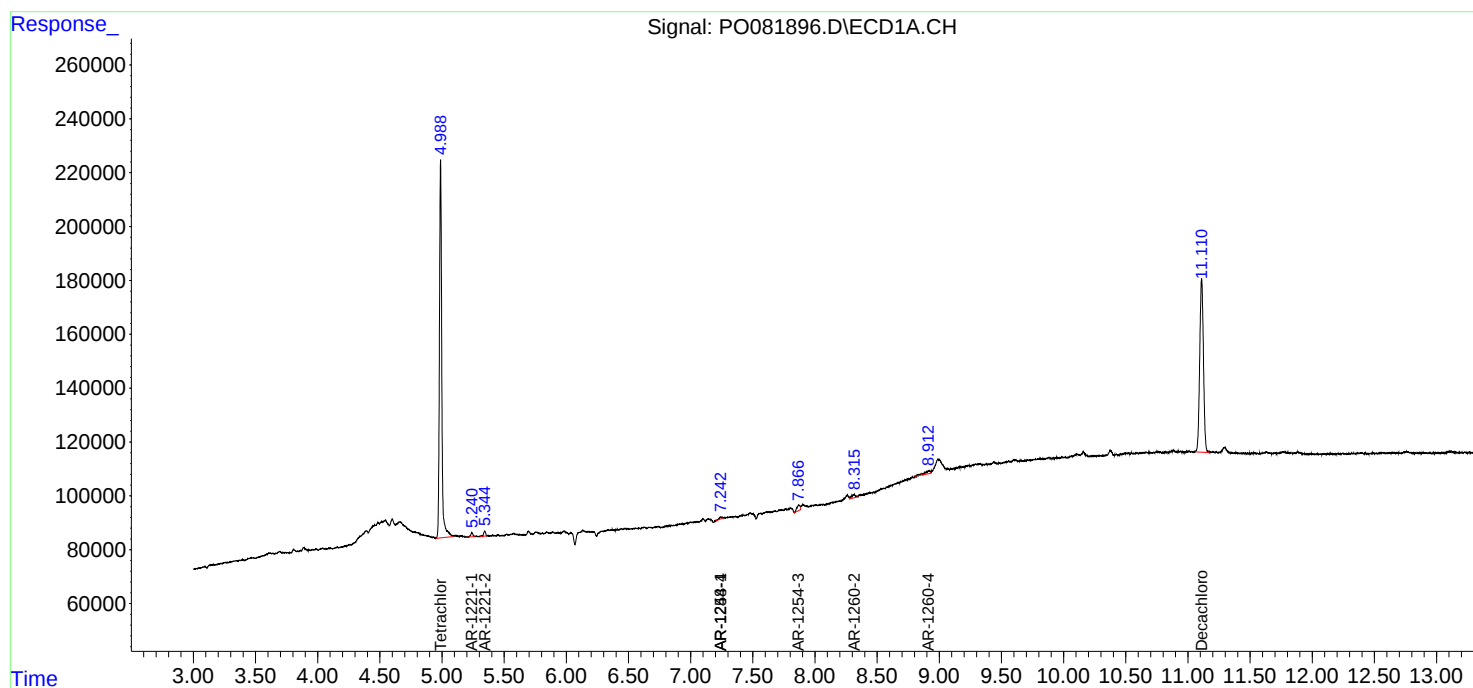


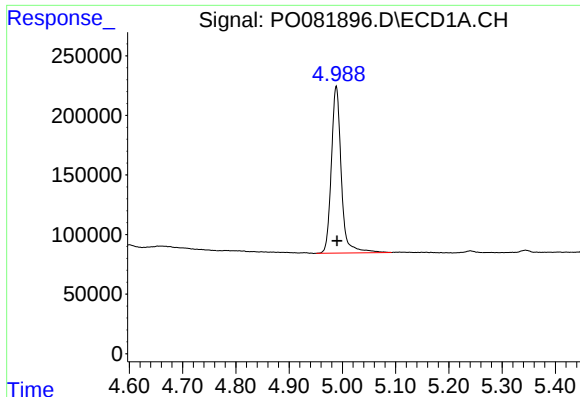

#1 Tetrachloro-m-xylene


R.T.: 4.989 min
Delta R.T.: -0.001 min
Response: 1818709
Conc: 21.92 ng/ml

Instrument :
ECD_O
ClientSampleId :

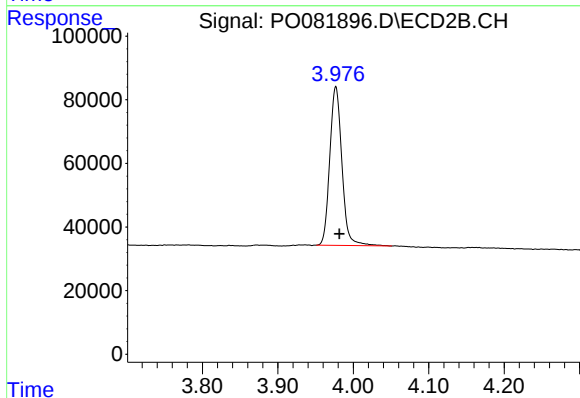


#1 Tetrachloro-m-xylene

R.T.: 3.977 min
Delta R.T.: -0.005 min
Response: 558311
Conc: 22.06 ng/ml

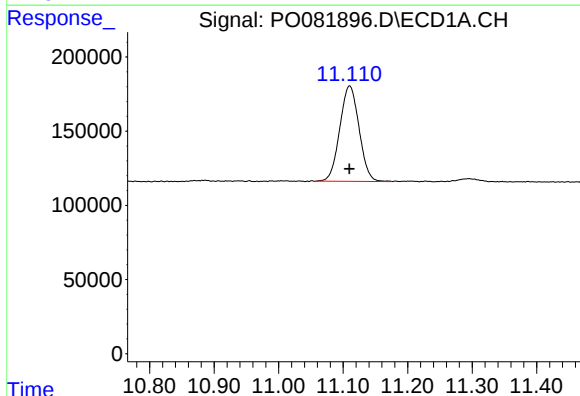


#2 Decachlorobiphenyl

R.T.: 11.110 min
Delta R.T.: 0.000 min
Response: 1333065
Conc: 22.47 ng/ml

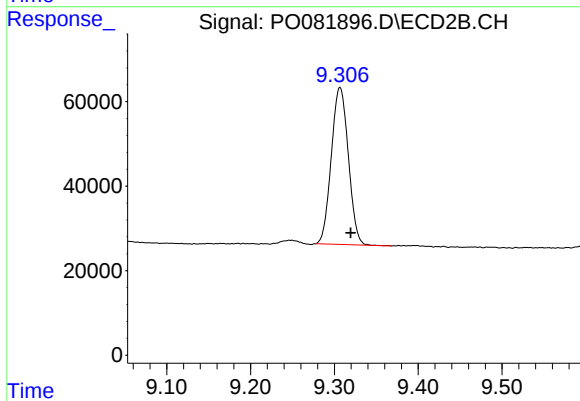

#2 Decachlorobiphenyl


R.T.: 9.307 min
Delta R.T.: -0.013 min
Response: 523853
Conc: 22.18 ng/ml

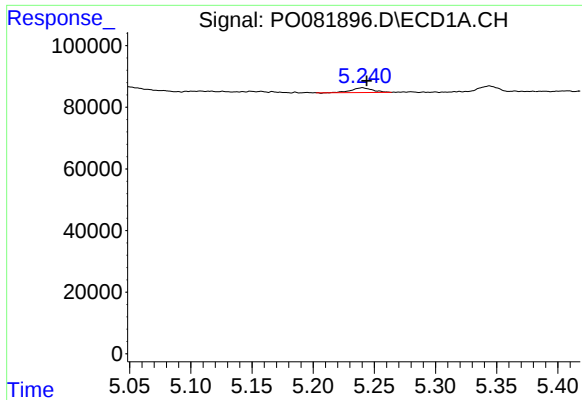

#8 AR-1221-1


R.T.: 5.240 min
Delta R.T.: -0.004 min
Response: 18677
Conc: 19.56 ng/ml

Instrument :
ECD_O
ClientSampleId :

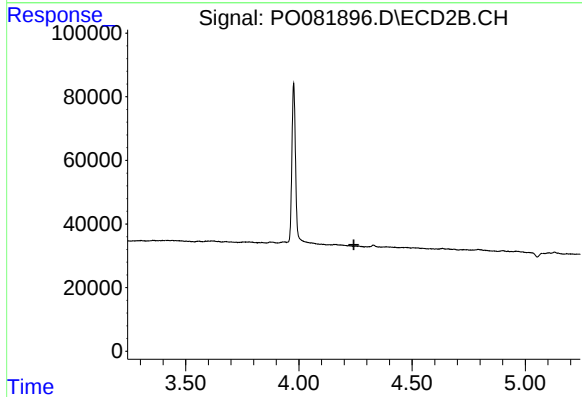


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.243 min
Response: 0
Conc: N.D.

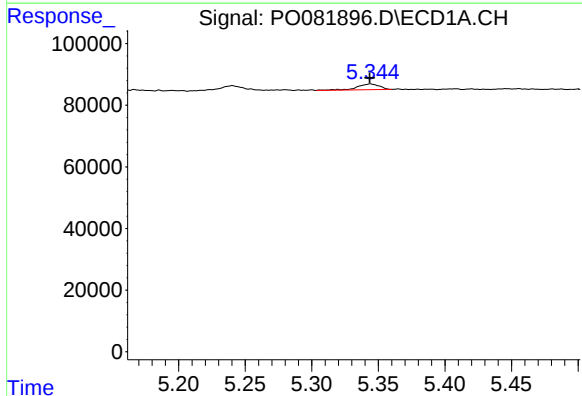


#9 AR-1221-2

R.T.: 5.344 min
Delta R.T.: 0.000 min
Response: 21755
Conc: 33.70 ng/ml

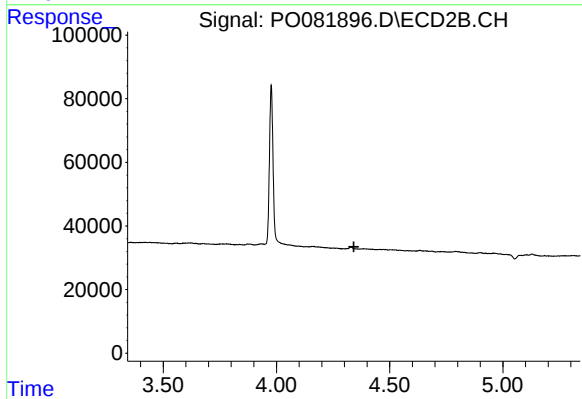

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.342 min
Response: 0
Conc: N.D.

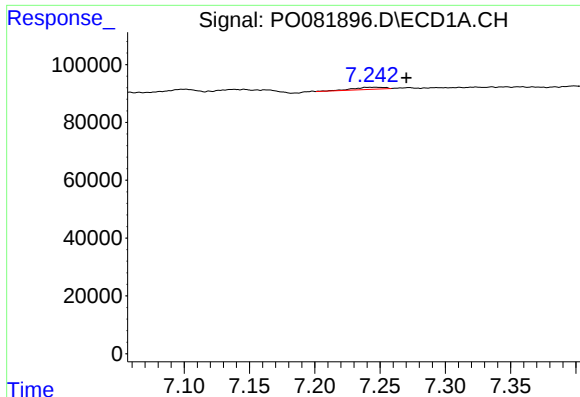

#24 AR-1248-4


R.T.: 7.242 min
Delta R.T.: -0.028 min
Response: 12305
Conc: 4.70 ng/ml

Instrument :
ECD_O
ClientSampleId :

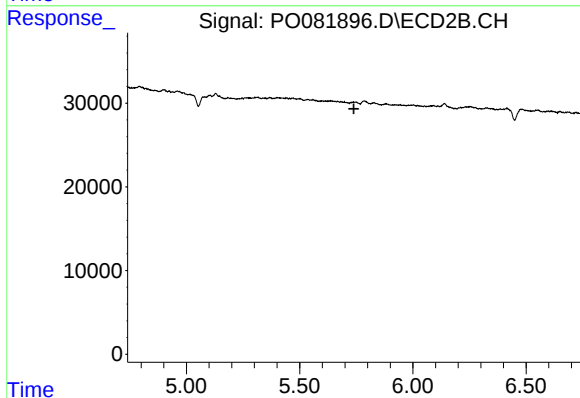


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.739 min
Response: 0
Conc: N.D.

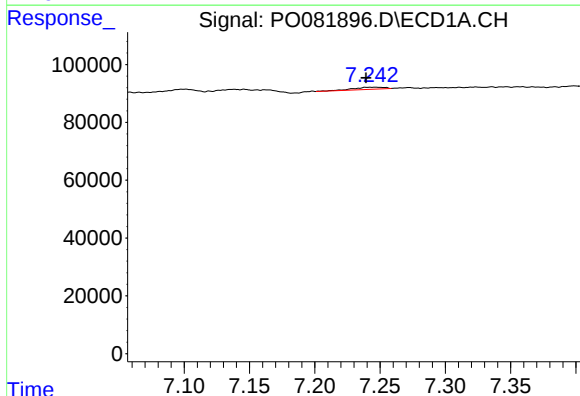


#26 AR-1254-1

R.T.: 7.242 min
Delta R.T.: 0.003 min
Response: 12305
Conc: 4.50 ng/ml

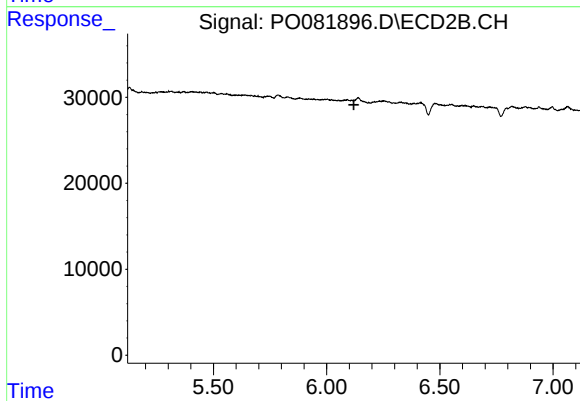

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.121 min
Response: 0
Conc: N.D.

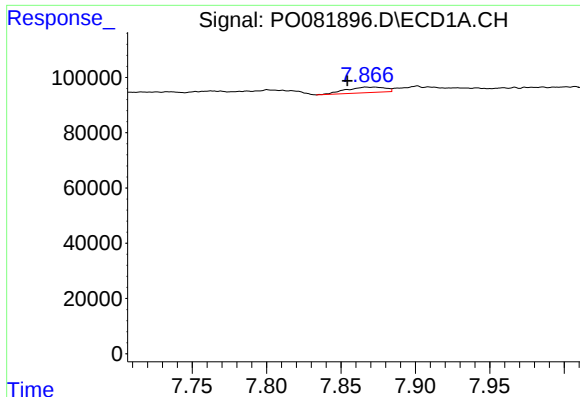

#28 AR-1254-3


R.T.: 7.873 min
Delta R.T.: 0.018 min
Response: 36723
Conc: 9.00 ng/ml

Instrument :
ECD_O
ClientSampleId :

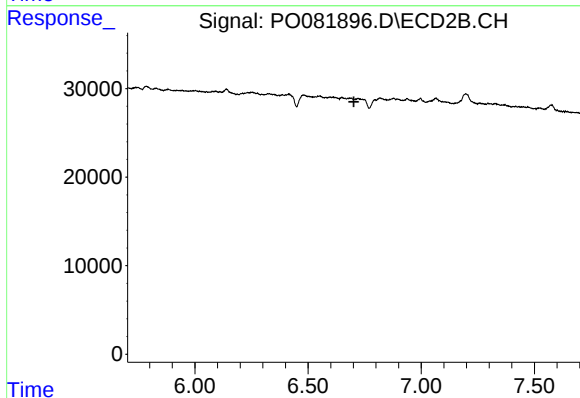


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.702 min
Response: 0
Conc: N.D.

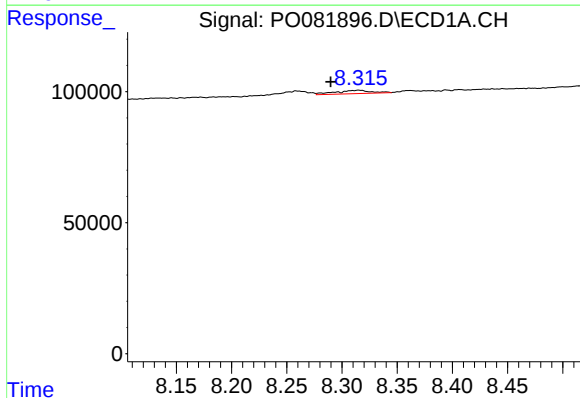


#32 AR-1260-2

R.T.: 8.315 min
Delta R.T.: 0.025 min
Response: 28886
Conc: 7.82 ng/ml

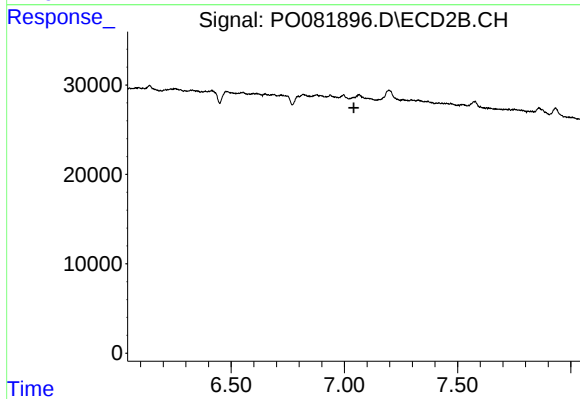

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.042 min
Response: 0
Conc: N.D.

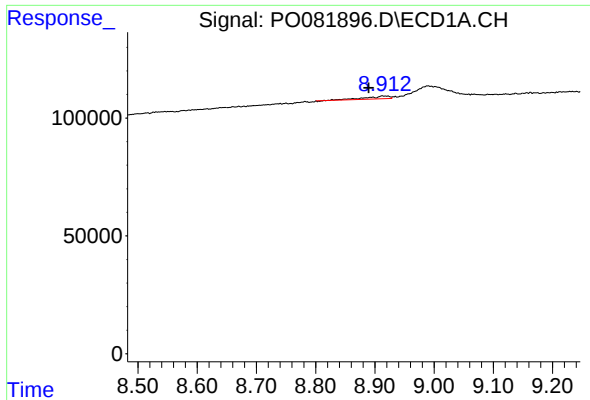

#34 AR-1260-4

R.T.: 8.912 min
Delta R.T.: 0.023 min
Response: 33705
Conc: 11.29 ng/ml

Instrument :
ECD_O
ClientSampleId :

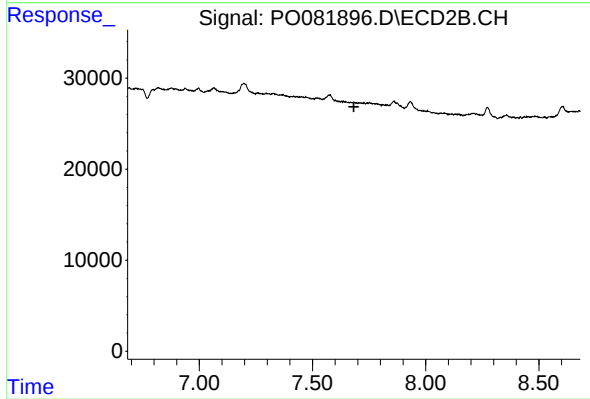

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.683 min
Response: 0
Conc: N.D.