

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100721\
 Data File : PO081868.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Oct 2021 20:47
 Operator : AJ\MA
 Sample : M4117-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-1(9.5-10.0)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 23:17:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 07 09:43:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.991	3.980	1851275	615456	22.309	24.322
2)	SA Decachlor...	11.114	9.311	1359774	520838	22.925	22.048

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100721\
Data File : P0081868.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Oct 2021 20:47
Operator : AJ\MA
Sample : M4117-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SB-1(9.5-10.0)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 23:17:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 07 09:43:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

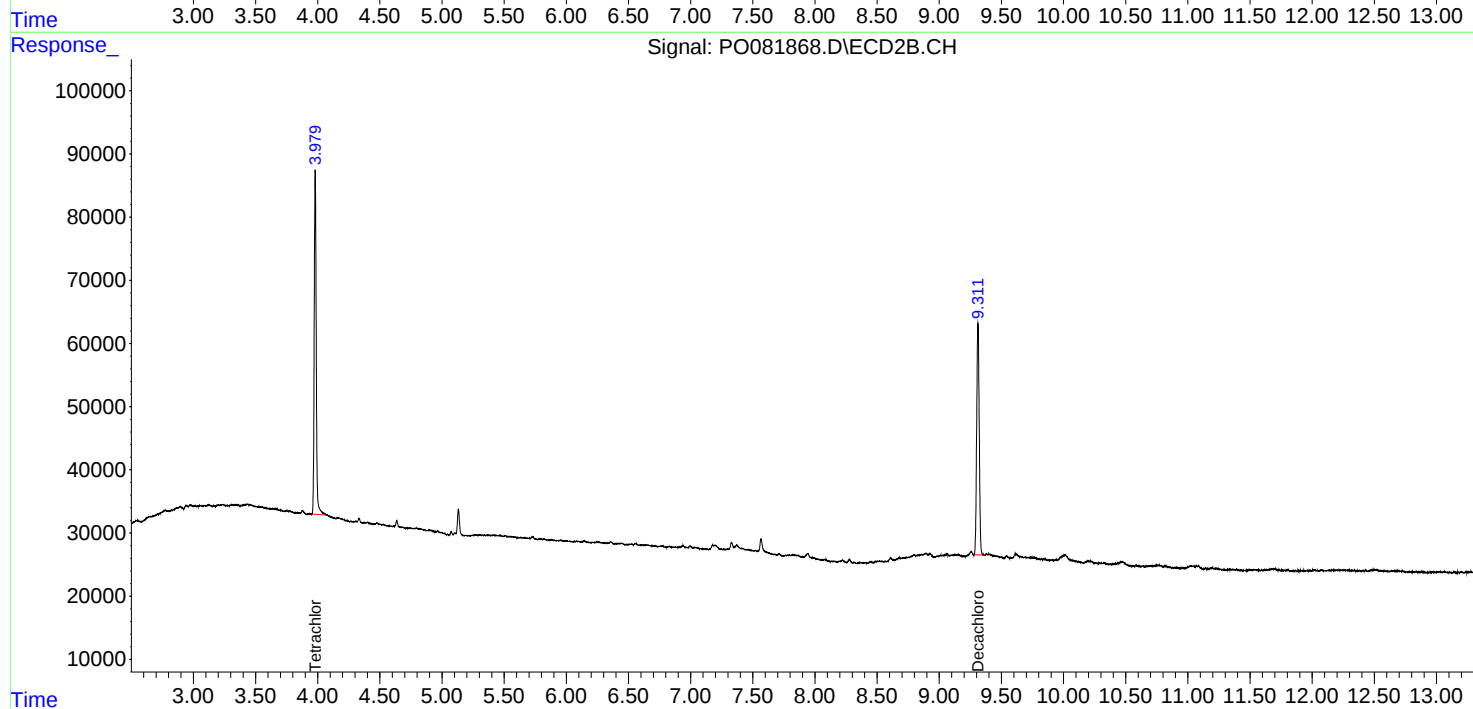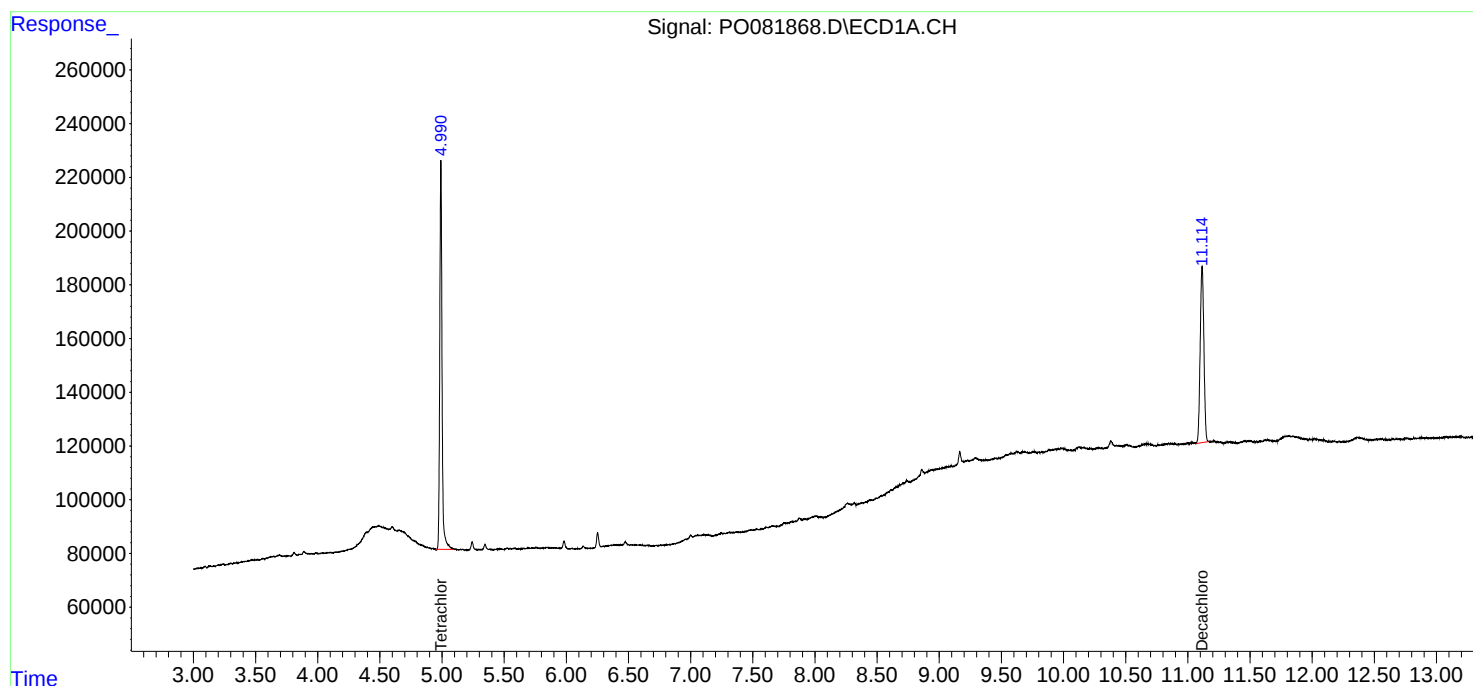


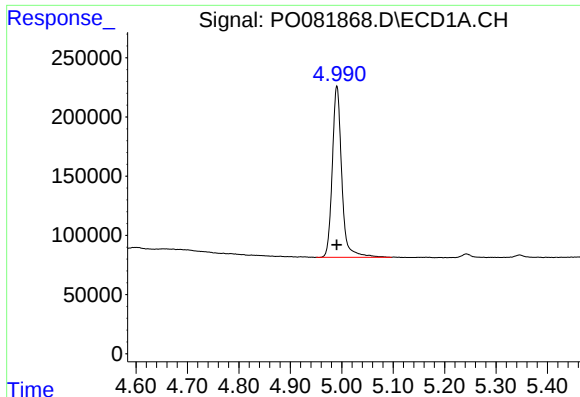

#1 Tetrachloro-m-xylene


R.T.: 4.991 min
Delta R.T.: 0.000 min
Response: 1851275
Conc: 22.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-1(9.5-10.0)

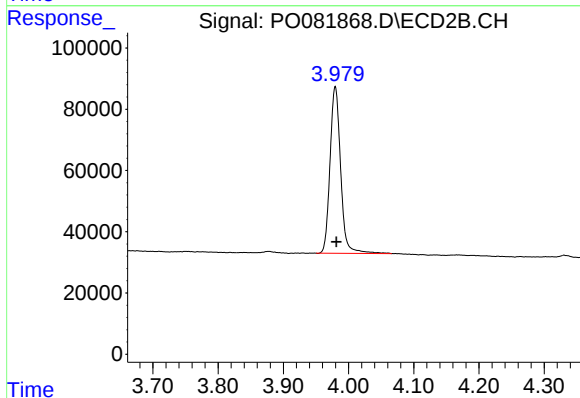


#1 Tetrachloro-m-xylene

R.T.: 3.980 min
Delta R.T.: -0.002 min
Response: 615456
Conc: 24.32 ng/ml

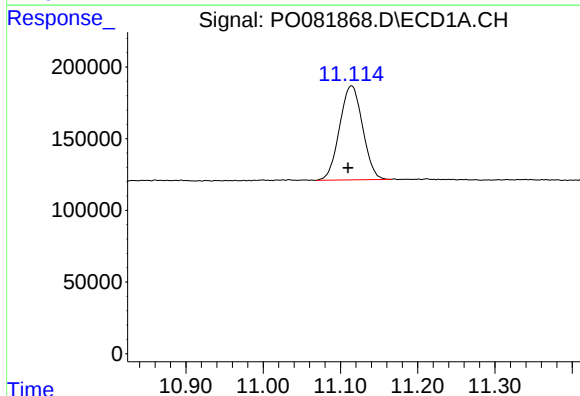

#2 Decachlorobiphenyl

R.T.: 11.114 min
Delta R.T.: 0.005 min
Response: 1359774
Conc: 22.92 ng/ml

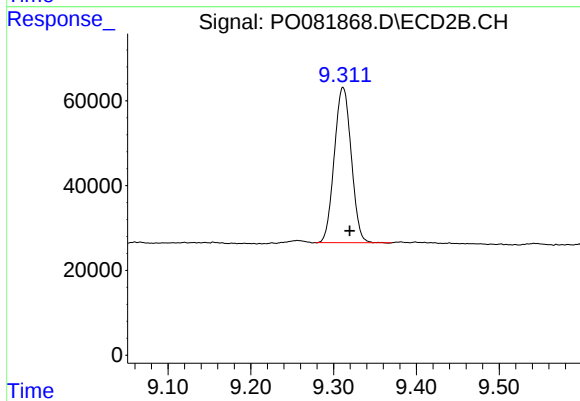

#2 Decachlorobiphenyl

R.T.: 9.311 min
Delta R.T.: -0.008 min
Response: 520838
Conc: 22.05 ng/ml