

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100721\
 Data File : PO081873.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Oct 2021 22:14
 Operator : AJ\MA
 Sample : M4117-07
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-3(1.5-2.0)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 23:20:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 07 09:43:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.991	3.979	1880953	590447	22.667	23.334
2)	SA Decachlor...	11.113	9.310	1265763	493669	21.340	20.898

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100721\
Data File : P0081873.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Oct 2021 22:14
Operator : AJ\MA
Sample : M4117-07
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SB-3(1.5-2.0)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 23:20:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 07 09:43:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

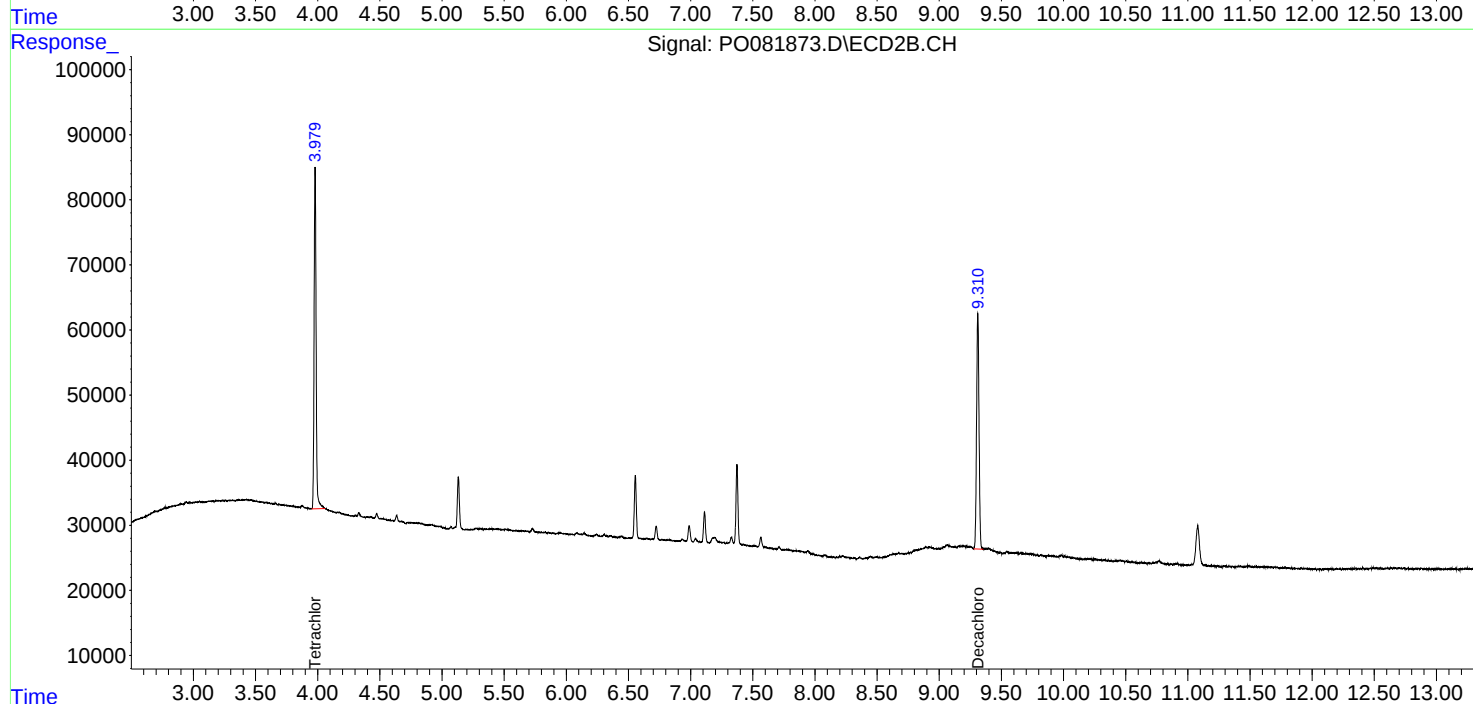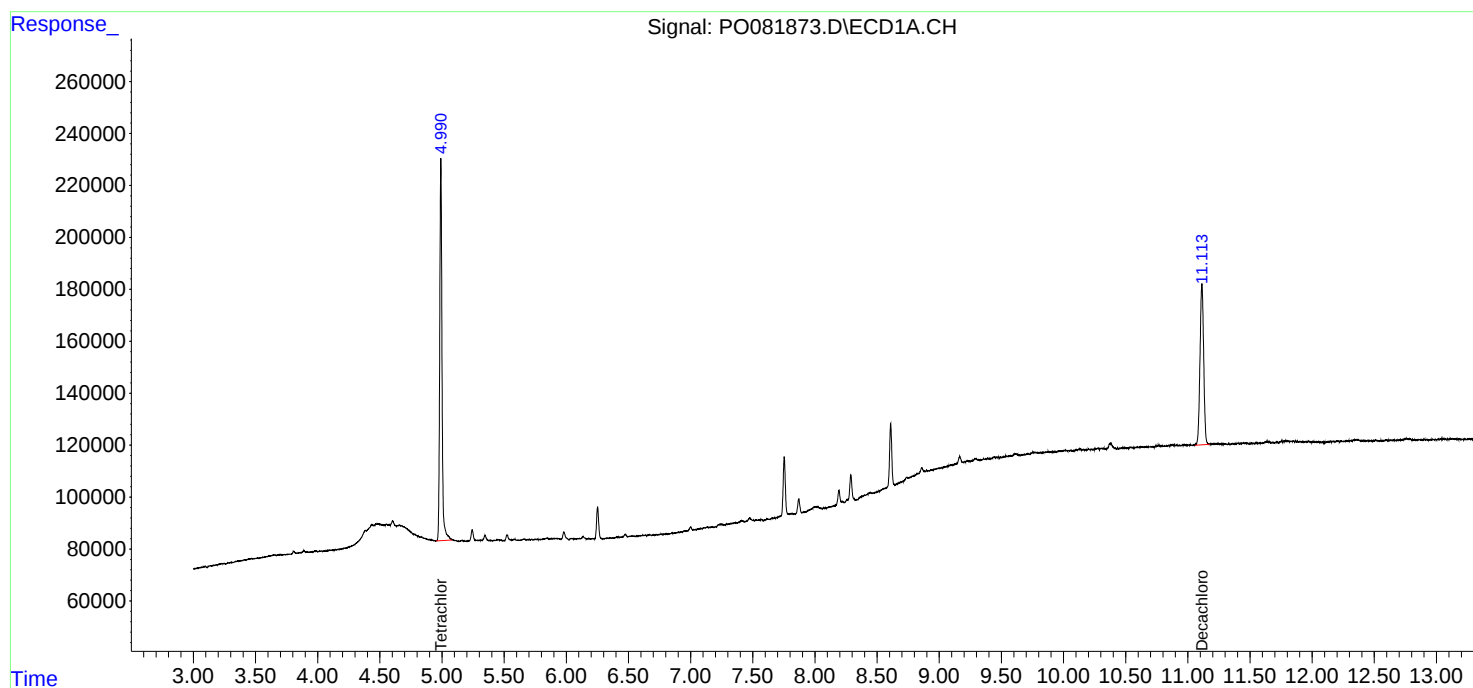


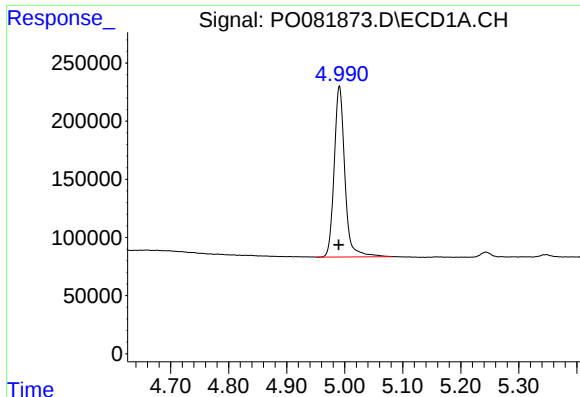

#1 Tetrachloro-m-xylene


R.T.: 4.991 min
Delta R.T.: 0.000 min
Response: 1880953
Conc: 22.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-3(1.5-2.0)

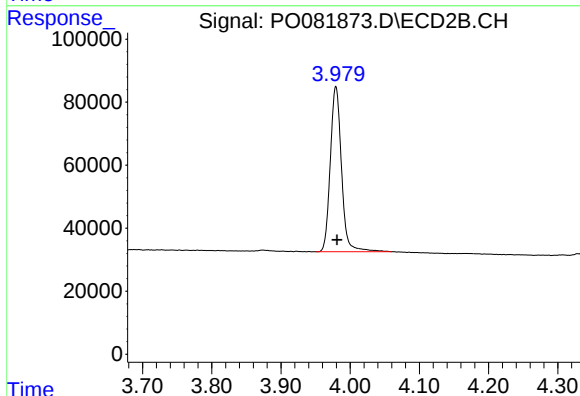


#1 Tetrachloro-m-xylene

R.T.: 3.979 min
Delta R.T.: -0.002 min
Response: 590447
Conc: 23.33 ng/ml

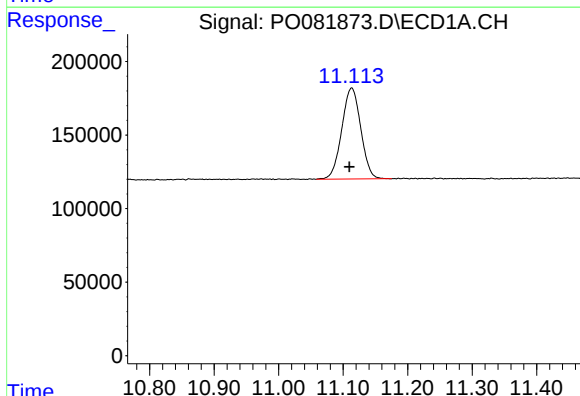

#2 Decachlorobiphenyl

R.T.: 11.113 min
Delta R.T.: 0.003 min
Response: 1265763
Conc: 21.34 ng/ml

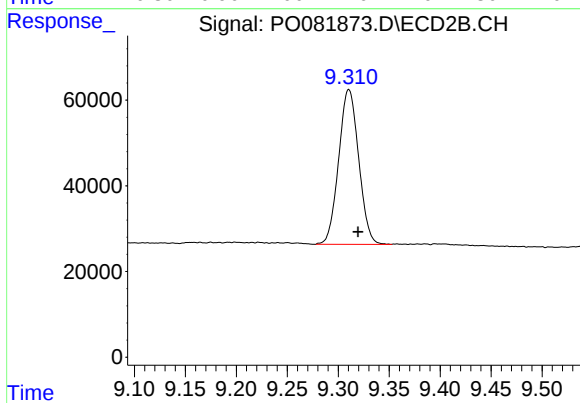

#2 Decachlorobiphenyl

R.T.: 9.310 min
Delta R.T.: -0.009 min
Response: 493669
Conc: 20.90 ng/ml