

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100721\
 Data File : PO081904.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Oct 2021 8:18
 Operator : AJ\MA
 Sample : M4118-01
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CONCRETE-100621-01

Manual Integrations
 APPROVED

mohammad
 10/10/2021 8:21:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 08 09:09:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 07 09:43:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.989	3.978	1883309	670888	22.695m	26.513
2) SA Decachlor...	11.111	9.305	1533083	702899	25.847	29.755m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100721\
Data File : P0081904.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Oct 2021 8:18
Operator : AJ\MA
Sample : M4118-01
Misc :
ALS Vial : 48 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CONCRETE-100621-01

Manual Integrations
APPROVED


mohammad
10/10/2021 8:21:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 09:09:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 07 09:43:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

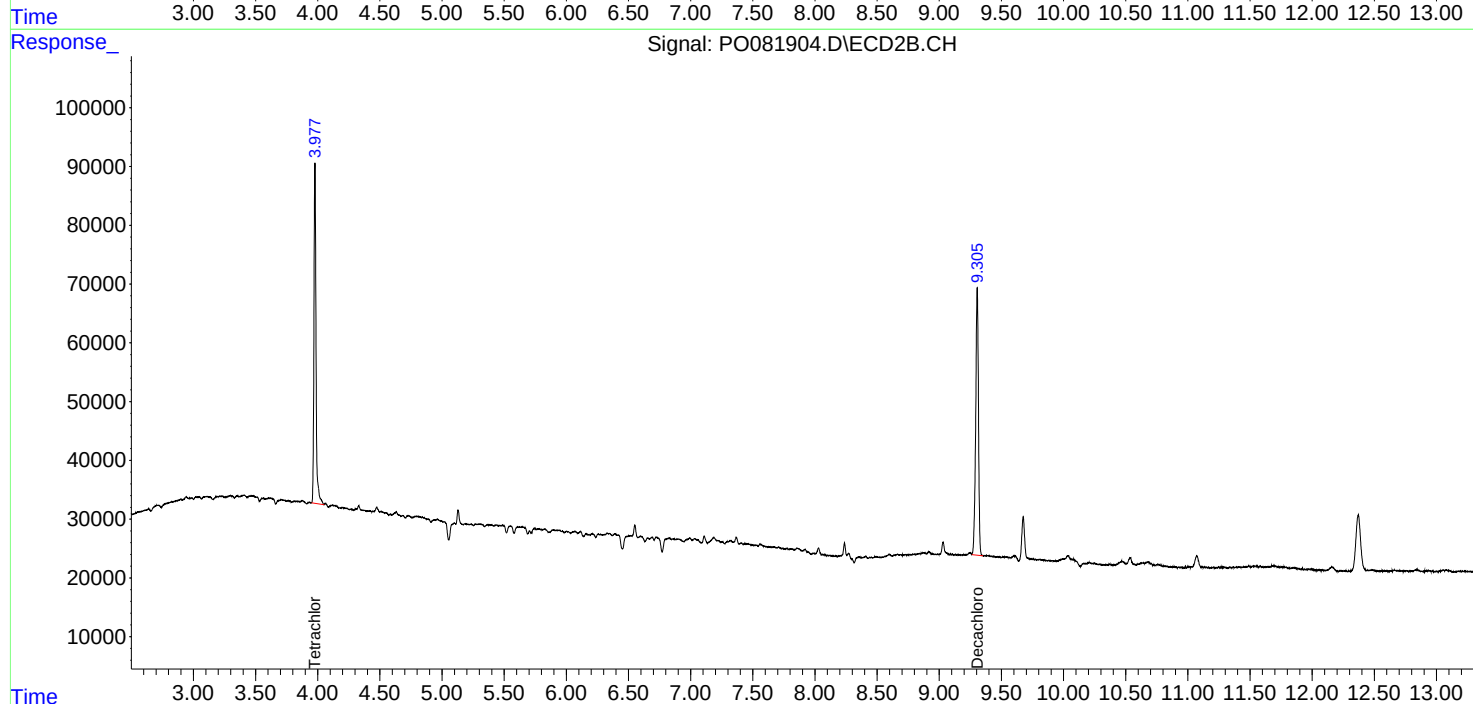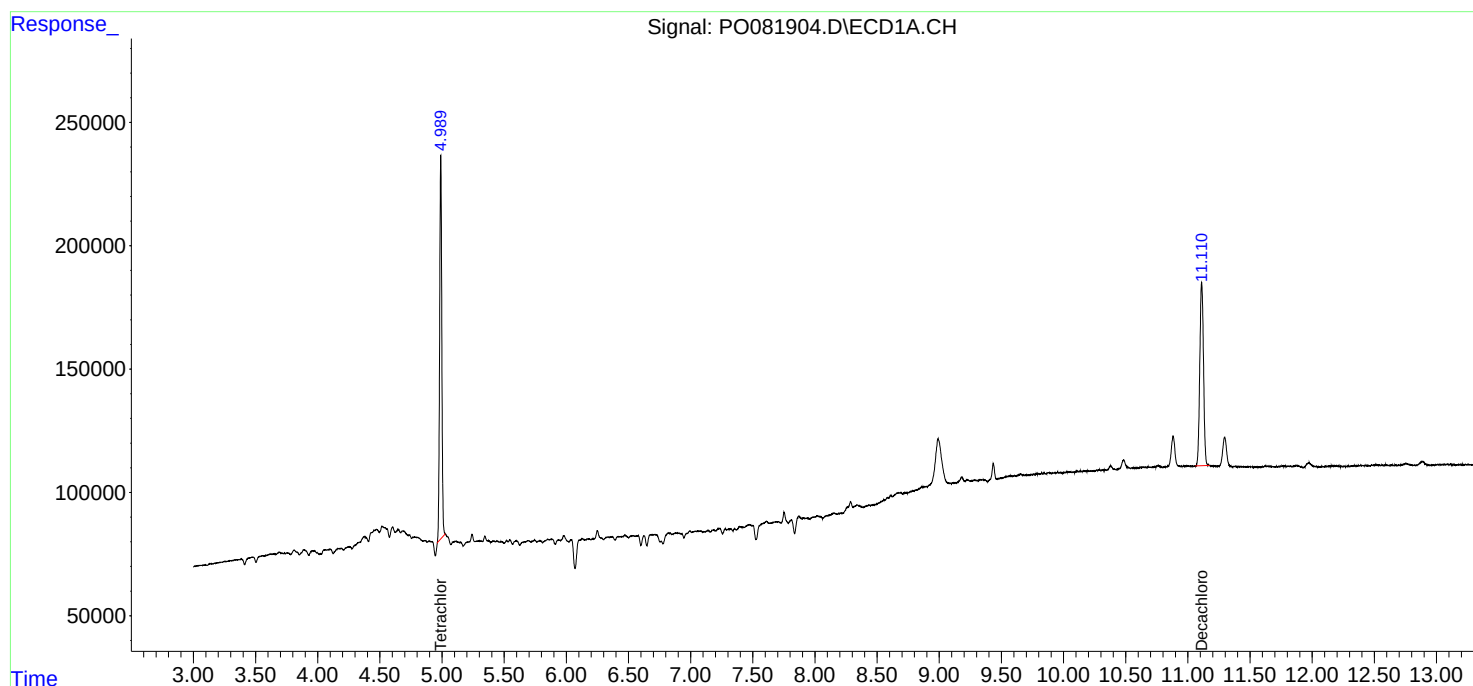

Response_

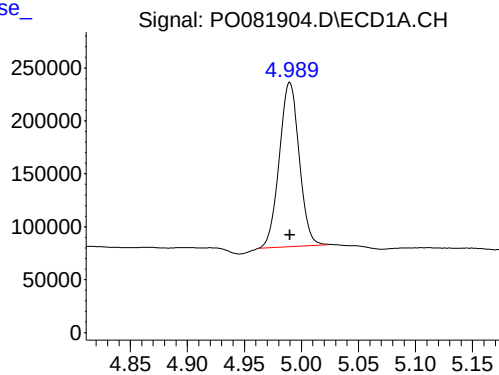

#1 Tetrachloro-m-xylene

R.T.: 4.989 min
Delta R.T.: 0.000 min
Response: 1883309
Conc: 22.70 ng/ml m


Instrument :
ECD_O
ClientSampleId :
CONCRETE-100621-01

Manual Integrations
APPROVED

mohammad
10/10/2021 8:21:40 PM

Time

Response_

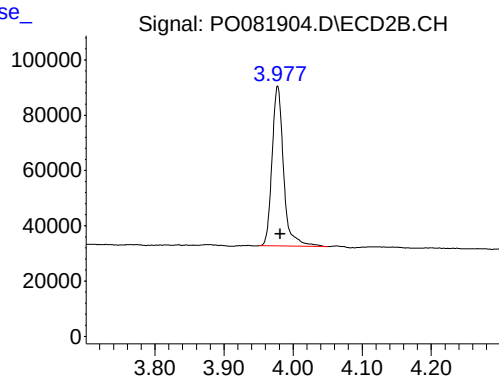


#1 Tetrachloro-m-xylene

R.T.: 3.978 min
Delta R.T.: -0.004 min
Response: 670888
Conc: 26.51 ng/ml

Time

Response_

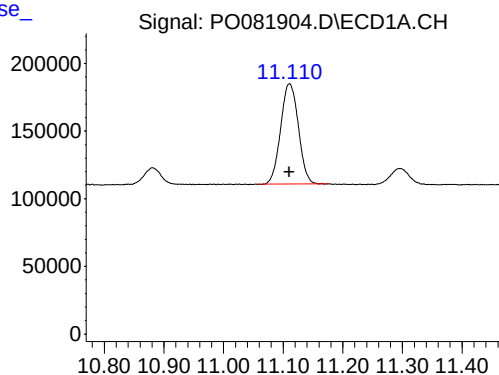


#2 Decachlorobiphenyl

R.T.: 11.111 min
Delta R.T.: 0.000 min
Response: 1533083
Conc: 25.85 ng/ml

Time

Response_

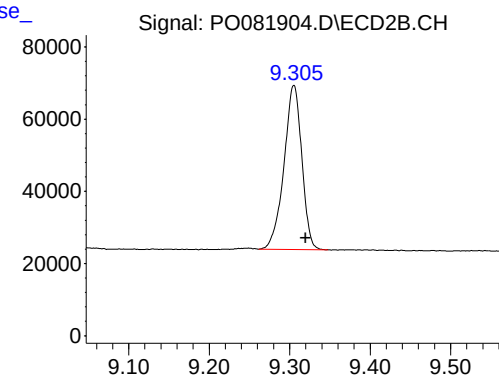

#2 Decachlorobiphenyl

R.T.: 9.305 min
Delta R.T.: -0.014 min
Response: 702899
Conc: 29.75 ng/ml m

Time