

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100721\
 Data File : PO081911.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Oct 2021 10:18
 Operator : AJ\MA
 Sample : M4099-02RE
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-092821-SR-02

Manual Integrations
 APPROVED

mohammad
 10/12/2021 8:36:38 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 08 16:26:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 07 09:43:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.991	3.979	1616473	433864	19.480	17.146
2) SA Decachlor...	11.121	9.308	1795325	422394	30.268m	17.881m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100721\
Data File : PO081911.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Oct 2021 10:18
Operator : AJ\MA
Sample : M4099-02RE
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PCB-092821-SR-02


Manual Integrations
APPROVED

mohammad
10/12/2021 8:36:38 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 16:26:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 07 09:43:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

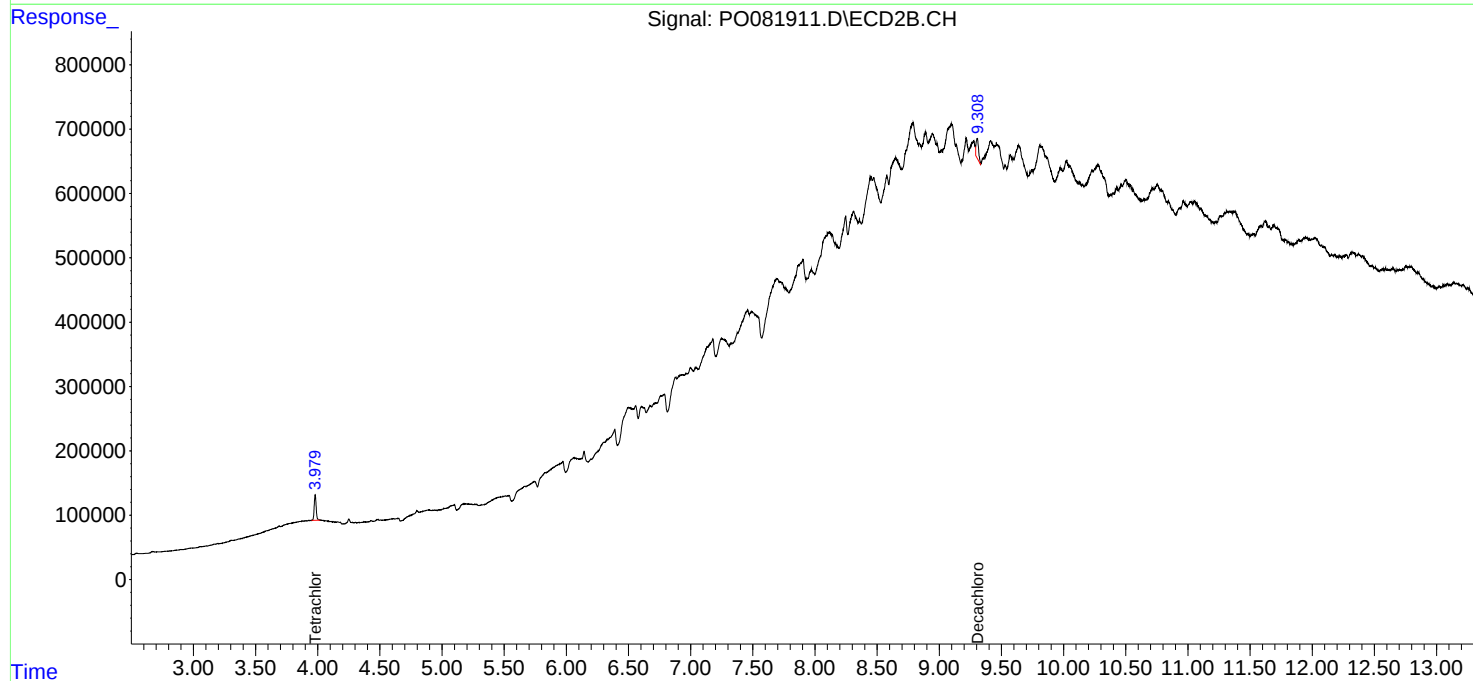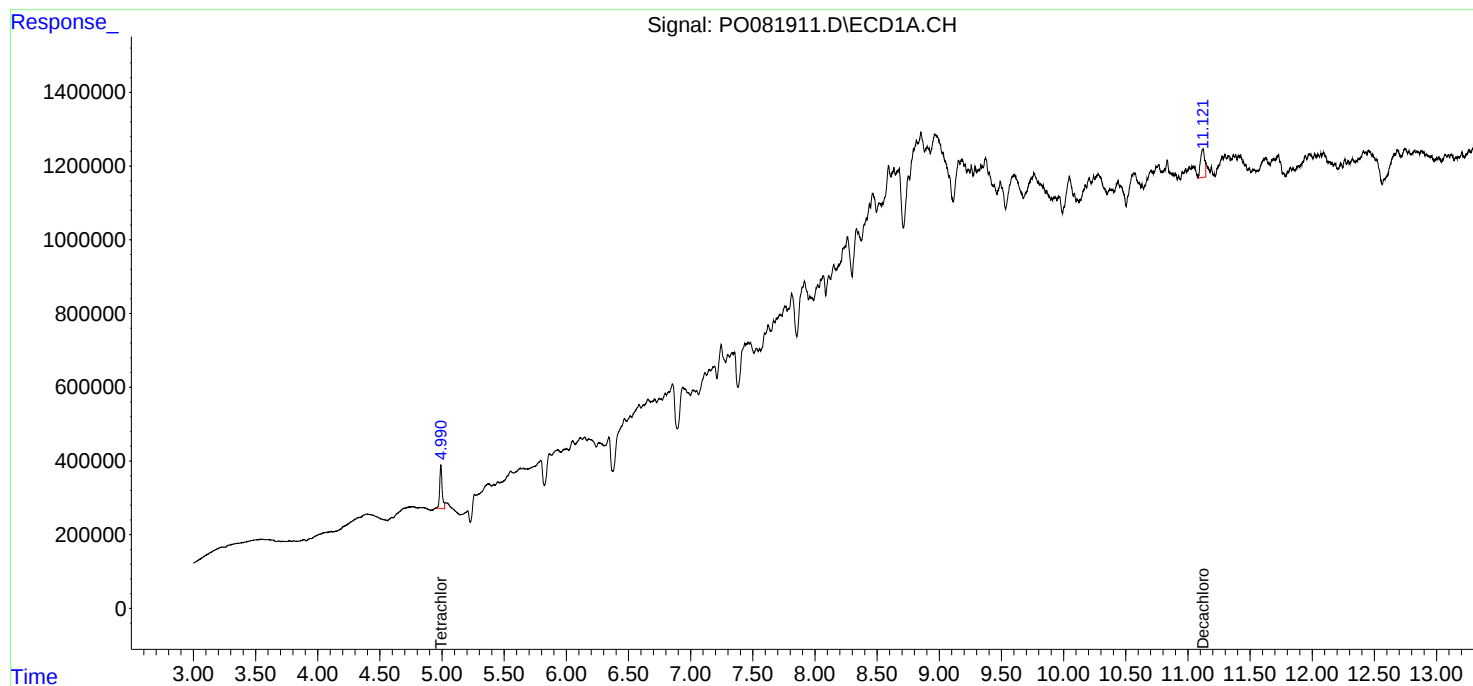

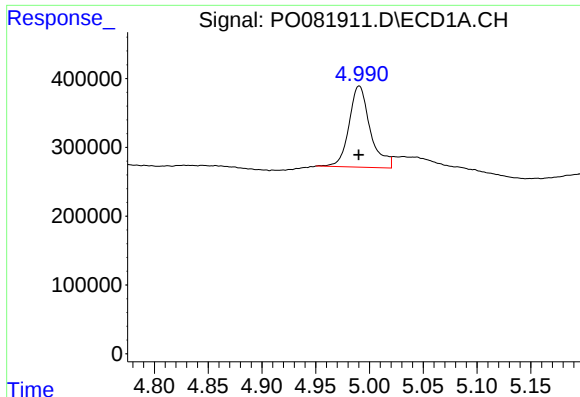


#1 Tetrachloro-m-xylene

R.T.: 4.991 min
Delta R.T.: 0.000 min
Response: 1616473
Conc: 19.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-092821-SR-02


Manual Integrations
APPROVED

mohammad
10/12/2021 8:36:38 AM

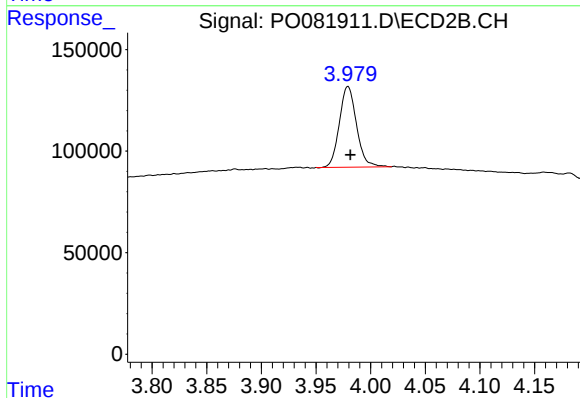


#1 Tetrachloro-m-xylene

R.T.: 3.979 min
Delta R.T.: -0.002 min
Response: 433864
Conc: 17.15 ng/ml

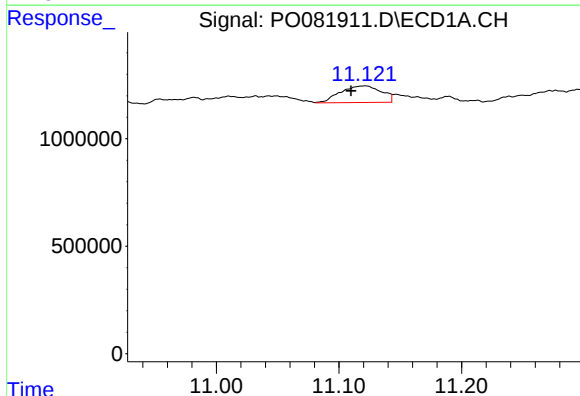

#2 Decachlorobiphenyl

R.T.: 11.121 min
Delta R.T.: 0.011 min
Response: 1795325
Conc: 30.27 ng/ml m

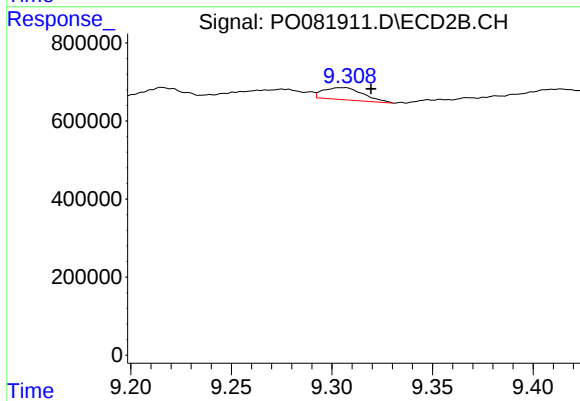

#2 Decachlorobiphenyl

R.T.: 9.308 min
Delta R.T.: -0.012 min
Response: 422394
Conc: 17.88 ng/ml m