

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100722\
 Data File : PO089803.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Oct 2022 12:40
 Operator : YP/AJ
 Sample : N5046-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 R-5

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/10/2022
 Supervised By :Ankita Jodhani 10/10/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 17:13:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 05 06:04:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.335	3.560	63735254	22926650	24.515	25.387
2) SA Decachlor...	10.098	8.590	28264696	17180605	26.294	21.621

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100722\
Data File : PO089803.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Oct 2022 12:40
Operator : YP/AJ
Sample : N5046-05
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
R-5


Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 10/10/2022
Supervised By : Ankita Jodhani 10/10/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 17:13:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100422.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 05 06:04:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

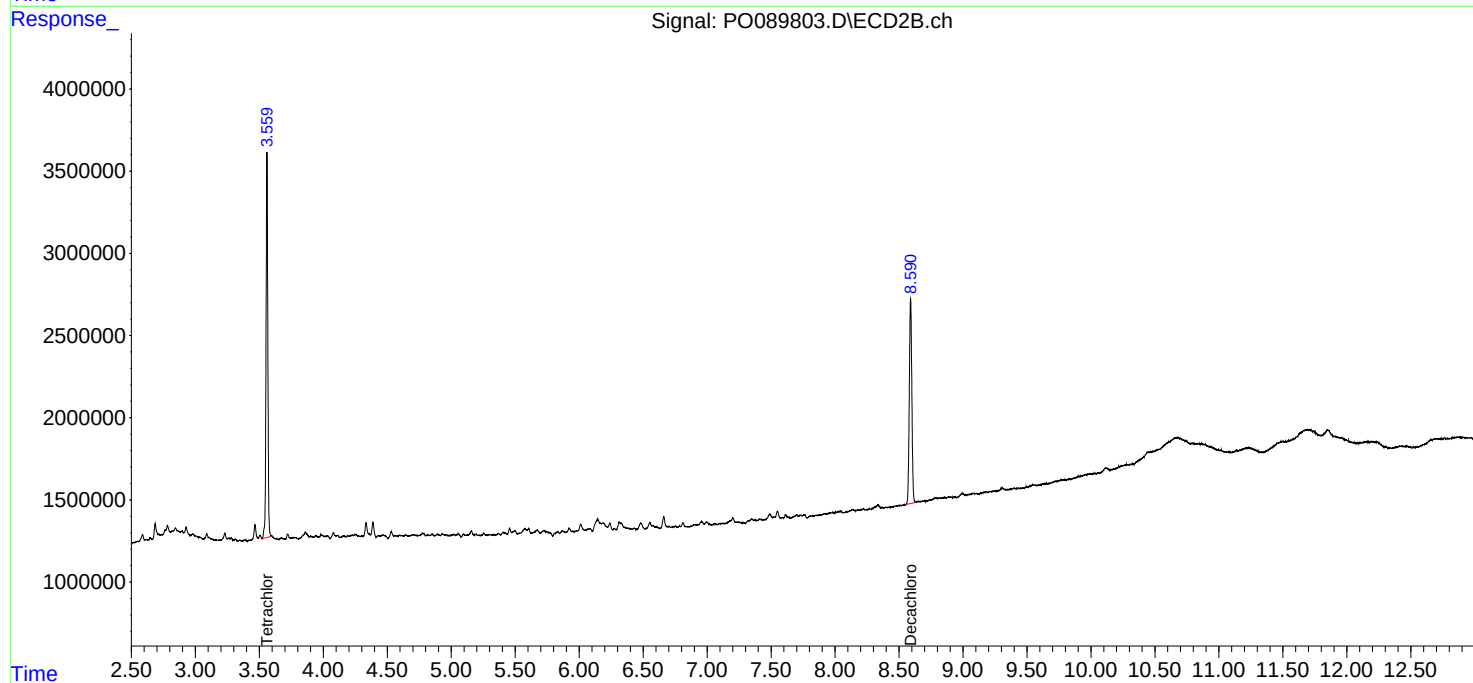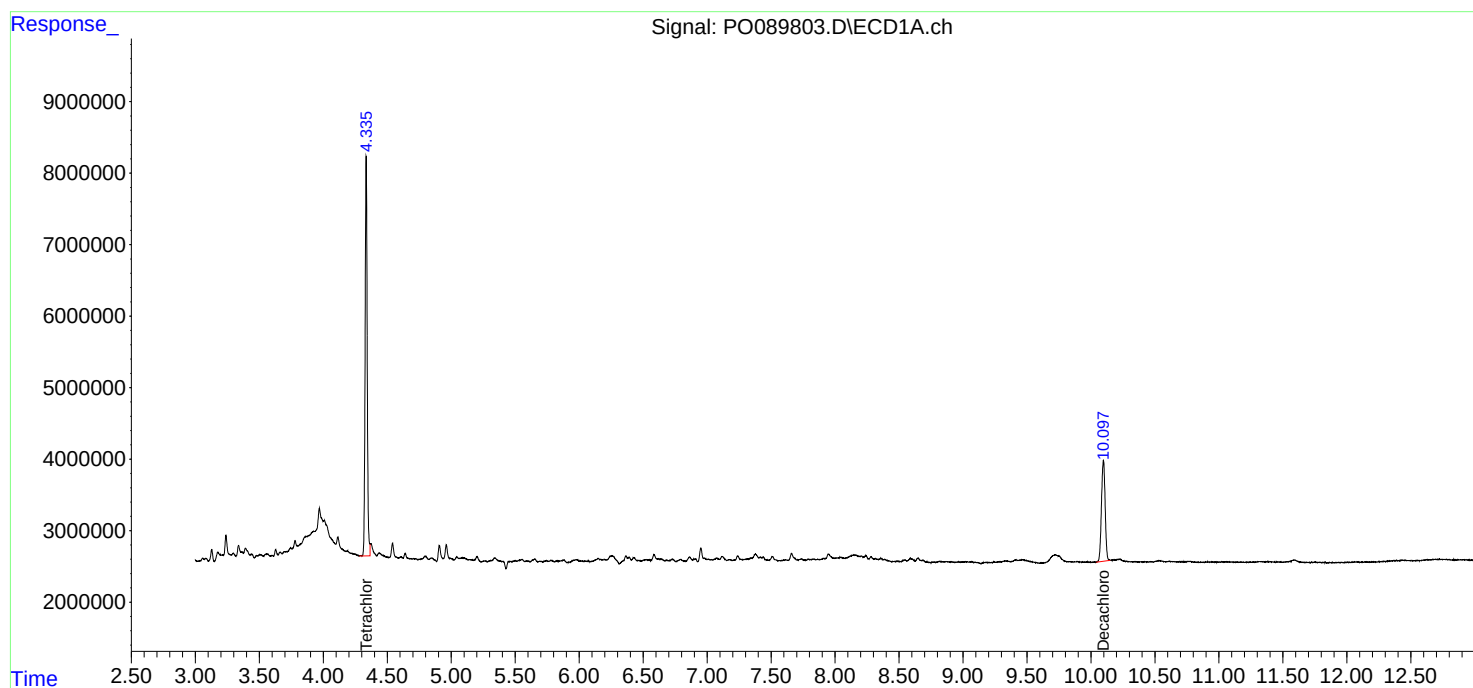

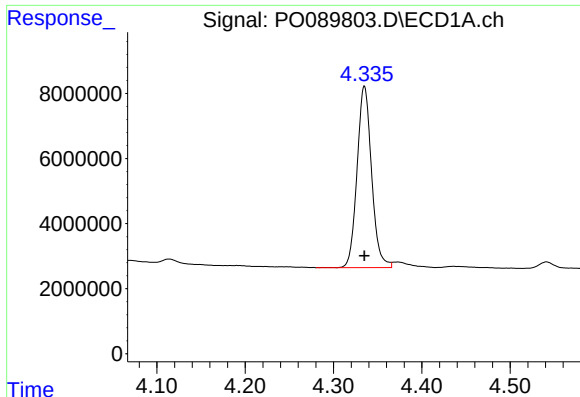


#1 Tetrachloro-m-xylene

R.T.: 4.335 min
Delta R.T.: 0.000 min
Response: 63735254
Conc: 24.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
R-5


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/10/2022
Supervised By :Ankita Jodhani 10/10/2022

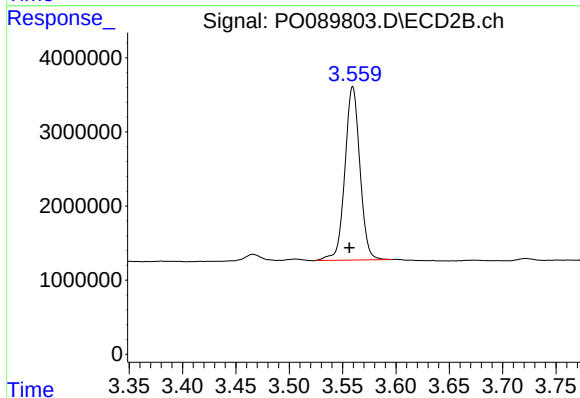


#1 Tetrachloro-m-xylene

R.T.: 3.560 min
Delta R.T.: 0.003 min
Response: 22926650
Conc: 25.39 ng/ml

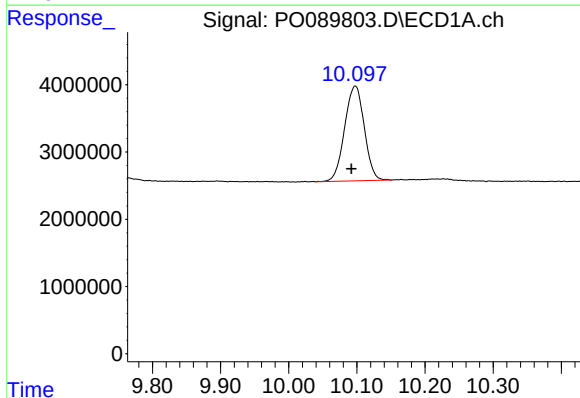

#2 Decachlorobiphenyl

R.T.: 10.098 min
Delta R.T.: 0.006 min
Response: 28264696
Conc: 26.29 ng/ml

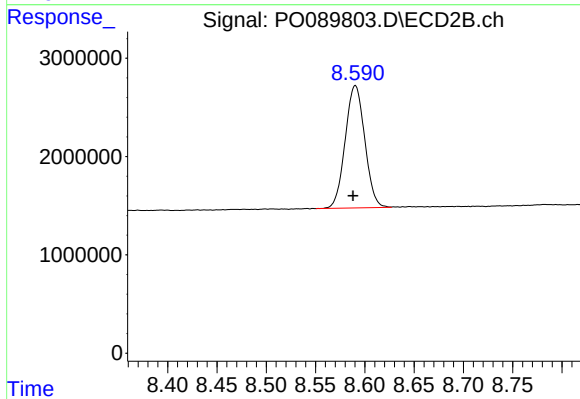

#2 Decachlorobiphenyl

R.T.: 8.590 min
Delta R.T.: 0.002 min
Response: 17180605
Conc: 21.62 ng/ml