

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100820\
 Data File : PO072111.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Oct 2020 13:54
 Operator : DD\AJ
 Sample : L4291-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PAV-B4-100620-10-20

Manual Integrations
 APPROVED

Ankita
 10/12/2020 9:17:17 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 08 16:33:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.325	3.510	1622180	824361	22.585m	22.009
2) SA Decachlor...	9.932	8.682	1865764	945879	16.945	16.630

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100820\
Data File : PO072111.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Oct 2020 13:54
Operator : DD\AJ
Sample : L4291-05
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PAV-B4-100620-10-20


Manual Integrations
APPROVED

Ankita
10/12/2020 9:17:17 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 16:33:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

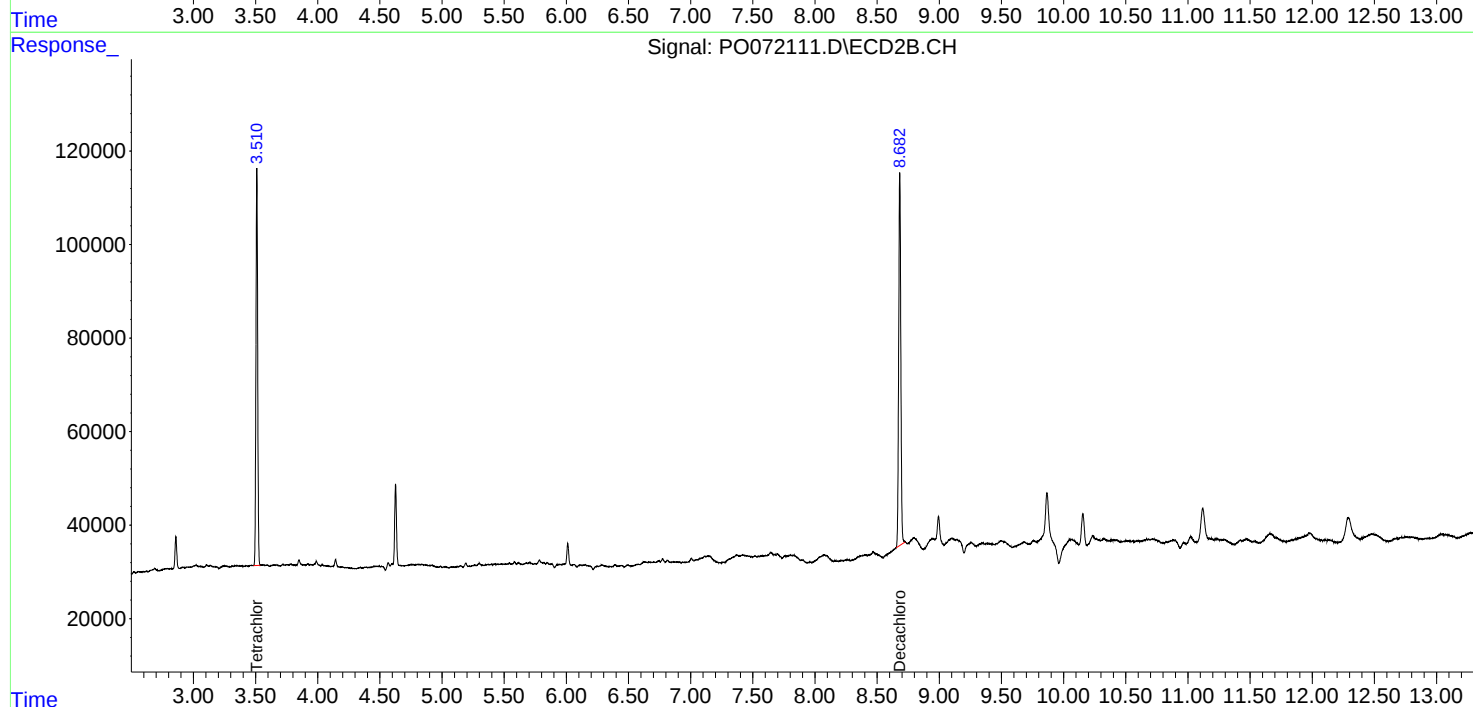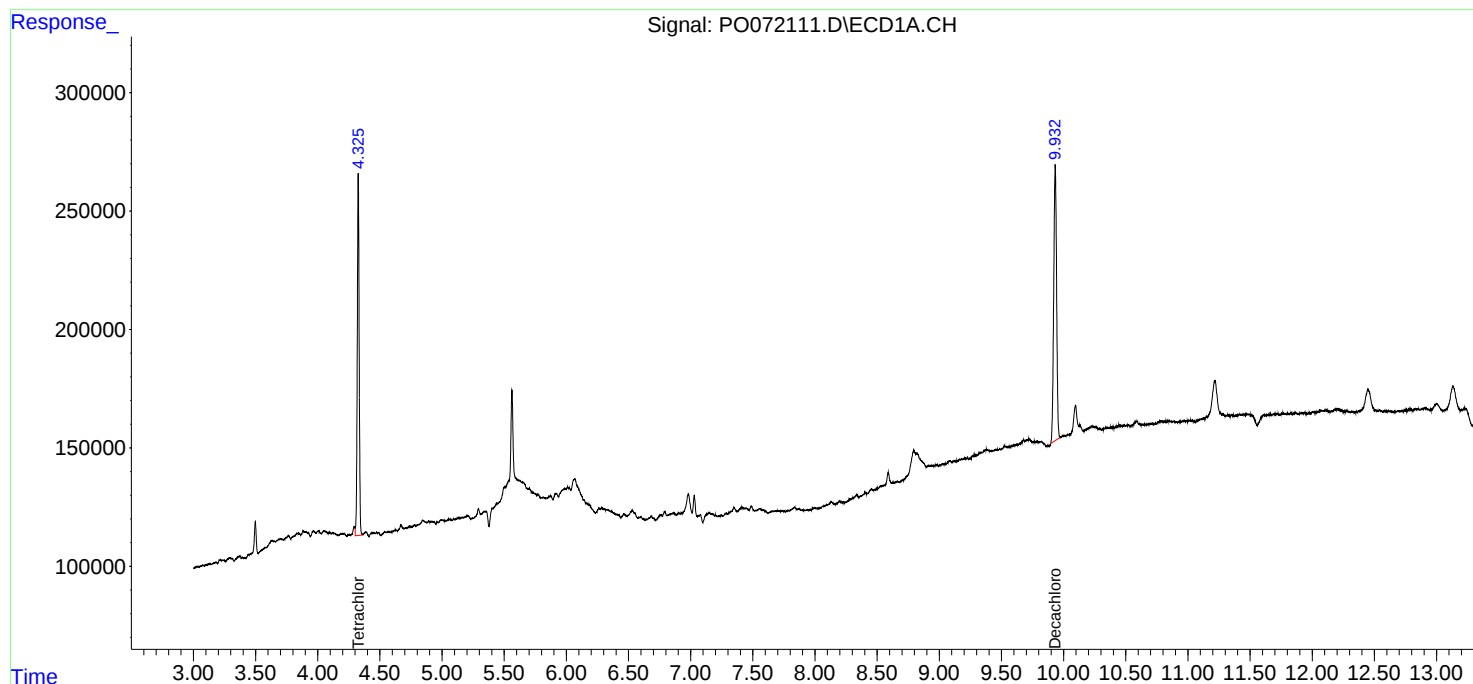

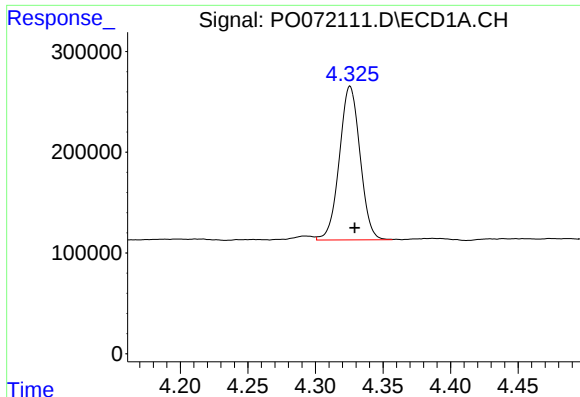


#1 Tetrachloro-m-xylene

R.T.: 4.325 min
Delta R.T.: -0.004 min
Response: 1622180
Conc: 22.58 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PAV-B4-100620-10-20


Manual Integrations
APPROVED

Ankita
10/12/2020 9:17:17 AM

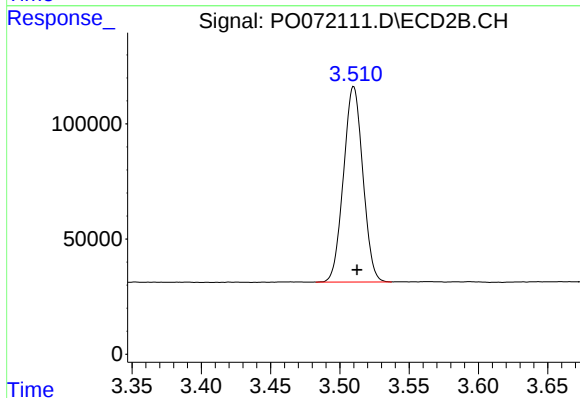


#1 Tetrachloro-m-xylene

R.T.: 3.510 min
Delta R.T.: -0.002 min
Response: 824361
Conc: 22.01 ng/ml

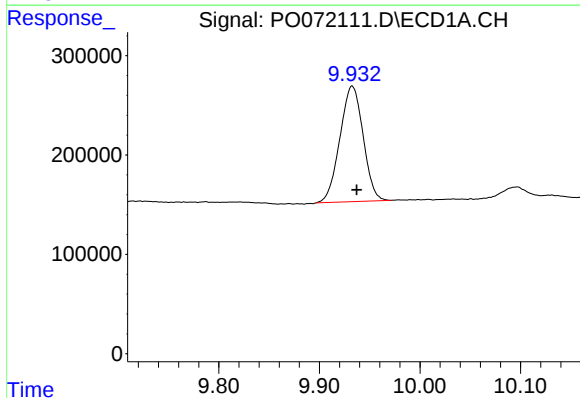

#2 Decachlorobiphenyl

R.T.: 9.932 min
Delta R.T.: -0.005 min
Response: 1865764
Conc: 16.95 ng/ml

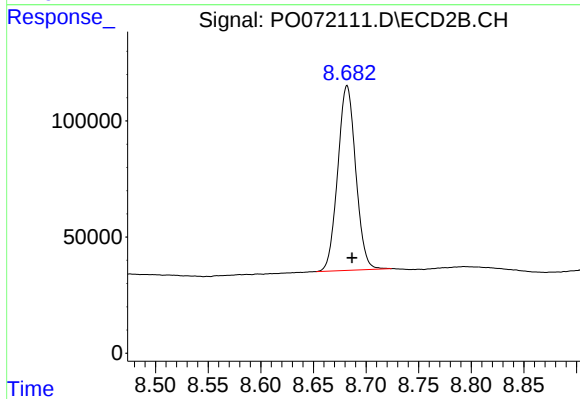

#2 Decachlorobiphenyl

R.T.: 8.682 min
Delta R.T.: -0.005 min
Response: 945879
Conc: 16.63 ng/ml