

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100820\
 Data File : PO072122.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Oct 2020 17:05
 Operator : DD\AJ
 Sample : L4297-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RO-RBR-200031

Manual Integrations
 APPROVED

Ankita
 10/12/2020 9:17:29 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 04:24:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.325	3.509	1327921	688124	18.488	18.371
2) SA Decachlor...	9.931	8.682	830813	362074	7.546m	6.366

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100820\
Data File : PO072122.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Oct 2020 17:05
Operator : DD\AJ
Sample : L4297-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
RO-RBR-200031


Manual Integrations
APPROVED

Ankita
10/12/2020 9:17:29 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 04:24:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

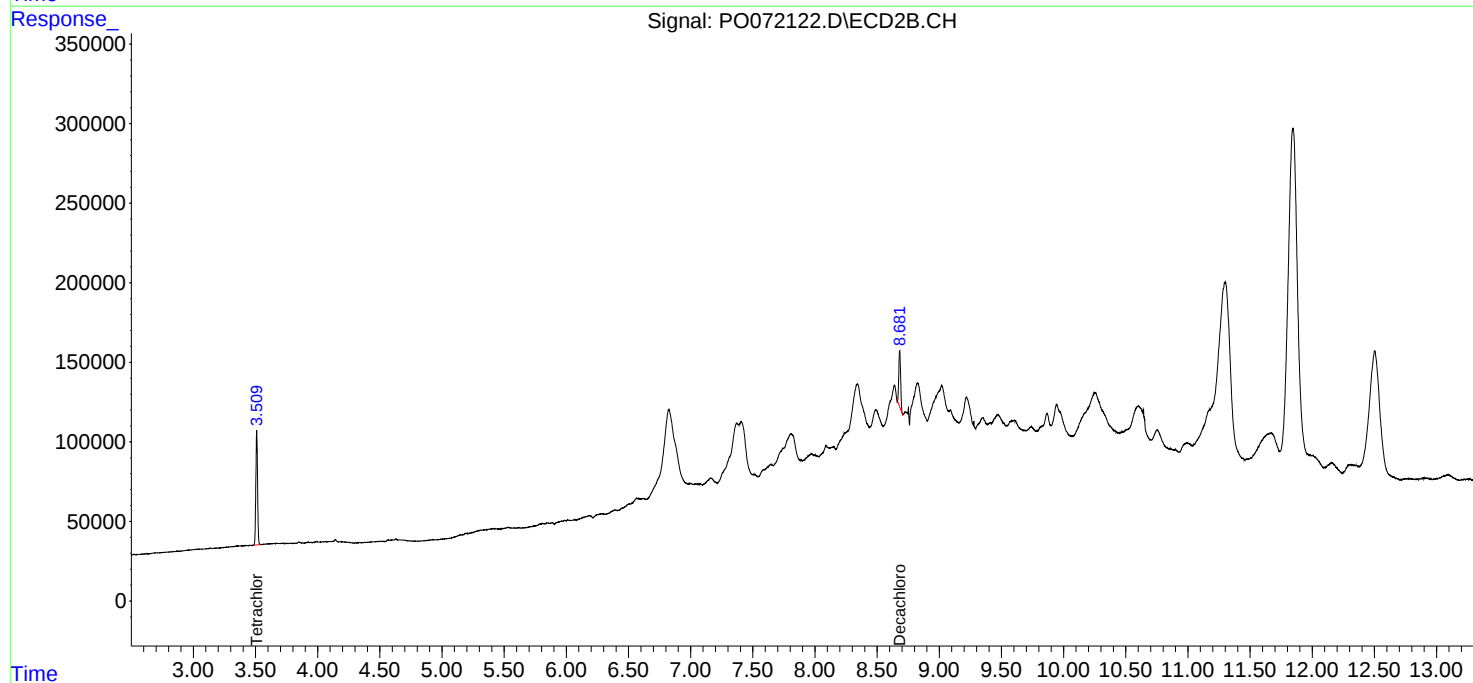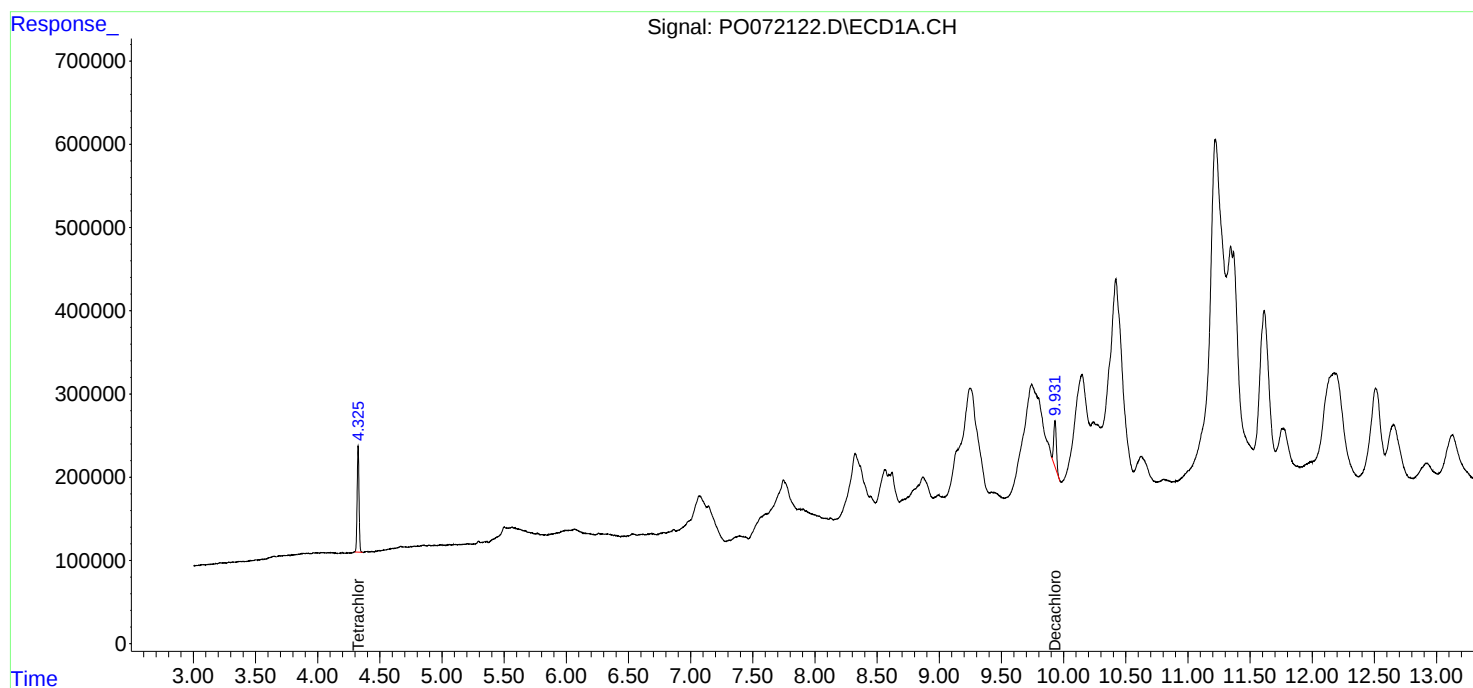

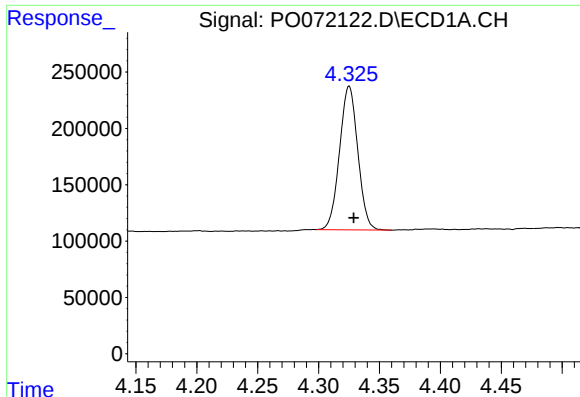


#1 Tetrachloro-m-xylene

R.T.: 4.325 min
Delta R.T.: -0.004 min
Response: 1327921
Conc: 18.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
RO-RBR-200031


Manual Integrations
APPROVED

Ankita
10/12/2020 9:17:29 AM

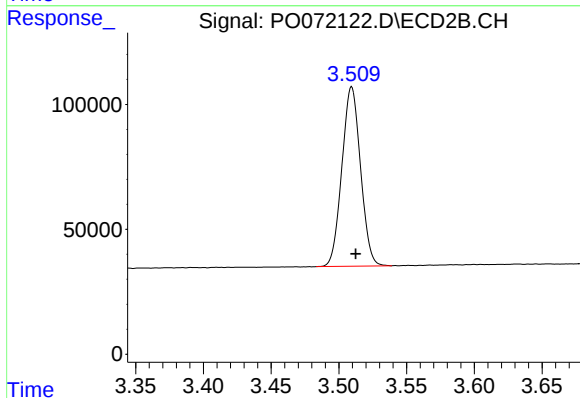


#1 Tetrachloro-m-xylene

R.T.: 3.509 min
Delta R.T.: -0.003 min
Response: 688124
Conc: 18.37 ng/ml

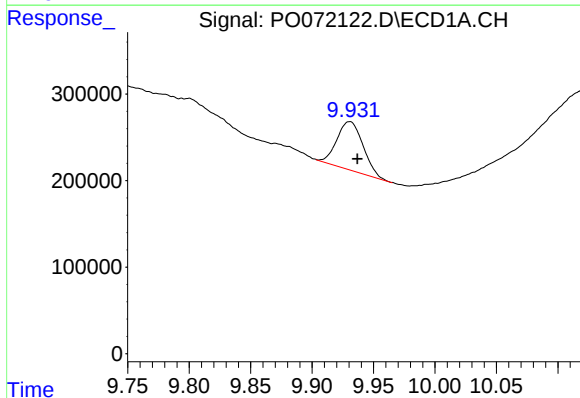

#2 Decachlorobiphenyl

R.T.: 9.931 min
Delta R.T.: -0.006 min
Response: 830813
Conc: 7.55 ng/ml m

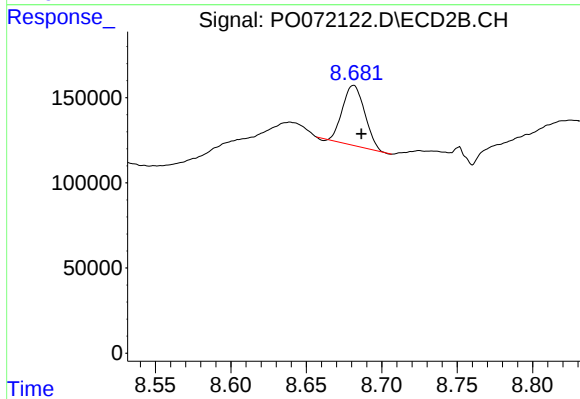

#2 Decachlorobiphenyl

R.T.: 8.682 min
Delta R.T.: -0.005 min
Response: 362074
Conc: 6.37 ng/ml