

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO100820\
 Data File : PO072125.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Oct 2020 17:56
 Operator : DD\AJ
 Sample : L4300-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 231-232-COMP

Manual Integrations
 APPROVED

Ankita
 10/12/2020 9:17:33 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 04:26:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.325	3.511	1117656	661917	15.561	17.672
2) SA Decachlor...	9.930	8.680	1664460	941788	15.117m	16.558
Target Compounds						
31) L7 AR-1260-1	7.284	6.288	135770	93824	28.329m	36.644 #
32) L7 AR-1260-2	7.551	6.489	266304	124004	35.554m	38.762
33) L7 AR-1260-3	7.908	6.634	212267	103584	33.295	35.099
34) L7 AR-1260-4	8.134	7.110	332880	79343	55.457	29.988 #
35) L7 AR-1260-5	8.449	7.363	423499	235276	30.562	35.412

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100820\
Data File : PO072125.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Oct 2020 17:56
Operator : DD\AJ
Sample : L4300-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
231-232-COMP


Manual Integrations
APPROVED

Ankita
10/12/2020 9:17:33 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 04:26:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

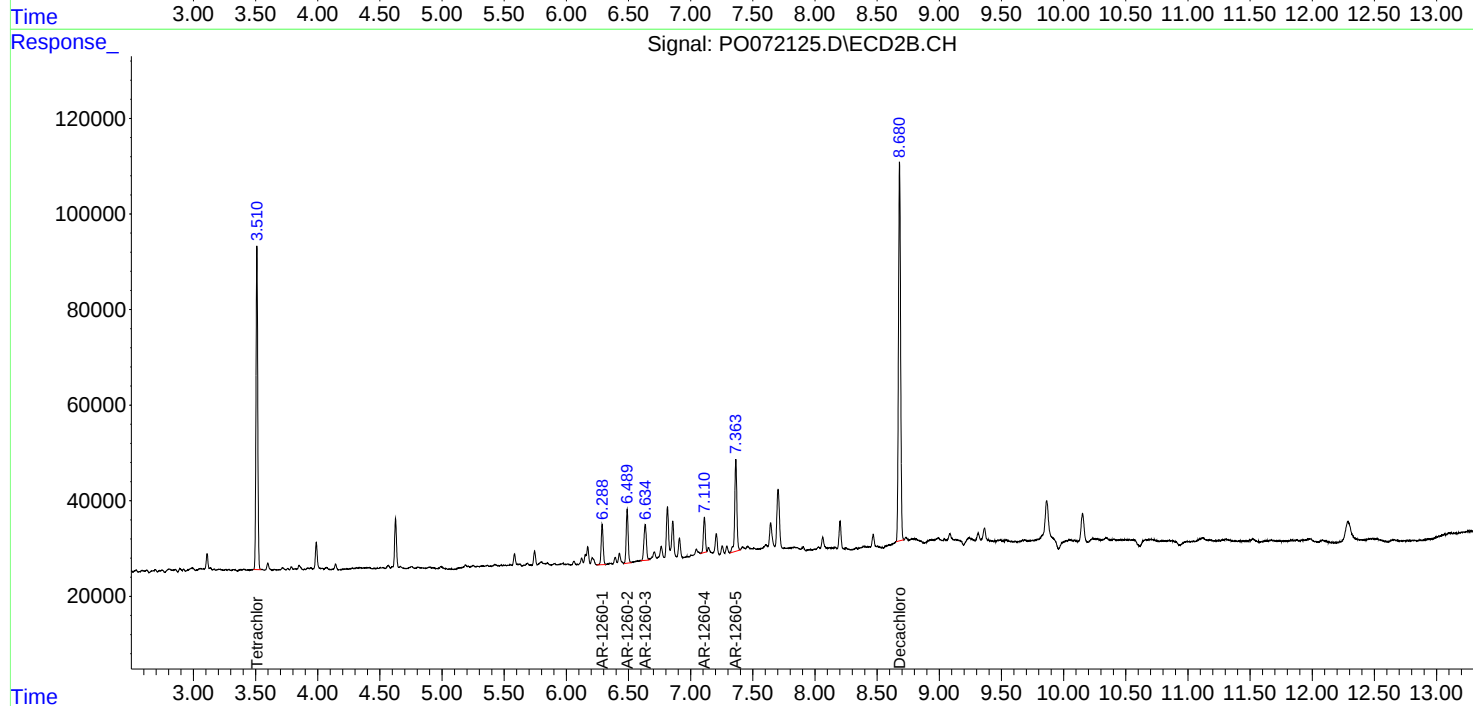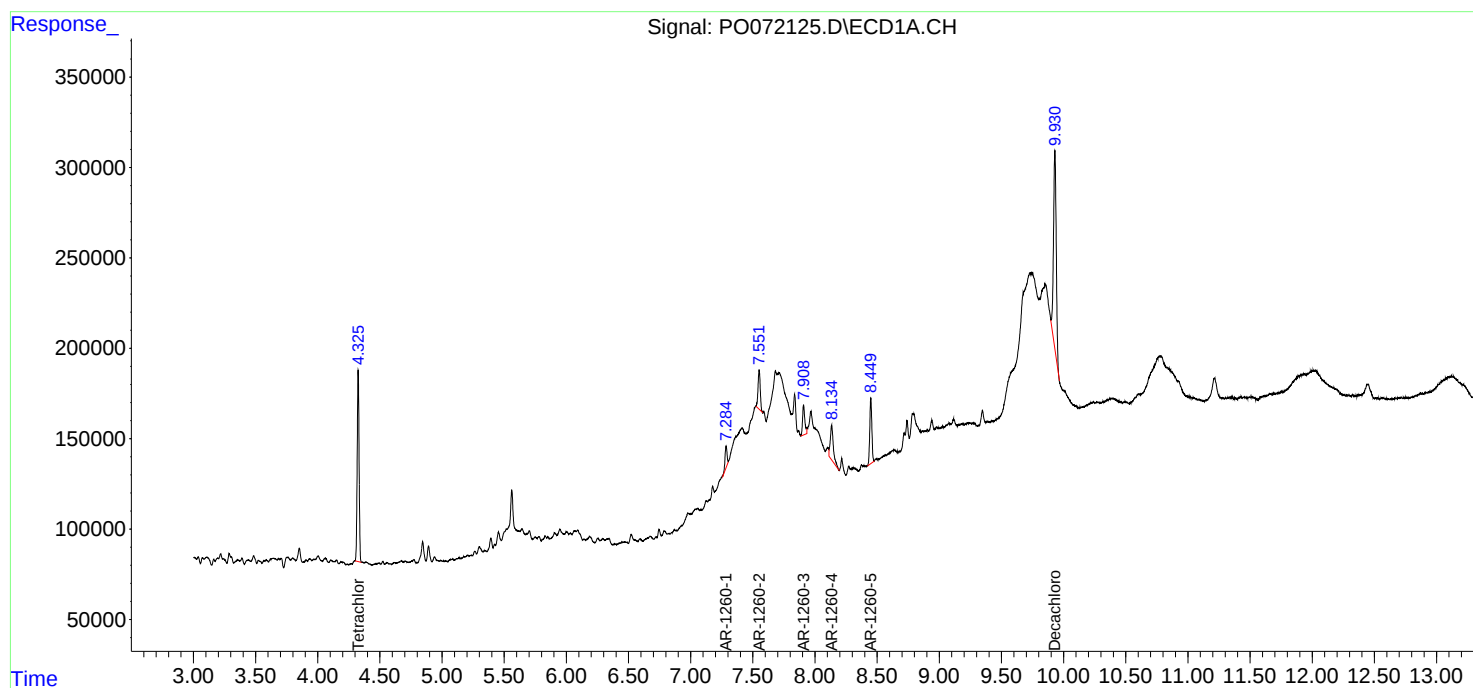

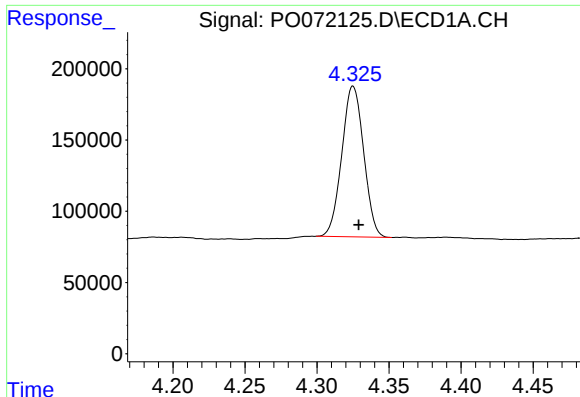


#1 Tetrachloro-m-xylene

R.T.: 4.325 min
Delta R.T.: -0.004 min
Response: 1117656
Conc: 15.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
231-232-COMP


Manual Integrations
APPROVED

Ankita
10/12/2020 9:17:33 AM

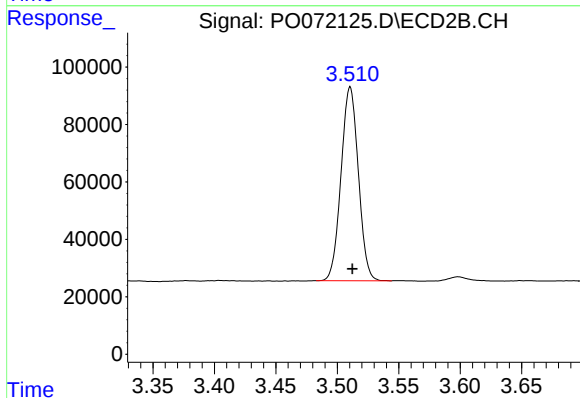


#1 Tetrachloro-m-xylene

R.T.: 3.511 min
Delta R.T.: -0.002 min
Response: 661917
Conc: 17.67 ng/ml

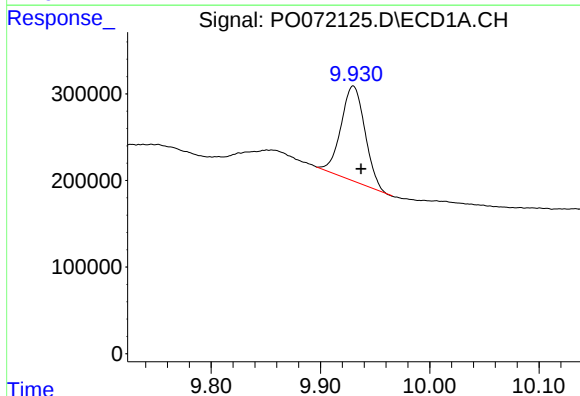


#2 Decachlorobiphenyl

R.T.: 9.930 min
Delta R.T.: -0.007 min
Response: 1664460
Conc: 15.12 ng/ml m

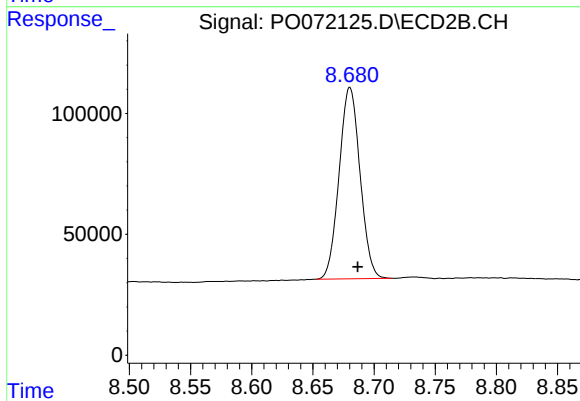

#2 Decachlorobiphenyl

R.T.: 8.680 min
Delta R.T.: -0.006 min
Response: 941788
Conc: 16.56 ng/ml

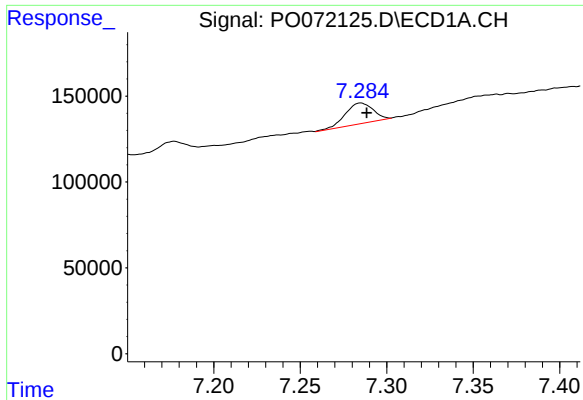


#31 AR-1260-1

R.T.: 7.284 min
Delta R.T.: -0.004 min
Response: 135770
Conc: 28.33 ng/ml m

Instrument :
ECD_O
ClientSampleId :
231-232-COMP


Manual Integrations
APPROVED

Ankita
10/12/2020 9:17:33 AM

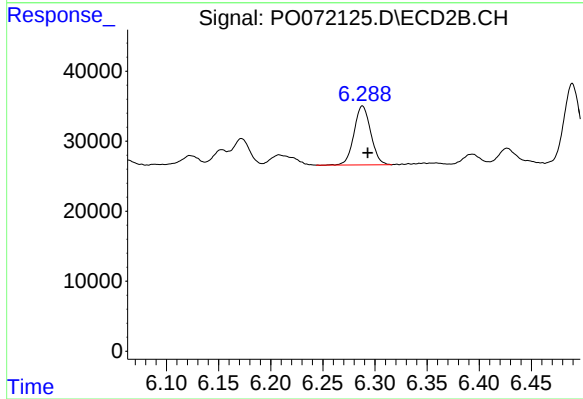


#31 AR-1260-1

R.T.: 6.288 min
Delta R.T.: -0.005 min
Response: 93824
Conc: 36.64 ng/ml

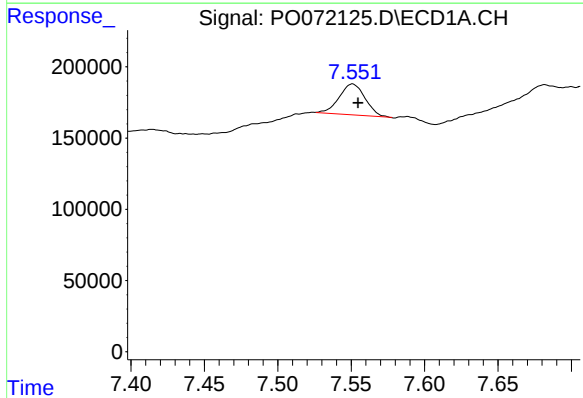


#32 AR-1260-2

R.T.: 7.551 min
Delta R.T.: -0.004 min
Response: 266304
Conc: 35.55 ng/ml m

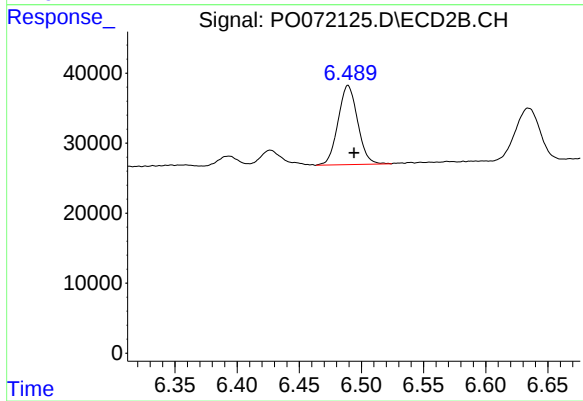

#32 AR-1260-2

R.T.: 6.489 min
Delta R.T.: -0.005 min
Response: 124004
Conc: 38.76 ng/ml

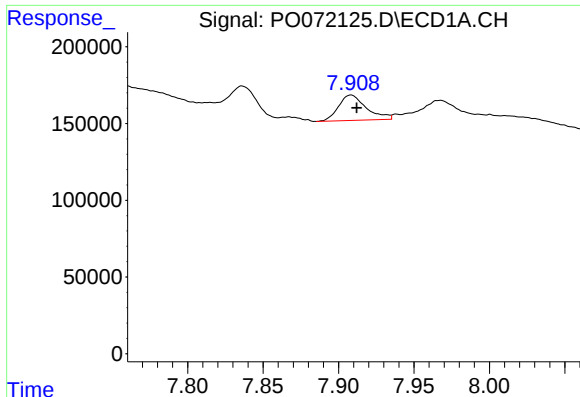


#33 AR-1260-3

R.T.: 7.908 min
Delta R.T.: -0.004 min
Response: 212267
Conc: 33.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
231-232-COMP


Manual Integrations
APPROVED

Ankita
10/12/2020 9:17:33 AM

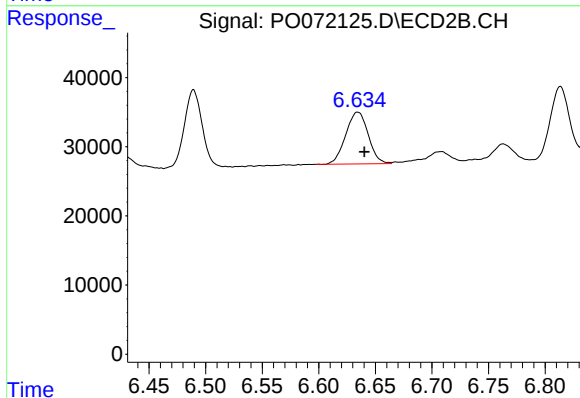


#33 AR-1260-3

R.T.: 6.634 min
Delta R.T.: -0.006 min
Response: 103584
Conc: 35.10 ng/ml

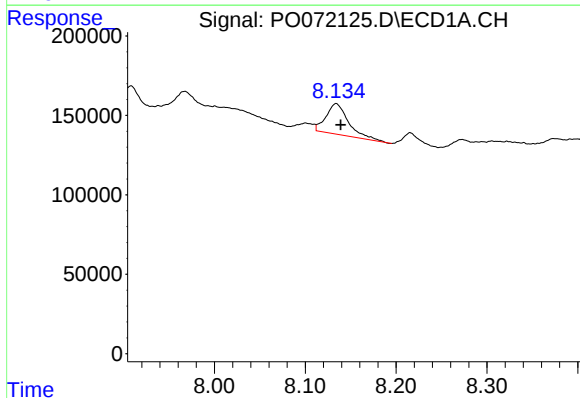


#34 AR-1260-4

R.T.: 8.134 min
Delta R.T.: -0.005 min
Response: 332880
Conc: 55.46 ng/ml

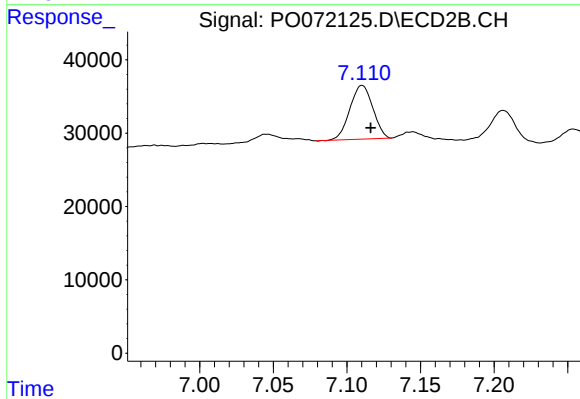

#34 AR-1260-4

R.T.: 7.110 min
Delta R.T.: -0.006 min
Response: 79343
Conc: 29.99 ng/ml

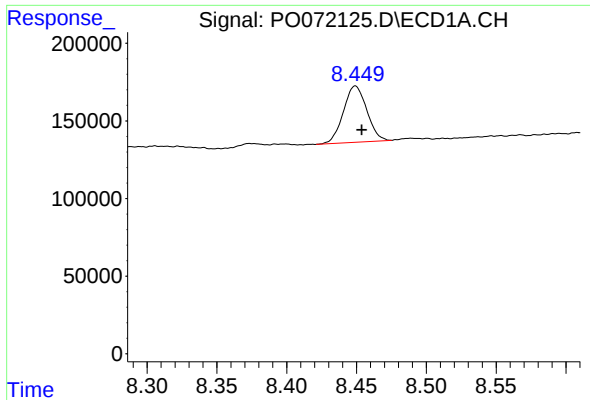


#35 AR-1260-5

R.T.: 8.449 min
Delta R.T.: -0.005 min
Response: 423499
Conc: 30.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
231-232-COMP

Manual Integrations
APPROVED

Ankita
10/12/2020 9:17:33 AM

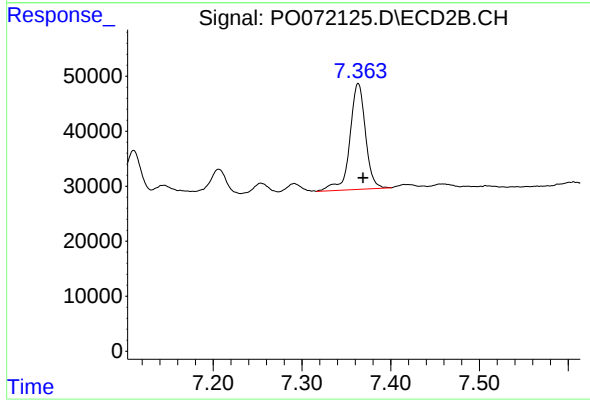

#35 AR-1260-5

R.T.: 7.363 min
Delta R.T.: -0.005 min
Response: 235276
Conc: 35.41 ng/ml