

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100820\
 Data File : PO072127.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Oct 2020 18:31
 Operator : DD\AJ
 Sample : L4311-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PAV-B10-100720-0-10

Manual Integrations
 APPROVED

Ankita
 10/12/2020 9:17:39 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 04:27:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.325	3.509	1770980	895441	24.657m	23.906
2) SA Decachlor...	9.930	8.681	1882300	1017299	17.095	17.885

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100820\
Data File : PO072127.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Oct 2020 18:31
Operator : DD\AJ
Sample : L4311-03
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PAV-B10-100720-0-10


Manual Integrations
APPROVED

Ankita
10/12/2020 9:17:39 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 04:27:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

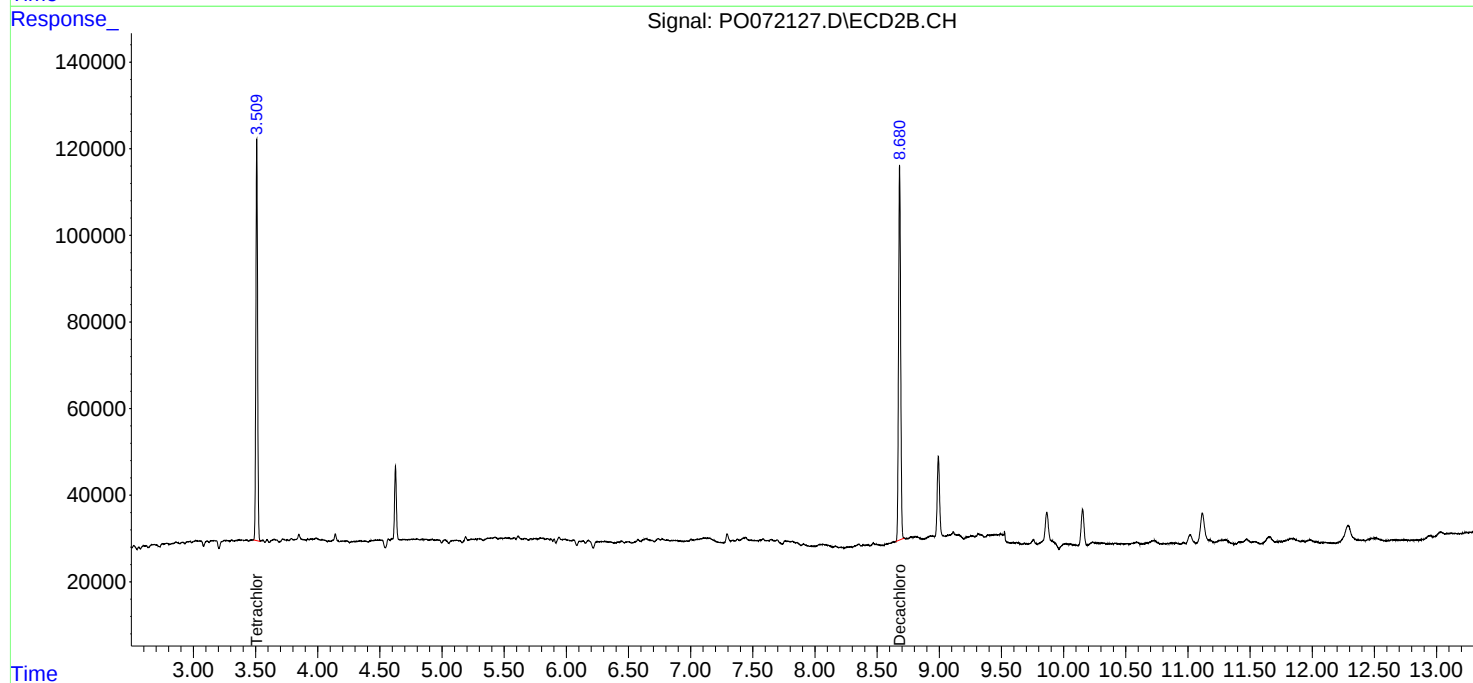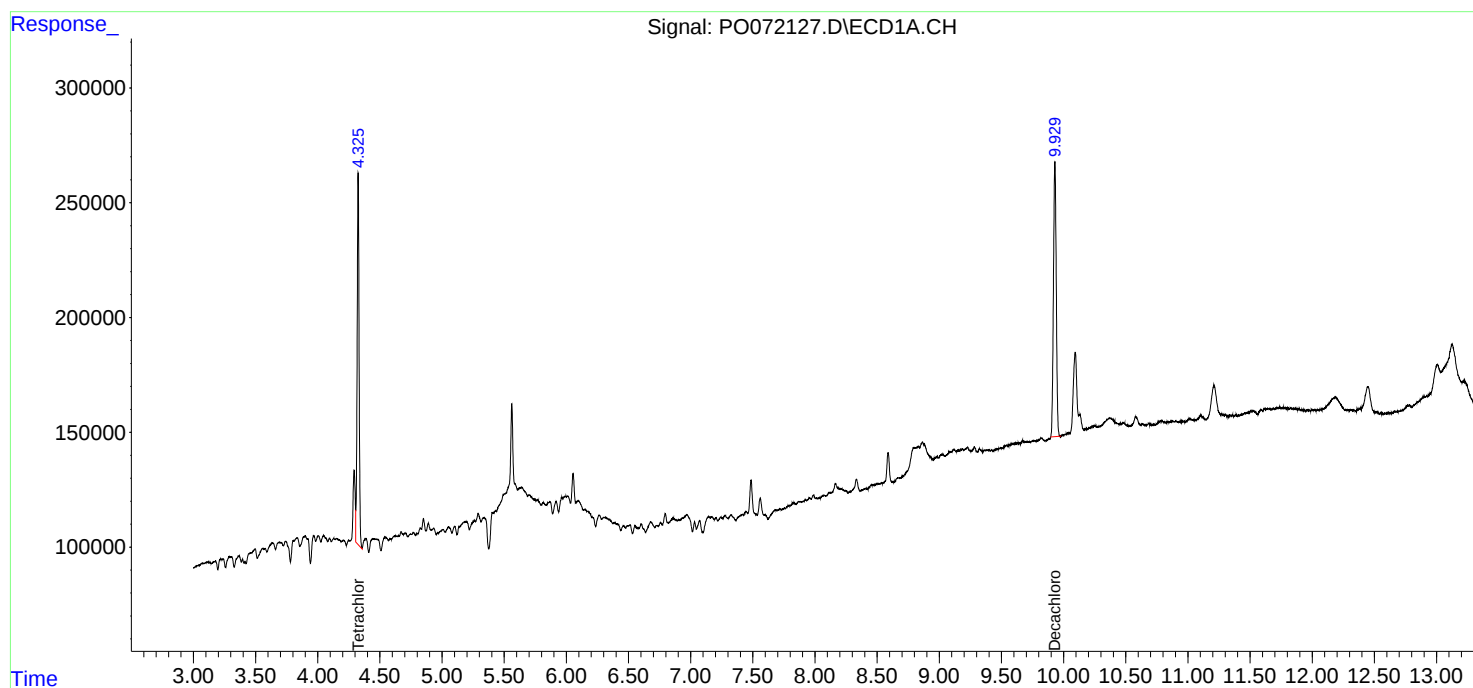

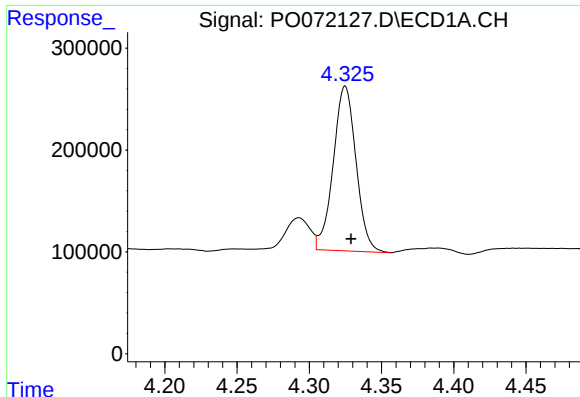


#1 Tetrachloro-m-xylene

R.T.: 4.325 min
Delta R.T.: -0.004 min
Response: 1770980
Conc: 24.66 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PAV-B10-100720-0-10


Manual Integrations
APPROVED

Ankita
10/12/2020 9:17:39 AM

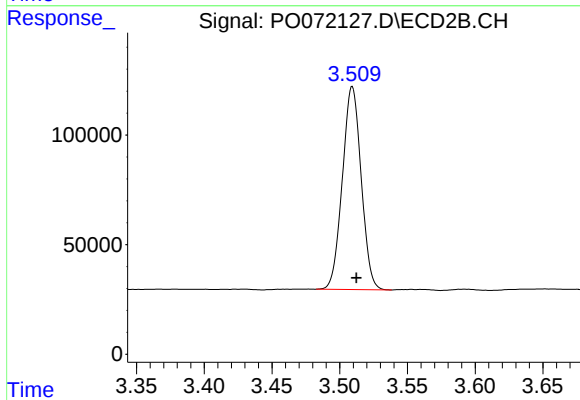


#1 Tetrachloro-m-xylene

R.T.: 3.509 min
Delta R.T.: -0.003 min
Response: 895441
Conc: 23.91 ng/ml

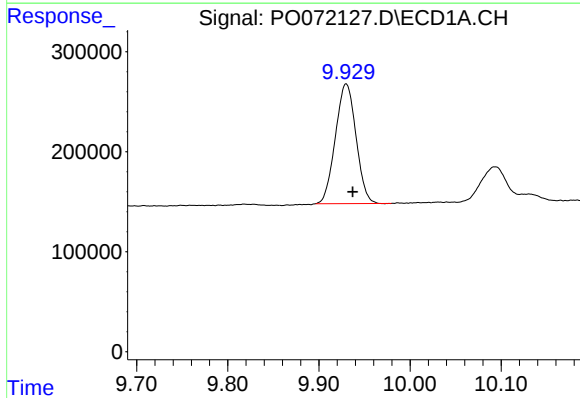

#2 Decachlorobiphenyl

R.T.: 9.930 min
Delta R.T.: -0.007 min
Response: 1882300
Conc: 17.10 ng/ml

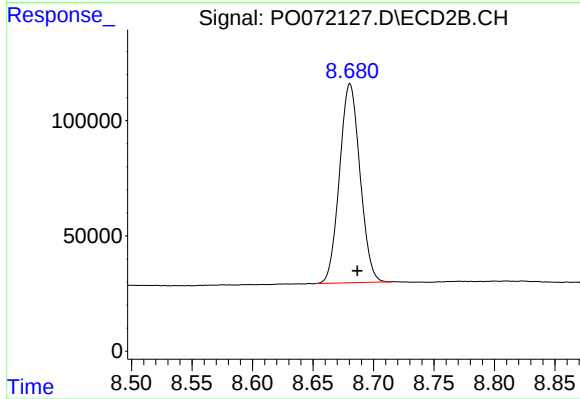

#2 Decachlorobiphenyl

R.T.: 8.681 min
Delta R.T.: -0.006 min
Response: 1017299
Conc: 17.89 ng/ml