

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100820\
 Data File : PO072131.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Oct 2020 19:39
 Operator : DD\AJ
 Sample : L4294-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-(0-3)-(3-5)-COMP

Manual Integrations
 APPROVED

Ankita
 10/12/2020 9:18:03 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 04:28:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.325	3.509	1951923	1007620	27.176	26.901
2) SA Decachlor...	9.931	8.680	2165804	1059218	19.670	18.622
Target Compounds						
31) L7 AR-1260-1	7.284	6.288	69042	54097	14.406	21.128 #
32) L7 AR-1260-2	7.558	6.489	242049	57224	32.316	17.888 #
33) L7 AR-1260-3	7.908	6.633	93796	56708	14.712	19.215 #
34) L7 AR-1260-4	8.132	7.109	93245	40763	15.534	15.407m
35) L7 AR-1260-5	8.449	7.362	164780	94632	11.891	14.243

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100820\
Data File : PO072131.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Oct 2020 19:39
Operator : DD\AJ
Sample : L4294-01
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-(0-3)-(3-5)-COMP


Manual Integrations
APPROVED

Ankita
10/12/2020 9:18:03 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 04:28:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

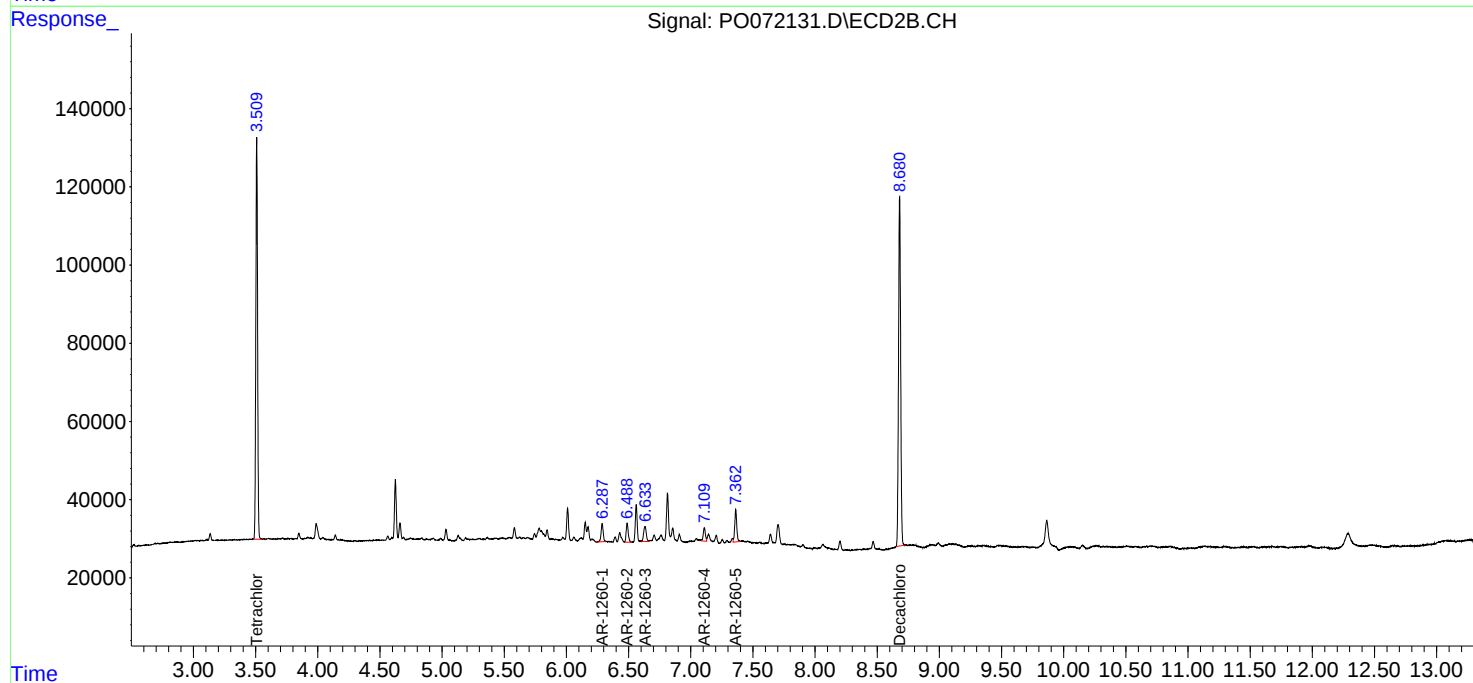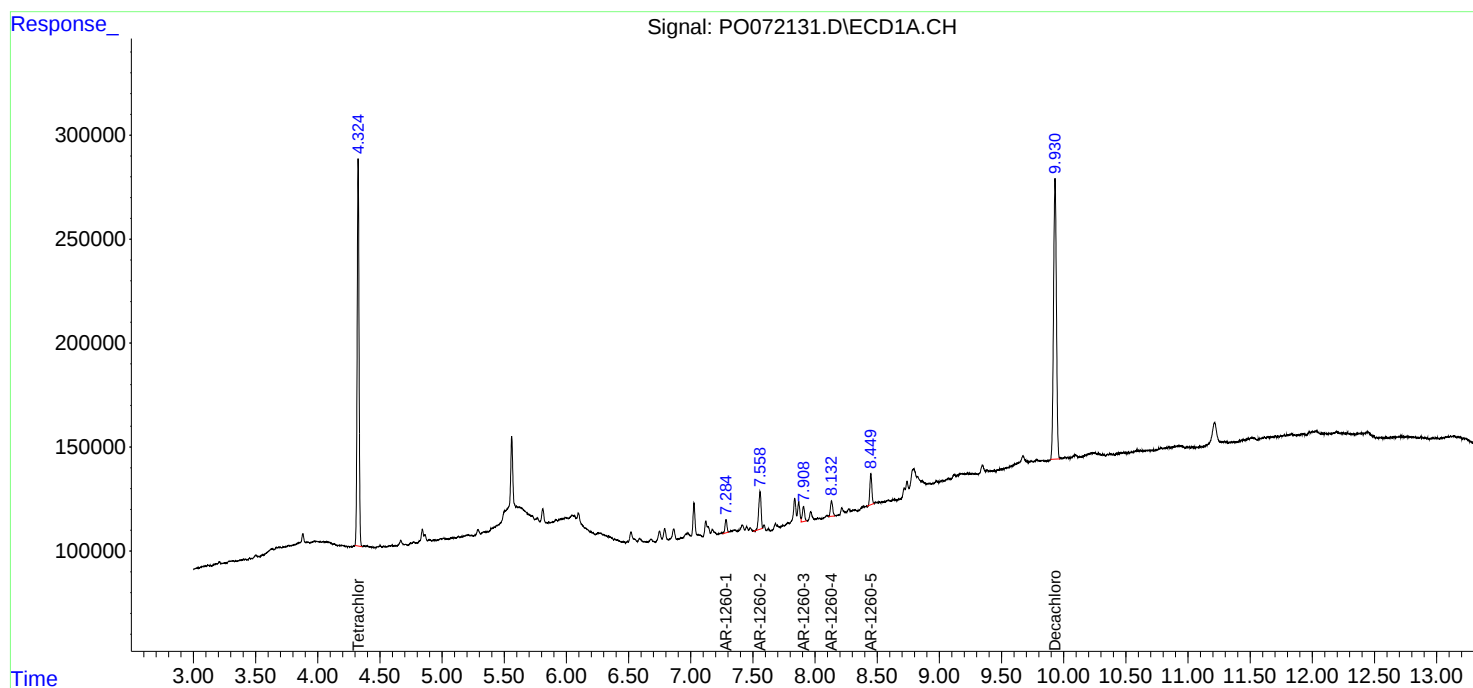

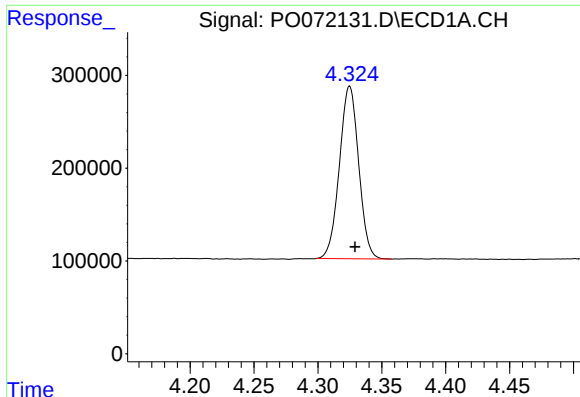


#1 Tetrachloro-m-xylene

R.T.: 4.325 min
Delta R.T.: -0.004 min
Response: 1951923
Conc: 27.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-(0-3)-(3-5)-COMP


Manual Integrations
APPROVED

Ankita
10/12/2020 9:18:03 AM

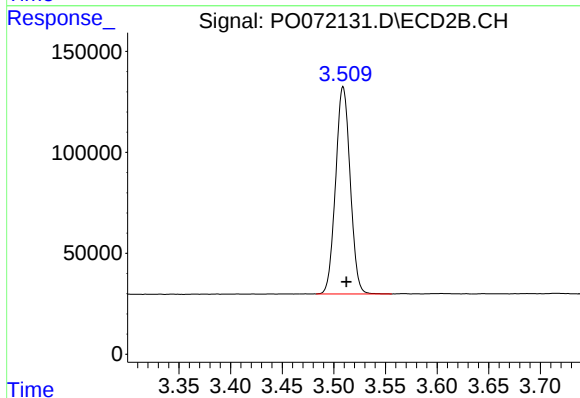


#1 Tetrachloro-m-xylene

R.T.: 3.509 min
Delta R.T.: -0.003 min
Response: 1007620
Conc: 26.90 ng/ml

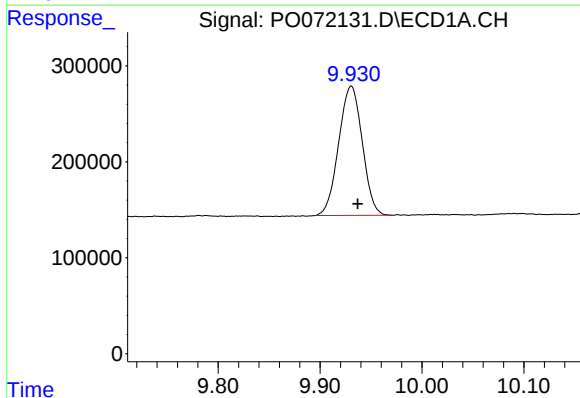


#2 Decachlorobiphenyl

R.T.: 9.931 min
Delta R.T.: -0.006 min
Response: 2165804
Conc: 19.67 ng/ml

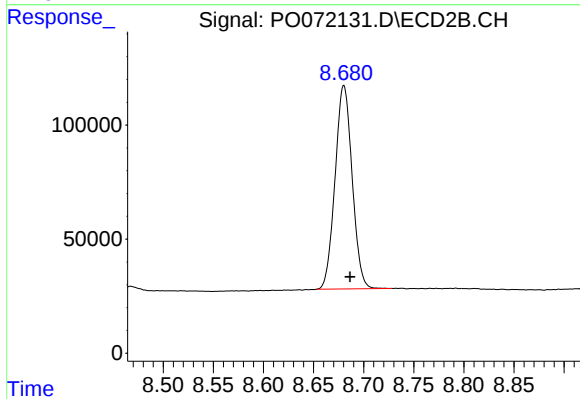

#2 Decachlorobiphenyl

R.T.: 8.680 min
Delta R.T.: -0.006 min
Response: 1059218
Conc: 18.62 ng/ml

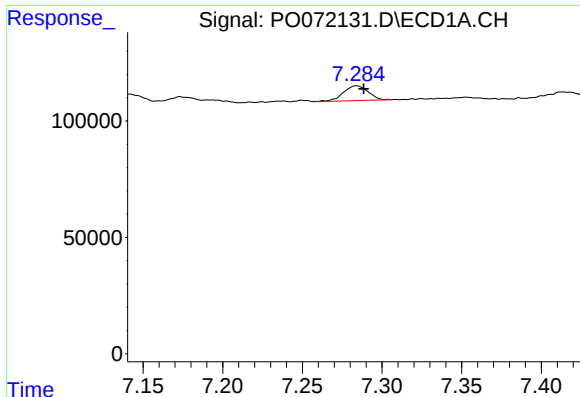


#31 AR-1260-1

R.T.: 7.284 min
Delta R.T.: -0.004 min
Response: 69042
Conc: 14.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-(0-3)-(3-5)-COMP


Manual Integrations
APPROVED

Ankita
10/12/2020 9:18:03 AM

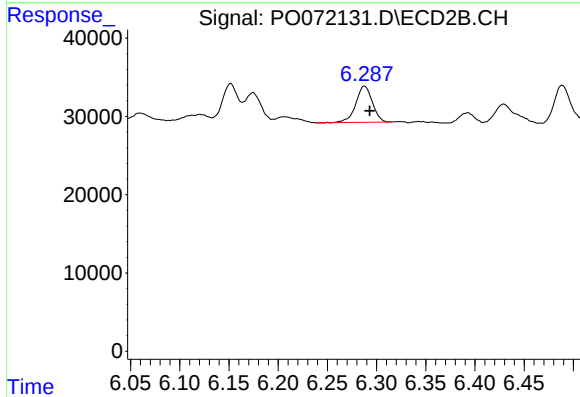


#31 AR-1260-1

R.T.: 6.288 min
Delta R.T.: -0.005 min
Response: 54097
Conc: 21.13 ng/ml

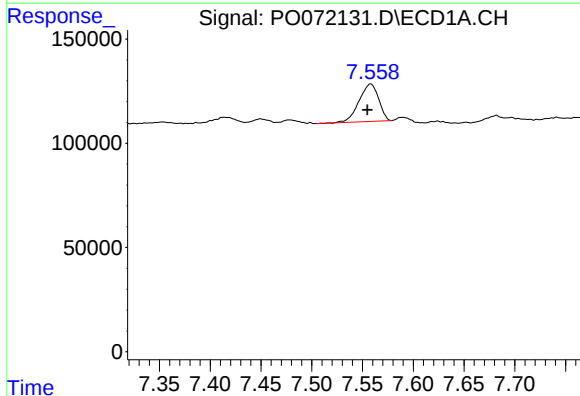


#32 AR-1260-2

R.T.: 7.558 min
Delta R.T.: 0.003 min
Response: 242049
Conc: 32.32 ng/ml

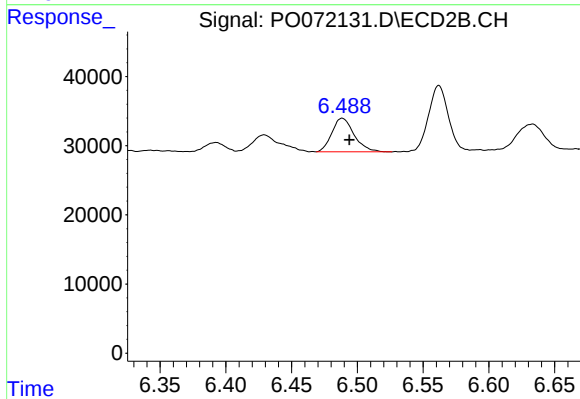

#32 AR-1260-2

R.T.: 6.489 min
Delta R.T.: -0.006 min
Response: 57224
Conc: 17.89 ng/ml

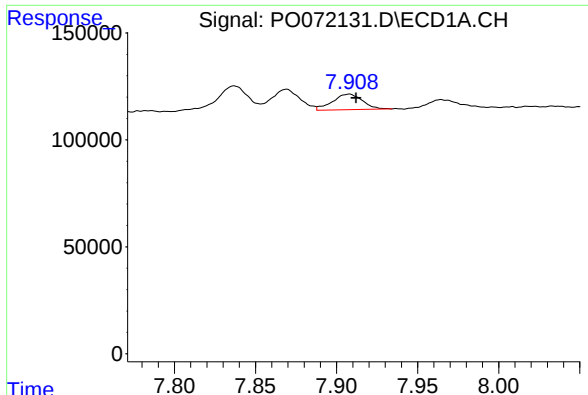


#33 AR-1260-3

R.T.: 7.908 min
Delta R.T.: -0.004 min
Response: 93796
Conc: 14.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-(0-3)-(3-5)-COMP


Manual Integrations
APPROVED

Ankita
10/12/2020 9:18:03 AM

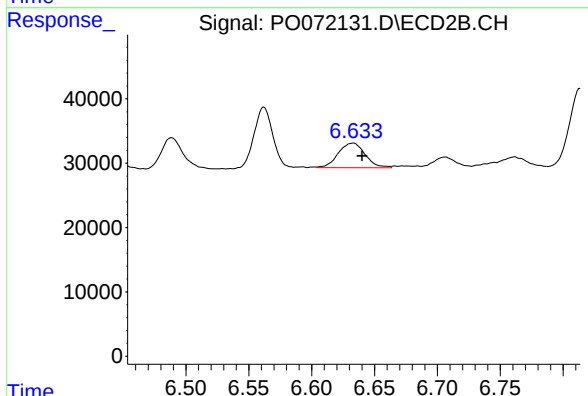


#33 AR-1260-3

R.T.: 6.633 min
Delta R.T.: -0.007 min
Response: 56708
Conc: 19.22 ng/ml

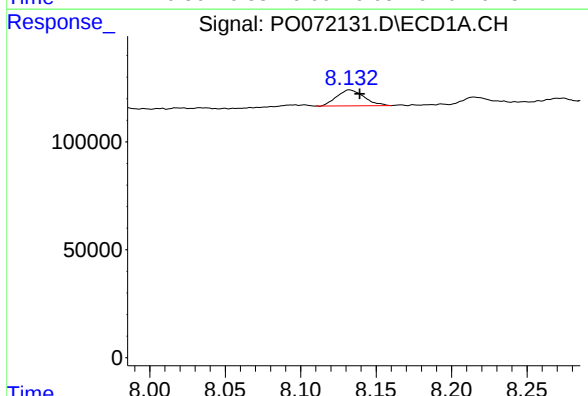


#34 AR-1260-4

R.T.: 8.132 min
Delta R.T.: -0.007 min
Response: 93245
Conc: 15.53 ng/ml

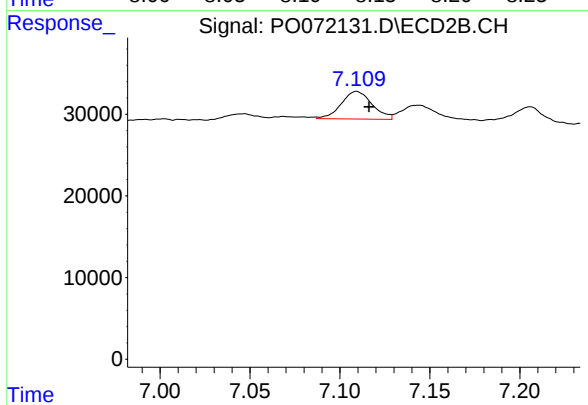

#34 AR-1260-4

R.T.: 7.109 min
Delta R.T.: -0.007 min
Response: 40763
Conc: 15.41 ng/ml m

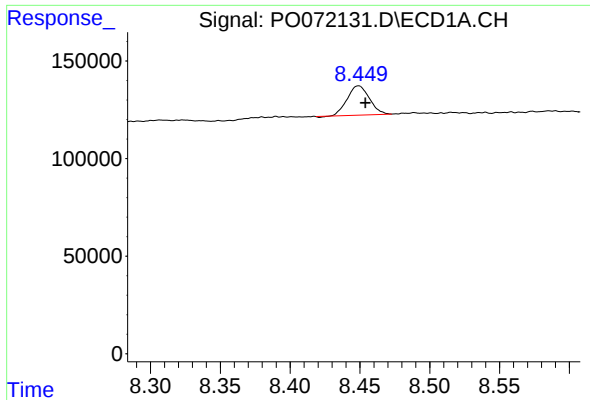


#35 AR-1260-5

R.T.: 8.449 min
Delta R.T.: -0.005 min
Response: 164780
Conc: 11.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-(0-3)-(3-5)-COMP

Manual Integrations
APPROVED

Ankita
10/12/2020 9:18:03 AM

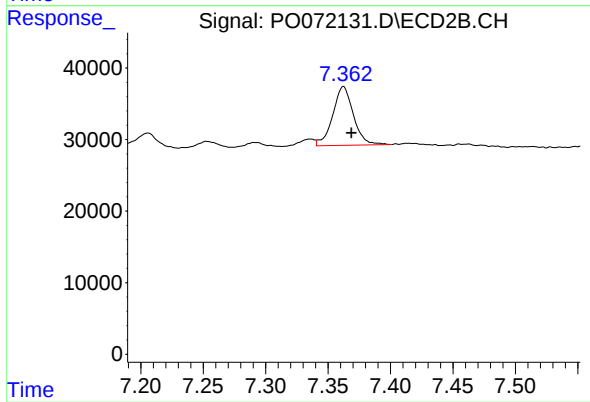

#35 AR-1260-5

R.T.: 7.362 min
Delta R.T.: -0.006 min
Response: 94632
Conc: 14.24 ng/ml