

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100820\
 Data File : PO072162.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Oct 2020 4:30
 Operator : DD\AJ
 Sample : L4299-06
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 86-96-COMP

Manual Integrations
 APPROVED

Ankita
 10/12/2020 9:17:49 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 07:28:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.324	3.510	1094808	394715	15.243m	10.538 #
2) SA Decachlor...	9.931	8.682	663144	321903	6.023	5.659

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100820\
Data File : PO072162.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Oct 2020 4:30
Operator : DD\AJ
Sample : L4299-06
Misc :
ALS Vial : 52 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
86-96-COMP


Manual Integrations
APPROVED

Ankita
10/12/2020 9:17:49 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 07:28:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

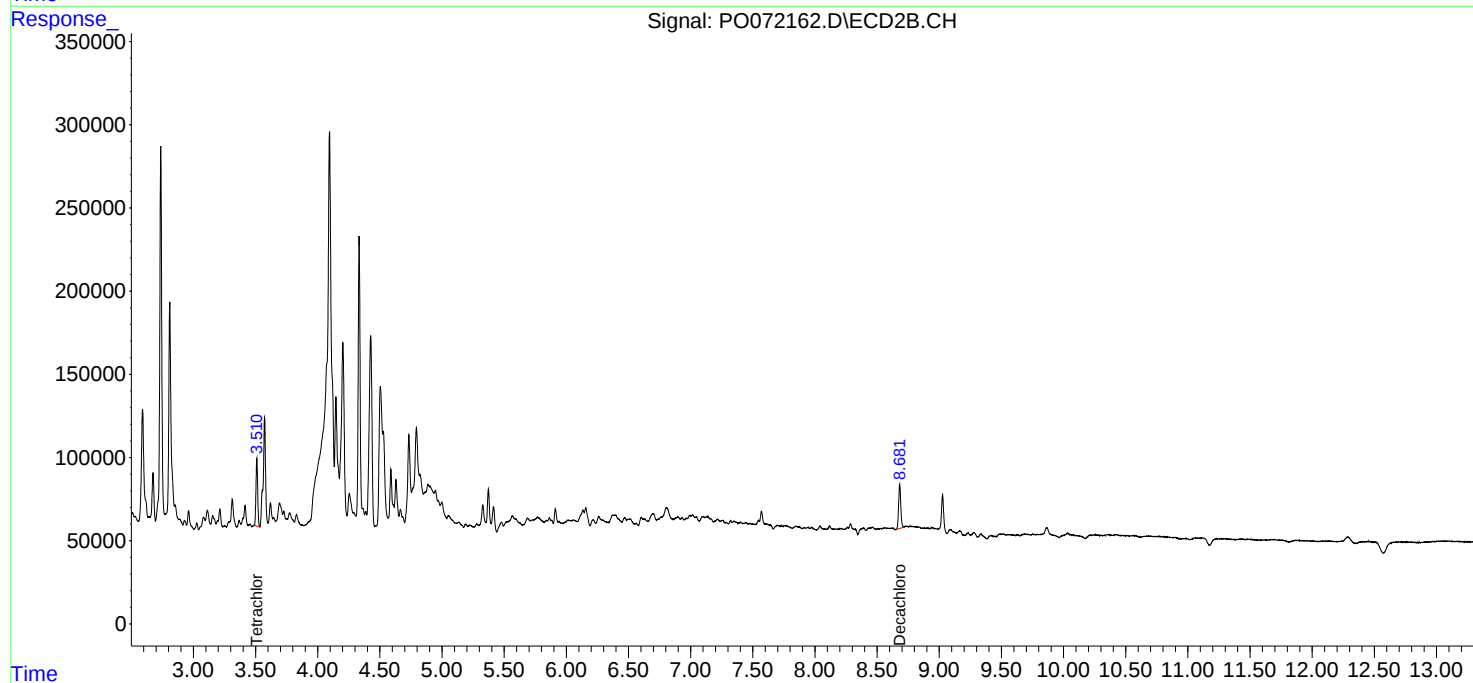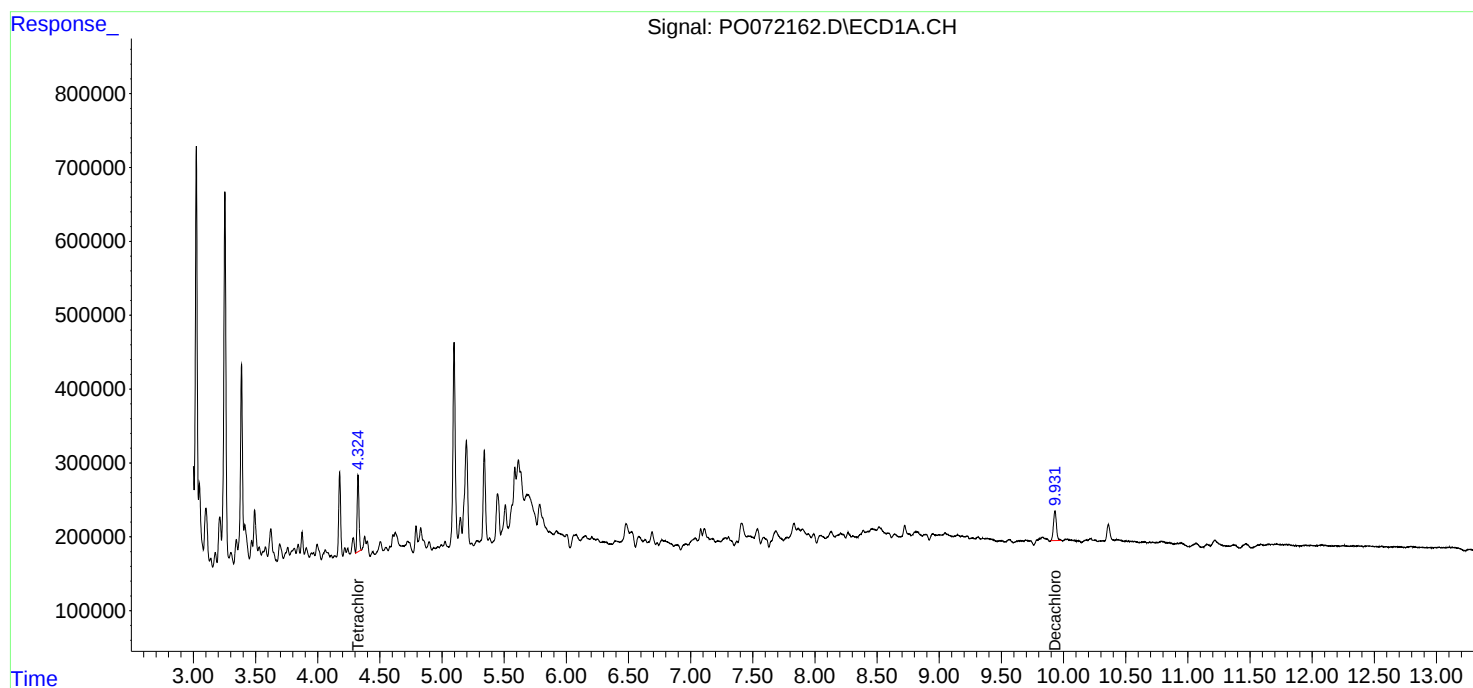

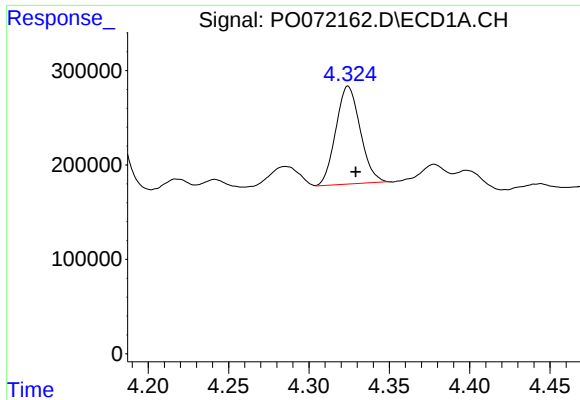


#1 Tetrachloro-m-xylene

R.T.: 4.324 min
Delta R.T.: -0.005 min
Response: 1094808
Conc: 15.24 ng/ml m

Instrument :
ECD_O
ClientSampleId :
86-96-COMP


Manual Integrations
APPROVED

Ankita
10/12/2020 9:17:49 AM

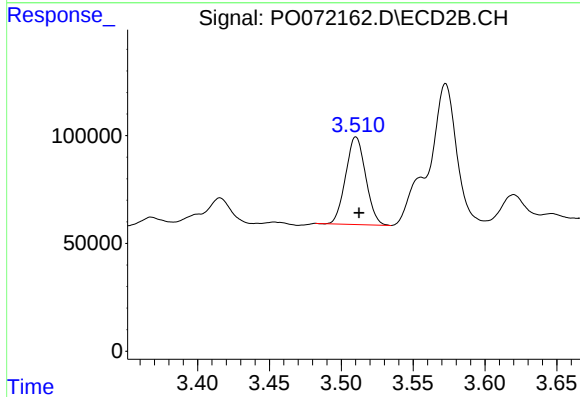


#1 Tetrachloro-m-xylene

R.T.: 3.510 min
Delta R.T.: -0.002 min
Response: 394715
Conc: 10.54 ng/ml

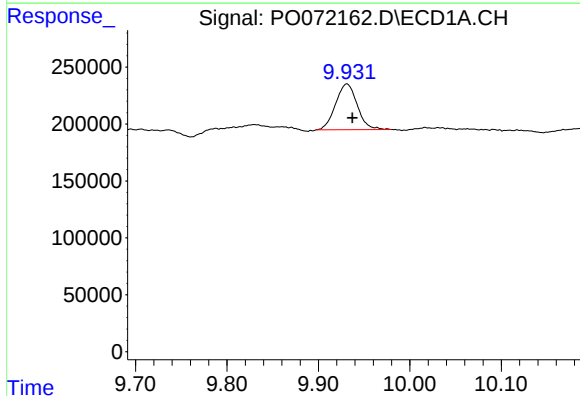

#2 Decachlorobiphenyl

R.T.: 9.931 min
Delta R.T.: -0.006 min
Response: 663144
Conc: 6.02 ng/ml

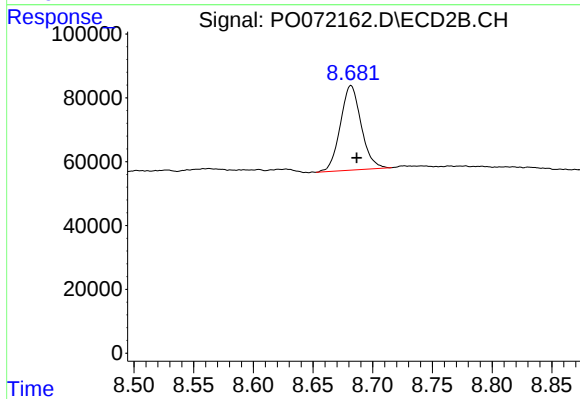

#2 Decachlorobiphenyl

R.T.: 8.682 min
Delta R.T.: -0.005 min
Response: 321903
Conc: 5.66 ng/ml