

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100820\
 Data File : PO072163.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Oct 2020 4:47
 Operator : DD\AJ
 Sample : L4300-02
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 223

Manual Integrations
 APPROVED

Ankita
 10/12/2020 9:17:51 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 07:28:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.328	3.516	994507	422916	13.846m	11.291
2) SA Decachlor...	9.929	8.679	893930	440520	8.119	7.745
Target Compounds						
31) L7 AR-1260-1	7.287	6.291	1061358	393608	221.454	153.729m#
32) L7 AR-1260-2	7.552	6.492	1648988	530157	220.154m	165.721m
33) L7 AR-1260-3	7.908	6.637	1555132	466802	243.931	158.173m#
34) L7 AR-1260-4	8.135	7.112	1159930	370947	193.240	140.200m#
35) L7 AR-1260-5	8.451	7.364	1932400	949878	139.453	142.970m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100820\
Data File : PO072163.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Oct 2020 4:47
Operator : DD\AJ
Sample : L4300-02
Misc :
ALS Vial : 53 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
223


Manual Integrations
APPROVED

Ankita
10/12/2020 9:17:51 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 07:28:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

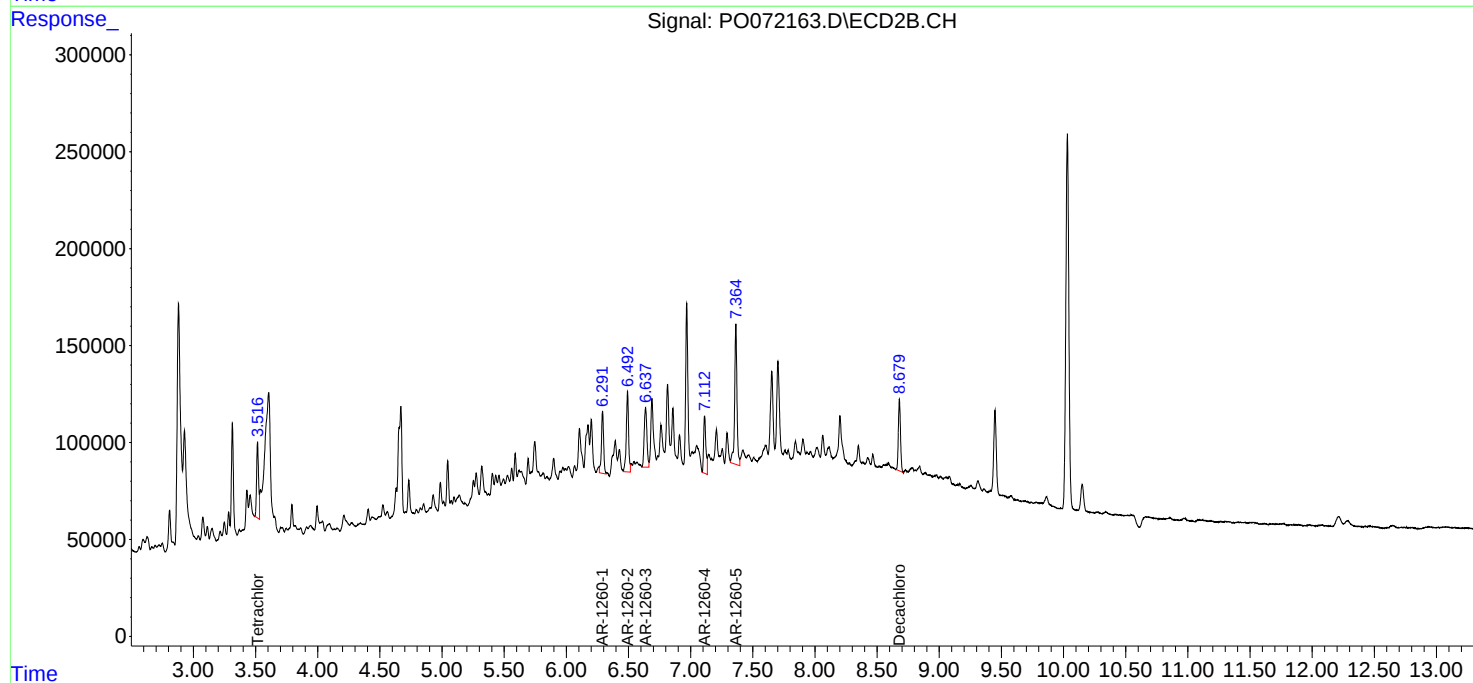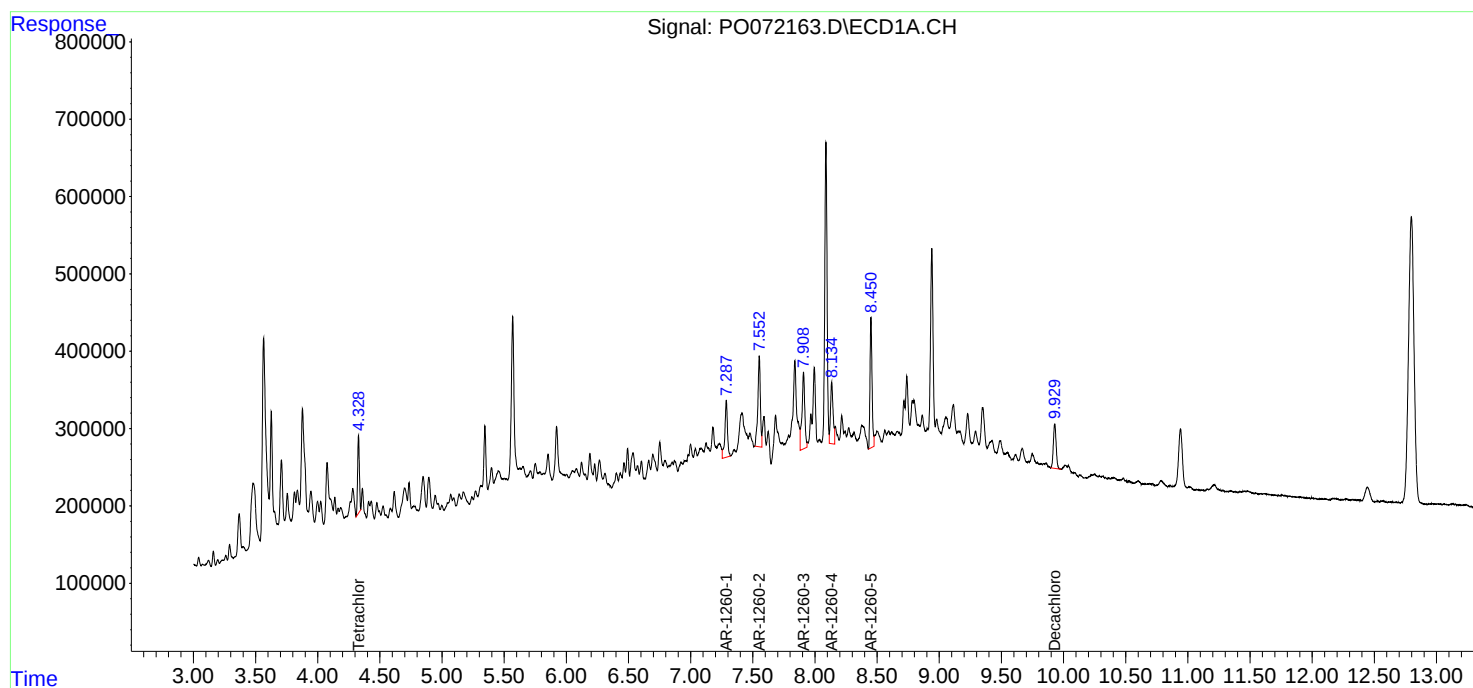

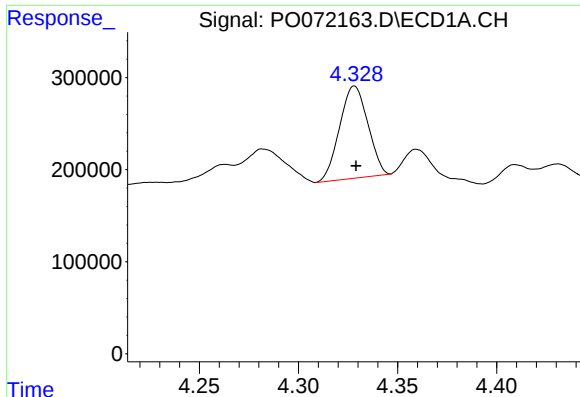


#1 Tetrachloro-m-xylene

R.T.: 4.328 min
Delta R.T.: -0.001 min
Response: 994507
Conc: 13.85 ng/ml m

Instrument :
ECD_O
ClientSampleId :
223


Manual Integrations
APPROVED

Ankita
10/12/2020 9:17:51 AM

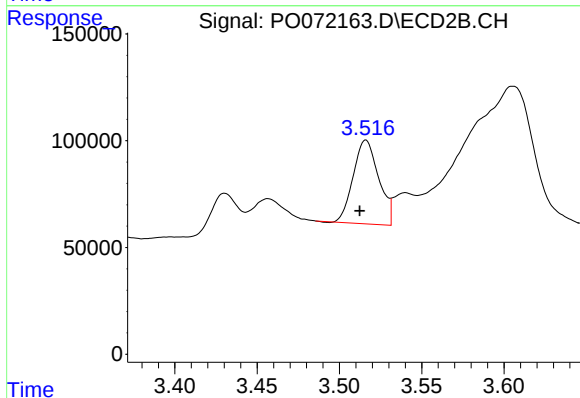


#1 Tetrachloro-m-xylene

R.T.: 3.516 min
Delta R.T.: 0.004 min
Response: 422916
Conc: 11.29 ng/ml

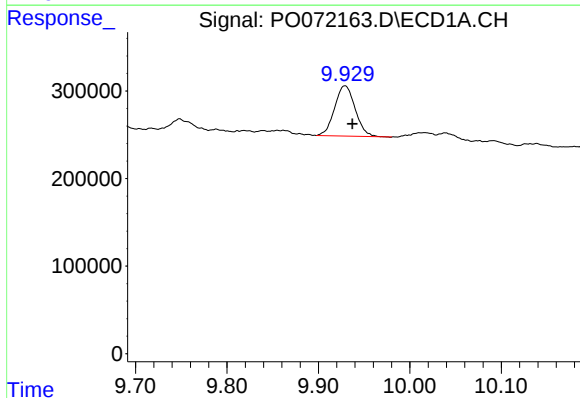


#2 Decachlorobiphenyl

R.T.: 9.929 min
Delta R.T.: -0.008 min
Response: 893930
Conc: 8.12 ng/ml

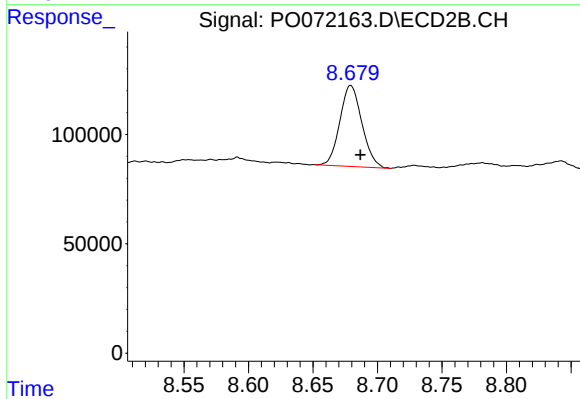

#2 Decachlorobiphenyl

R.T.: 8.679 min
Delta R.T.: -0.007 min
Response: 440520
Conc: 7.74 ng/ml

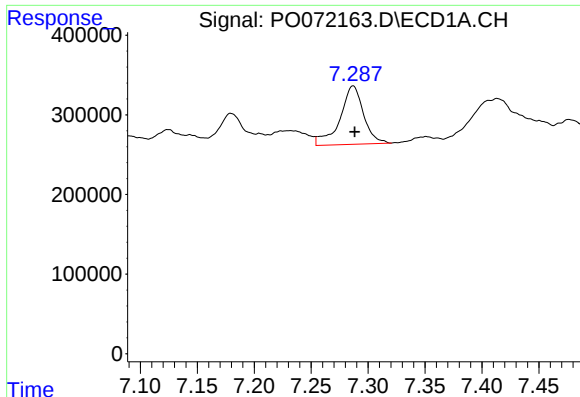


#31 AR-1260-1

R.T.: 7.287 min
Delta R.T.: -0.002 min
Response: 1061358
Conc: 221.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
223


Manual Integrations
APPROVED

Ankita
10/12/2020 9:17:51 AM

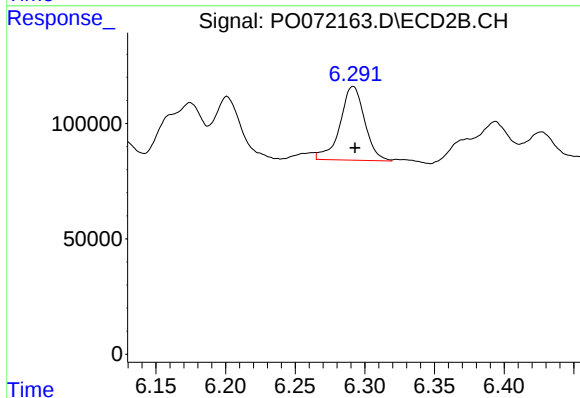


#31 AR-1260-1

R.T.: 6.291 min
Delta R.T.: -0.002 min
Response: 393608
Conc: 153.73 ng/ml m

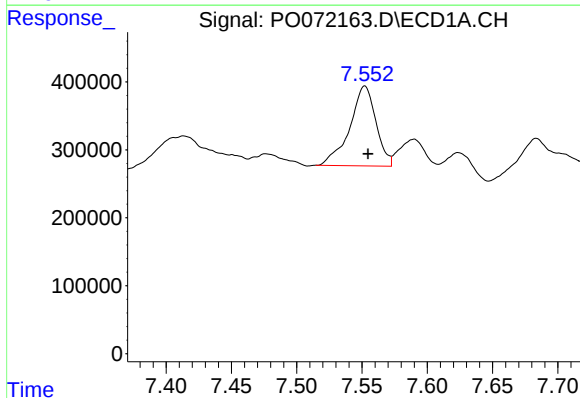


#32 AR-1260-2

R.T.: 7.552 min
Delta R.T.: -0.003 min
Response: 1648988
Conc: 220.15 ng/ml m

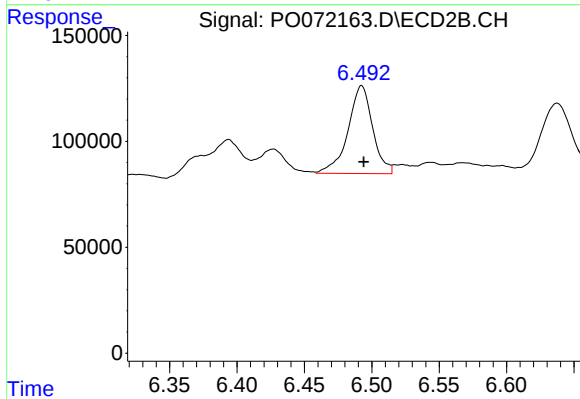

#32 AR-1260-2

R.T.: 6.492 min
Delta R.T.: -0.002 min
Response: 530157
Conc: 165.72 ng/ml m

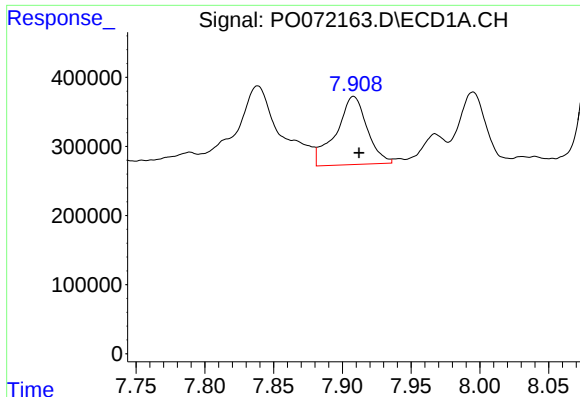


#33 AR-1260-3

R.T.: 7.908 min
Delta R.T.: -0.004 min
Response: 1555132
Conc: 243.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
223


Manual Integrations
APPROVED

Ankita
10/12/2020 9:17:51 AM

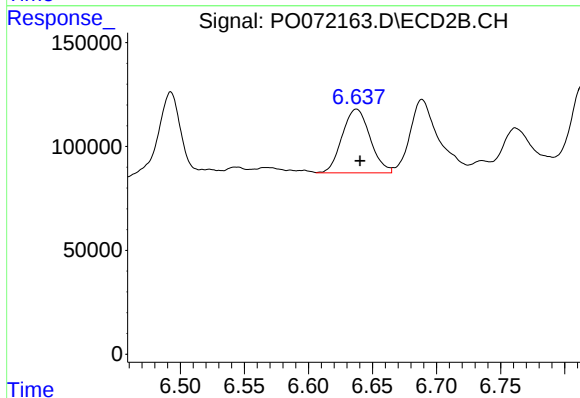


#33 AR-1260-3

R.T.: 6.637 min
Delta R.T.: -0.003 min
Response: 466802
Conc: 158.17 ng/ml m

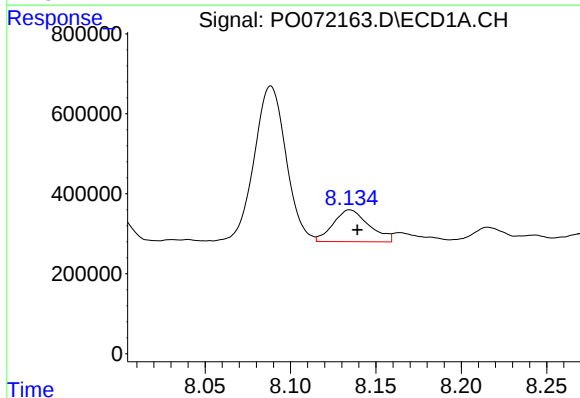


#34 AR-1260-4

R.T.: 8.135 min
Delta R.T.: -0.004 min
Response: 1159930
Conc: 193.24 ng/ml

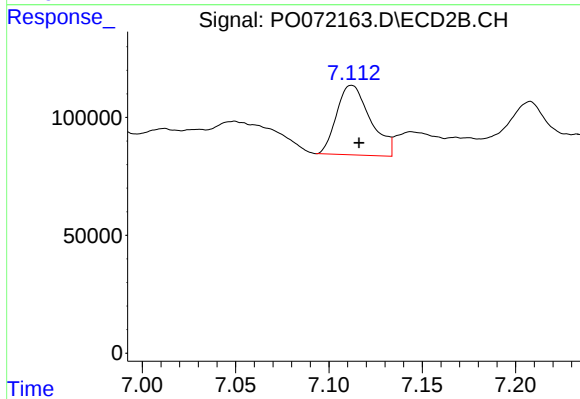

#34 AR-1260-4

R.T.: 7.112 min
Delta R.T.: -0.004 min
Response: 370947
Conc: 140.20 ng/ml m

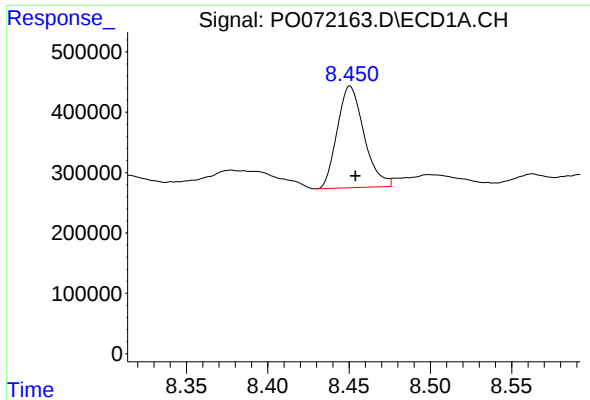


#35 AR-1260-5

R.T.: 8.451 min
Delta R.T.: -0.003 min
Response: 1932400
Conc: 139.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
223

Manual Integrations
APPROVED

Ankita
10/12/2020 9:17:51 AM

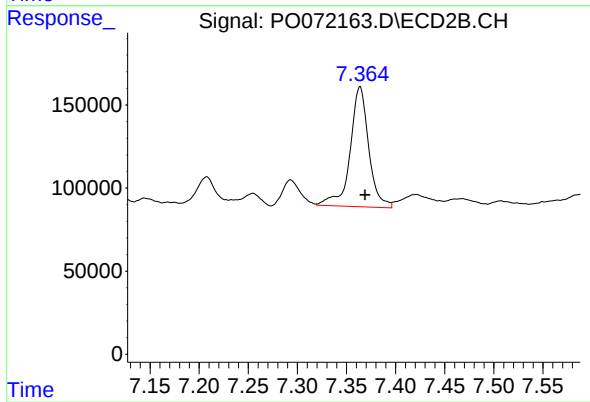

#35 AR-1260-5

R.T.: 7.364 min
Delta R.T.: -0.005 min
Response: 949878
Conc: 142.97 ng/ml m