

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100821\
 Data File : PO081940.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Oct 2021 21:37
 Operator : AJ\MA
 Sample : M4144-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IDW-LIQ-DRUM-2-100721

Manual Integrations
 APPROVED

mohammad
 10/12/2021 9:41:49 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 05:24:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 07 09:43:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.990	3.979	1604507	611286	19.336m	24.157m
2) SA Decachlor...	11.113	9.303	693321	447891	11.689m	18.960m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100821\
Data File : PO081940.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Oct 2021 21:37
Operator : AJ\MA
Sample : M4144-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
IDW-LIQ-DRUM-2-100721


Manual Integrations
APPROVED

mohammad
10/12/2021 9:41:49 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 05:24:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 07 09:43:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

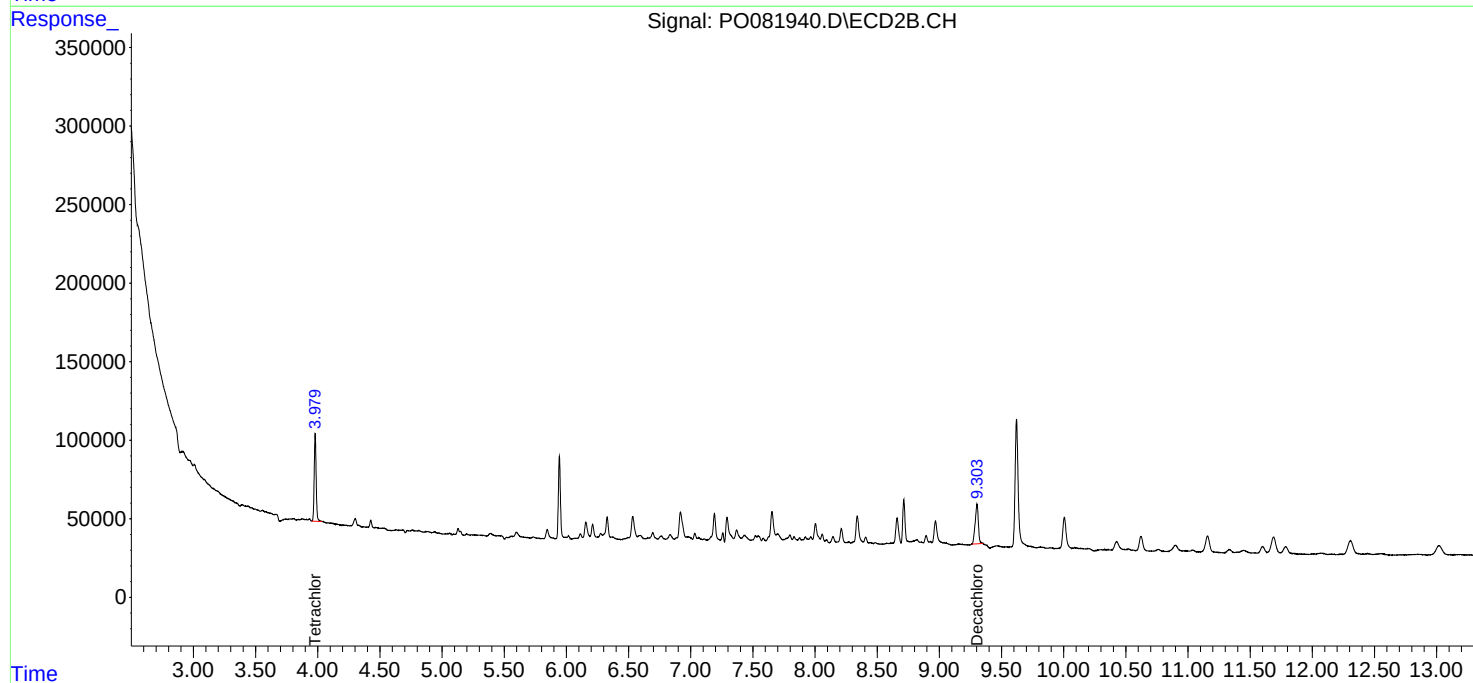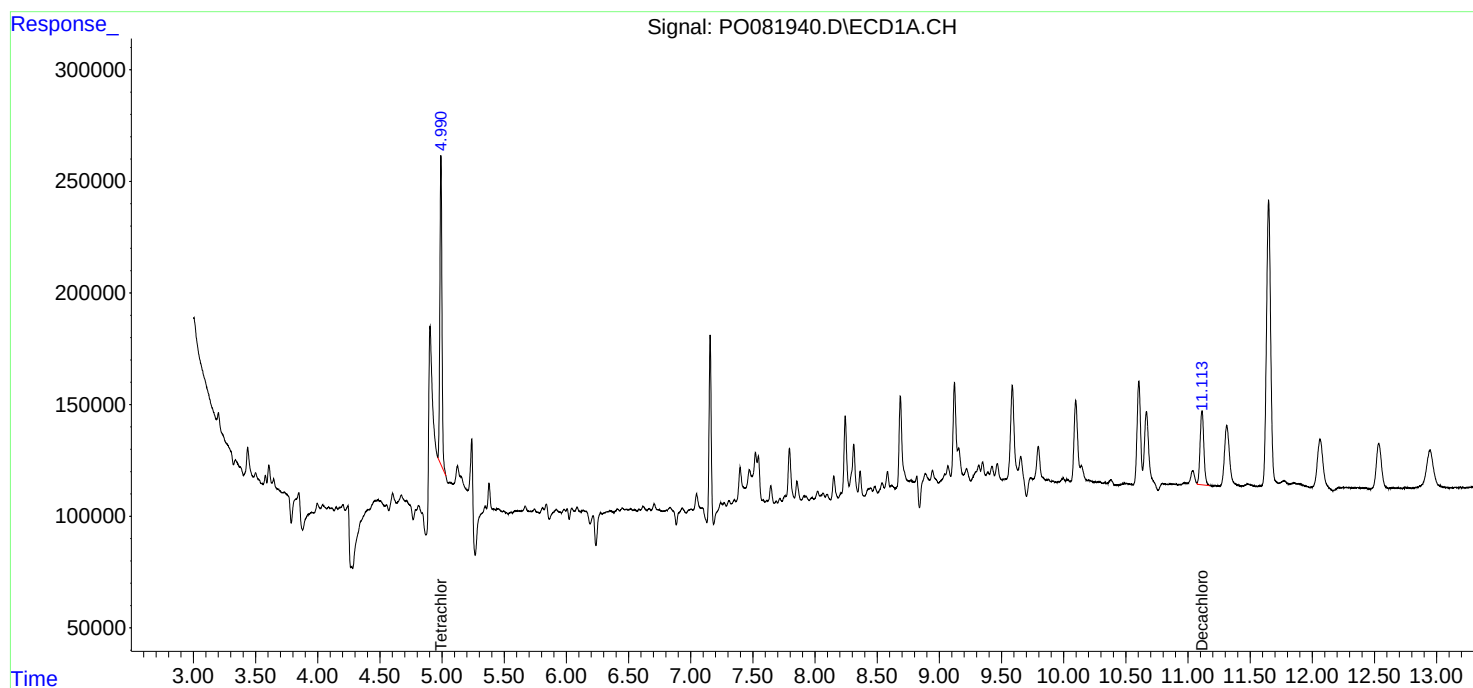

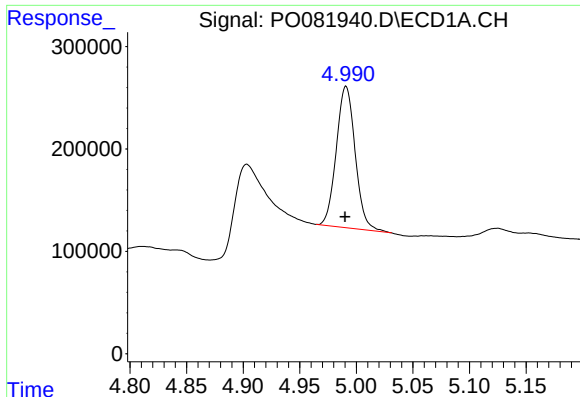


#1 Tetrachloro-m-xylene

R.T.: 4.990 min
Delta R.T.: 0.000 min
Response: 1604507
Conc: 19.34 ng/ml m

Instrument :
ECD_O
ClientSampleId :
IDW-LIQ-DRUM-2-100721


Manual Integrations
APPROVED

mohammad
10/12/2021 9:41:49 AM

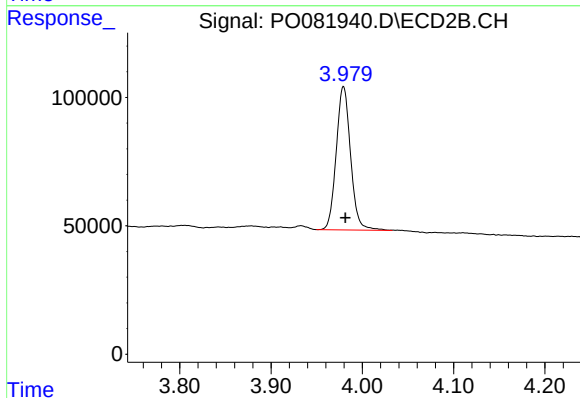


#1 Tetrachloro-m-xylene

R.T.: 3.979 min
Delta R.T.: -0.002 min
Response: 611286
Conc: 24.16 ng/ml m

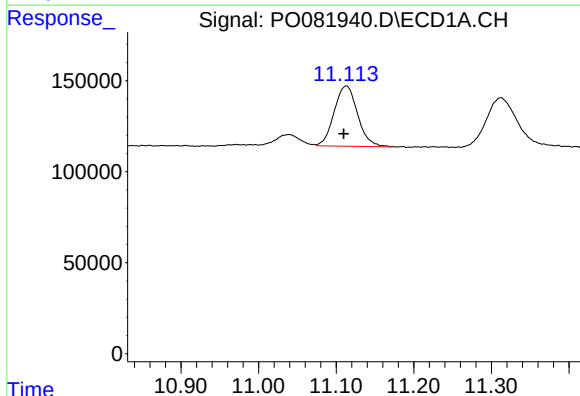

#2 Decachlorobiphenyl

R.T.: 11.113 min
Delta R.T.: 0.003 min
Response: 693321
Conc: 11.69 ng/ml m

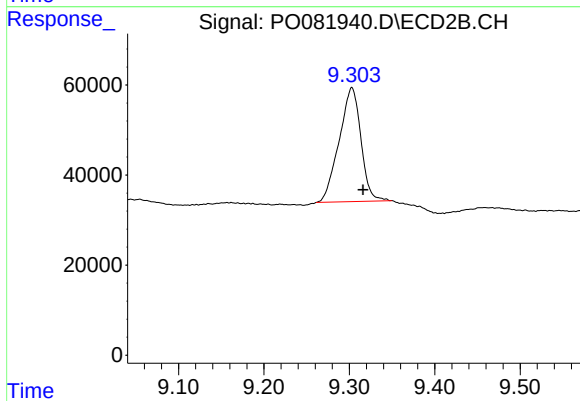

#2 Decachlorobiphenyl

R.T.: 9.303 min
Delta R.T.: -0.013 min
Response: 447891
Conc: 18.96 ng/ml m