

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100920\
 Data File : PO072226.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Oct 2020 1:43
 Operator : DD\AJ
 Sample : L4329-01
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 05:55:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.322	3.507	1646148	827816	22.919	22.101
2)	SA Decachlor...	9.926	8.677	1395737	672742	12.676	11.828
Target Compounds							
29)	L6 AR-1254-4	7.416	6.388	86266	70520	14.807	29.042 #
30)	L6 AR-1254-5	7.832	6.807	113832	91071	21.151	27.833 #
31)	L7 AR-1260-1	0.000	6.266f	0	2872	N.D.	1.122 #
32)	L7 AR-1260-2	7.550	0.000	134603	0	17.971	N.D. #
34)	L7 AR-1260-4	0.000	7.136f	0	4153	N.D.	1.570 #
36)	L8 AR-1262-1	0.000	6.807	0	91071	N.D.	51.423 #
39)	L8 AR-1262-4	0.000	7.697	0	3734	N.D.	0.771 #
42)	L9 AR-1268-2	0.000	7.697f	0	3734	N.D.	0.535 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100920\
Data File : PO072226.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Oct 2020 1:43
Operator : DD\AJ
Sample : L4329-01
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 05:55:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

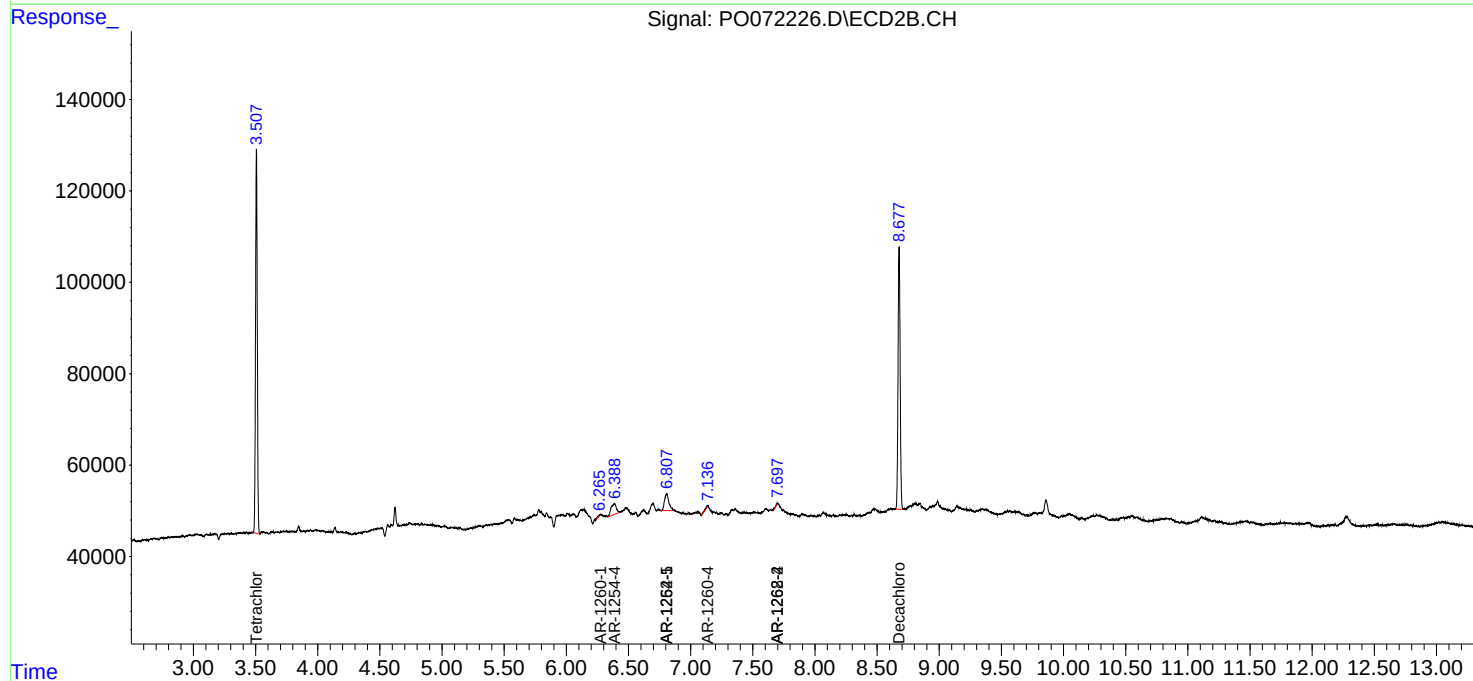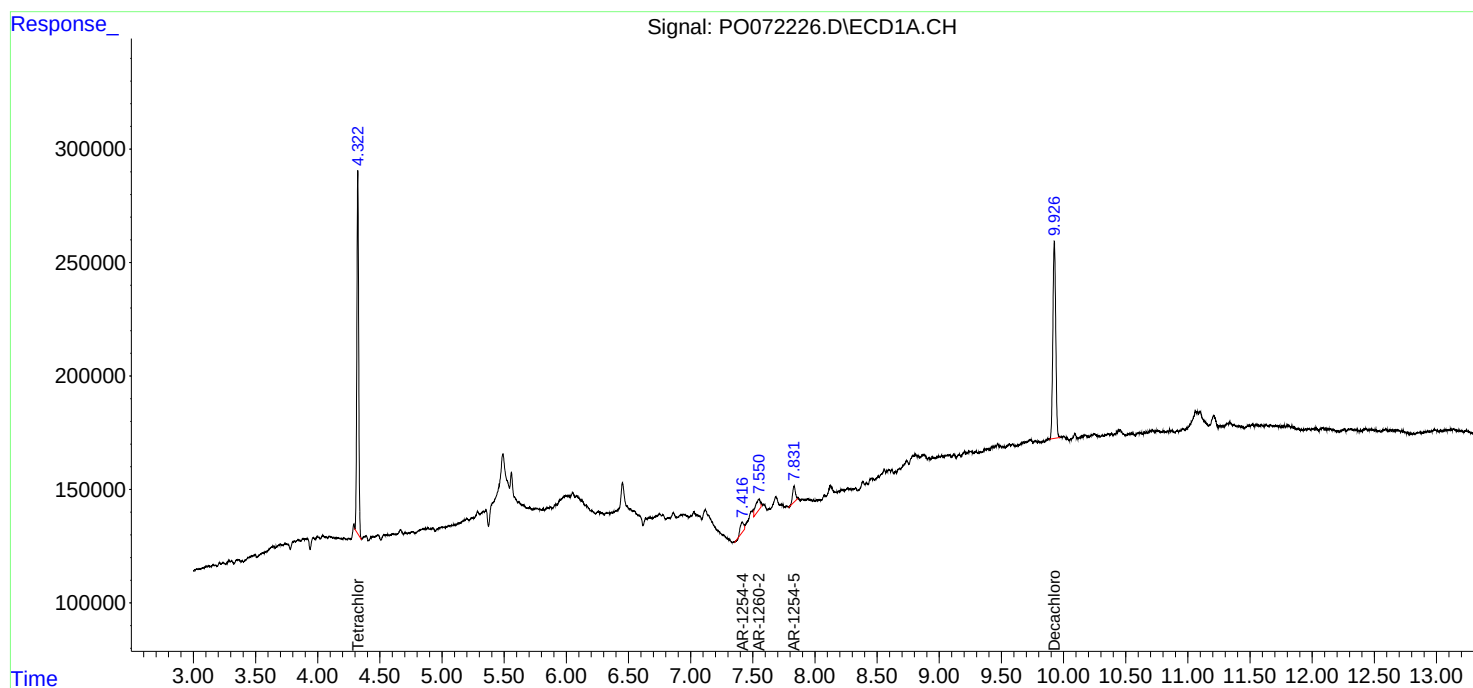


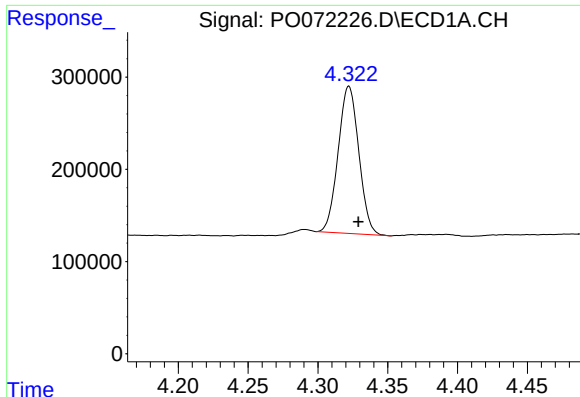

#1 Tetrachloro-m-xylene


R.T.: 4.322 min
Delta R.T.: -0.007 min
Response: 1646148
Conc: 22.92 ng/ml

Instrument :
ECD_O
ClientSampleId :

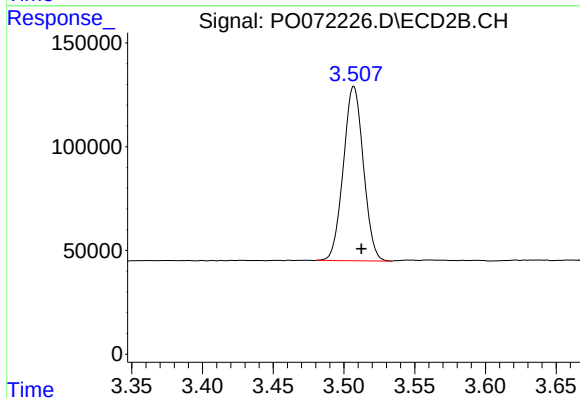


#1 Tetrachloro-m-xylene

R.T.: 3.507 min
Delta R.T.: -0.005 min
Response: 827816
Conc: 22.10 ng/ml

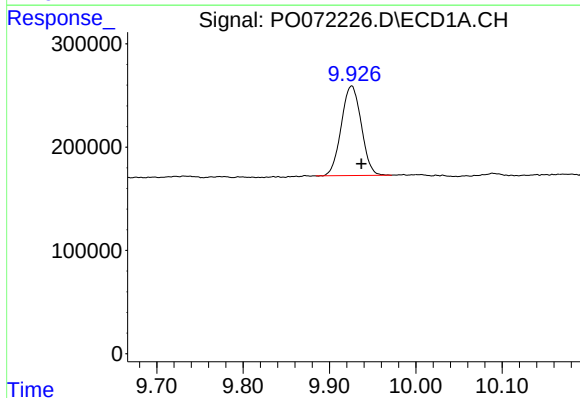


#2 Decachlorobiphenyl

R.T.: 9.926 min
Delta R.T.: -0.011 min
Response: 1395737
Conc: 12.68 ng/ml

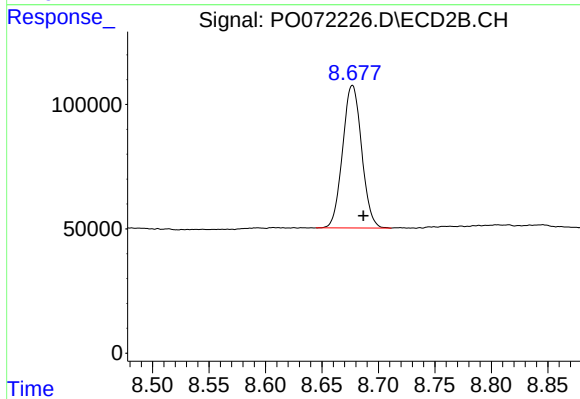

#2 Decachlorobiphenyl


R.T.: 8.677 min
Delta R.T.: -0.010 min
Response: 672742
Conc: 11.83 ng/ml

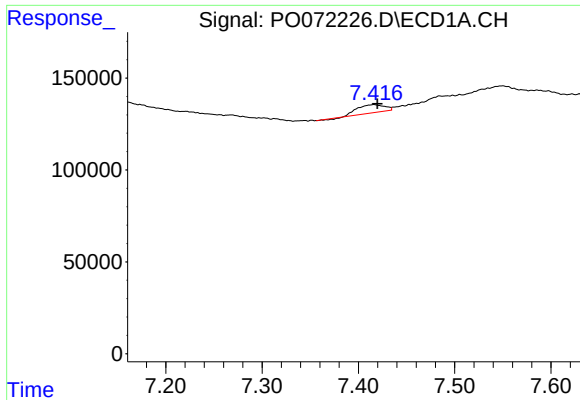

#29 AR-1254-4


R.T.: 7.416 min
Delta R.T.: -0.004 min
Response: 86266
Conc: 14.81 ng/ml

Instrument :
ECD_O
ClientSampleId :

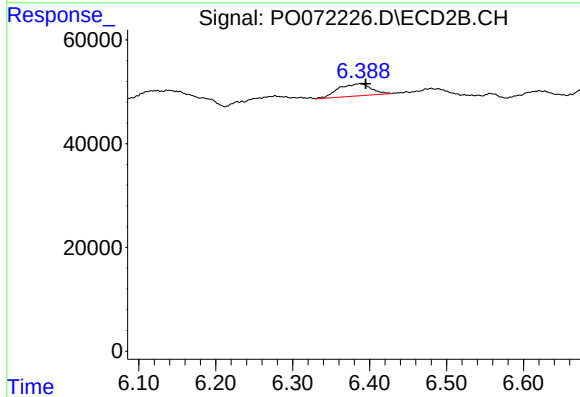


#29 AR-1254-4

R.T.: 6.388 min
Delta R.T.: -0.007 min
Response: 70520
Conc: 29.04 ng/ml

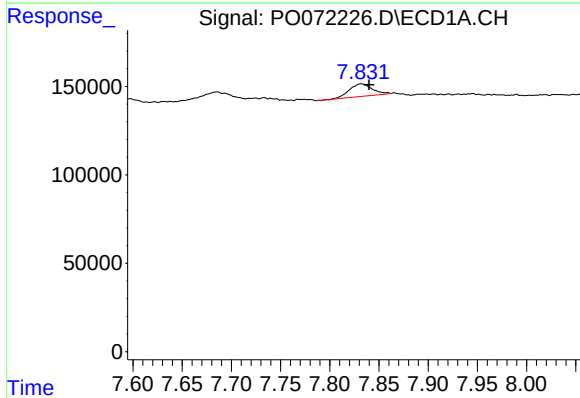


#30 AR-1254-5

R.T.: 7.832 min
Delta R.T.: -0.008 min
Response: 113832
Conc: 21.15 ng/ml

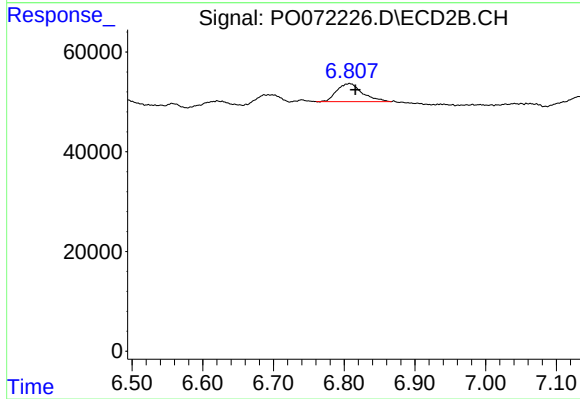

#30 AR-1254-5


R.T.: 6.807 min
Delta R.T.: -0.008 min
Response: 91071
Conc: 27.83 ng/ml

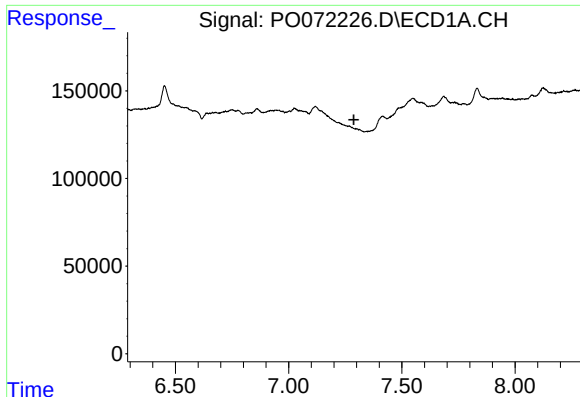

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.288 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

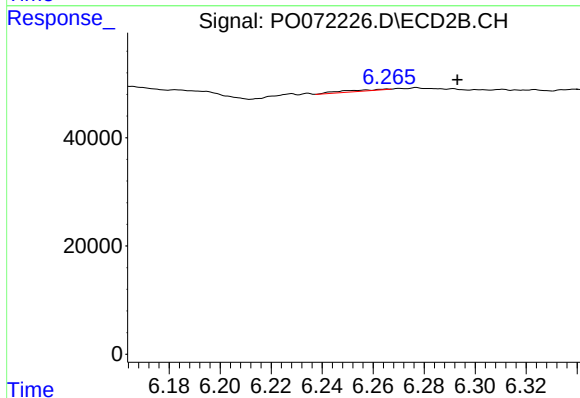


#31 AR-1260-1

R.T.: 6.266 min
Delta R.T.: -0.027 min
Response: 2872
Conc: 1.12 ng/ml

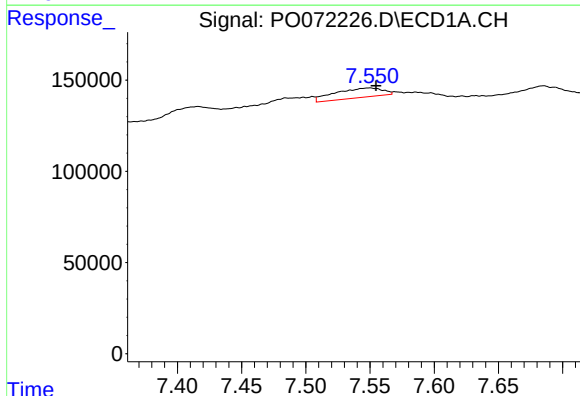


#32 AR-1260-2

R.T.: 7.550 min
Delta R.T.: -0.005 min
Response: 134603
Conc: 17.97 ng/ml

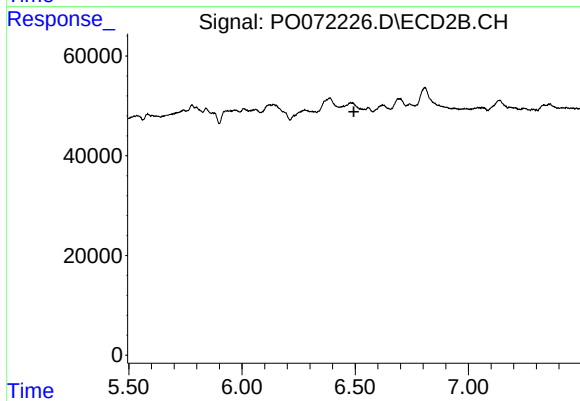

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 6.494 min
Response: 0
Conc: N.D.

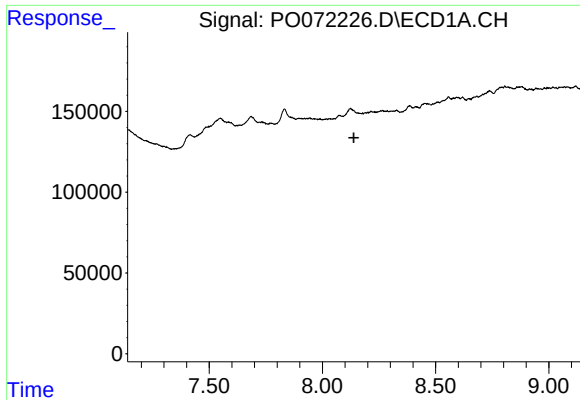

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T.: 8.139 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

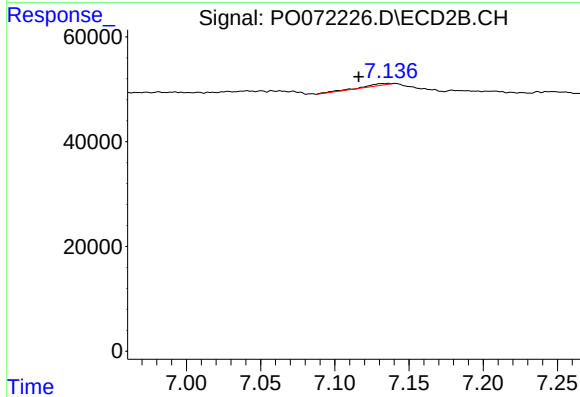


#34 AR-1260-4

R.T.: 7.136 min
Delta R.T.: 0.020 min
Response: 4153
Conc: 1.57 ng/ml

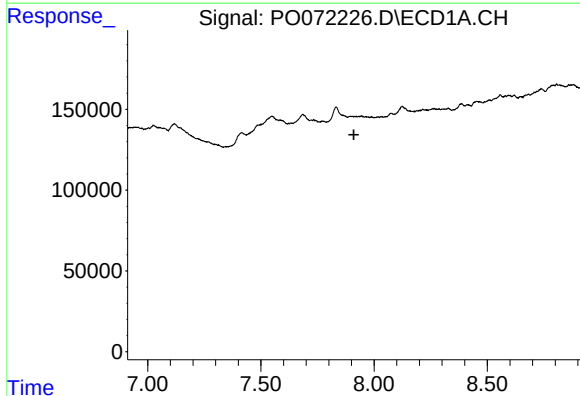


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.911 min
Response: 0
Conc: N.D.

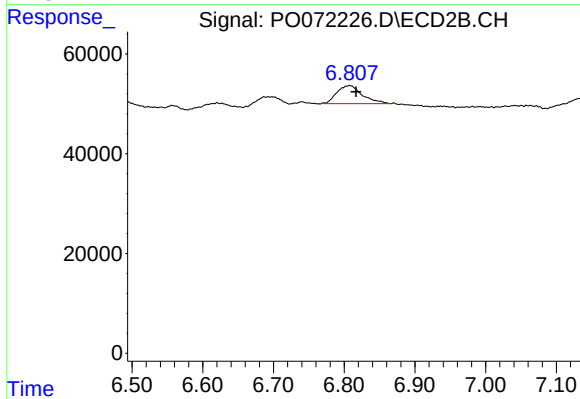

#36 AR-1262-1


R.T.: 6.807 min
Delta R.T.: -0.009 min
Response: 91071
Conc: 51.42 ng/ml

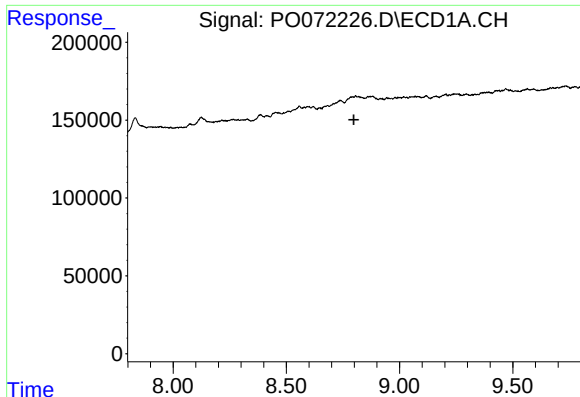

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 8.798 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

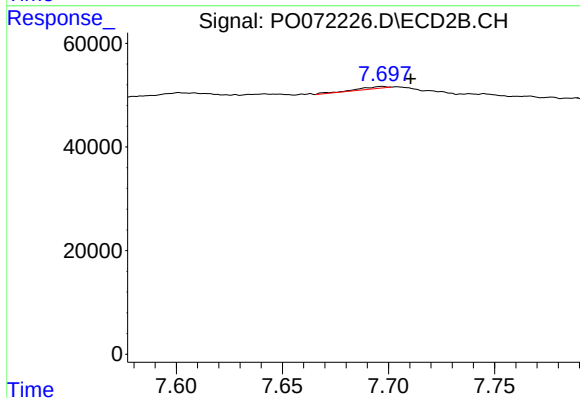


#39 AR-1262-4

R.T.: 7.697 min
Delta R.T.: -0.013 min
Response: 3734
Conc: 0.77 ng/ml

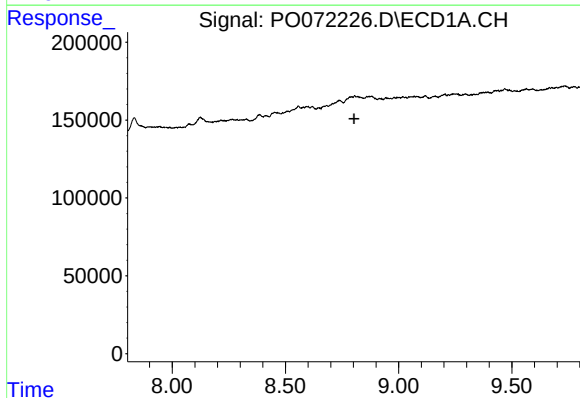

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.803 min
Response: 0
Conc: N.D.

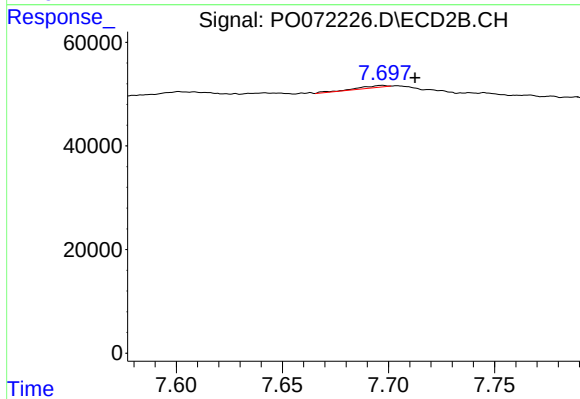

#42 AR-1268-2

R.T.: 7.697 min
Delta R.T.: -0.015 min
Response: 3734
Conc: 0.53 ng/ml