

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100920\
 Data File : PO072197.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Oct 2020 17:10
 Operator : DD\AJ
 Sample : L4309-04
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OWLS-HEAD-BH-04-B

Manual Integrations
 APPROVED

Ankita
 10/13/2020 9:41:13 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 18:14:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.322	3.507	1723073	806066	23.990	21.520
2) SA Decachlor...	9.926	8.676	2235143	1117081	20.300m	19.639m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100920\
Data File : PO072197.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Oct 2020 17:10
Operator : DD\AJ
Sample : L4309-04
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OWLS-HEAD-BH-04-B


Manual Integrations
APPROVED

Ankita
10/13/2020 9:41:13 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 18:14:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

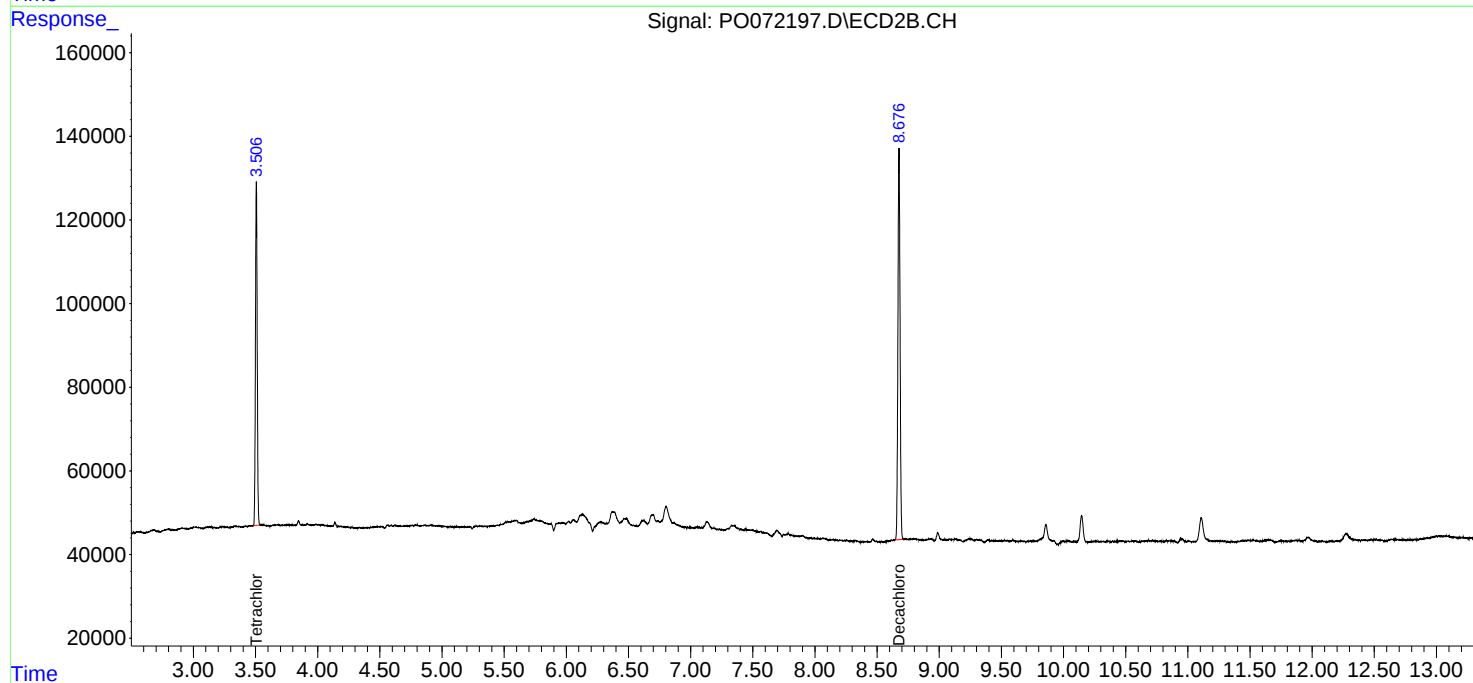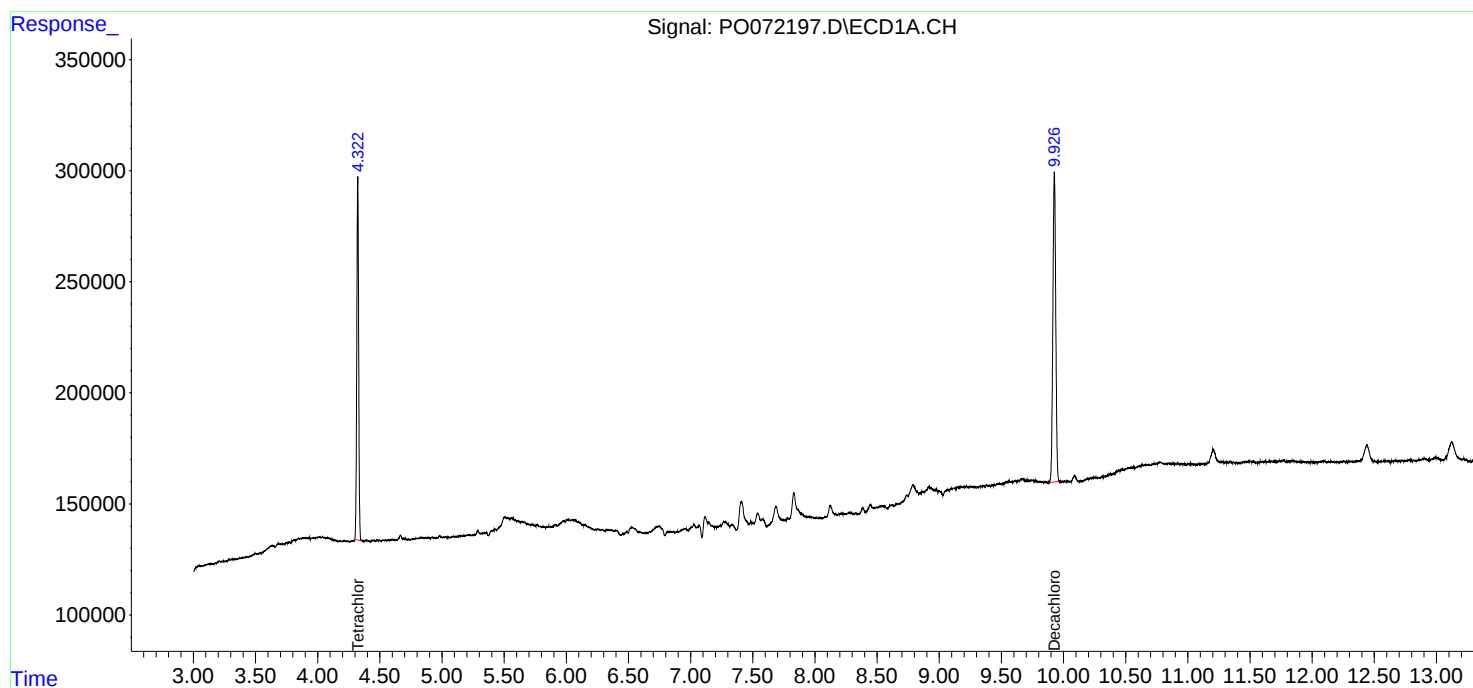

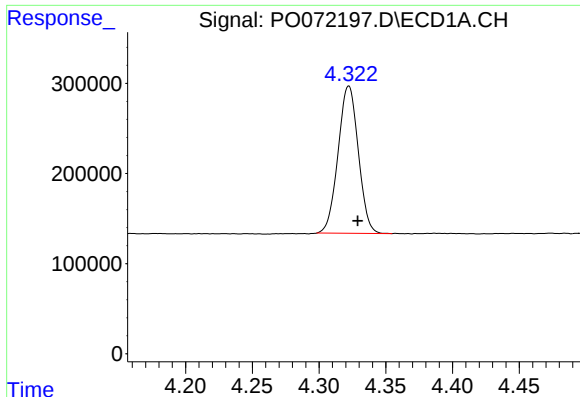


#1 Tetrachloro-m-xylene

R.T.: 4.322 min
Delta R.T.: -0.007 min
Response: 1723073
Conc: 23.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
OWLS-HEAD-BH-04-B


Manual Integrations
APPROVED

Ankita
10/13/2020 9:41:13 AM

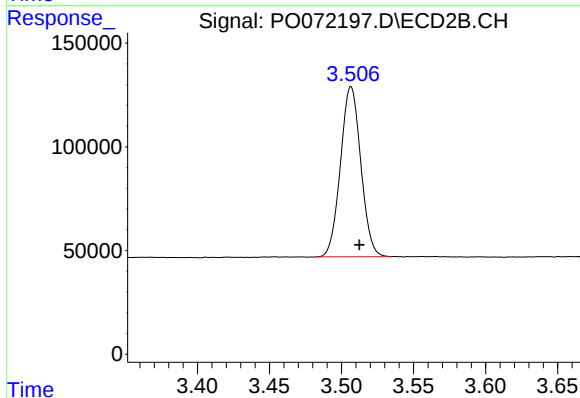


#1 Tetrachloro-m-xylene

R.T.: 3.507 min
Delta R.T.: -0.006 min
Response: 806066
Conc: 21.52 ng/ml

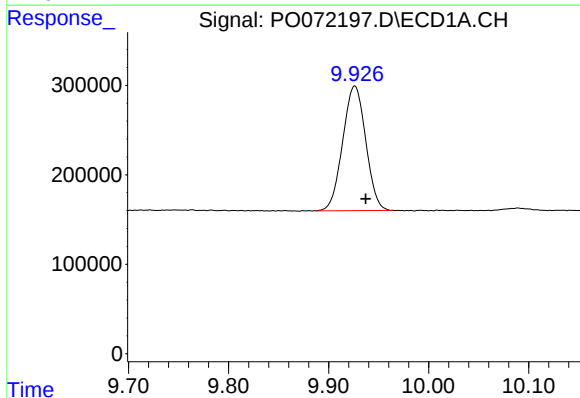

#2 Decachlorobiphenyl

R.T.: 9.926 min
Delta R.T.: -0.011 min
Response: 2235143
Conc: 20.30 ng/ml m

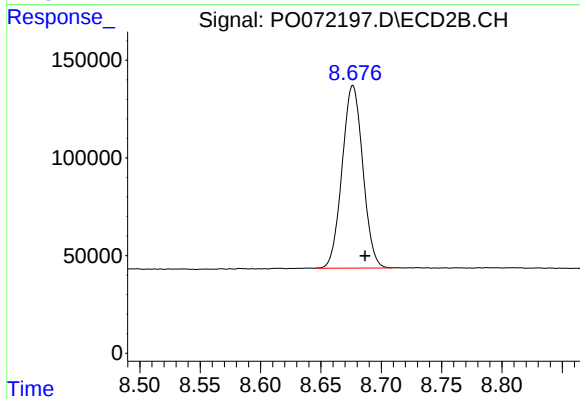

#2 Decachlorobiphenyl

R.T.: 8.676 min
Delta R.T.: -0.010 min
Response: 1117081
Conc: 19.64 ng/ml m