

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100920\
 Data File : PO072200.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Oct 2020 18:01
 Operator : DD\AJ
 Sample : L4316-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 11929

Manual Integrations
 APPROVED

Ankita
 10/13/2020 9:41:19 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 18:43:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.323	3.508	1766452	839062	24.594	22.401
2) SA Decachlor...	9.928	8.677	2237011	1140646	20.317	20.054m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100920\
Data File : PO072200.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Oct 2020 18:01
Operator : DD\AJ
Sample : L4316-01
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
11929


Manual Integrations
APPROVED

Ankita
10/13/2020 9:41:19 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 18:43:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

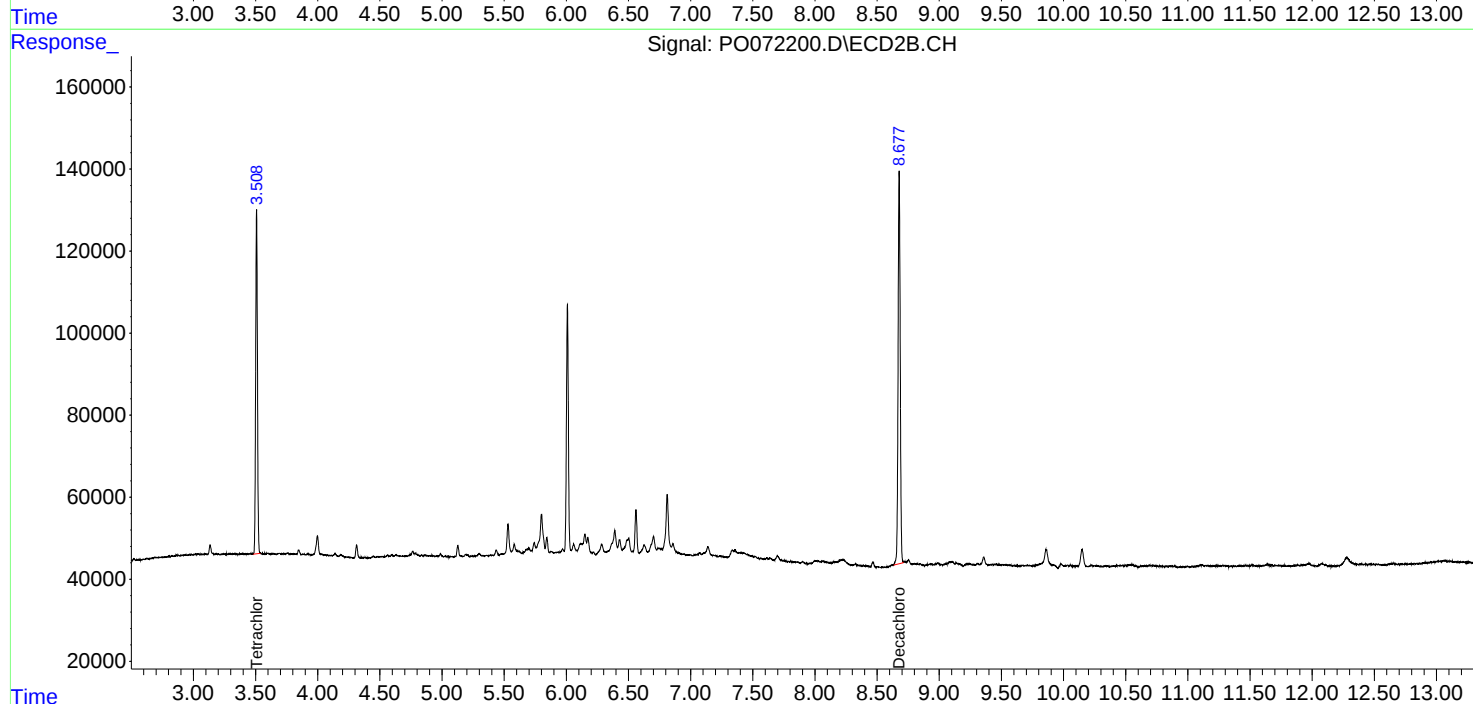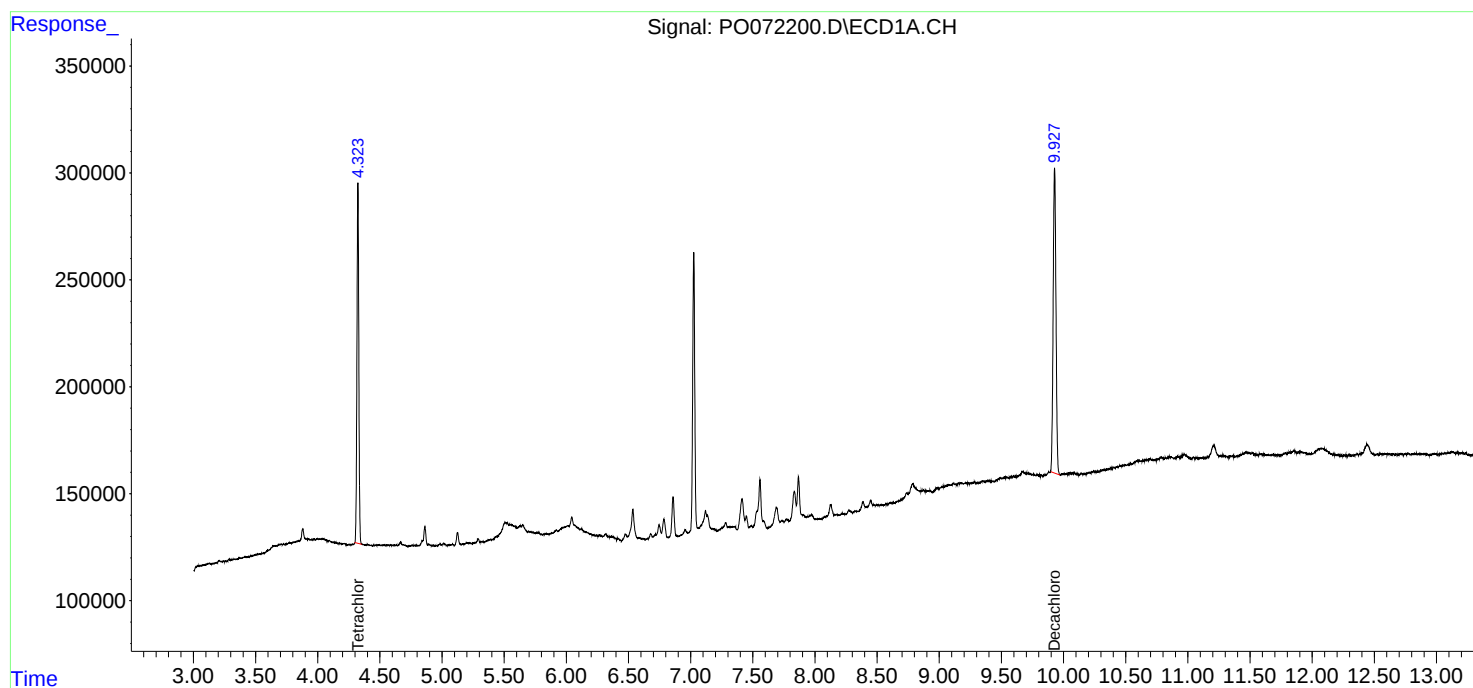

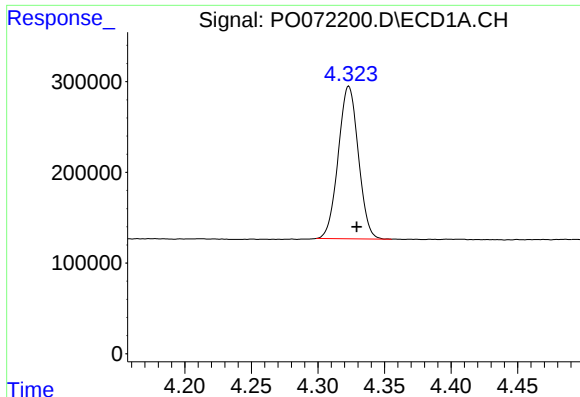


#1 Tetrachloro-m-xylene

R.T.: 4.323 min
Delta R.T.: -0.006 min
Response: 1766452
Conc: 24.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
11929


Manual Integrations
APPROVED

Ankita
10/13/2020 9:41:19 AM

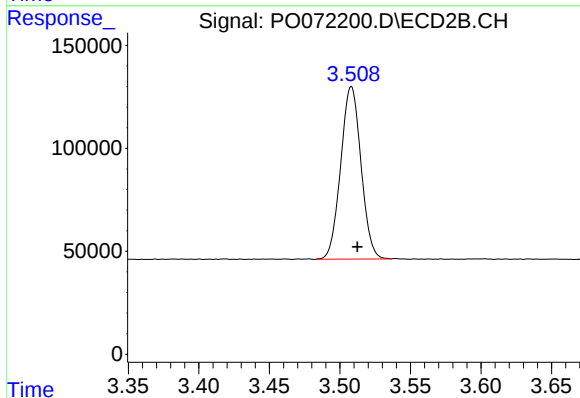


#1 Tetrachloro-m-xylene

R.T.: 3.508 min
Delta R.T.: -0.004 min
Response: 839062
Conc: 22.40 ng/ml

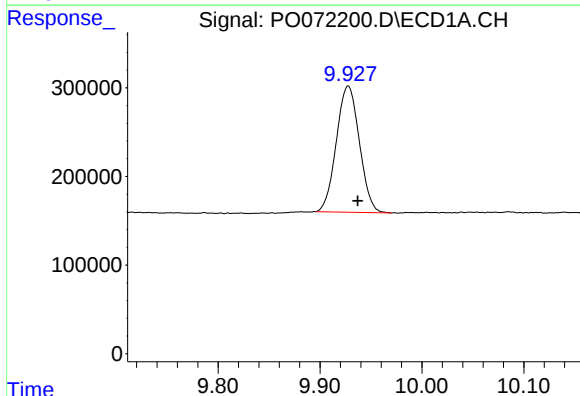

#2 Decachlorobiphenyl

R.T.: 9.928 min
Delta R.T.: -0.009 min
Response: 2237011
Conc: 20.32 ng/ml

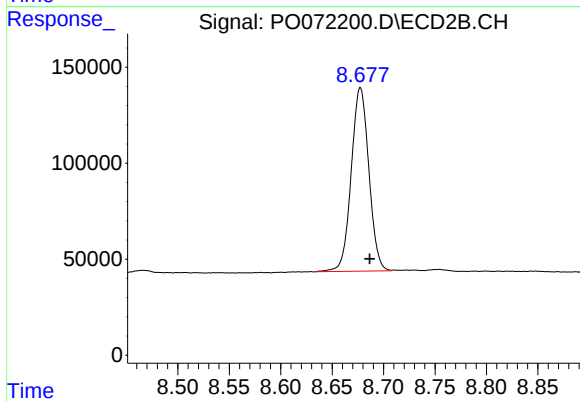

#2 Decachlorobiphenyl

R.T.: 8.677 min
Delta R.T.: -0.010 min
Response: 1140646
Conc: 20.05 ng/ml m