

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100920\
 Data File : PO072204.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Oct 2020 19:09
 Operator : DD\AJ
 Sample : L4318-01
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 214

Manual Integrations
 APPROVED

Ankita
 10/13/2020 9:41:22 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 00:54:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.322	3.507	1433404	684118	19.957	18.264
2) SA Decachlor...	9.926	8.677	2024482	971661	18.387	17.083
Target Compounds						
26) L6 AR-1254-1	6.516	5.580	131360	90966	37.599m	38.064
27) L6 AR-1254-2	6.742	5.740	285328	89389	51.826	41.791
28) L6 AR-1254-3	7.118	6.149	358642	170872	62.101	50.328
29) L6 AR-1254-4	7.413	6.389	490308	197603	84.159	81.379
30) L6 AR-1254-5	7.832	6.810	402824	260698	74.848m	79.673

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100920\
Data File : PO072204.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Oct 2020 19:09
Operator : DD\AJ
Sample : L4318-01
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
214


Manual Integrations
APPROVED

Ankita
10/13/2020 9:41:22 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 00:54:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

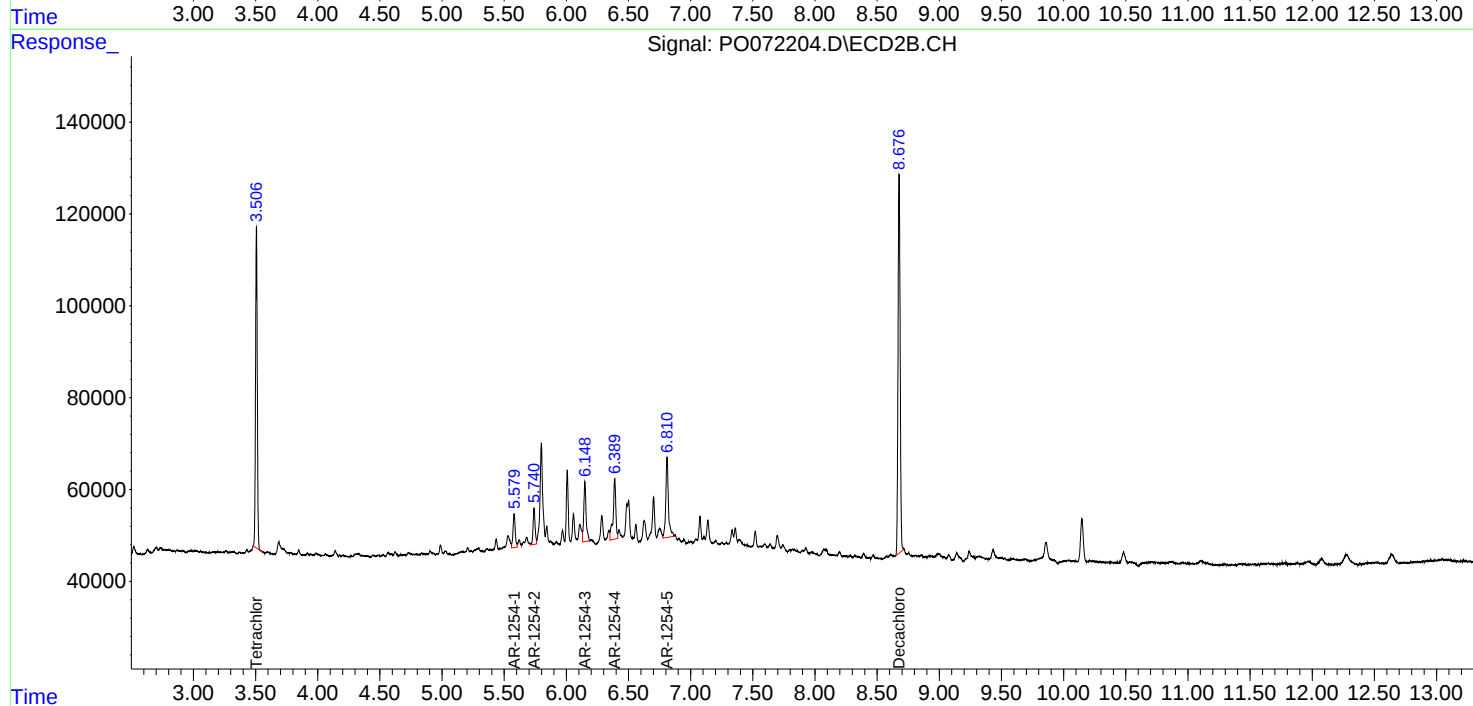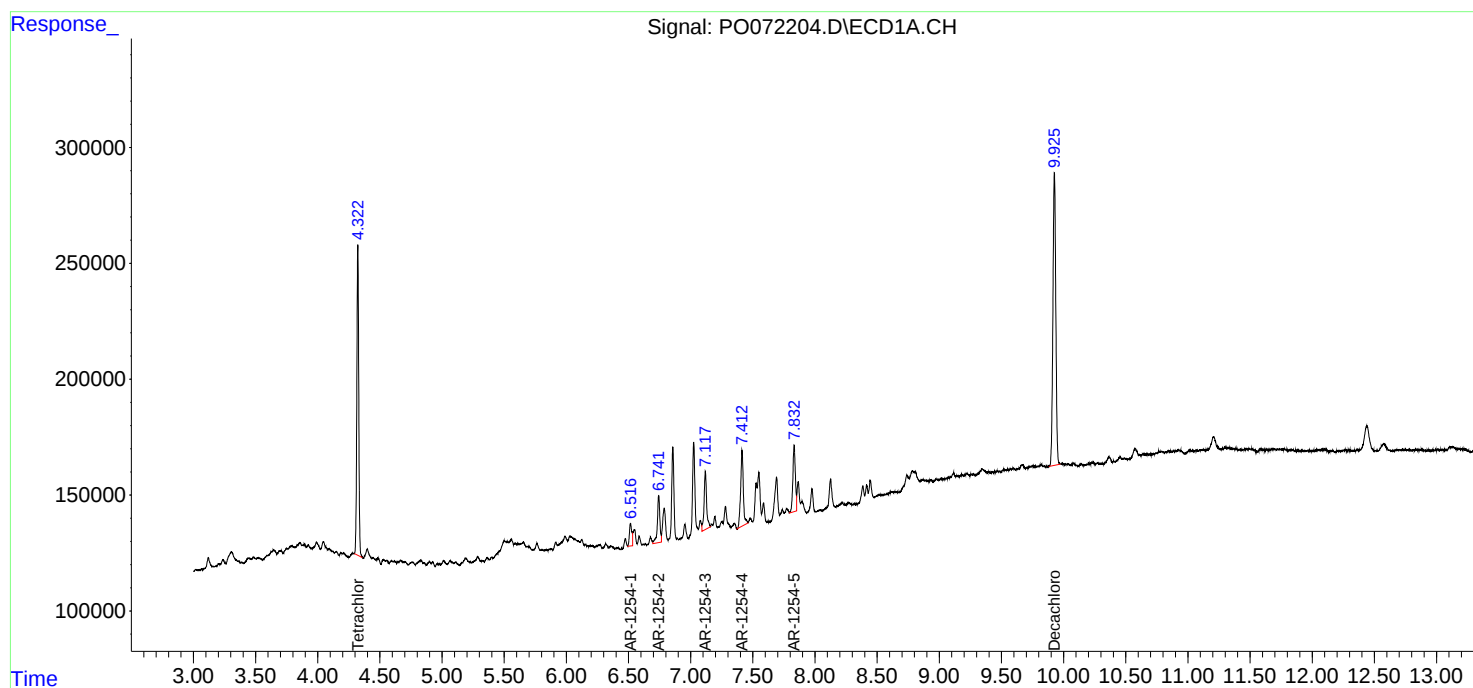

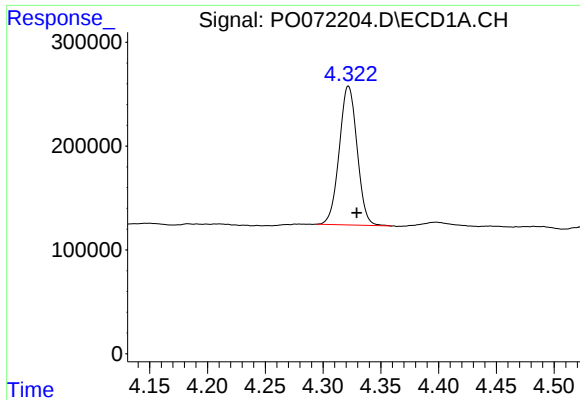


#1 Tetrachloro-m-xylene

R.T.: 4.322 min
Delta R.T.: -0.007 min
Response: 1433404
Conc: 19.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
214


Manual Integrations
APPROVED

Ankita
10/13/2020 9:41:22 AM

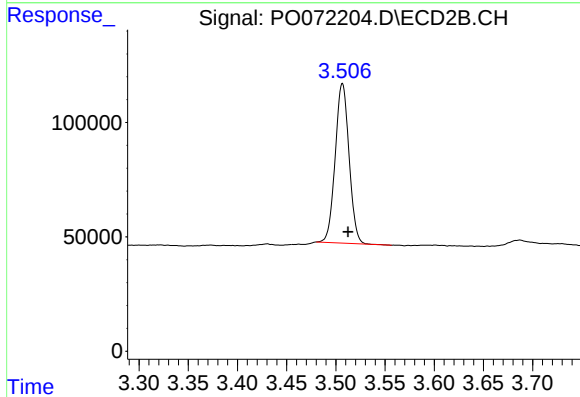


#1 Tetrachloro-m-xylene

R.T.: 3.507 min
Delta R.T.: -0.006 min
Response: 684118
Conc: 18.26 ng/ml

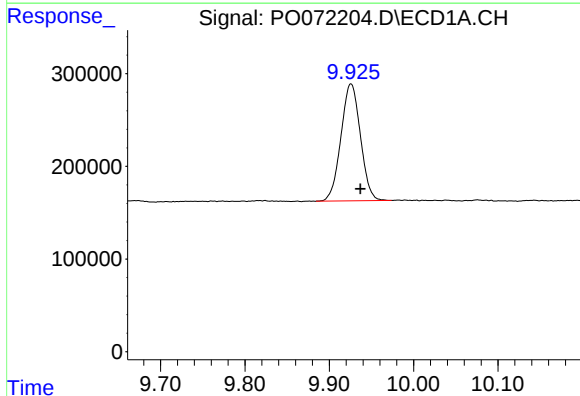


#2 Decachlorobiphenyl

R.T.: 9.926 min
Delta R.T.: -0.011 min
Response: 2024482
Conc: 18.39 ng/ml

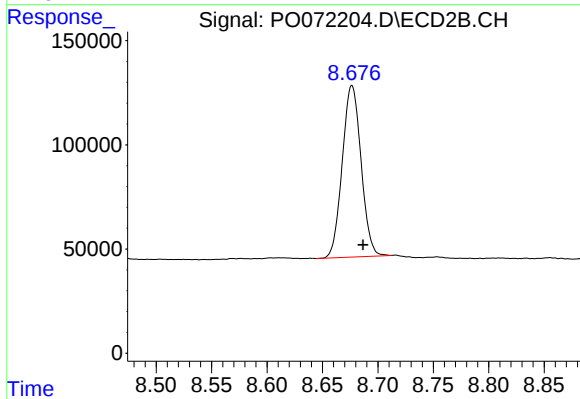

#2 Decachlorobiphenyl

R.T.: 8.677 min
Delta R.T.: -0.010 min
Response: 971661
Conc: 17.08 ng/ml

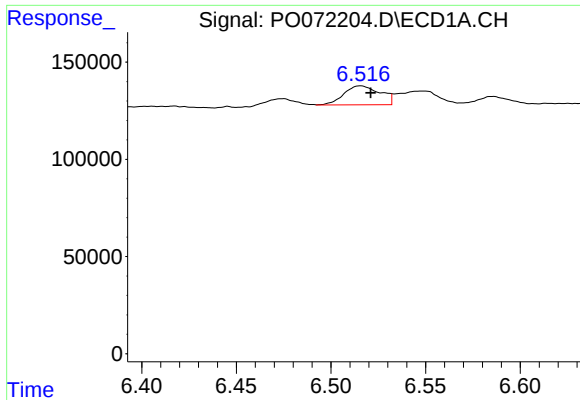


#26 AR-1254-1

R.T.: 6.516 min
Delta R.T.: -0.005 min
Response: 131360
Conc: 37.60 ng/ml m

Instrument :
ECD_O
ClientSampleId :
214


Manual Integrations
APPROVED

Ankita
10/13/2020 9:41:22 AM

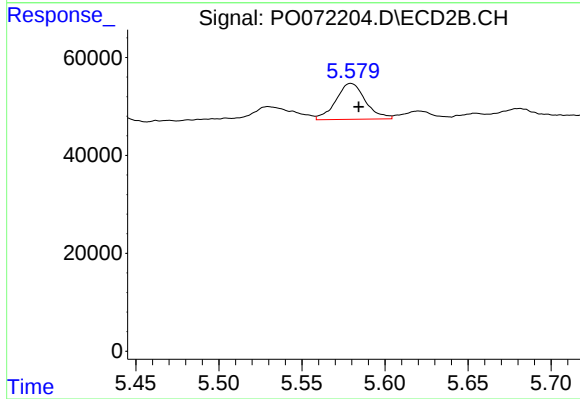


#26 AR-1254-1

R.T.: 5.580 min
Delta R.T.: -0.005 min
Response: 90966
Conc: 38.06 ng/ml

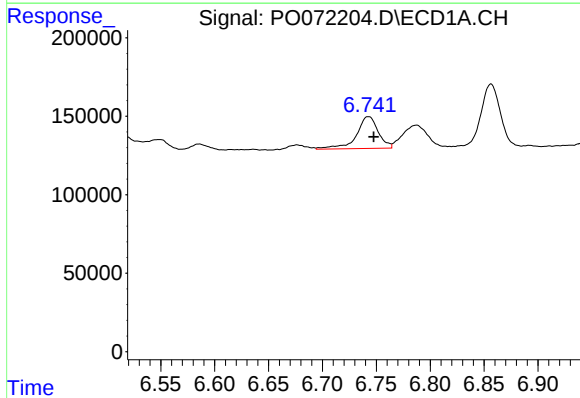


#27 AR-1254-2

R.T.: 6.742 min
Delta R.T.: -0.006 min
Response: 285328
Conc: 51.83 ng/ml

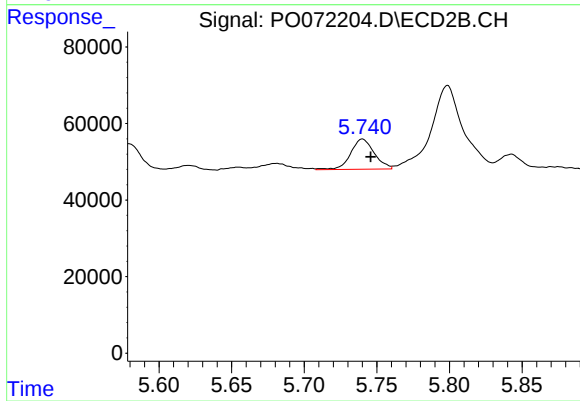

#27 AR-1254-2

R.T.: 5.740 min
Delta R.T.: -0.006 min
Response: 89389
Conc: 41.79 ng/ml

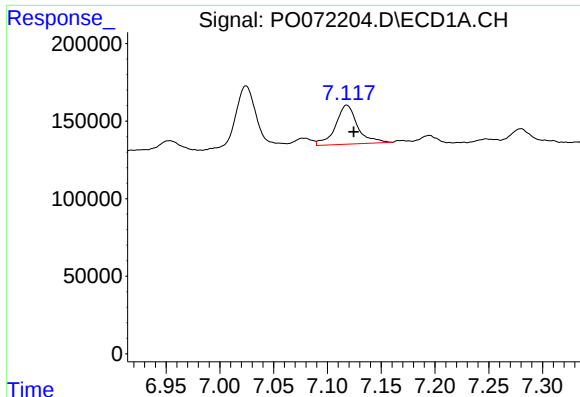


#28 AR-1254-3

R.T.: 7.118 min
Delta R.T.: -0.007 min
Response: 358642
Conc: 62.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
214


Manual Integrations
APPROVED

Ankita
10/13/2020 9:41:22 AM

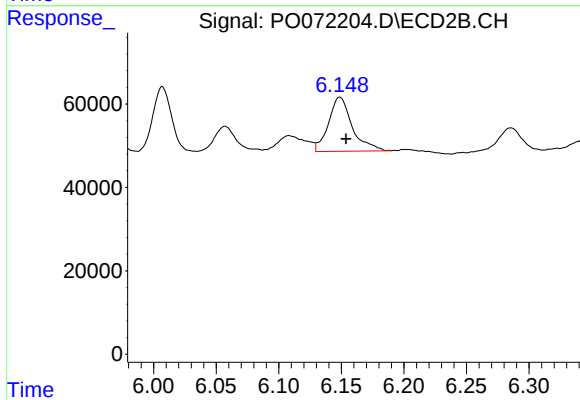


#28 AR-1254-3

R.T.: 6.149 min
Delta R.T.: -0.005 min
Response: 170872
Conc: 50.33 ng/ml

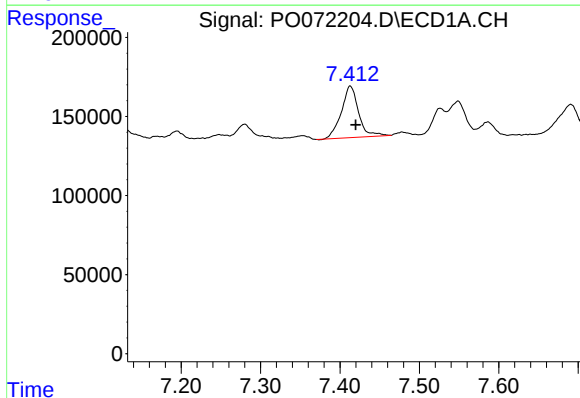


#29 AR-1254-4

R.T.: 7.413 min
Delta R.T.: -0.007 min
Response: 490308
Conc: 84.16 ng/ml

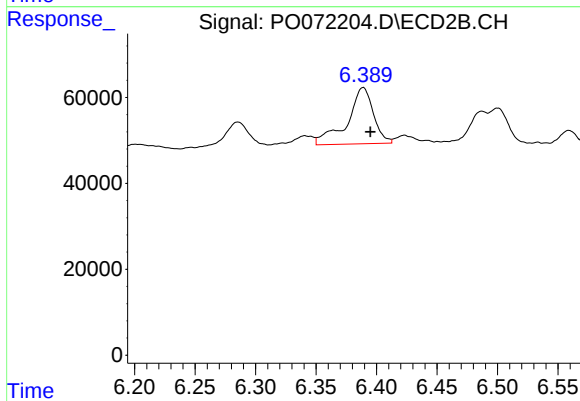

#29 AR-1254-4

R.T.: 6.389 min
Delta R.T.: -0.006 min
Response: 197603
Conc: 81.38 ng/ml

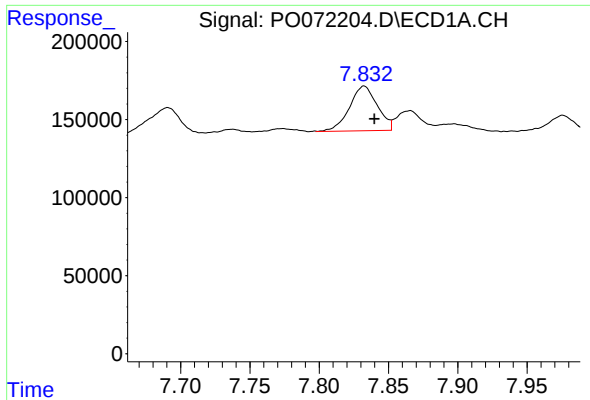


#30 AR-1254-5

R.T.: 7.832 min
Delta R.T.: -0.008 min
Response: 402824
Conc: 74.85 ng/ml m

Instrument :
ECD_O
ClientSampleId :
214

Manual Integrations
APPROVED

Ankita
10/13/2020 9:41:22 AM

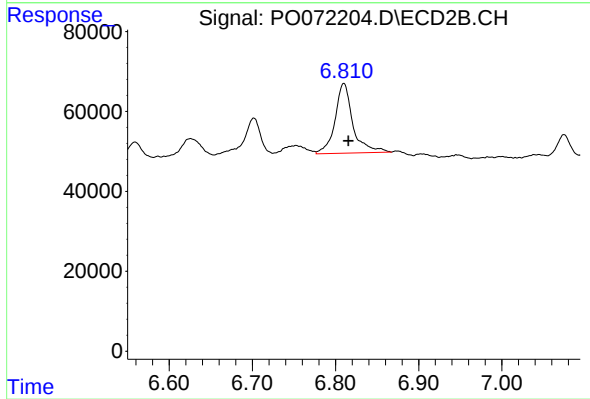

#30 AR-1254-5

R.T.: 6.810 min
Delta R.T.: -0.005 min
Response: 260698
Conc: 79.67 ng/ml