

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100920\
 Data File : PO072221.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Oct 2020 00:18
 Operator : DD\AJ
 Sample : L4300-01
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 231-232-COMP

Manual Integrations
 APPROVED

Ankita
 10/13/2020 9:42:29 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 01:02:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.325	3.510	1164415	625142	16.212	16.690
2) SA Decachlor...	9.928	8.679	1673315	878095	15.197	15.438
Target Compounds						
31) L7 AR-1260-1	7.283	6.288	178446	97127	37.233	37.934
32) L7 AR-1260-2	7.548	6.488	339330	148783	45.303	46.508
33) L7 AR-1260-3	7.906	6.634	198242	114851	31.095	38.916 #
34) L7 AR-1260-4	8.133	7.109	249066	86821	41.493	32.814m
35) L7 AR-1260-5	8.448	7.362	443774	223580	32.025	33.652

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100920\
Data File : PO072221.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Oct 2020 00:18
Operator : DD\AJ
Sample : L4300-01
Misc :
ALS Vial : 53 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
231-232-COMP


Manual Integrations
APPROVED

Ankita
10/13/2020 9:42:29 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 01:02:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

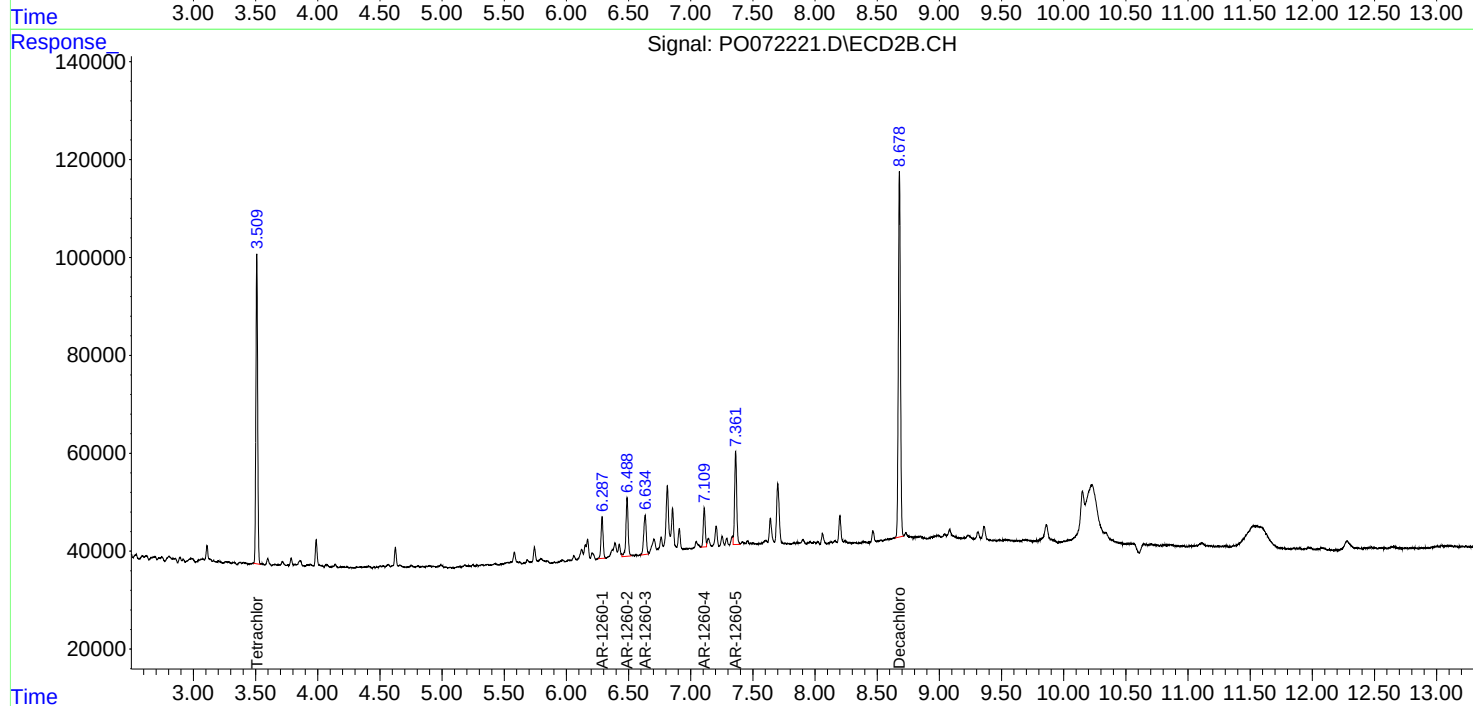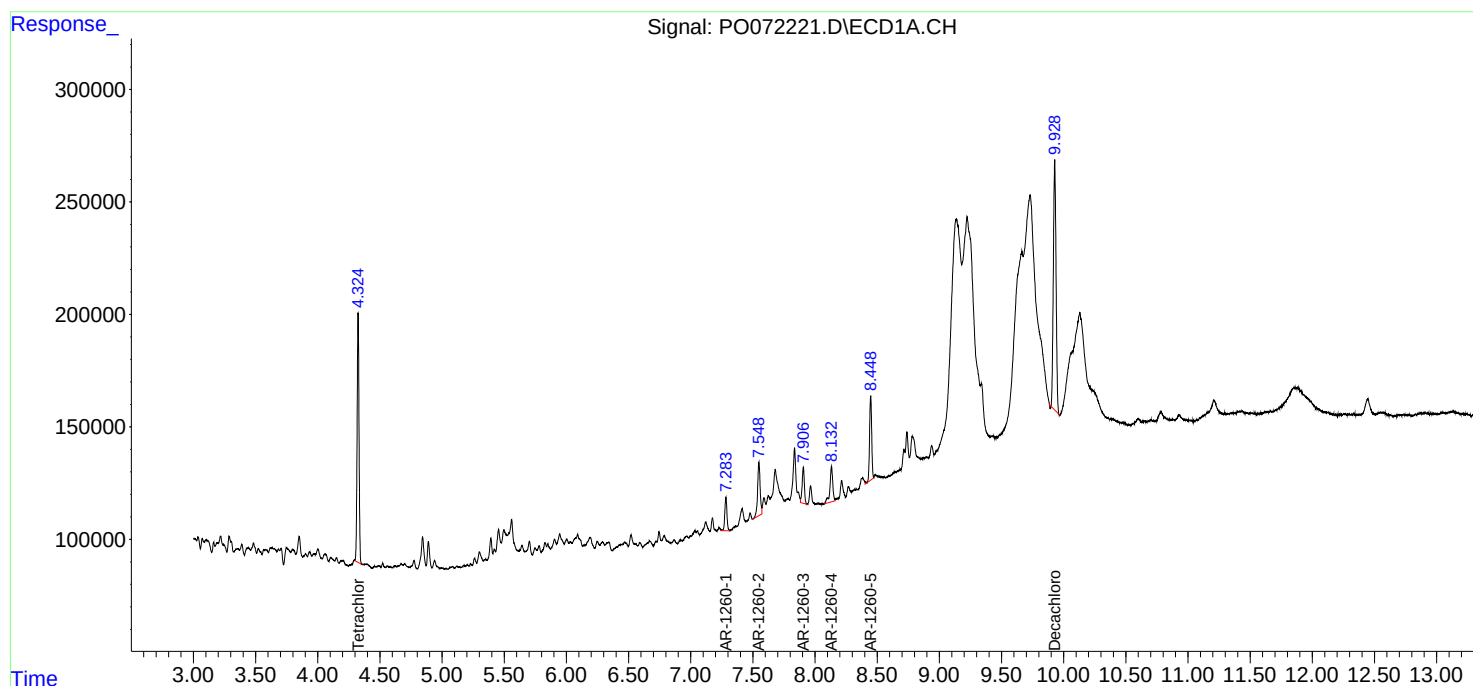

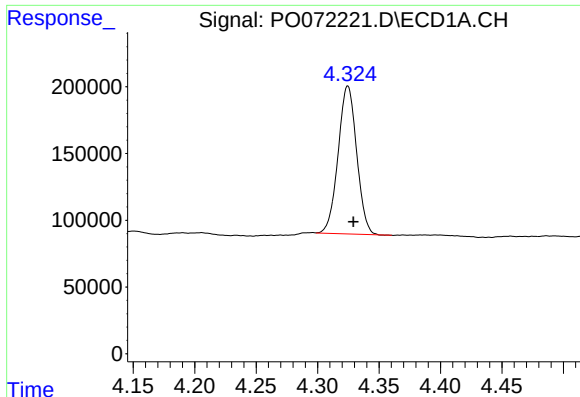


#1 Tetrachloro-m-xylene

R.T.: 4.325 min
Delta R.T.: -0.004 min
Response: 1164415
Conc: 16.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
231-232-COMP


Manual Integrations
APPROVED

Ankita
10/13/2020 9:42:29 AM

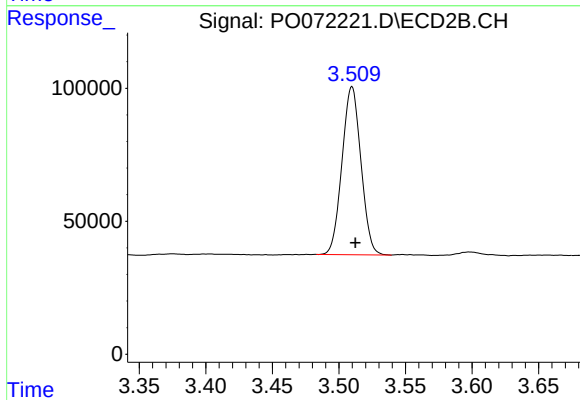


#1 Tetrachloro-m-xylene

R.T.: 3.510 min
Delta R.T.: -0.003 min
Response: 625142
Conc: 16.69 ng/ml

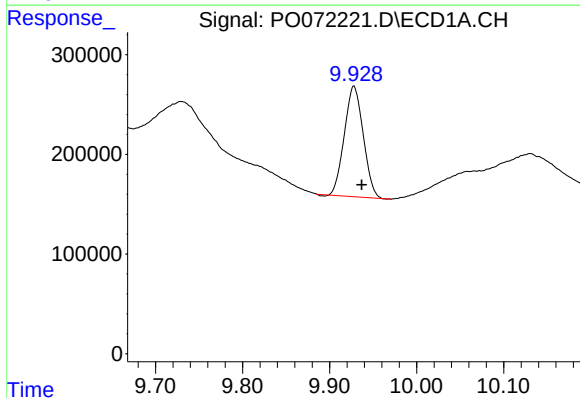


#2 Decachlorobiphenyl

R.T.: 9.928 min
Delta R.T.: -0.009 min
Response: 1673315
Conc: 15.20 ng/ml

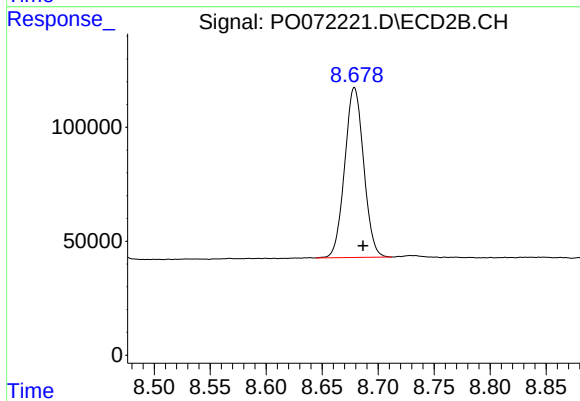

#2 Decachlorobiphenyl

R.T.: 8.679 min
Delta R.T.: -0.008 min
Response: 878095
Conc: 15.44 ng/ml

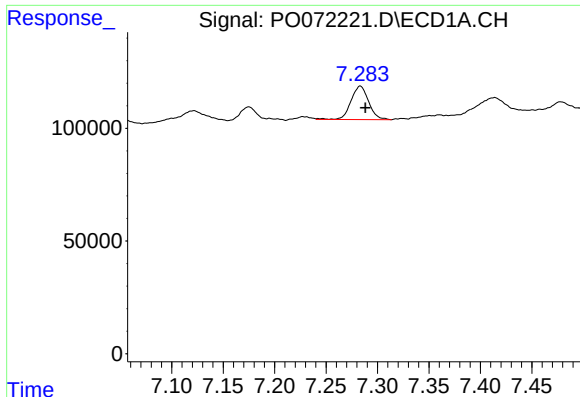


#31 AR-1260-1

R.T.: 7.283 min
Delta R.T.: -0.005 min
Response: 178446
Conc: 37.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
231-232-COMP


Manual Integrations
APPROVED

Ankita
10/13/2020 9:42:29 AM

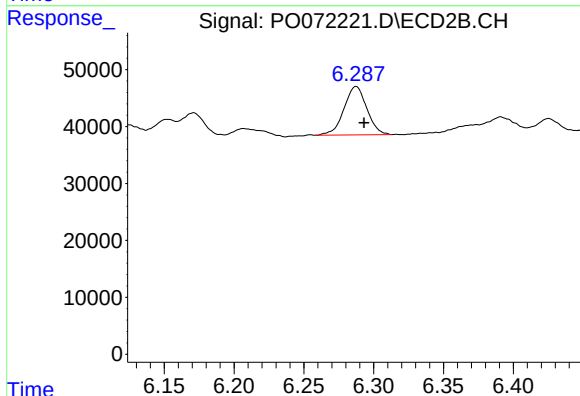


#31 AR-1260-1

R.T.: 6.288 min
Delta R.T.: -0.006 min
Response: 97127
Conc: 37.93 ng/ml

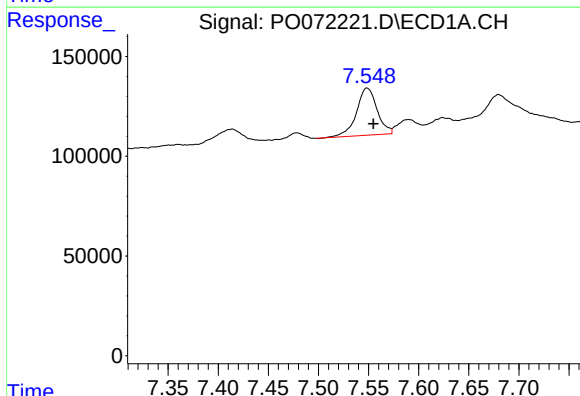


#32 AR-1260-2

R.T.: 7.548 min
Delta R.T.: -0.006 min
Response: 339330
Conc: 45.30 ng/ml

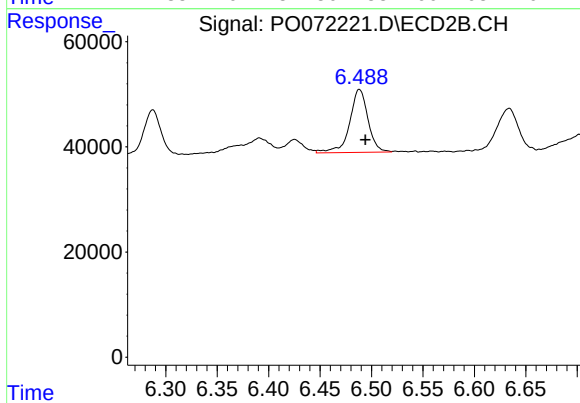

#32 AR-1260-2

R.T.: 6.488 min
Delta R.T.: -0.006 min
Response: 148783
Conc: 46.51 ng/ml

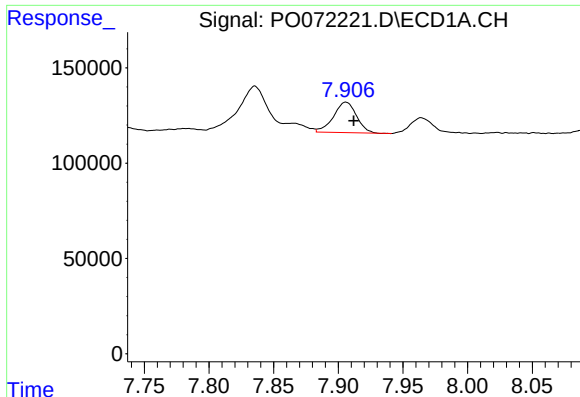


#33 AR-1260-3

R.T.: 7.906 min
Delta R.T.: -0.006 min
Response: 198242
Conc: 31.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
231-232-COMP


Manual Integrations
APPROVED

Ankita
10/13/2020 9:42:29 AM

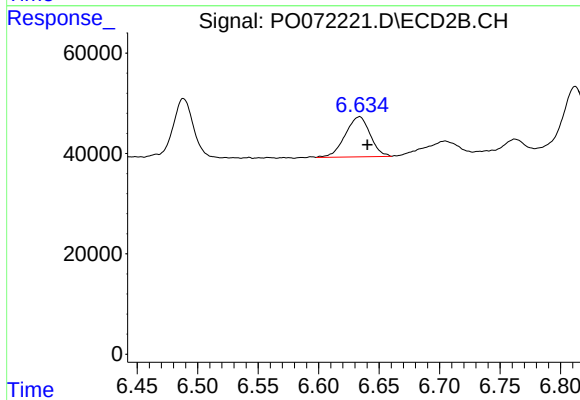


#33 AR-1260-3

R.T.: 6.634 min
Delta R.T.: -0.006 min
Response: 114851
Conc: 38.92 ng/ml

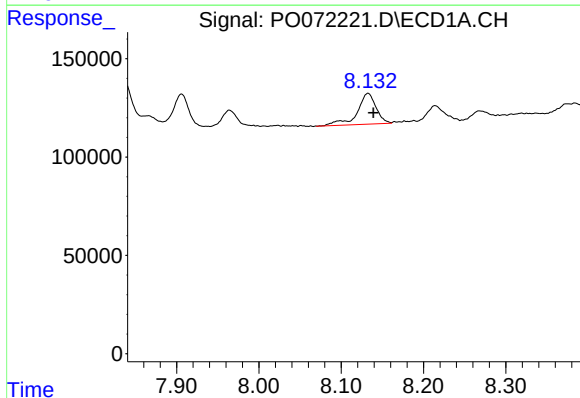


#34 AR-1260-4

R.T.: 8.133 min
Delta R.T.: -0.006 min
Response: 249066
Conc: 41.49 ng/ml

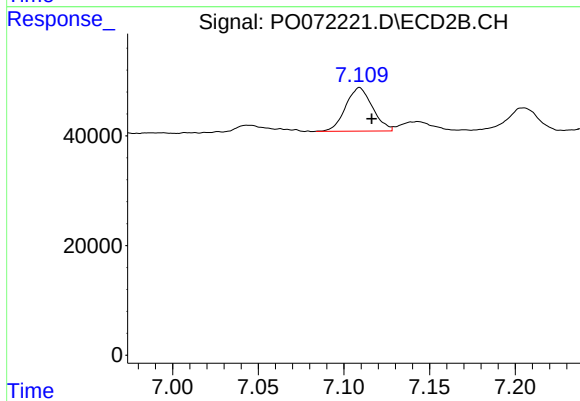

#34 AR-1260-4

R.T.: 7.109 min
Delta R.T.: -0.007 min
Response: 86821
Conc: 32.81 ng/ml m

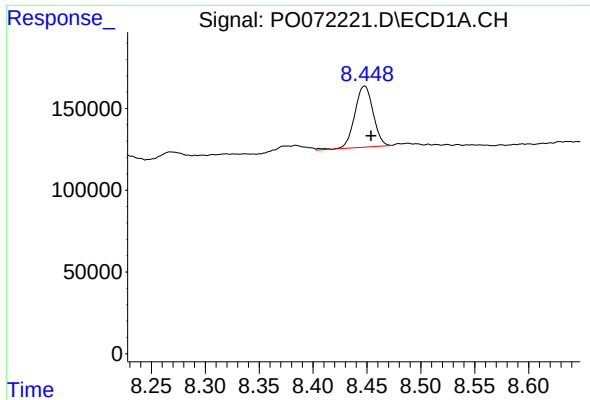


#35 AR-1260-5

R.T.: 8.448 min
Delta R.T.: -0.006 min
Response: 443774
Conc: 32.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
231-232-COMP

Manual Integrations
APPROVED

Ankita
10/13/2020 9:42:29 AM

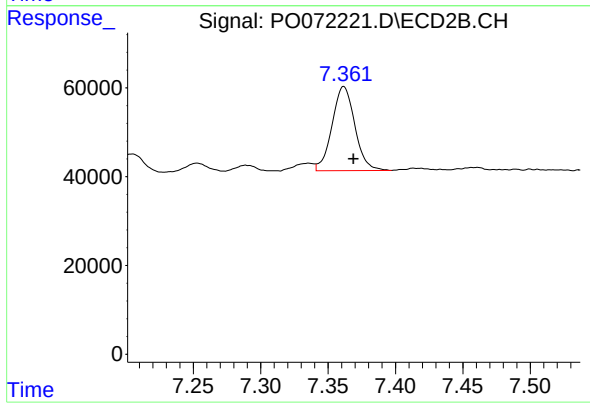

#35 AR-1260-5

R.T.: 7.362 min
Delta R.T.: -0.007 min
Response: 223580
Conc: 33.65 ng/ml