

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100920\
 Data File : PO072224.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Oct 2020 1:09
 Operator : DD\AJ
 Sample : L4299-06RE
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 86-96-COMP

Manual Integrations
 APPROVED

Ankita
 10/13/2020 9:42:34 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 05:54:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.322	3.508	1240060	400262	17.265m	10.686 #
2) SA Decachlor...	9.928	8.679	592242	290621	5.379	5.109

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100920\
Data File : PO072224.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Oct 2020 1:09
Operator : DD\AJ
Sample : L4299-06RE
Misc :
ALS Vial : 56 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
86-96-COMPRE


Manual Integrations
APPROVED

Ankita
10/13/2020 9:42:34 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 05:54:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

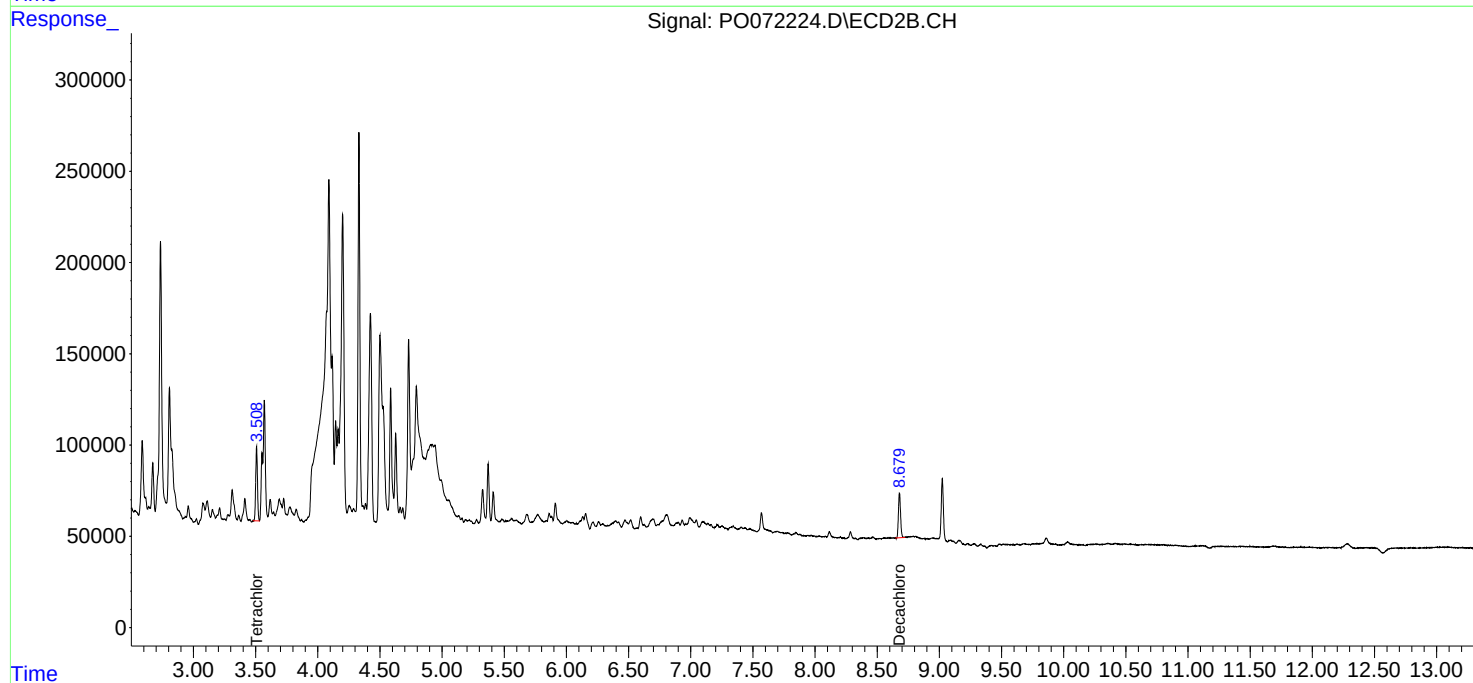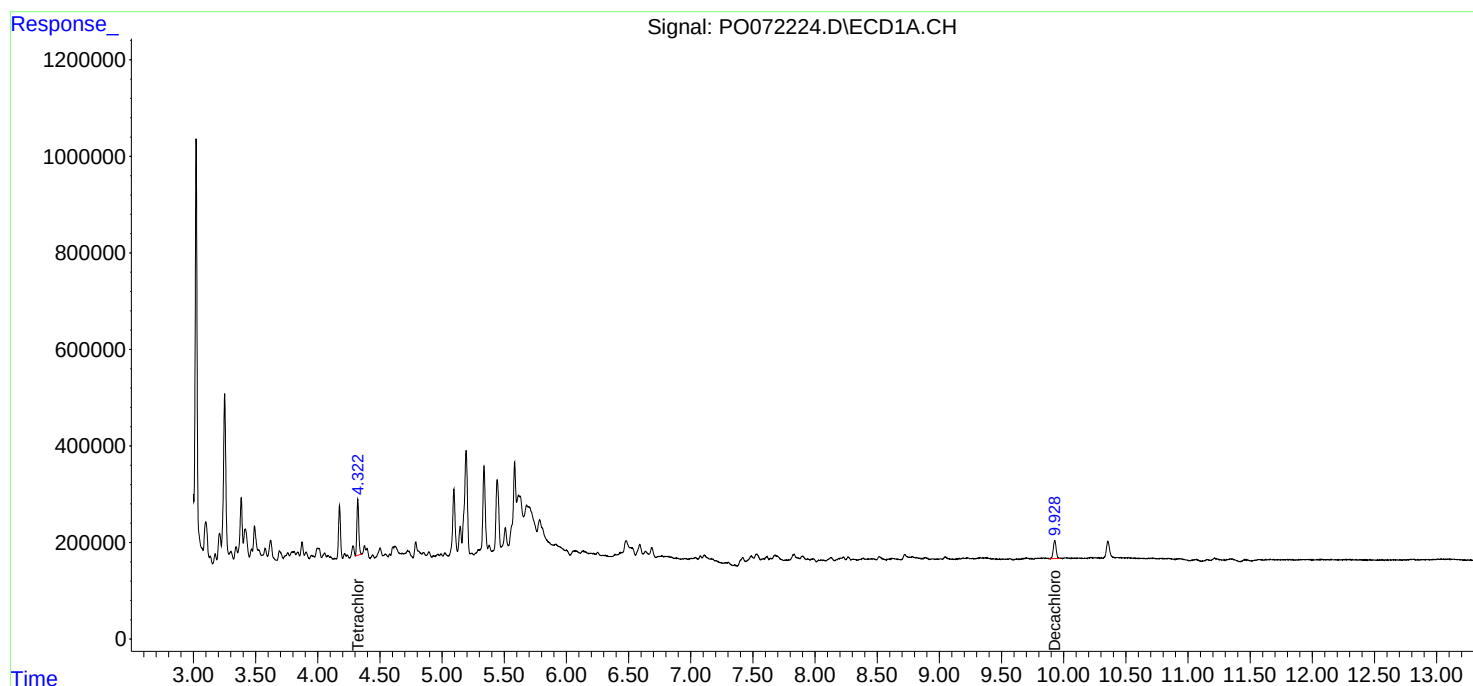

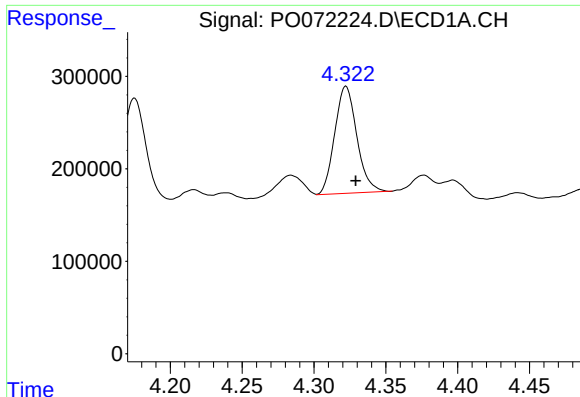


#1 Tetrachloro-m-xylene

R.T.: 4.322 min
Delta R.T.: -0.007 min
Response: 1240060
Conc: 17.26 ng/ml m

Instrument :
ECD_O
ClientSampleId :
86-96-COMP


Manual Integrations
APPROVED

Ankita
10/13/2020 9:42:34 AM

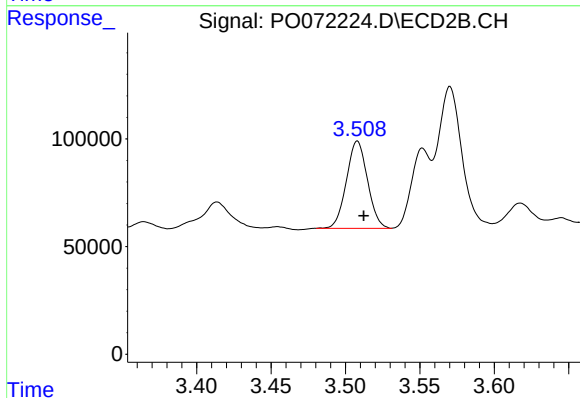


#1 Tetrachloro-m-xylene

R.T.: 3.508 min
Delta R.T.: -0.004 min
Response: 400262
Conc: 10.69 ng/ml

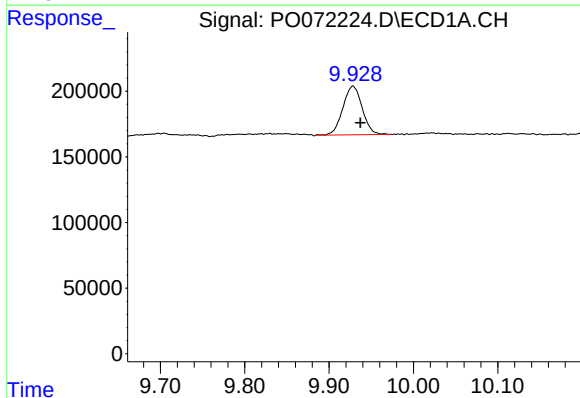

#2 Decachlorobiphenyl

R.T.: 9.928 min
Delta R.T.: -0.009 min
Response: 592242
Conc: 5.38 ng/ml

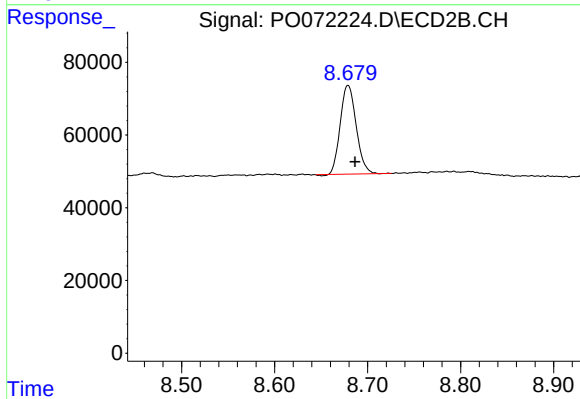

#2 Decachlorobiphenyl

R.T.: 8.679 min
Delta R.T.: -0.008 min
Response: 290621
Conc: 5.11 ng/ml