

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100920\
 Data File : PO072225.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Oct 2020 1:26
 Operator : DD\AJ
 Sample : L4300-02
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 223

Manual Integrations
 APPROVED

Ankita
 10/13/2020 9:42:36 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 05:55:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.326	3.515	914159	444467	12.727m	11.866
2) SA Decachlor...	9.926	8.677	896230	439372	8.140m	7.725
Target Compounds						
31) L7 AR-1260-1	7.285	6.289	956086	380132	199.489	148.466m#
32) L7 AR-1260-2	7.550	6.490	1520540	510270	203.005m	159.505m
33) L7 AR-1260-3	7.907	6.635	1553685	496184	243.704m	168.128m#
34) L7 AR-1260-4	8.135	7.110	929724	379580	154.888m	143.463m
35) L7 AR-1260-5	8.449	7.361	2059398	929872	148.618	139.959m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100920\
Data File : P0072225.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Oct 2020 1:26
Operator : DD\AJ
Sample : L4300-02
Misc :
ALS Vial : 57 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
223


Manual Integrations
APPROVED

Ankita
10/13/2020 9:42:36 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 05:55:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

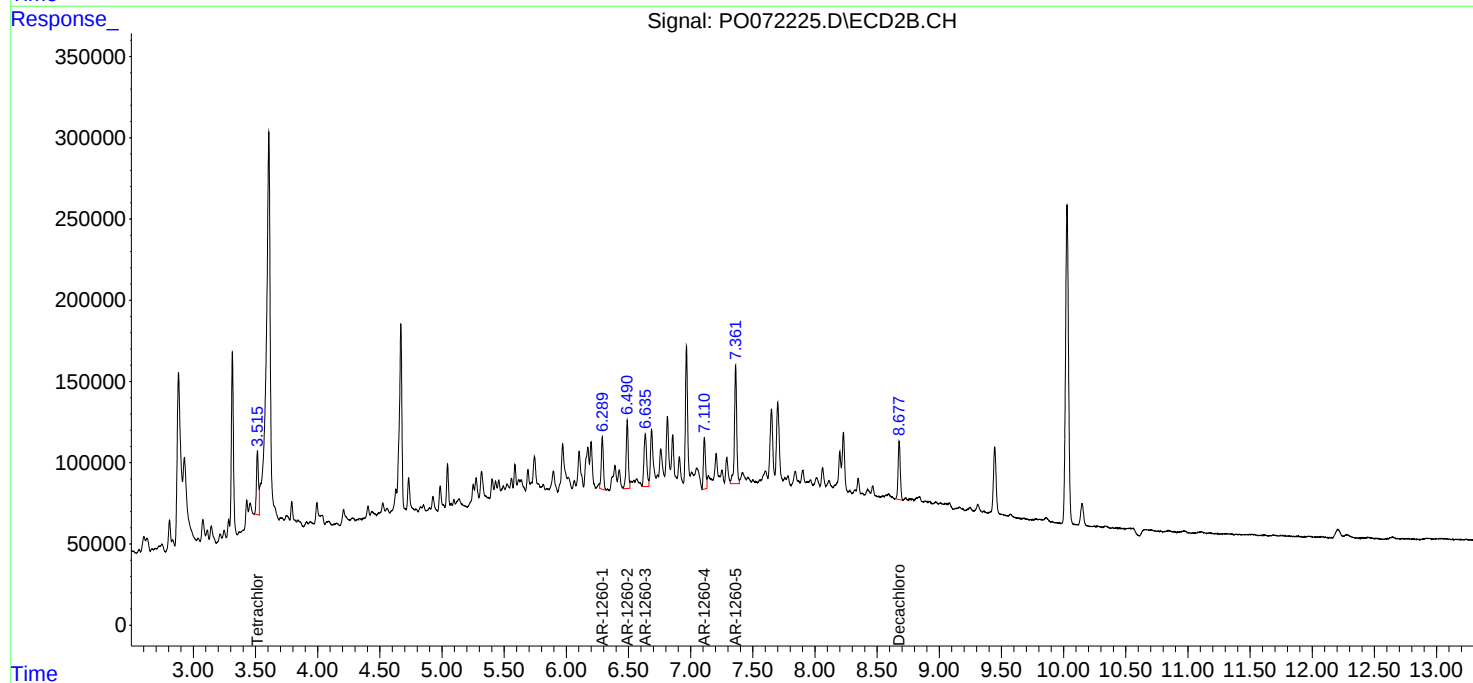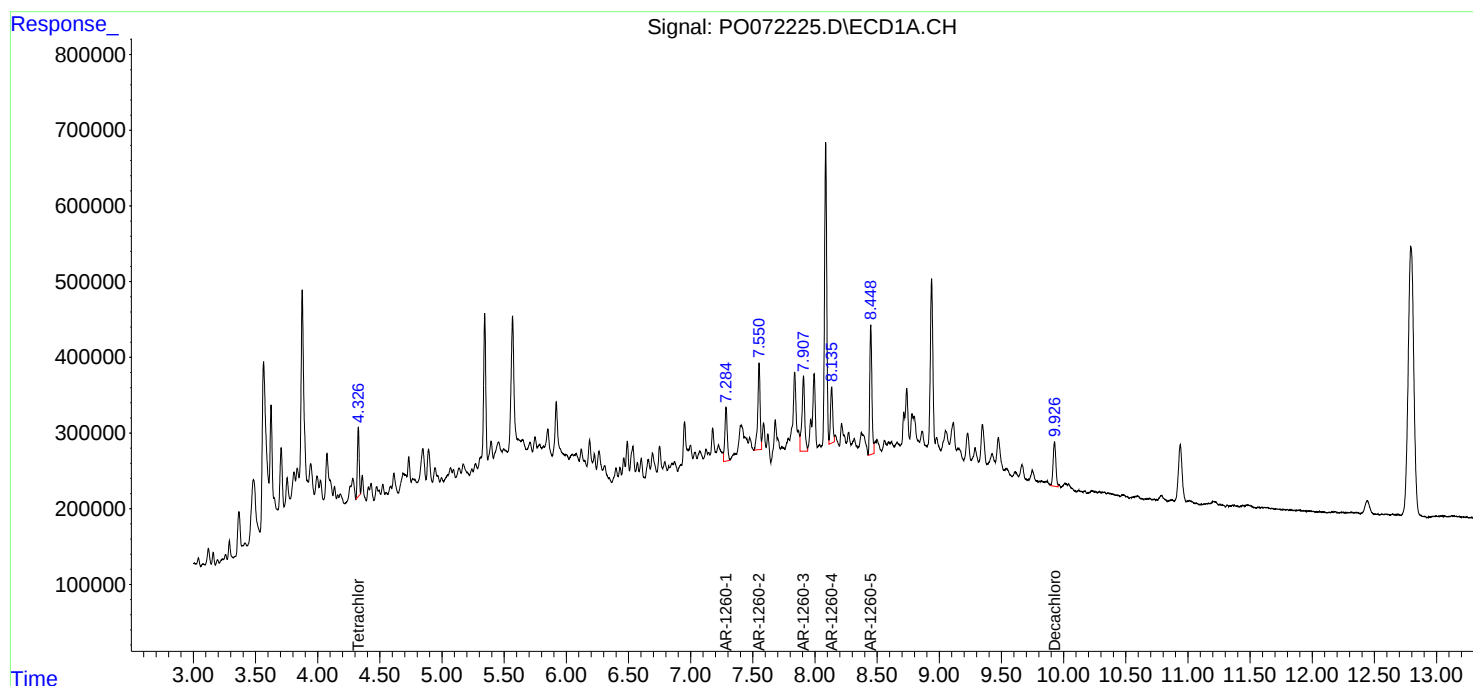

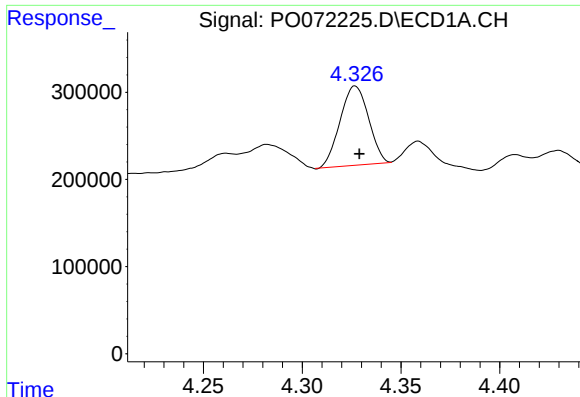


#1 Tetrachloro-m-xylene

R.T.: 4.326 min
Delta R.T.: -0.003 min
Response: 914159
Conc: 12.73 ng/ml m

Instrument :
ECD_O
ClientSampleId :
223


Manual Integrations
APPROVED

Ankita
10/13/2020 9:42:36 AM

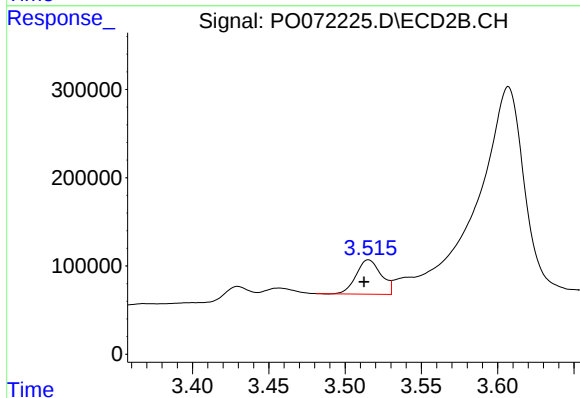


#1 Tetrachloro-m-xylene

R.T.: 3.515 min
Delta R.T.: 0.003 min
Response: 444467
Conc: 11.87 ng/ml

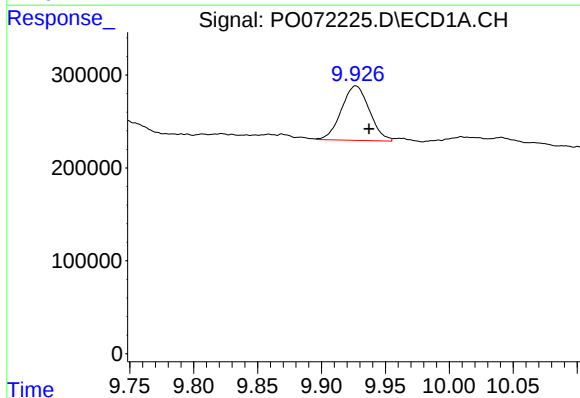


#2 Decachlorobiphenyl

R.T.: 9.926 min
Delta R.T.: -0.011 min
Response: 896230
Conc: 8.14 ng/ml m

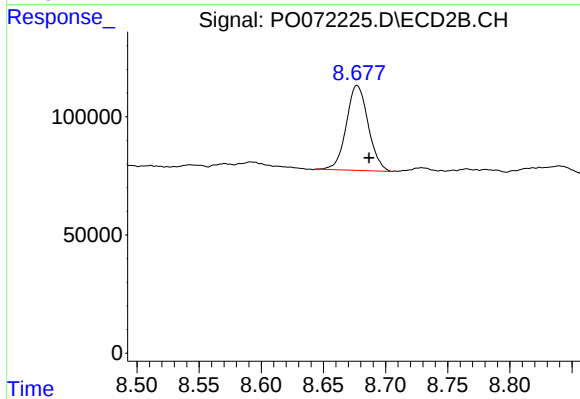

#2 Decachlorobiphenyl

R.T.: 8.677 min
Delta R.T.: -0.009 min
Response: 439372
Conc: 7.72 ng/ml

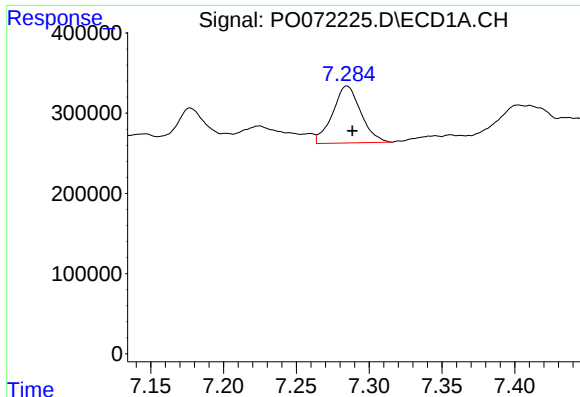


#31 AR-1260-1

R.T.: 7.285 min
Delta R.T.: -0.004 min
Response: 956086
Conc: 199.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
223


Manual Integrations
APPROVED

Ankita
10/13/2020 9:42:36 AM

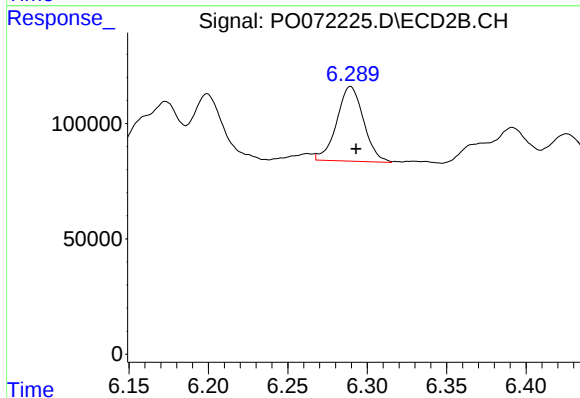


#31 AR-1260-1

R.T.: 6.289 min
Delta R.T.: -0.004 min
Response: 380132
Conc: 148.47 ng/ml m

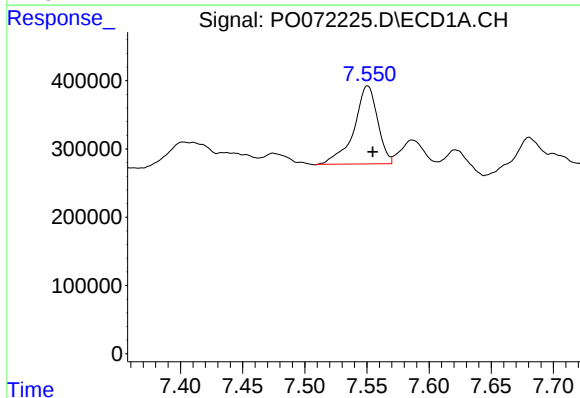


#32 AR-1260-2

R.T.: 7.550 min
Delta R.T.: -0.005 min
Response: 1520540
Conc: 203.00 ng/ml m

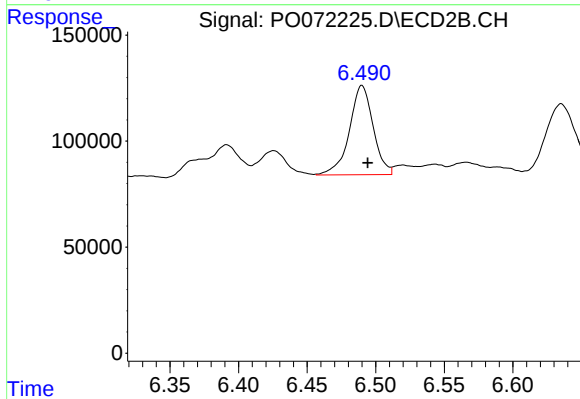

#32 AR-1260-2

R.T.: 6.490 min
Delta R.T.: -0.005 min
Response: 510270
Conc: 159.50 ng/ml m

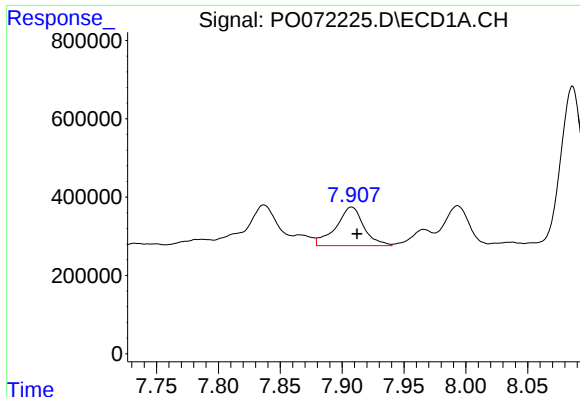


#33 AR-1260-3

R.T.: 7.907 min
Delta R.T.: -0.005 min
Response: 1553685
Conc: 243.70 ng/ml m

Instrument :
ECD_O
ClientSampleId :
223


Manual Integrations
APPROVED

Ankita
10/13/2020 9:42:36 AM

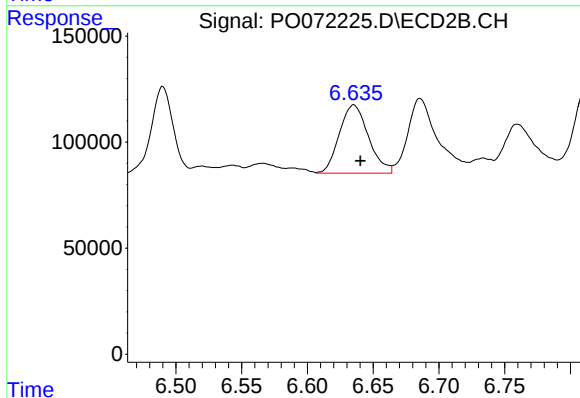


#33 AR-1260-3

R.T.: 6.635 min
Delta R.T.: -0.005 min
Response: 496184
Conc: 168.13 ng/ml m

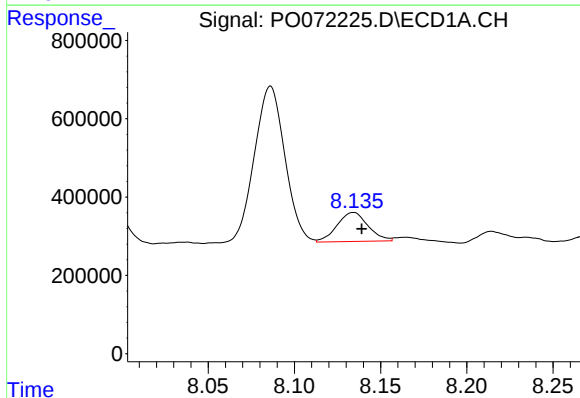


#34 AR-1260-4

R.T.: 8.135 min
Delta R.T.: -0.004 min
Response: 929724
Conc: 154.89 ng/ml m

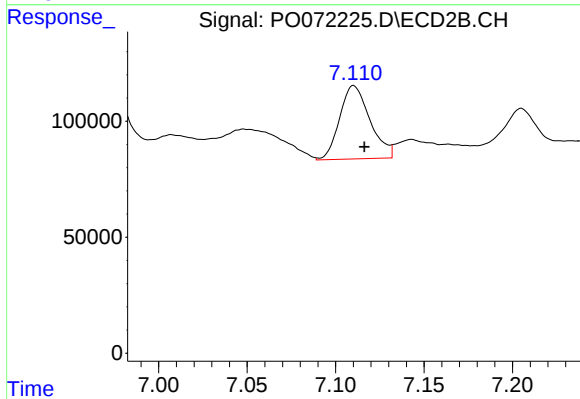

#34 AR-1260-4

R.T.: 7.110 min
Delta R.T.: -0.006 min
Response: 379580
Conc: 143.46 ng/ml m

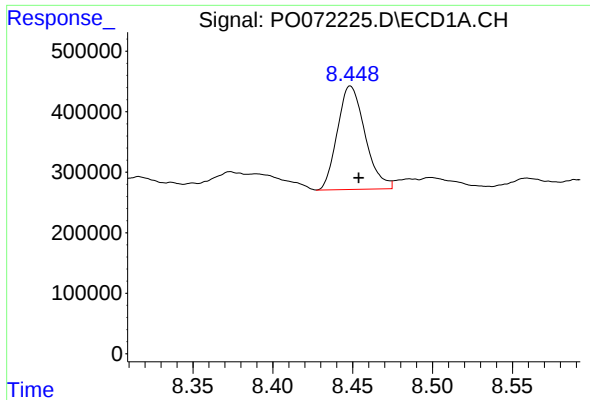


#35 AR-1260-5

R.T.: 8.449 min
Delta R.T.: -0.005 min
Response: 2059398
Conc: 148.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
223

Manual Integrations
APPROVED

Ankita
10/13/2020 9:42:36 AM

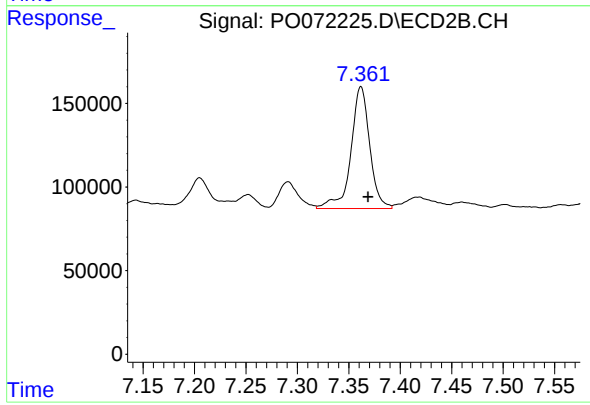

#35 AR-1260-5

R.T.: 7.361 min
Delta R.T.: -0.007 min
Response: 929872
Conc: 139.96 ng/ml m