

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO100925\
 Data File : PO114346.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2025 01:51
 Operator : YP/AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 05:10:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO100925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 10 05:04:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.350	3.636	25102	229754	0.005	0.057 #
2)	SA Decachlor...	9.943	8.680	343884	535987	0.094	0.161 #
Target Compounds							
3)	L1 AR-1016-1	5.464	4.710	744941	11545	4.130	0.069 #
4)	L1 AR-1016-2	5.521	4.779	433518	585914	1.425	2.421 #
5)	L1 AR-1016-3	5.570	4.918	141417	180797	0.800	1.456 #
6)	L1 AR-1016-4	5.668	4.960	80039	482464	0.582	4.998 #
7)	L1 AR-1016-5	5.972	5.194	499212	-131139	3.954	N.D. #
8)	L2 AR-1221-1	4.563	3.866	304461	872495	4.682	15.912 #
9)	L2 AR-1221-2	4.644	3.961	1804071	2380479	39.346	58.828 #
10)	L2 AR-1221-3	4.717	4.063	1885753	1409818	12.532	10.976
11)	L3 AR-1232-1	4.717	4.063	1885753	1409818	15.449	13.471
12)	L3 AR-1232-2	5.252	4.779	93312	585914	1.726	5.695 #
13)	L3 AR-1232-3	5.521	4.918	433518	180797	3.572	3.529
14)	L3 AR-1232-4	5.668	5.024	80039	1698463	1.481	38.925 #
15)	L3 AR-1232-5	5.768	5.194	431193	-131139	11.545	N.D. #
16)	L4 AR-1242-1	5.521	4.710	433518	11545	3.295	0.088 #
17)	L4 AR-1242-2	5.521	4.779	433518	585914	1.975	3.137 #
18)	L4 AR-1242-3	5.583	4.918	148784	180797	1.206	1.889 #
19)	L4 AR-1242-4	5.668	5.024	80039	1698463	0.780	18.393 #
20)	L4 AR-1242-5	6.405	5.528	9721933	5113523	83.930	41.722 #
21)	L5 AR-1248-1	5.521	4.710	433518	11545	4.408	0.117 #
22)	L5 AR-1248-2	5.757	4.960	145195	482464	1.011	3.599 #
23)	L5 AR-1248-3	5.972	5.024	499212	1698463	3.143	12.172 #
24)	L5 AR-1248-4	6.405f	5.194	9721933	-131139	49.655	N.D. #
25)	L5 AR-1248-5	6.405	5.561	9721933	1960522	48.563	11.561 #
26)	L6 AR-1254-1	6.311	5.528	4369994	5113523	25.050	19.246
27)	L6 AR-1254-2	6.546	5.688	11165140	1500793	43.835	6.300 #
28)	L6 AR-1254-3	6.918	6.111	8881917	19177128	30.740	54.110 #
29)	L6 AR-1254-4	7.186	6.300	2331463	13314486	9.852	51.575 #
30)	L6 AR-1254-5	7.624	6.739	1746.3E6	2017.8E6	7956.662	6301.639
31)	L7 AR-1260-1	7.074	6.231	1351189	15172960	6.200	64.433 #
32)	L7 AR-1260-2	7.310	6.416	2264.3E6	6783510	7339.720	20.286 #
33)	L7 AR-1260-3	7.687	6.548	807001	9186521	3.147	31.147 #
34)	L7 AR-1260-4	7.896	7.036	276149	145096	1.186	0.651 #
35)	L7 AR-1260-5	8.213	7.277	279248	694427	0.481	1.133 #
36)	L8 AR-1262-1	7.687	6.739f	807001	2017.8E6	2.210	4740.481 #
37)	L8 AR-1262-2	8.213	7.277	279248	694427	0.462	1.031 #
38)	L8 AR-1262-3	8.527	7.566	58822	252651	0.161	0.912 #
39)	L8 AR-1262-4	8.571	7.620	113717	95962	0.431	0.210 #
40)	L8 AR-1262-5	9.212	8.126	15509572	45395	72.187	0.215 #
41)	L9 AR-1268-1	8.527	7.566	58822	252651	0.080	0.309 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100925\
Data File : PO114346.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2025 01:51
Operator : YP/AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 05:10:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100925.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 10 05:04:59 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.571	7.631	113717	25398	0.183	0.037 #
43)	L9 AR-1268-3	8.811	7.821	703036	8127945	1.229	13.767 #
44)	L9 AR-1268-4	9.212	8.126	15509572	45395	62.781	0.190 #
45)	L9 AR-1268-5	9.621	8.401	3129147	386118	1.826	0.237 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100925\
Data File : PO114346.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2025 01:51
Operator : YP/AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 05:10:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100925.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 10 05:04:59 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

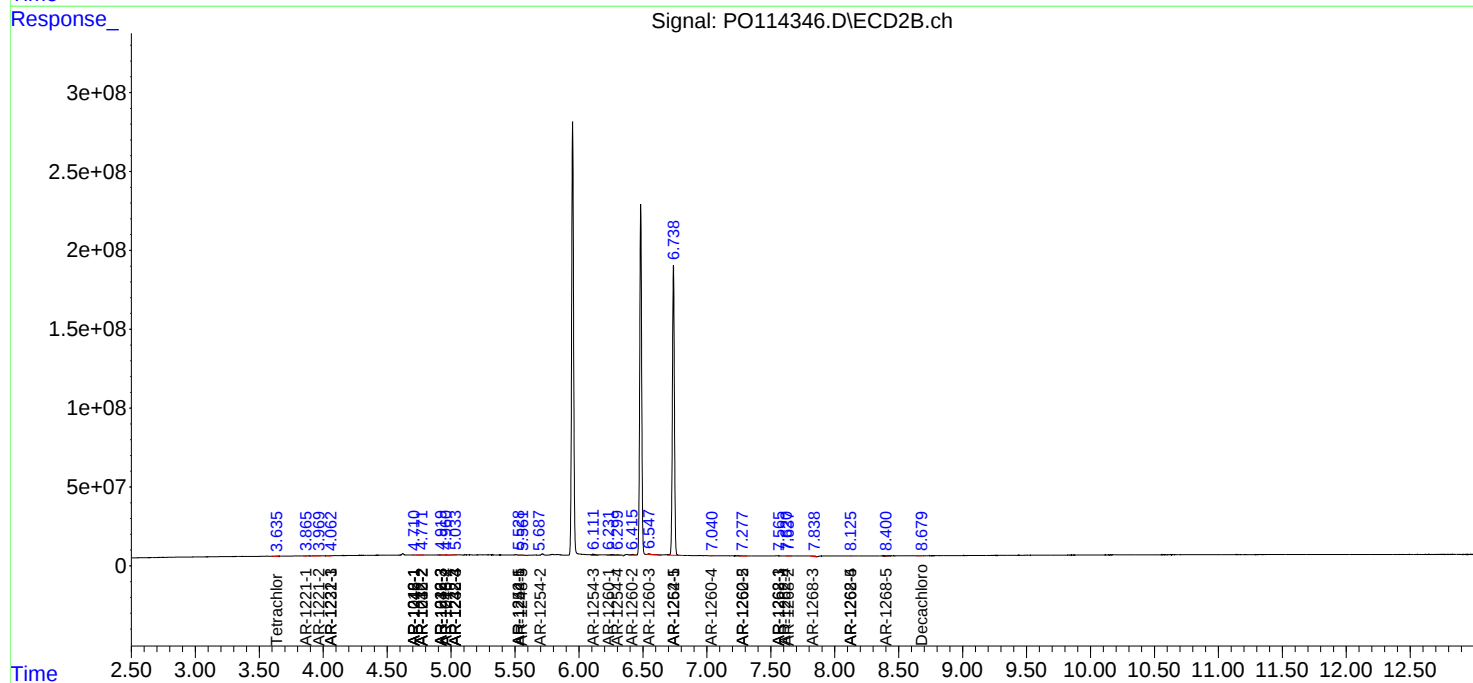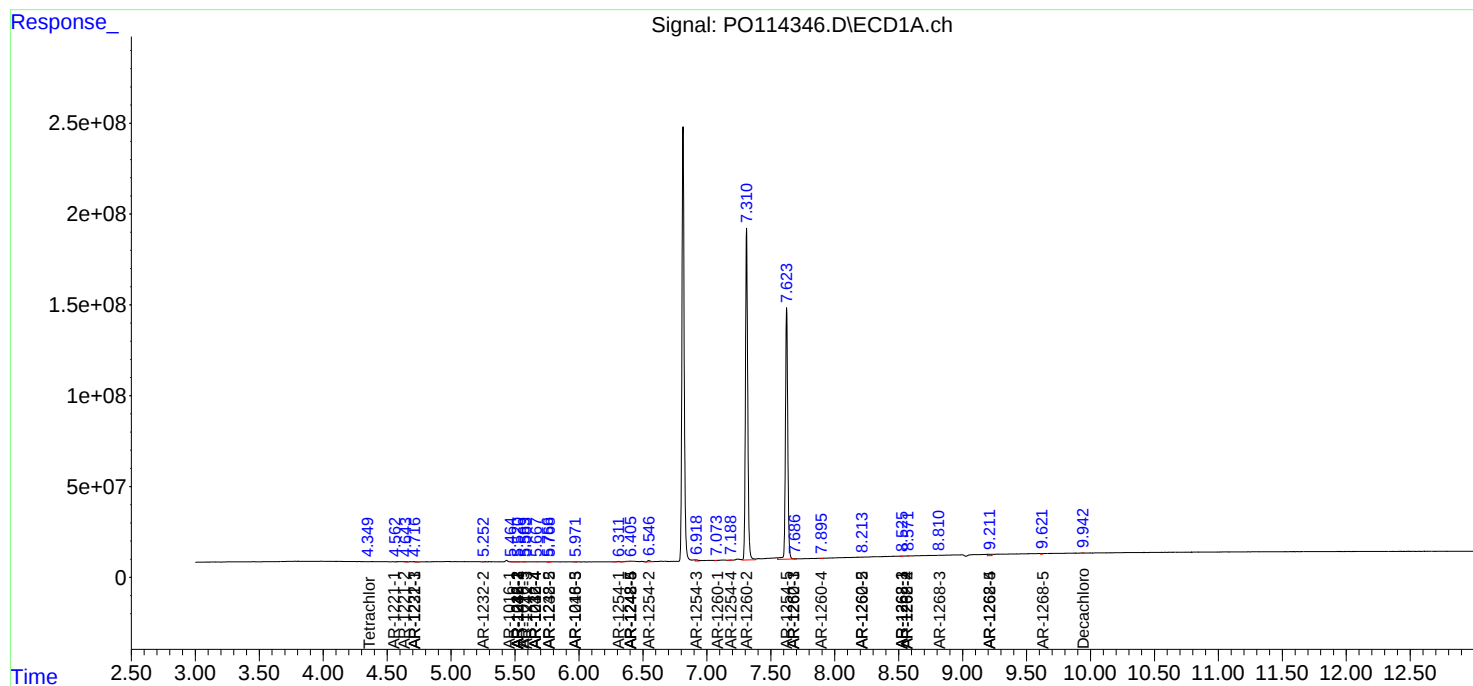


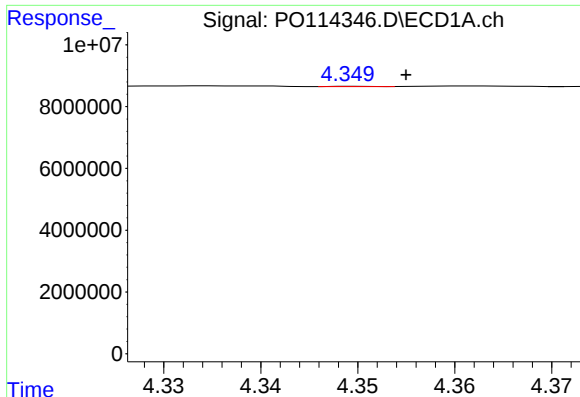

#1 Tetrachloro-m-xylene


R.T.: 4.350 min
Delta R.T.: -0.005 min
Response: 25102
Conc: 0.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

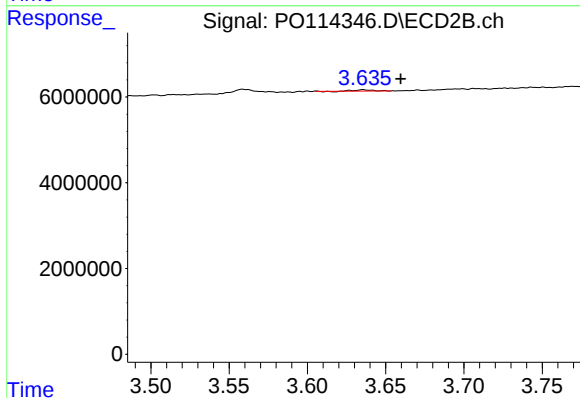


#1 Tetrachloro-m-xylene

R.T.: 3.636 min
Delta R.T.: -0.024 min
Response: 229754
Conc: 0.06 ng/ml

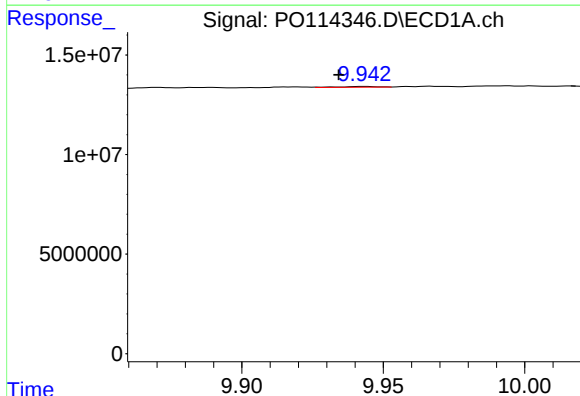


#2 Decachlorobiphenyl

R.T.: 9.943 min
Delta R.T.: 0.009 min
Response: 343884
Conc: 0.09 ng/ml

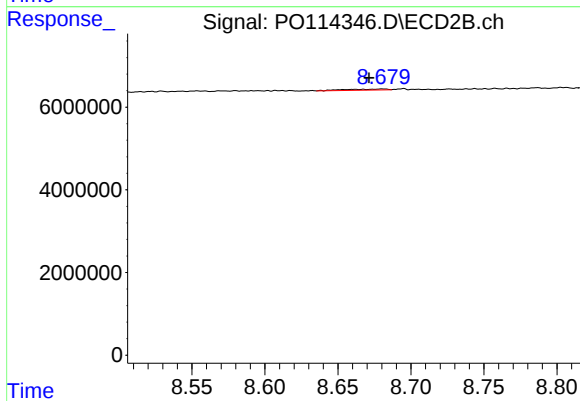

#2 Decachlorobiphenyl


R.T.: 8.680 min
Delta R.T.: 0.009 min
Response: 535987
Conc: 0.16 ng/ml

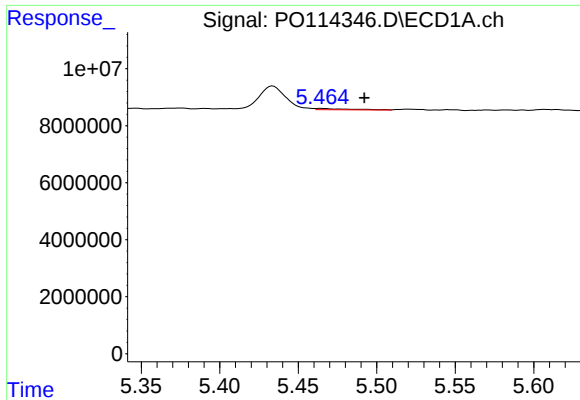

#3 AR-1016-1


R.T.: 5.464 min
Delta R.T.: -0.028 min
Response: 744941
Conc: 4.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

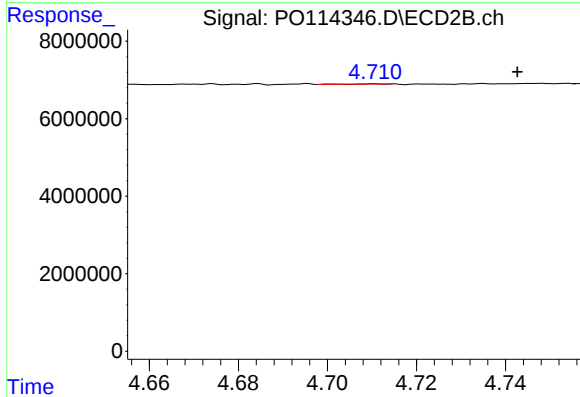


#3 AR-1016-1

R.T.: 4.710 min
Delta R.T.: -0.032 min
Response: 11545
Conc: 0.07 ng/ml

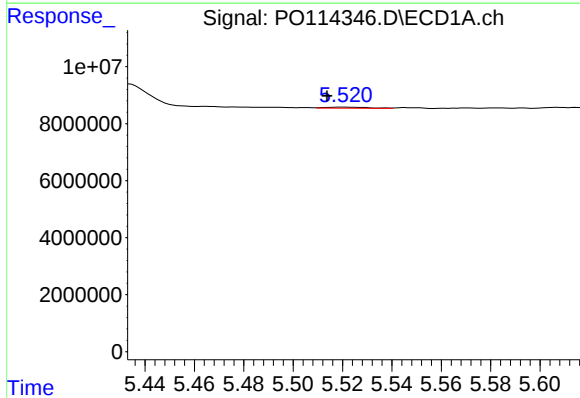


#4 AR-1016-2

R.T.: 5.521 min
Delta R.T.: 0.007 min
Response: 433518
Conc: 1.42 ng/ml

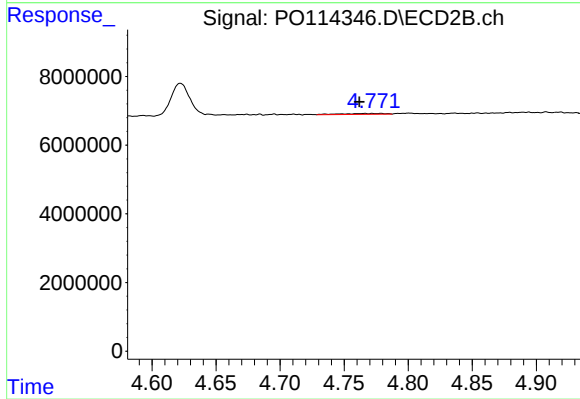

#4 AR-1016-2


R.T.: 4.779 min
Delta R.T.: 0.017 min
Response: 585914
Conc: 2.42 ng/ml

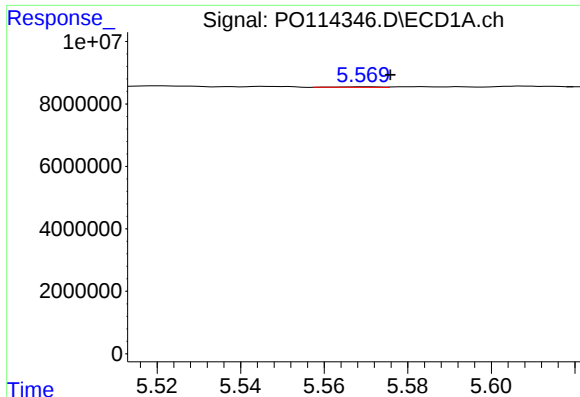

#5 AR-1016-3


R.T.: 5.570 min
Delta R.T.: -0.006 min
Response: 141417
Conc: 0.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

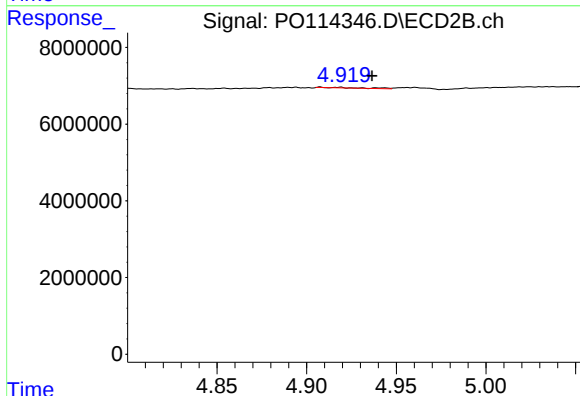


#5 AR-1016-3

R.T.: 4.918 min
Delta R.T.: -0.018 min
Response: 180797
Conc: 1.46 ng/ml

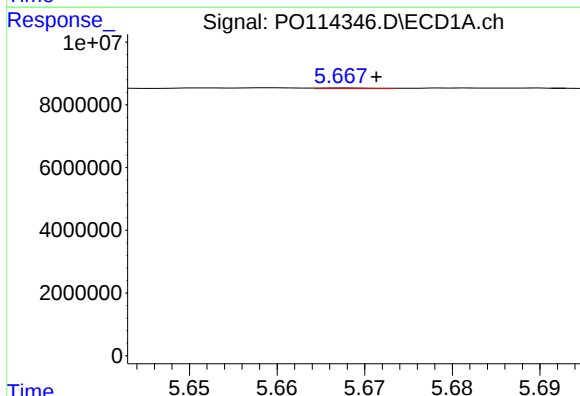


#6 AR-1016-4

R.T.: 5.668 min
Delta R.T.: -0.004 min
Response: 80039
Conc: 0.58 ng/ml

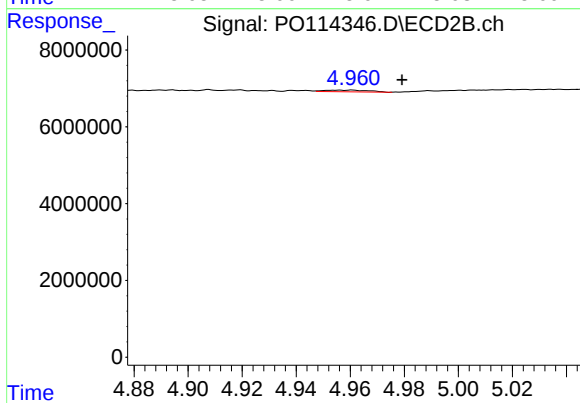

#6 AR-1016-4


R.T.: 4.960 min
Delta R.T.: -0.019 min
Response: 482464
Conc: 5.00 ng/ml

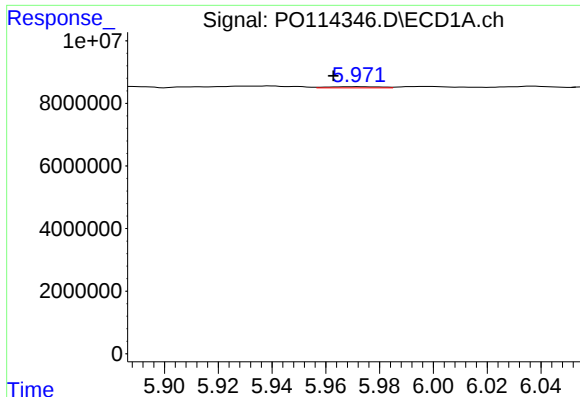

#7 AR-1016-5


R.T.: 5.972 min
Delta R.T.: 0.009 min
Response: 499212
Conc: 3.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

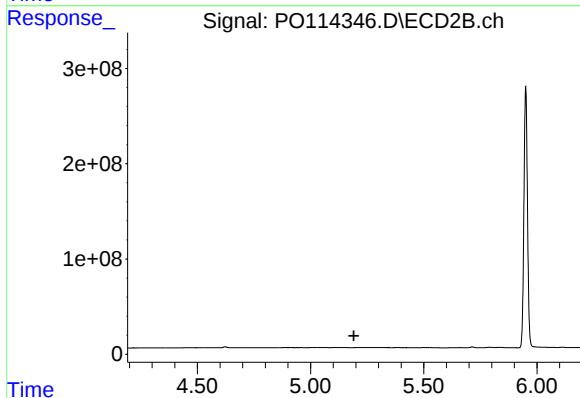


#7 AR-1016-5

R.T.: 5.194 min
Delta R.T.: 0.002 min
Response: -131139
Conc: N.D.

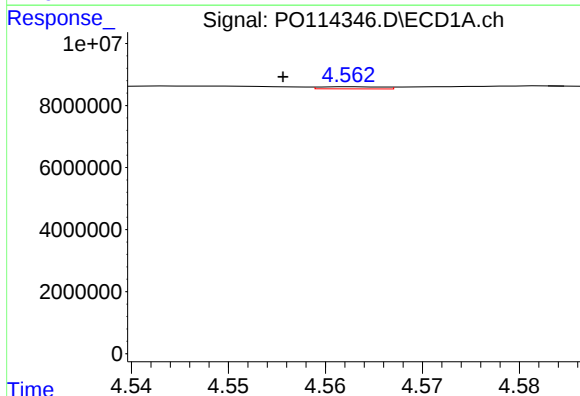


#8 AR-1221-1

R.T.: 4.563 min
Delta R.T.: 0.007 min
Response: 304461
Conc: 4.68 ng/ml

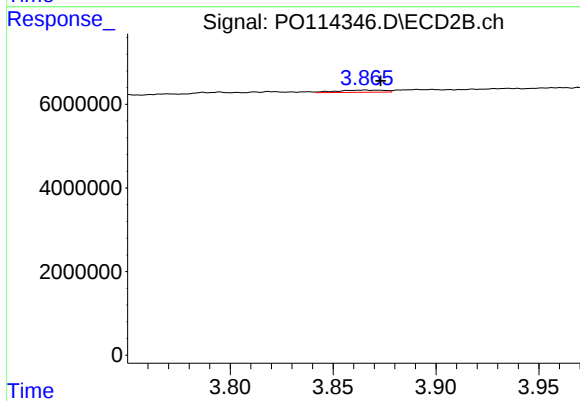

#8 AR-1221-1


R.T.: 3.866 min
Delta R.T.: -0.008 min
Response: 872495
Conc: 15.91 ng/ml

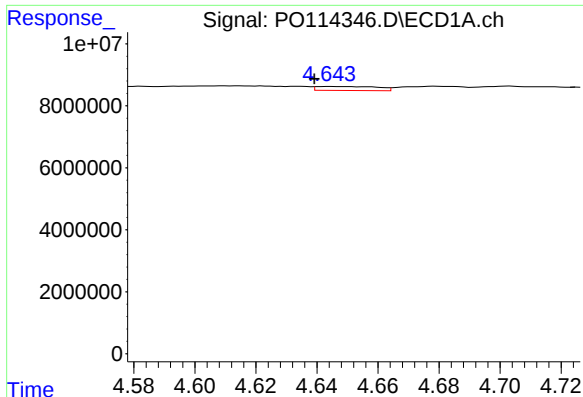

#9 AR-1221-2


R.T.: 4.644 min
Delta R.T.: 0.005 min
Response: 1804071
Conc: 39.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

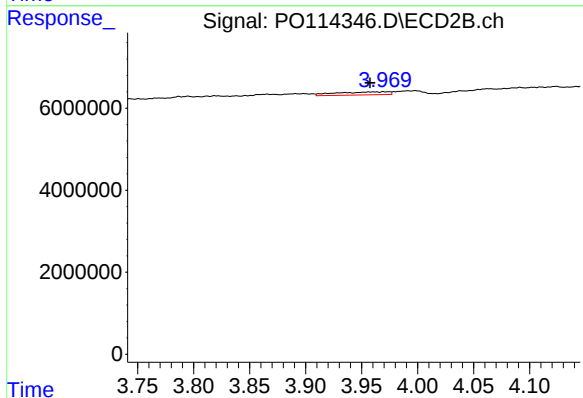


#9 AR-1221-2

R.T.: 3.961 min
Delta R.T.: 0.004 min
Response: 2380479
Conc: 58.83 ng/ml

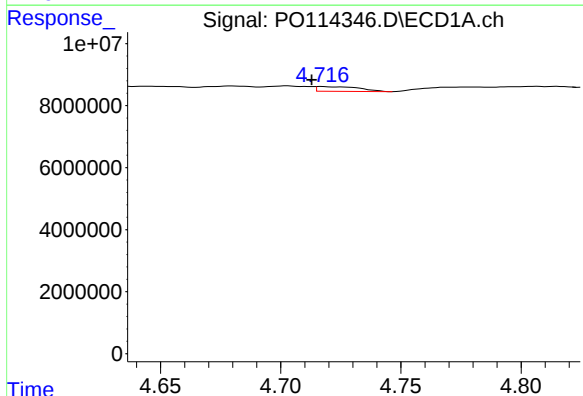


#10 AR-1221-3

R.T.: 4.717 min
Delta R.T.: 0.004 min
Response: 1885753
Conc: 12.53 ng/ml

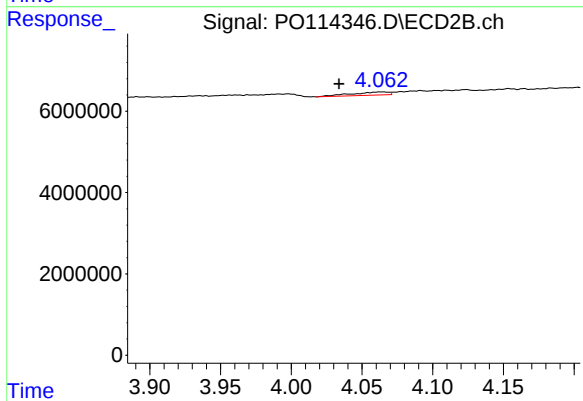

#10 AR-1221-3


R.T.: 4.063 min
Delta R.T.: 0.030 min
Response: 1409818
Conc: 10.98 ng/ml

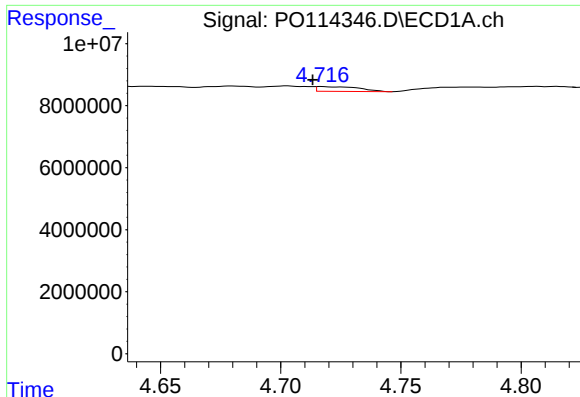

#11 AR-1232-1


R.T.: 4.717 min
Delta R.T.: 0.004 min
Response: 1885753
Conc: 15.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

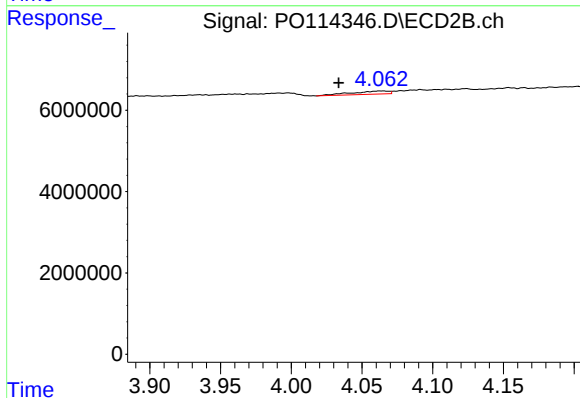


#11 AR-1232-1

R.T.: 4.063 min
Delta R.T.: 0.030 min
Response: 1409818
Conc: 13.47 ng/ml

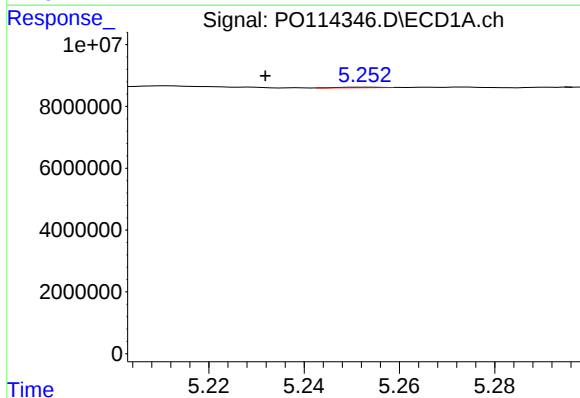


#12 AR-1232-2

R.T.: 5.252 min
Delta R.T.: 0.021 min
Response: 93312
Conc: 1.73 ng/ml

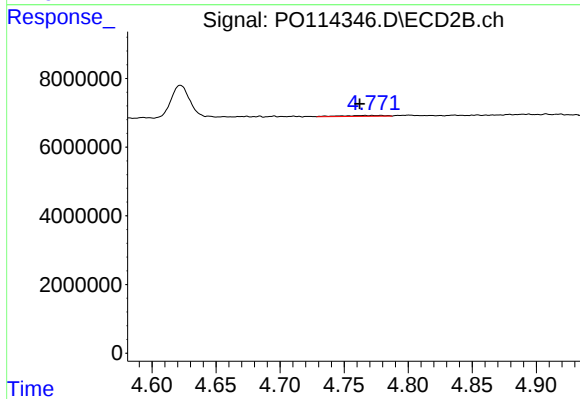

#12 AR-1232-2


R.T.: 4.779 min
Delta R.T.: 0.017 min
Response: 585914
Conc: 5.70 ng/ml

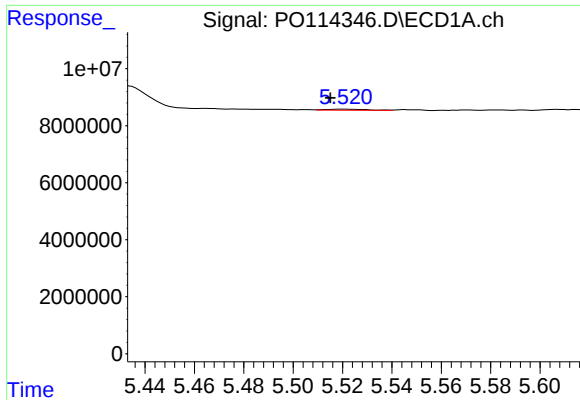

#13 AR-1232-3


R.T.: 5.521 min
Delta R.T.: 0.005 min
Response: 433518
Conc: 3.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

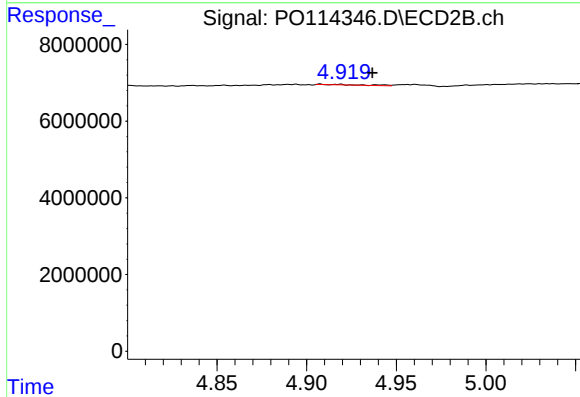


#13 AR-1232-3

R.T.: 4.918 min
Delta R.T.: -0.018 min
Response: 180797
Conc: 3.53 ng/ml

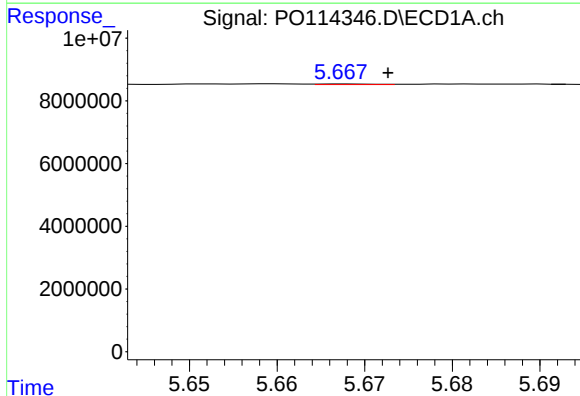


#14 AR-1232-4

R.T.: 5.668 min
Delta R.T.: -0.005 min
Response: 80039
Conc: 1.48 ng/ml

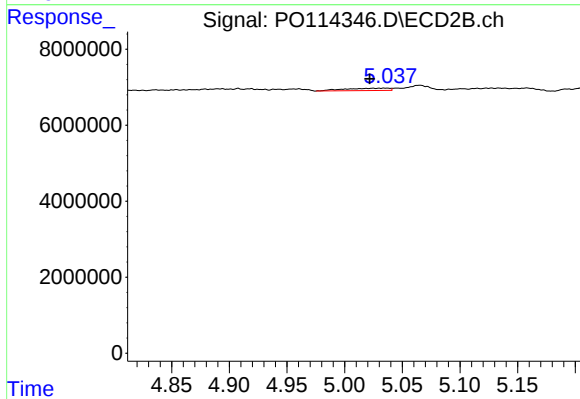

#14 AR-1232-4


R.T.: 5.024 min
Delta R.T.: 0.003 min
Response: 1698463
Conc: 38.92 ng/ml

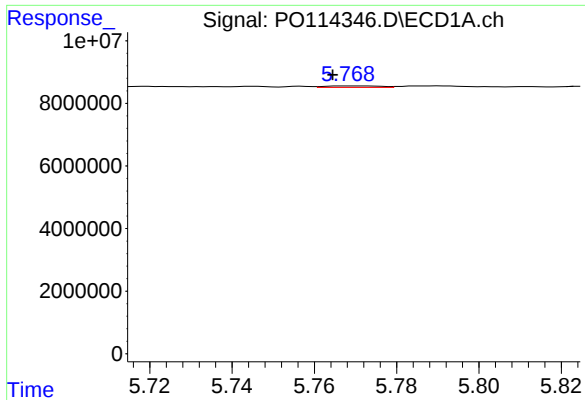

#15 AR-1232-5


R.T.: 5.768 min
Delta R.T.: 0.004 min
Response: 431193
Conc: 11.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

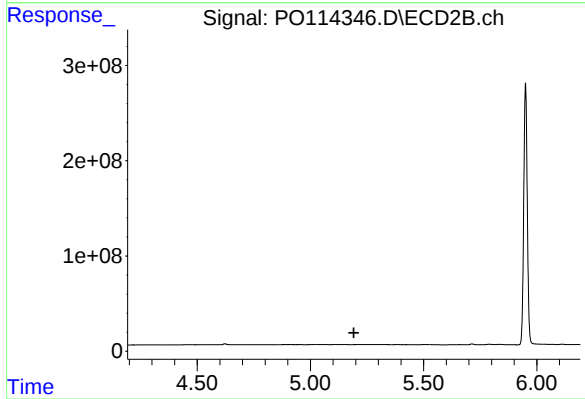


#15 AR-1232-5

R.T.: 5.194 min
Delta R.T.: 0.001 min
Response: -131139
Conc: N.D.

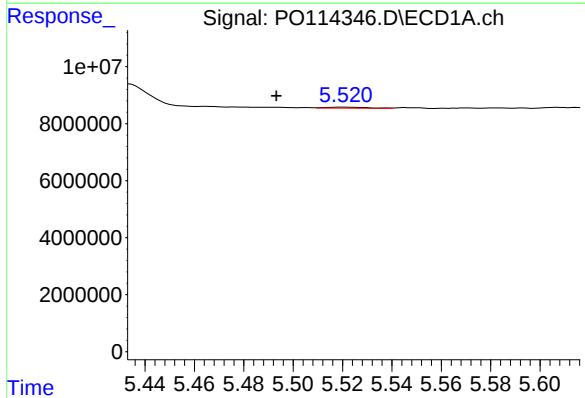


#16 AR-1242-1

R.T.: 5.521 min
Delta R.T.: 0.027 min
Response: 433518
Conc: 3.30 ng/ml

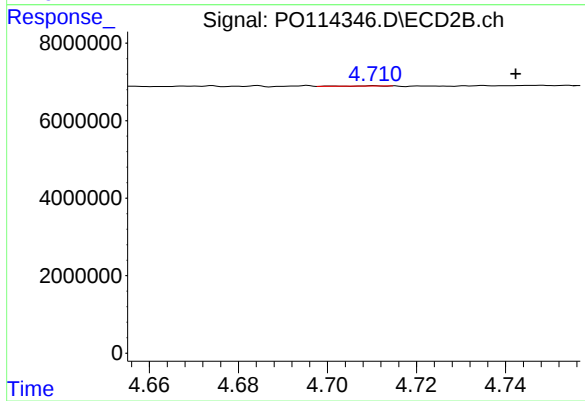

#16 AR-1242-1


R.T.: 4.710 min
Delta R.T.: -0.032 min
Response: 11545
Conc: 0.09 ng/ml

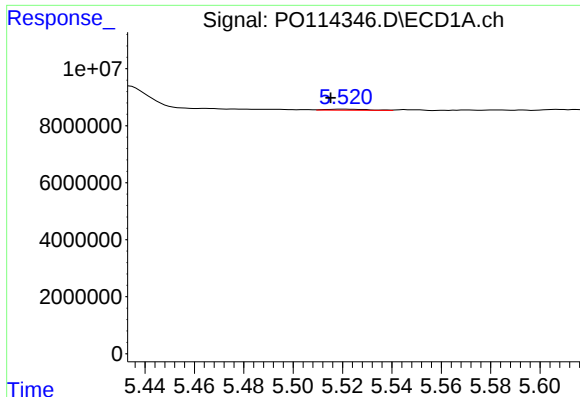

#17 AR-1242-2


R.T.: 5.521 min
Delta R.T.: 0.005 min
Response: 433518
Conc: 1.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

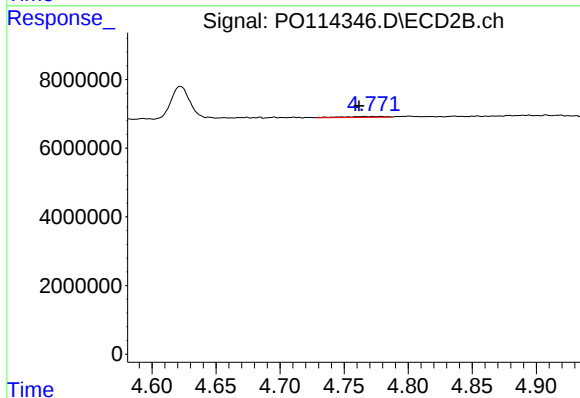


#17 AR-1242-2

R.T.: 4.779 min
Delta R.T.: 0.017 min
Response: 585914
Conc: 3.14 ng/ml

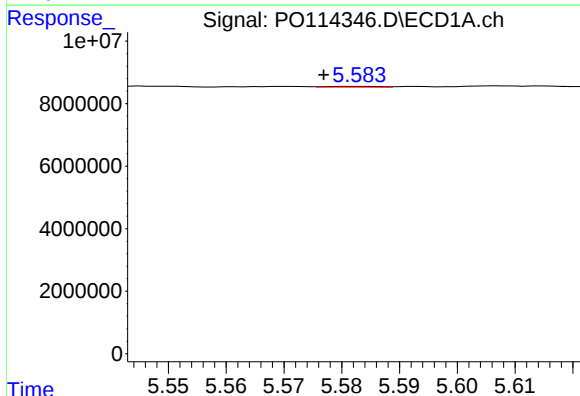


#18 AR-1242-3

R.T.: 5.583 min
Delta R.T.: 0.006 min
Response: 148784
Conc: 1.21 ng/ml

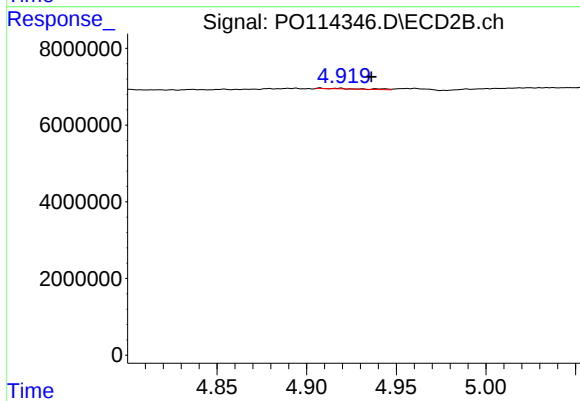

#18 AR-1242-3


R.T.: 4.918 min
Delta R.T.: -0.018 min
Response: 180797
Conc: 1.89 ng/ml

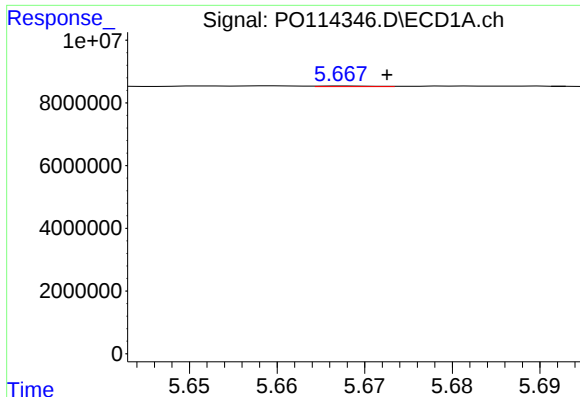

#19 AR-1242-4


R.T.: 5.668 min
Delta R.T.: -0.005 min
Response: 80039
Conc: 0.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

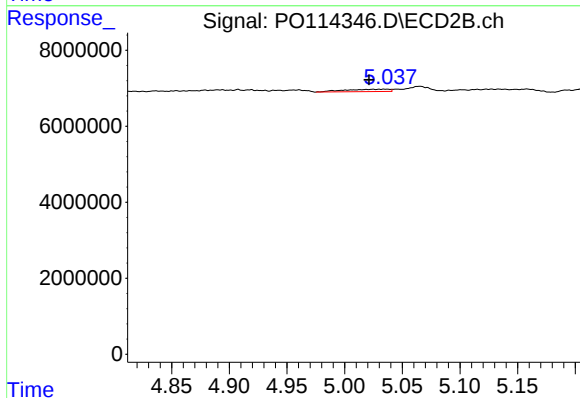


#19 AR-1242-4

R.T.: 5.024 min
Delta R.T.: 0.003 min
Response: 1698463
Conc: 18.39 ng/ml

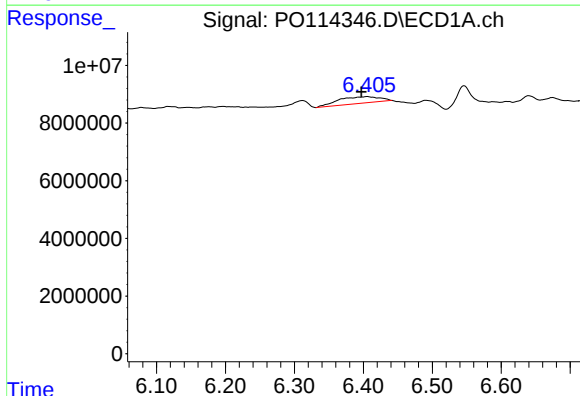


#20 AR-1242-5

R.T.: 6.405 min
Delta R.T.: 0.008 min
Response: 9721933
Conc: 83.93 ng/ml

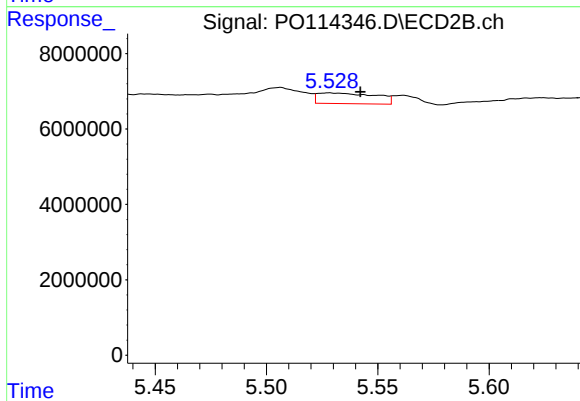

#20 AR-1242-5


R.T.: 5.528 min
Delta R.T.: -0.014 min
Response: 5113523
Conc: 41.72 ng/ml

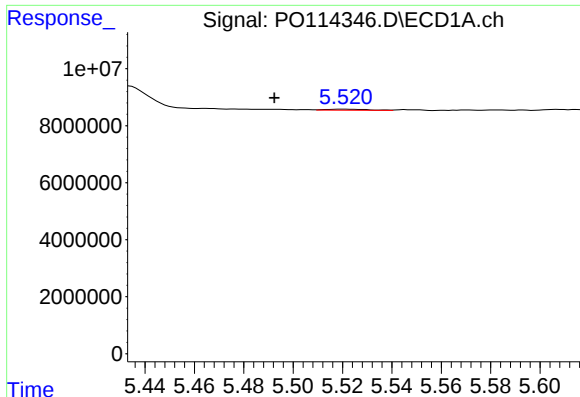

#21 AR-1248-1


R.T.: 5.521 min
Delta R.T.: 0.028 min
Response: 433518
Conc: 4.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

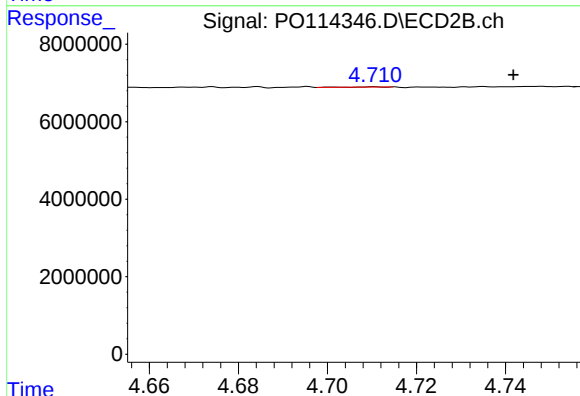


#21 AR-1248-1

R.T.: 4.710 min
Delta R.T.: -0.031 min
Response: 11545
Conc: 0.12 ng/ml

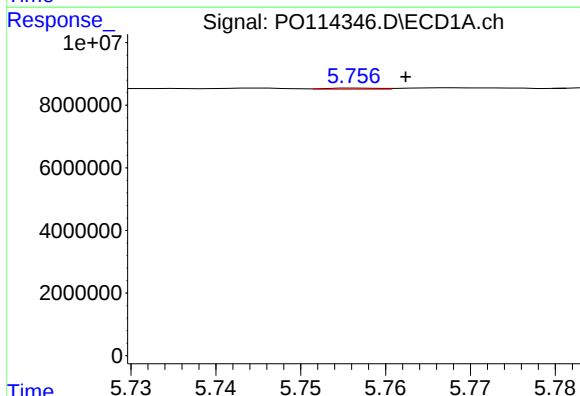


#22 AR-1248-2

R.T.: 5.757 min
Delta R.T.: -0.006 min
Response: 145195
Conc: 1.01 ng/ml

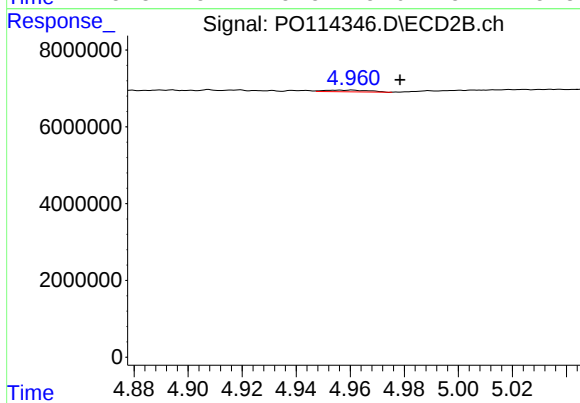

#22 AR-1248-2


R.T.: 4.960 min
Delta R.T.: -0.018 min
Response: 482464
Conc: 3.60 ng/ml

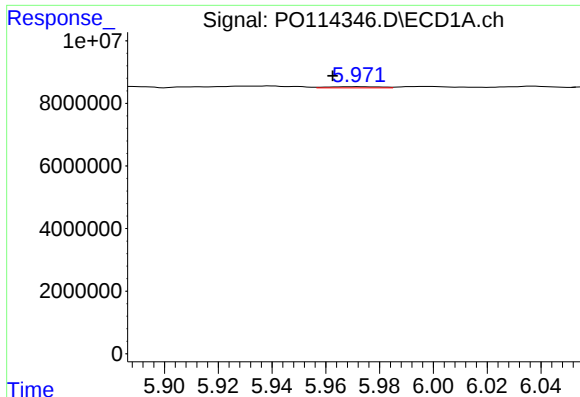

#23 AR-1248-3


R.T.: 5.972 min
Delta R.T.: 0.009 min
Response: 499212
Conc: 3.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

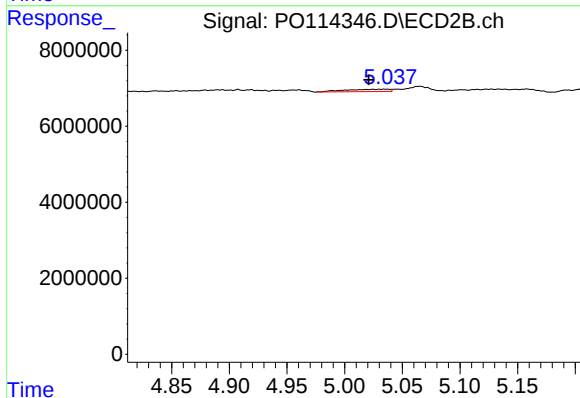


#23 AR-1248-3

R.T.: 5.024 min
Delta R.T.: 0.004 min
Response: 1698463
Conc: 12.17 ng/ml

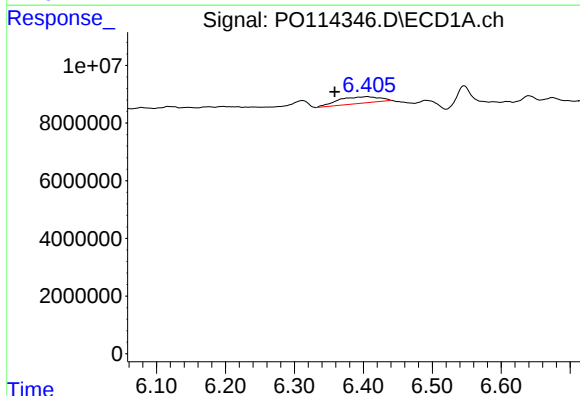


#24 AR-1248-4

R.T.: 6.405 min
Delta R.T.: 0.047 min
Response: 9721933
Conc: 49.65 ng/ml

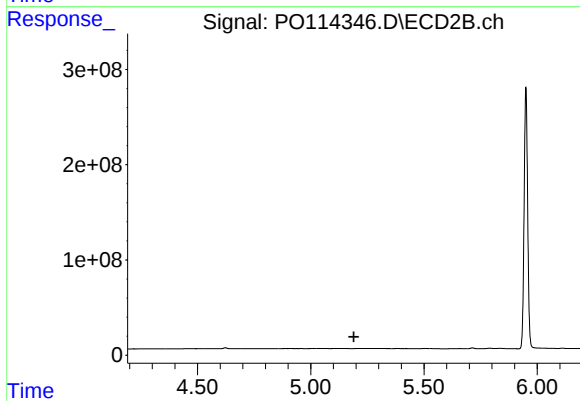

#24 AR-1248-4


R.T.: 5.194 min
Delta R.T.: 0.003 min
Response: -131139
Conc: N.D.

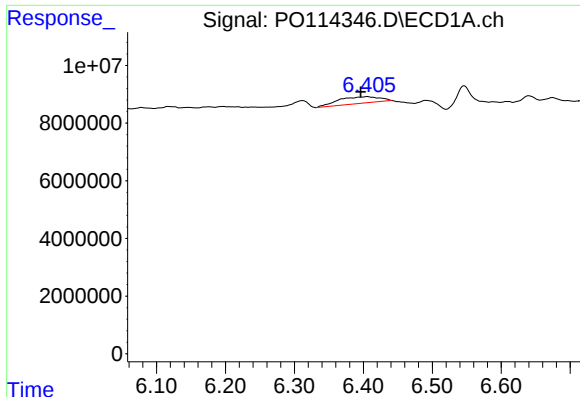

#25 AR-1248-5


R.T.: 6.405 min
Delta R.T.: 0.009 min
Response: 9721933
Conc: 48.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

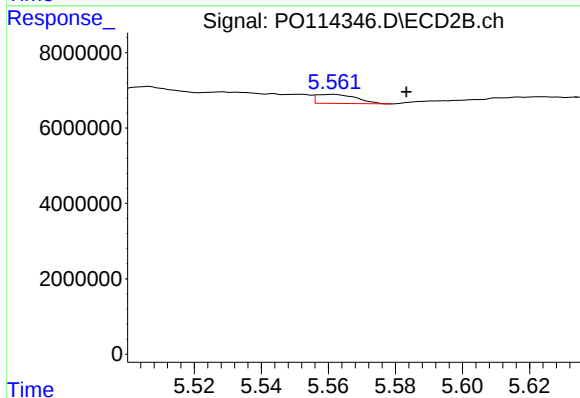


#25 AR-1248-5

R.T.: 5.561 min
Delta R.T.: -0.022 min
Response: 1960522
Conc: 11.56 ng/ml

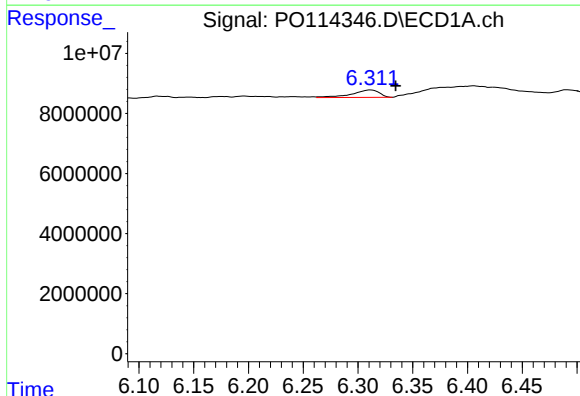


#26 AR-1254-1

R.T.: 6.311 min
Delta R.T.: -0.023 min
Response: 4369994
Conc: 25.05 ng/ml

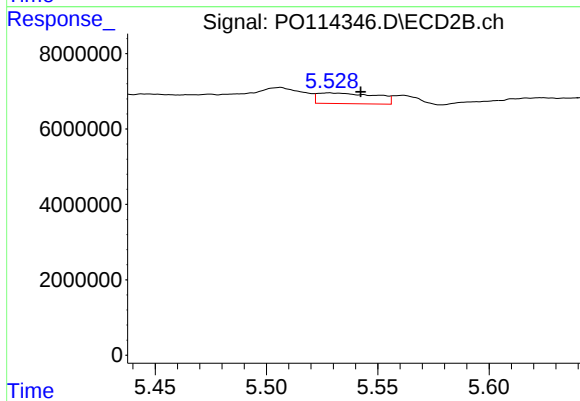

#26 AR-1254-1


R.T.: 5.528 min
Delta R.T.: -0.014 min
Response: 5113523
Conc: 19.25 ng/ml

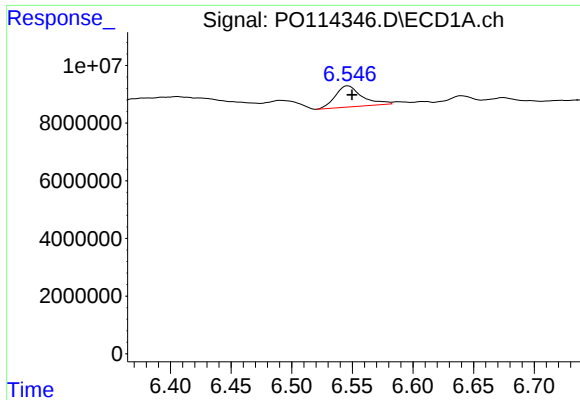

#27 AR-1254-2


R.T.: 6.546 min
Delta R.T.: -0.003 min
Response: 11165140
Conc: 43.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

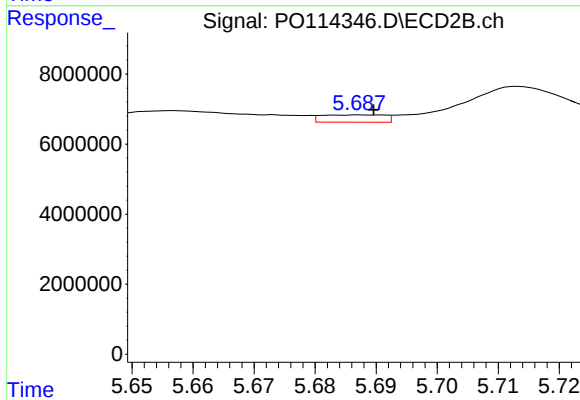


#27 AR-1254-2

R.T.: 5.688 min
Delta R.T.: -0.002 min
Response: 1500793
Conc: 6.30 ng/ml

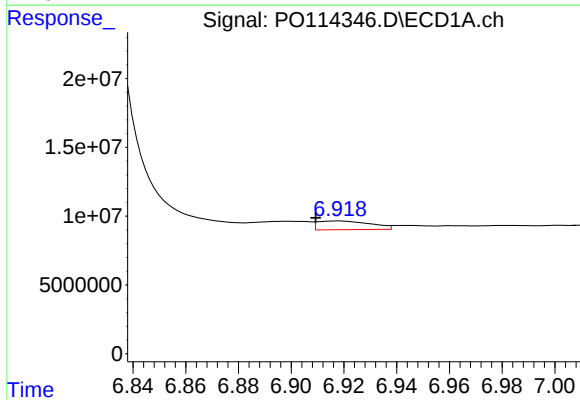


#28 AR-1254-3

R.T.: 6.918 min
Delta R.T.: 0.009 min
Response: 8881917
Conc: 30.74 ng/ml

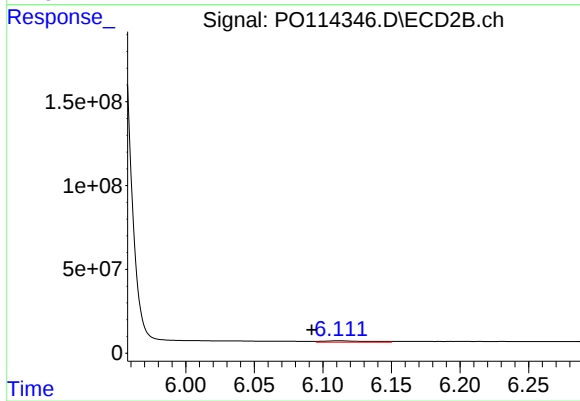

#28 AR-1254-3


R.T.: 6.111 min
Delta R.T.: 0.020 min
Response: 19177128
Conc: 54.11 ng/ml

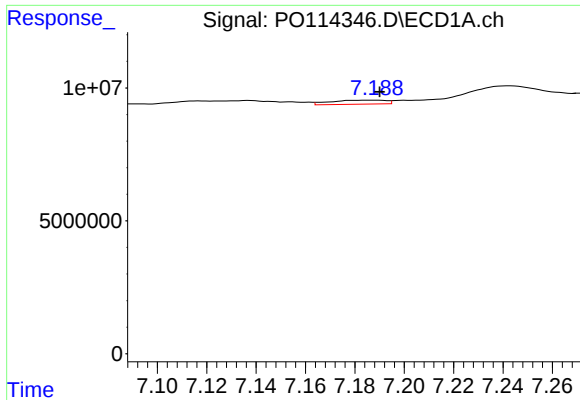

#29 AR-1254-4


R.T.: 7.186 min
Delta R.T.: -0.004 min
Response: 2331463
Conc: 9.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

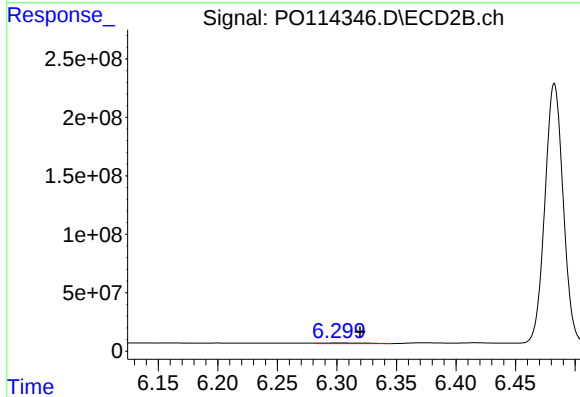


#29 AR-1254-4

R.T.: 6.300 min
Delta R.T.: -0.019 min
Response: 13314486
Conc: 51.58 ng/ml

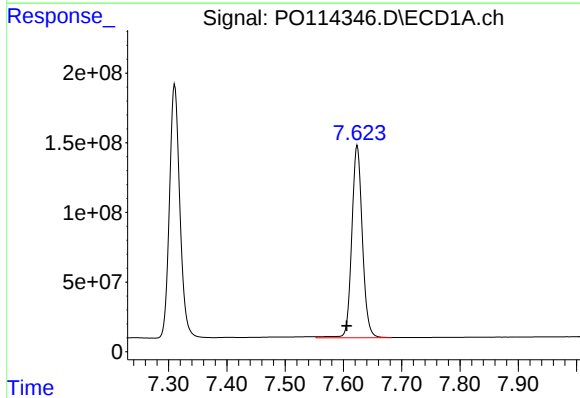


#30 AR-1254-5

R.T.: 7.624 min
Delta R.T.: 0.018 min
Response: 1746294846
Conc: 7956.66 ng/ml

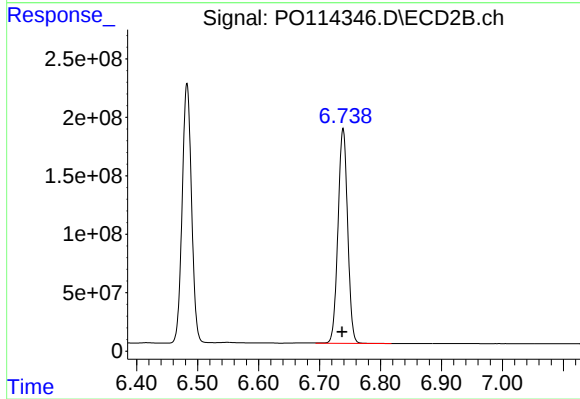

#30 AR-1254-5


R.T.: 6.739 min
Delta R.T.: 0.001 min
Response: 2017807082
Conc: 6301.64 ng/ml

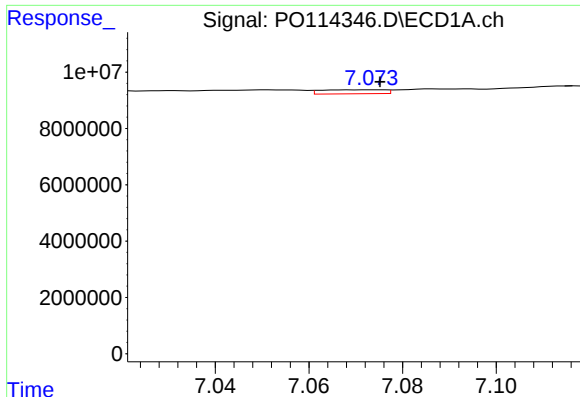

#31 AR-1260-1


R.T.: 7.074 min
Delta R.T.: -0.002 min
Response: 1351189
Conc: 6.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

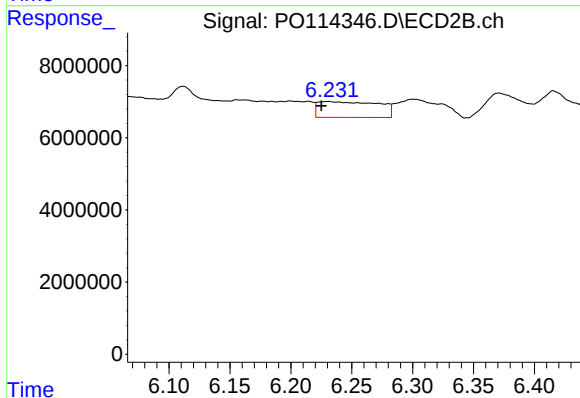


#31 AR-1260-1

R.T.: 6.231 min
Delta R.T.: 0.006 min
Response: 15172960
Conc: 64.43 ng/ml

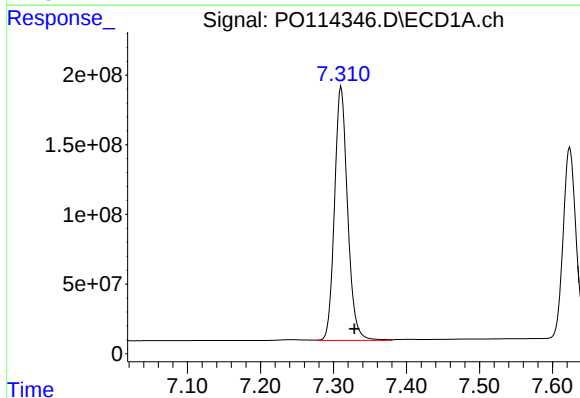


#32 AR-1260-2

R.T.: 7.310 min
Delta R.T.: -0.018 min
Response: 2264336118
Conc: 7339.72 ng/ml

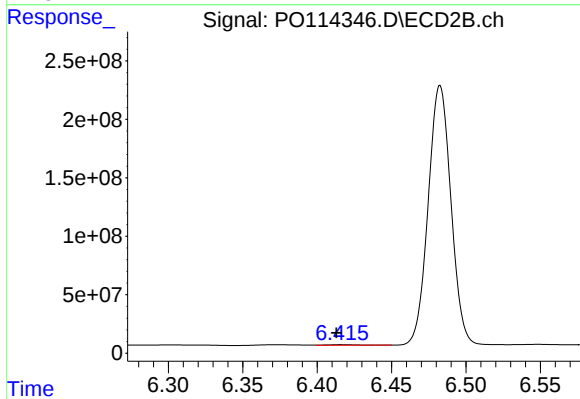

#32 AR-1260-2


R.T.: 6.416 min
Delta R.T.: 0.003 min
Response: 6783510
Conc: 20.29 ng/ml

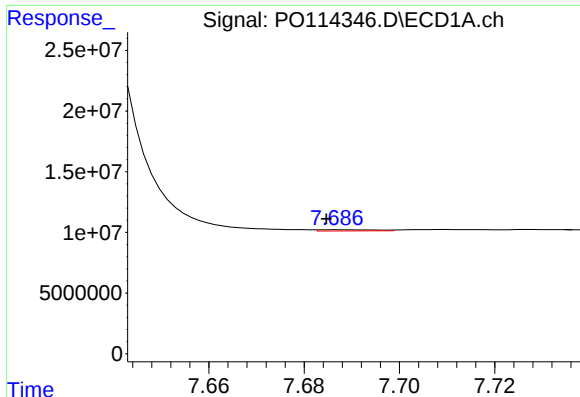

#33 AR-1260-3


R.T.: 7.687 min
Delta R.T.: 0.002 min
Response: 807001
Conc: 3.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

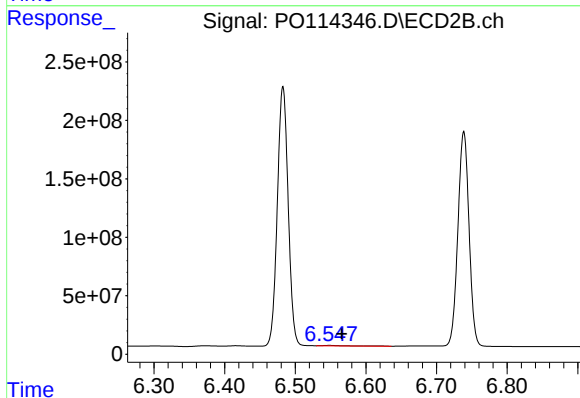


#33 AR-1260-3

R.T.: 6.548 min
Delta R.T.: -0.018 min
Response: 9186521
Conc: 31.15 ng/ml

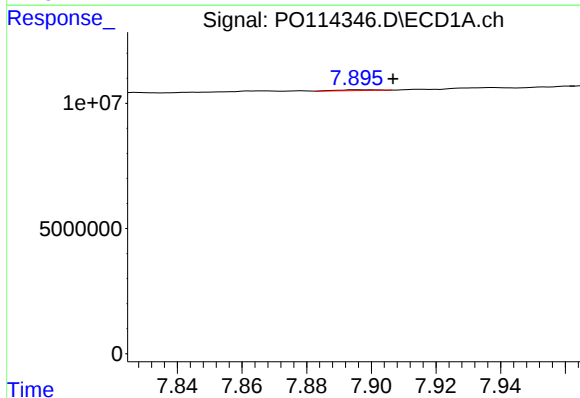


#34 AR-1260-4

R.T.: 7.896 min
Delta R.T.: -0.011 min
Response: 276149
Conc: 1.19 ng/ml

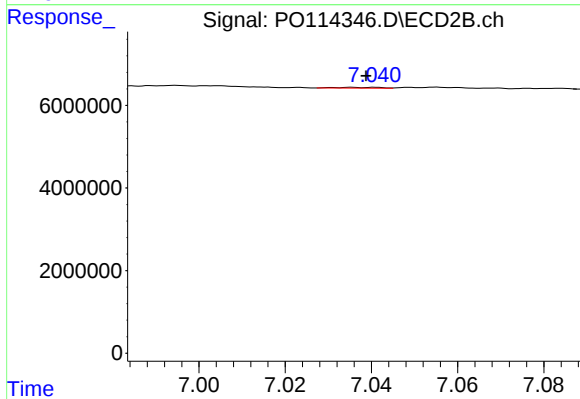

#34 AR-1260-4


R.T.: 7.036 min
Delta R.T.: -0.003 min
Response: 145096
Conc: 0.65 ng/ml

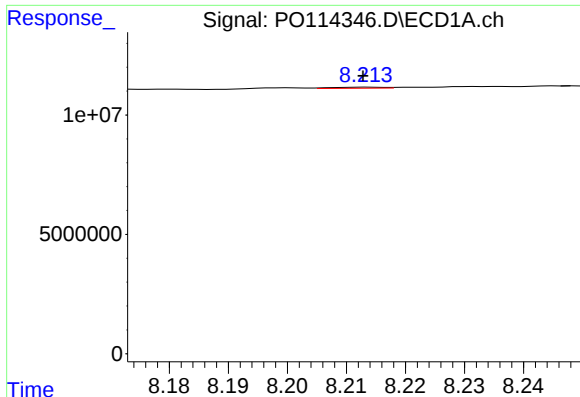

#35 AR-1260-5


R.T.: 8.213 min
Delta R.T.: 0.000 min
Response: 279248
Conc: 0.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

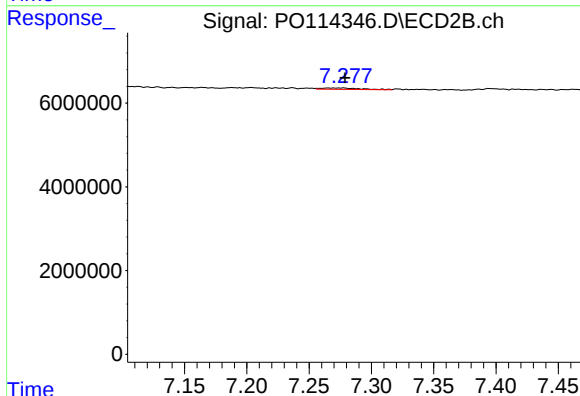


#35 AR-1260-5

R.T.: 7.277 min
Delta R.T.: -0.001 min
Response: 694427
Conc: 1.13 ng/ml

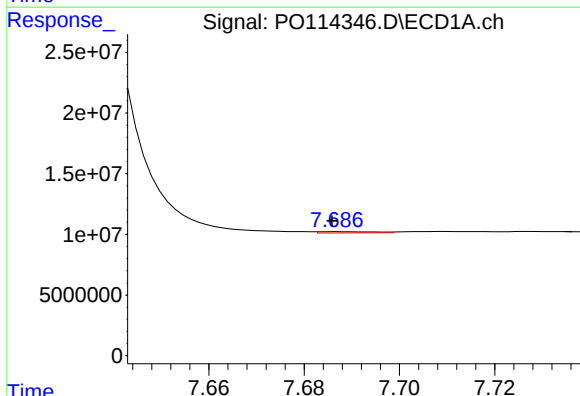


#36 AR-1262-1

R.T.: 7.687 min
Delta R.T.: 0.000 min
Response: 807001
Conc: 2.21 ng/ml

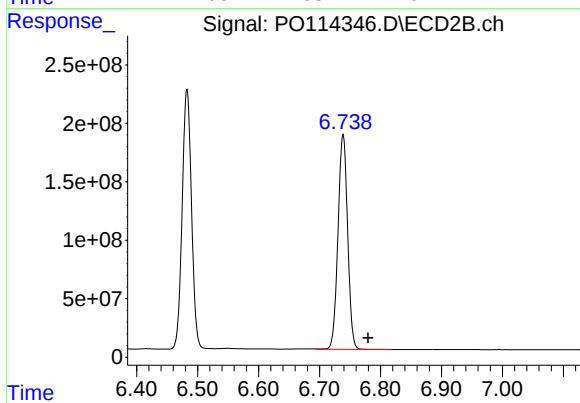

#36 AR-1262-1


R.T.: 6.739 min
Delta R.T.: -0.041 min
Response: 2017807082
Conc: 4740.48 ng/ml

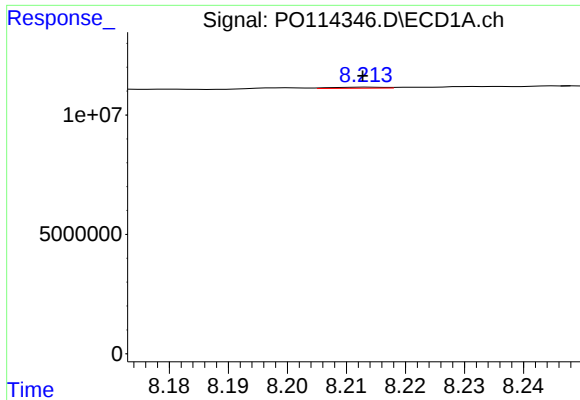

#37 AR-1262-2


R.T.: 8.213 min
Delta R.T.: 0.000 min
Response: 279248
Conc: 0.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

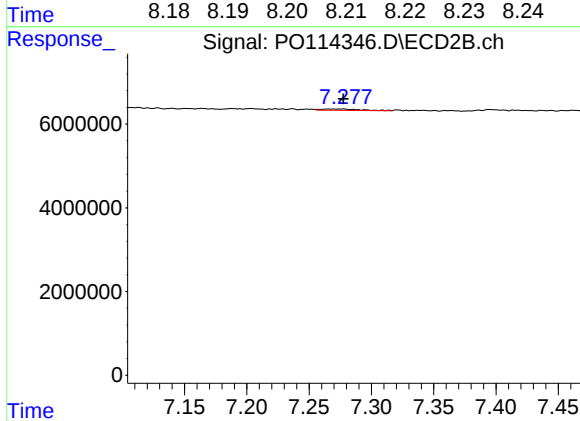


#37 AR-1262-2

R.T.: 7.277 min
Delta R.T.: 0.000 min
Response: 694427
Conc: 1.03 ng/ml

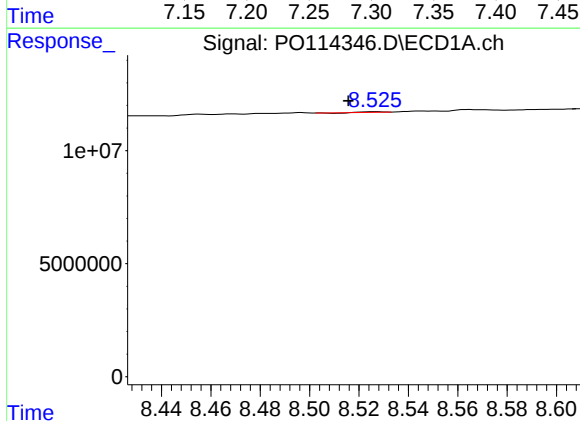


#38 AR-1262-3

R.T.: 8.527 min
Delta R.T.: 0.011 min
Response: 58822
Conc: 0.16 ng/ml

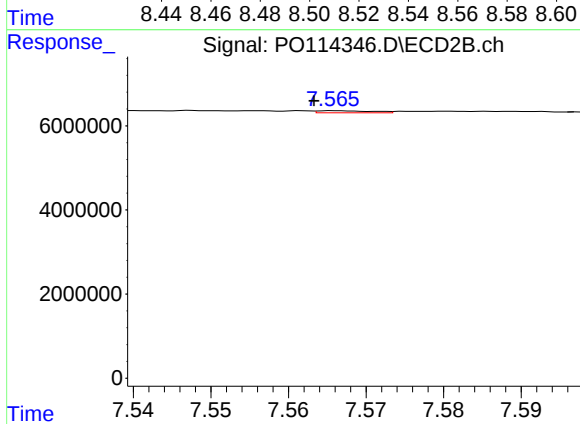

#38 AR-1262-3


R.T.: 7.566 min
Delta R.T.: 0.003 min
Response: 252651
Conc: 0.91 ng/ml

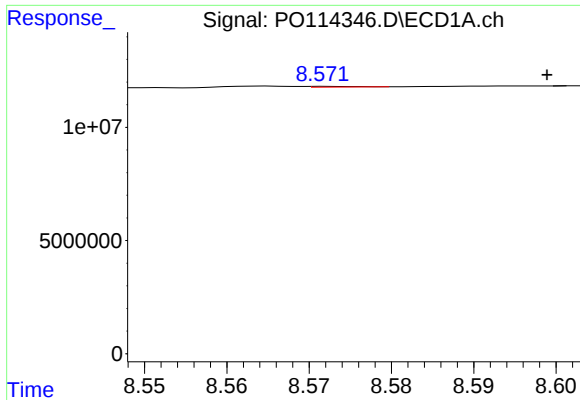

#39 AR-1262-4


R.T.: 8.571 min
Delta R.T.: -0.028 min
Response: 113717
Conc: 0.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

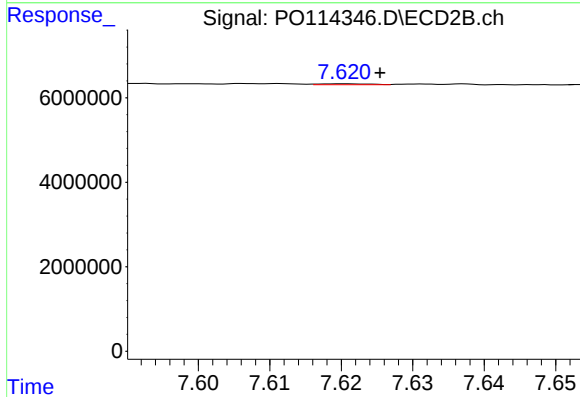


#39 AR-1262-4

R.T.: 7.620 min
Delta R.T.: -0.005 min
Response: 95962
Conc: 0.21 ng/ml

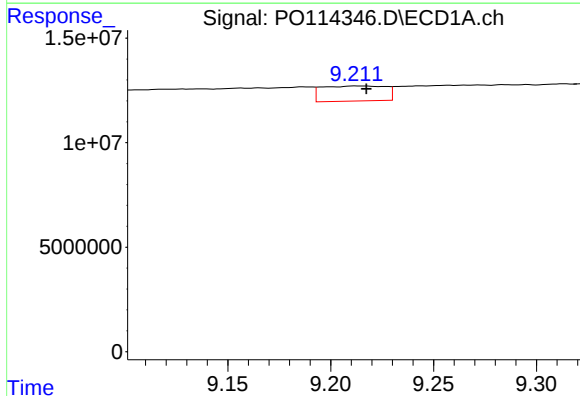


#40 AR-1262-5

R.T.: 9.212 min
Delta R.T.: -0.005 min
Response: 15509572
Conc: 72.19 ng/ml

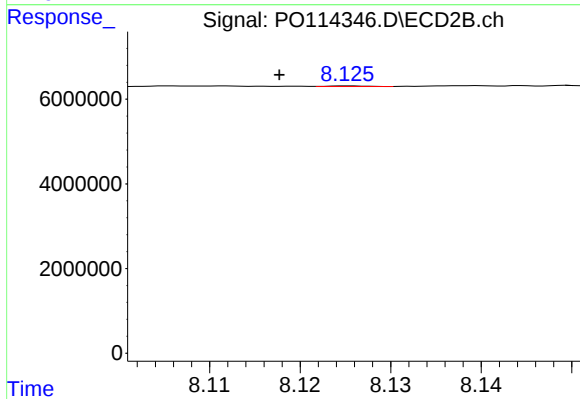

#40 AR-1262-5


R.T.: 8.126 min
Delta R.T.: 0.008 min
Response: 45395
Conc: 0.22 ng/ml

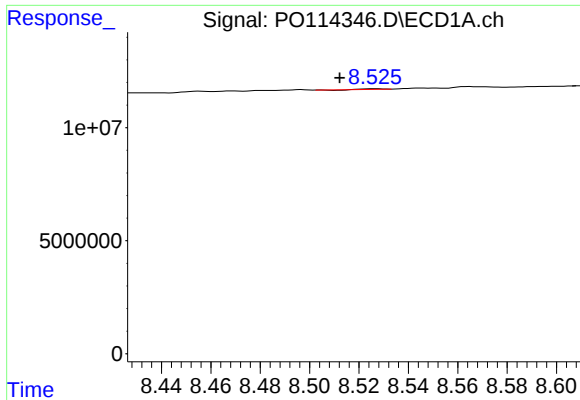

#41 AR-1268-1


R.T.: 8.527 min
Delta R.T.: 0.014 min
Response: 58822
Conc: 0.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

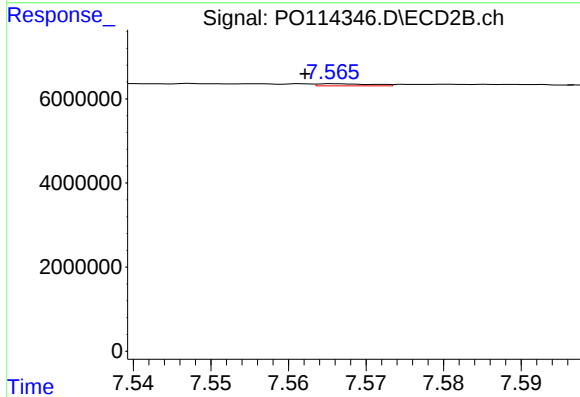


#41 AR-1268-1

R.T.: 7.566 min
Delta R.T.: 0.004 min
Response: 252651
Conc: 0.31 ng/ml

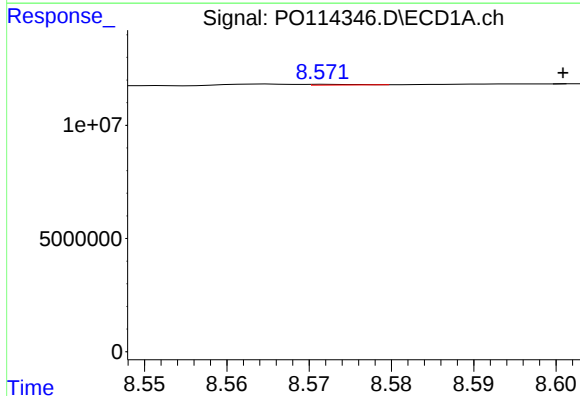


#42 AR-1268-2

R.T.: 8.571 min
Delta R.T.: -0.030 min
Response: 113717
Conc: 0.18 ng/ml

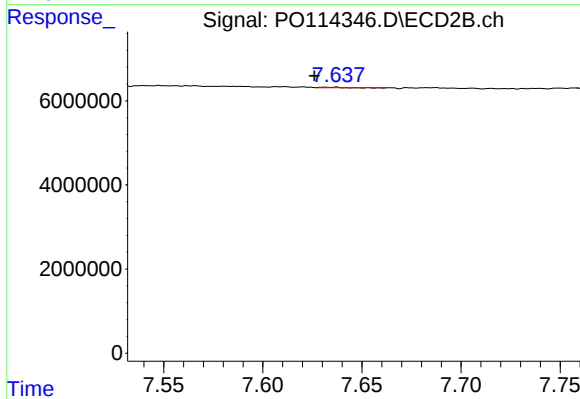

#42 AR-1268-2


R.T.: 7.631 min
Delta R.T.: 0.005 min
Response: 25398
Conc: 0.04 ng/ml

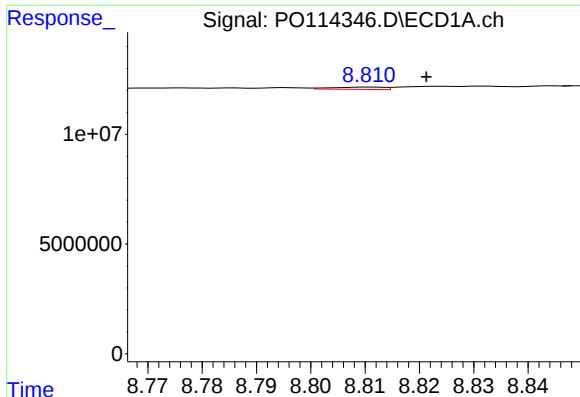

#43 AR-1268-3


R.T.: 8.811 min
Delta R.T.: -0.010 min
Response: 703036
Conc: 1.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

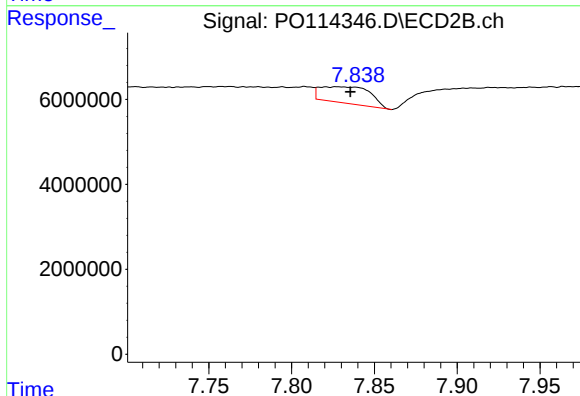


#43 AR-1268-3

R.T.: 7.821 min
Delta R.T.: -0.015 min
Response: 8127945
Conc: 13.77 ng/ml

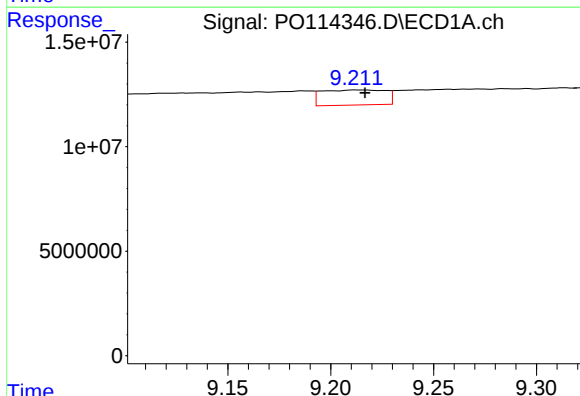


#44 AR-1268-4

R.T.: 9.212 min
Delta R.T.: -0.004 min
Response: 15509572
Conc: 62.78 ng/ml

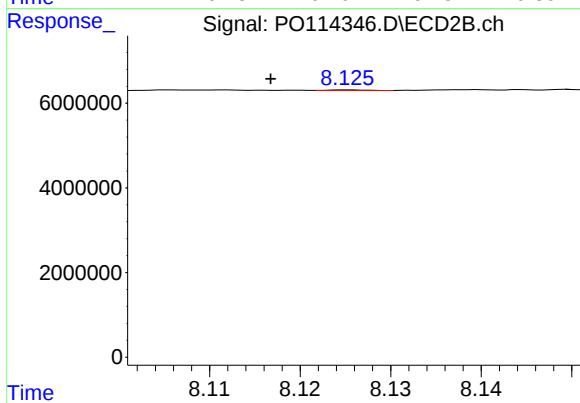

#44 AR-1268-4


R.T.: 8.126 min
Delta R.T.: 0.009 min
Response: 45395
Conc: 0.19 ng/ml

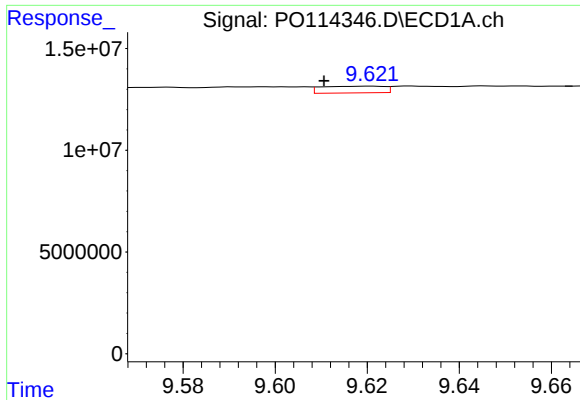

#45 AR-1268-5

R.T.: 9.621 min
Delta R.T.: 0.010 min
Response: 3129147
Conc: 1.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

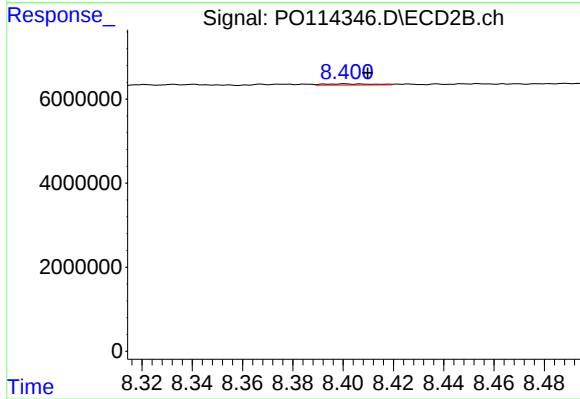

#45 AR-1268-5

R.T.: 8.401 min
Delta R.T.: -0.009 min
Response: 386118
Conc: 0.24 ng/ml