

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101018\
 Data File : PO049856.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Oct 2018 10:48
 Operator : SM/SJ
 Sample : J5293-03DL 4X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 VW-CONCRETE-FLOORDL

Manual Integrations
 APPROVED

Sohil
 10/11/2018 3:00:14 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 11:04:28 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 08 15:27:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.384	3.514	1939851	1093471	8.581m	4.534m#
2) SA Decachlor...	10.093	8.439	2177405	1140175	6.535	4.359 #
Target Compounds						
26) L6 AR-1254-1	6.411	5.371	12043068	11927727	875.771	608.446 #
27) L6 AR-1254-2	6.631	5.518	22487905	10041914	1018.499	599.969 #
28) L6 AR-1254-3	6.997	5.917	17358216	16461237	711.428	589.717
29) L6 AR-1254-4	7.280	6.143	22991550	7767497	1121.052	387.092 #
30) L6 AR-1254-5	7.700	6.556	16920867	10842775	878.044	405.220 #
31) L7 AR-1260-1	7.160	6.044	21082580	10426916	1142.634	504.970 #
32) L7 AR-1260-2	7.417	6.232	12441732	11773670	518.827	419.903
33) L7 AR-1260-3	7.775	6.383	5653353	6985172	299.017	286.639
34) L7 AR-1260-4	7.997	6.850	7340206	2651292	386.578	137.280 #
35) L7 AR-1260-5	8.318	7.090	7395978	8700699	174.829	169.705

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101018\
Data File : P0049856.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Oct 2018 10:48
Operator : SM/SJ
Sample : J5293-03DL 4X
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
VW-CONCRETE-FLOORDL


Manual Integrations
APPROVED

Sohil
10/11/2018 3:00:14 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 11:04:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100818.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 08 15:27:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

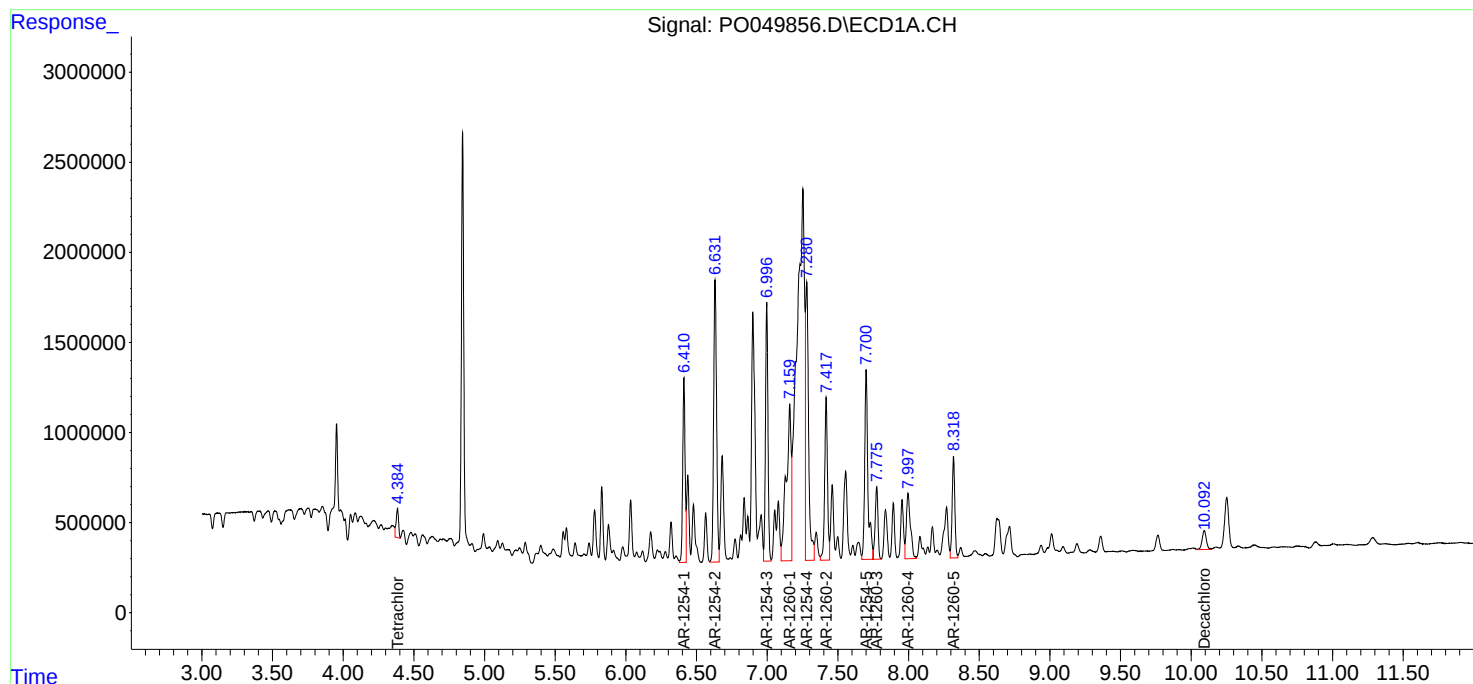

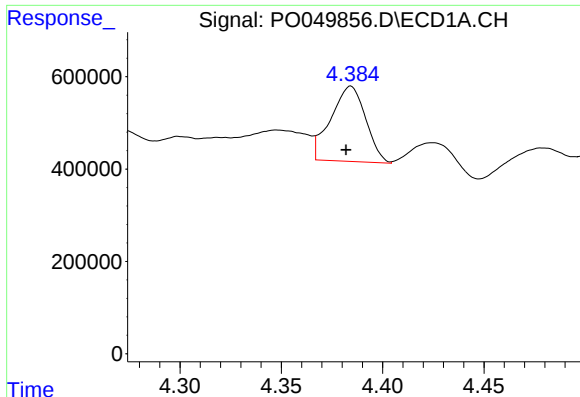


#1 Tetrachloro-m-xylene

R.T.: 4.384 min
Delta R.T.: 0.002 min
Response: 1939851
Conc: 8.58 ng/ml m

Instrument :
ECD_O
ClientSampleId :
VW-CONCRETE-FLOORDL


Manual Integrations
APPROVED

Sohil
10/11/2018 3:00:14 PM

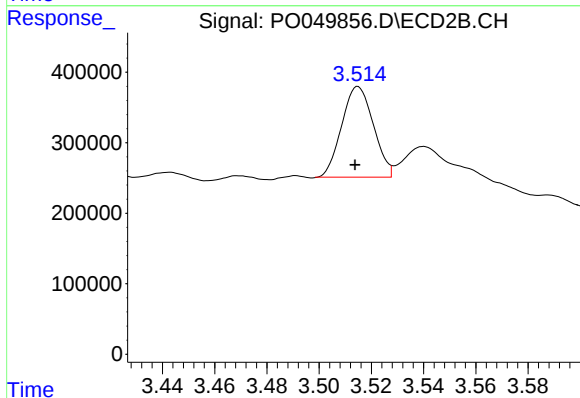


#1 Tetrachloro-m-xylene

R.T.: 3.514 min
Delta R.T.: 0.000 min
Response: 1093471
Conc: 4.53 ng/ml m

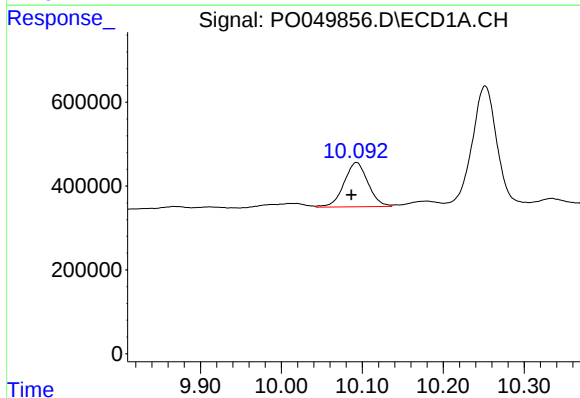


#2 Decachlorobiphenyl

R.T.: 10.093 min
Delta R.T.: 0.006 min
Response: 2177405
Conc: 6.53 ng/ml

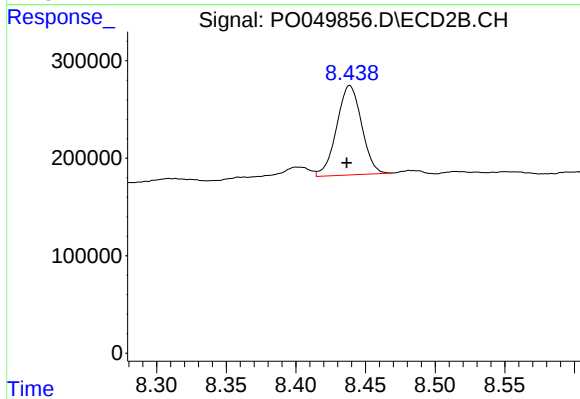

#2 Decachlorobiphenyl

R.T.: 8.439 min
Delta R.T.: 0.002 min
Response: 1140175
Conc: 4.36 ng/ml

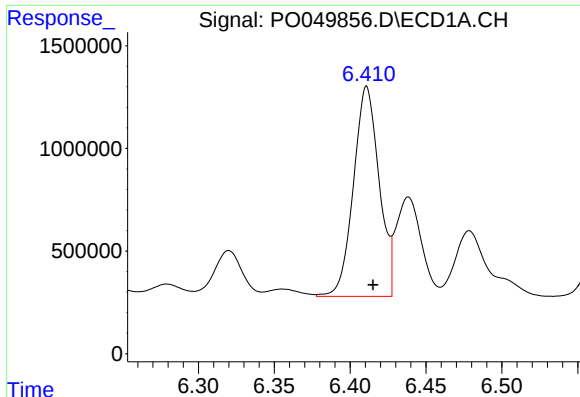


#26 AR-1254-1

R.T.: 6.411 min
Delta R.T.: -0.004 min
Response: 12043068
Conc: 875.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
VW-CONCRETE-FLOORDL


Manual Integrations
APPROVED

Sohil
10/11/2018 3:00:14 PM

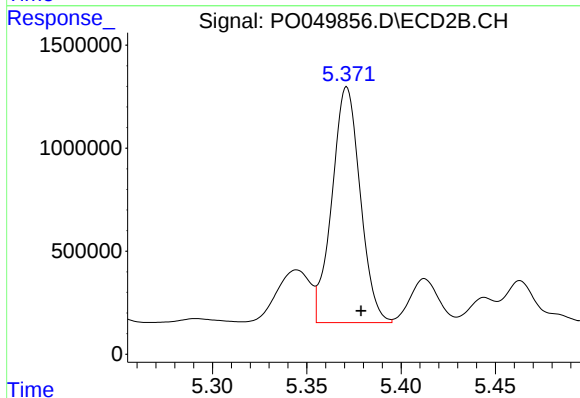


#26 AR-1254-1

R.T.: 5.371 min
Delta R.T.: -0.008 min
Response: 11927727
Conc: 608.45 ng/ml

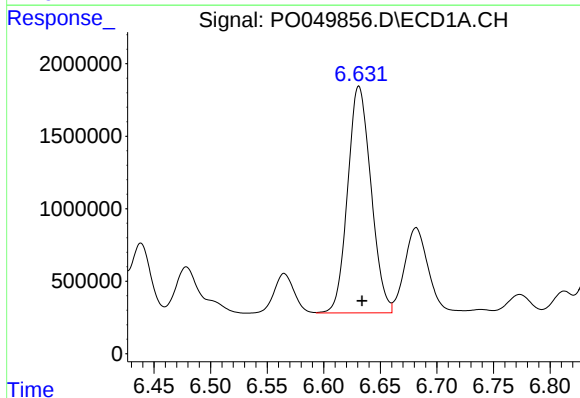


#27 AR-1254-2

R.T.: 6.631 min
Delta R.T.: -0.003 min
Response: 22487905
Conc: 1018.50 ng/ml

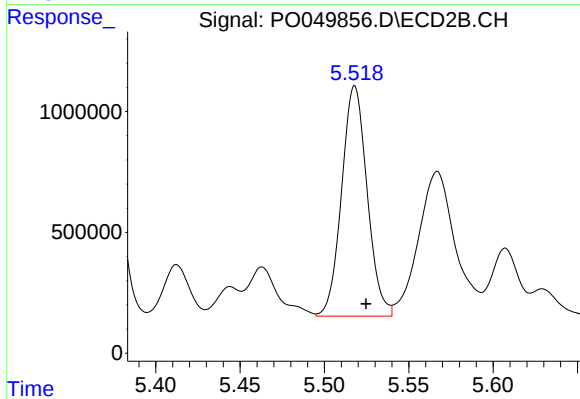

#27 AR-1254-2

R.T.: 5.518 min
Delta R.T.: -0.007 min
Response: 10041914
Conc: 599.97 ng/ml

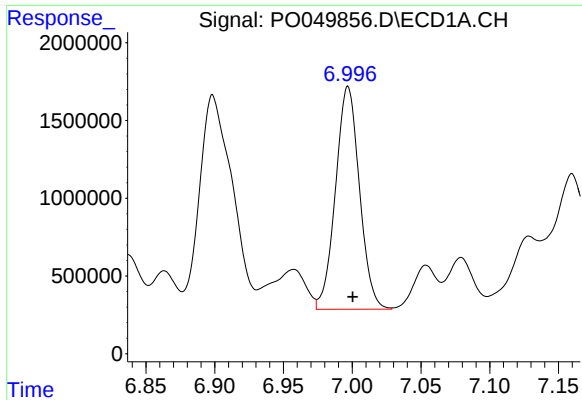


#28 AR-1254-3

R.T.: 6.997 min
Delta R.T.: -0.003 min
Response: 17358216
Conc: 711.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
VW-CONCRETE-FLOORDL


Manual Integrations
APPROVED

Sohil
10/11/2018 3:00:14 PM

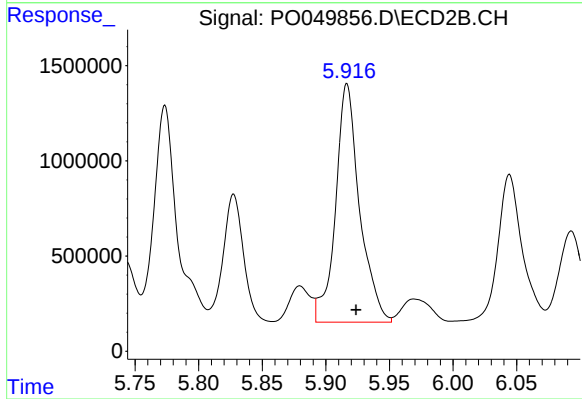


#28 AR-1254-3

R.T.: 5.917 min
Delta R.T.: -0.007 min
Response: 16461237
Conc: 589.72 ng/ml

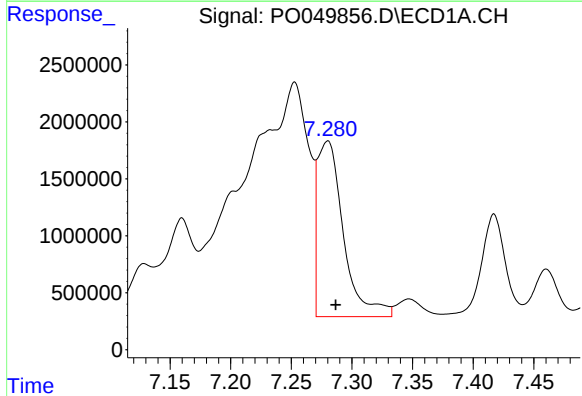


#29 AR-1254-4

R.T.: 7.280 min
Delta R.T.: -0.007 min
Response: 22991550
Conc: 1121.05 ng/ml

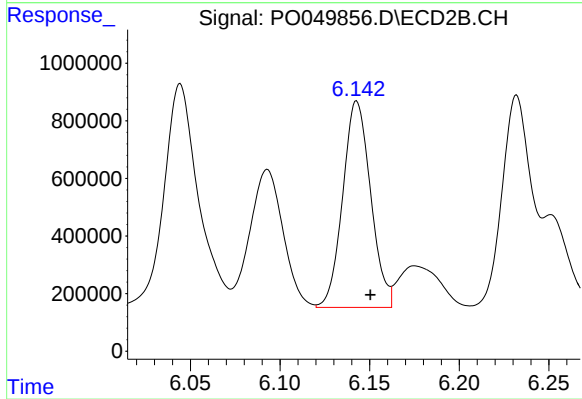

#29 AR-1254-4

R.T.: 6.143 min
Delta R.T.: -0.008 min
Response: 7767497
Conc: 387.09 ng/ml

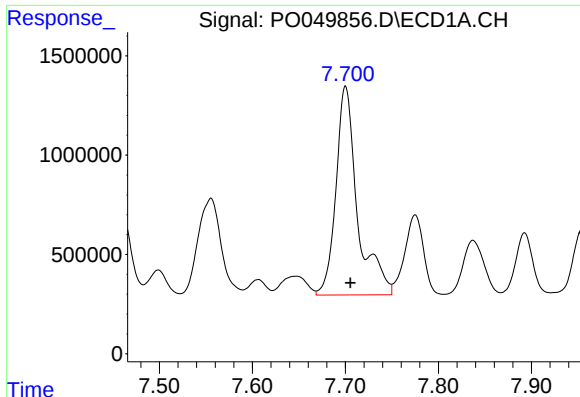


#30 AR-1254-5

R.T.: 7.700 min
Delta R.T.: -0.005 min
Response: 16920867
Conc: 878.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
VW-CONCRETE-FLOORDL


Manual Integrations
APPROVED

Sohil
10/11/2018 3:00:14 PM

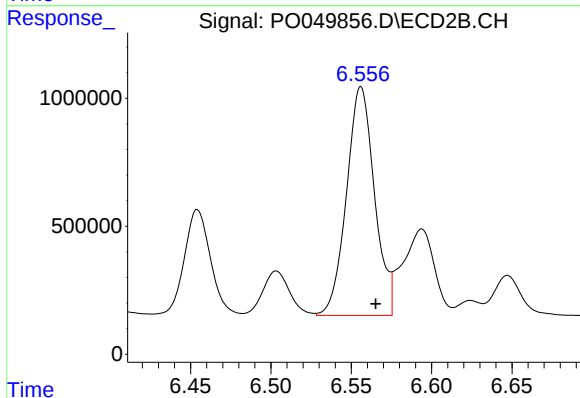


#30 AR-1254-5

R.T.: 6.556 min
Delta R.T.: -0.009 min
Response: 10842775
Conc: 405.22 ng/ml

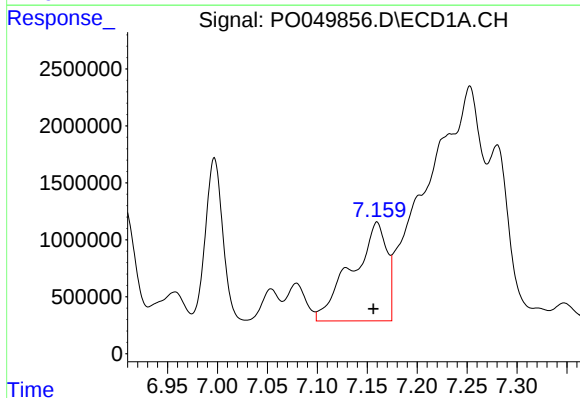


#31 AR-1260-1

R.T.: 7.160 min
Delta R.T.: 0.003 min
Response: 21082580
Conc: 1142.63 ng/ml

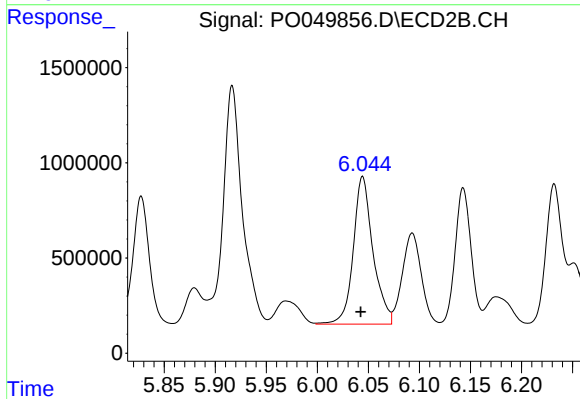

#31 AR-1260-1

R.T.: 6.044 min
Delta R.T.: 0.002 min
Response: 10426916
Conc: 504.97 ng/ml

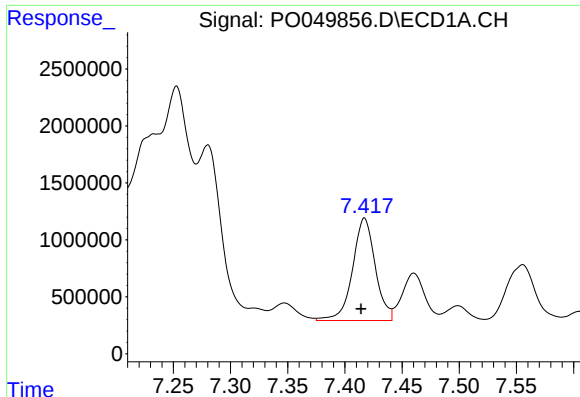


#32 AR-1260-2

R.T.: 7.417 min
Delta R.T.: 0.003 min
Response: 12441732
Conc: 518.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
VW-CONCRETE-FLOORDL


Manual Integrations
APPROVED

Sohil
10/11/2018 3:00:14 PM

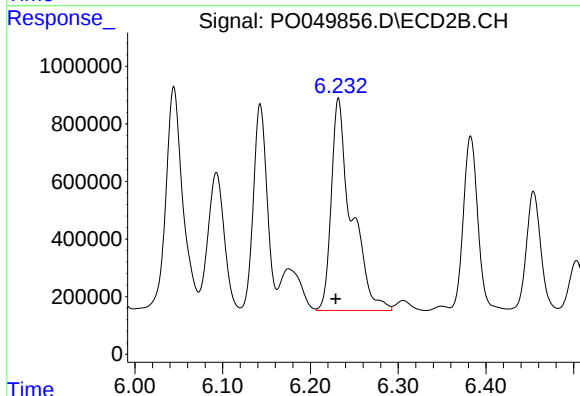


#32 AR-1260-2

R.T.: 6.232 min
Delta R.T.: 0.003 min
Response: 11773670
Conc: 419.90 ng/ml

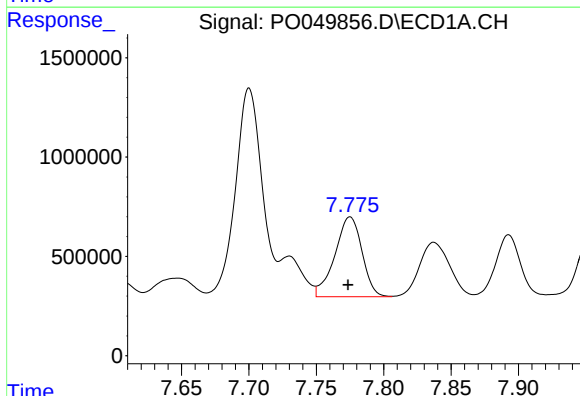


#33 AR-1260-3

R.T.: 7.775 min
Delta R.T.: 0.001 min
Response: 5653353
Conc: 299.02 ng/ml

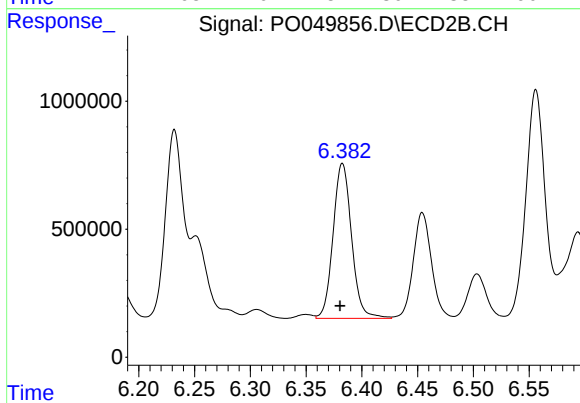

#33 AR-1260-3

R.T.: 6.383 min
Delta R.T.: 0.002 min
Response: 6985172
Conc: 286.64 ng/ml

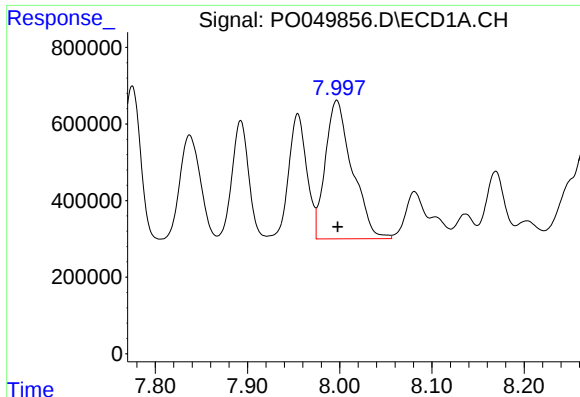


#34 AR-1260-4

R.T.: 7.997 min
Delta R.T.: -0.001 min
Response: 7340206
Conc: 386.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
VW-CONCRETE-FLOORDL


Manual Integrations
APPROVED

Sohil
10/11/2018 3:00:14 PM

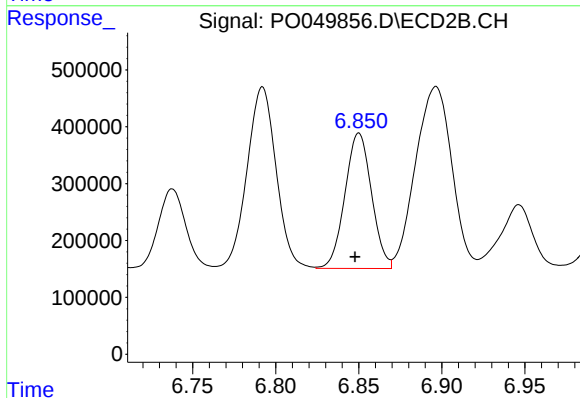


#34 AR-1260-4

R.T.: 6.850 min
Delta R.T.: 0.002 min
Response: 2651292
Conc: 137.28 ng/ml

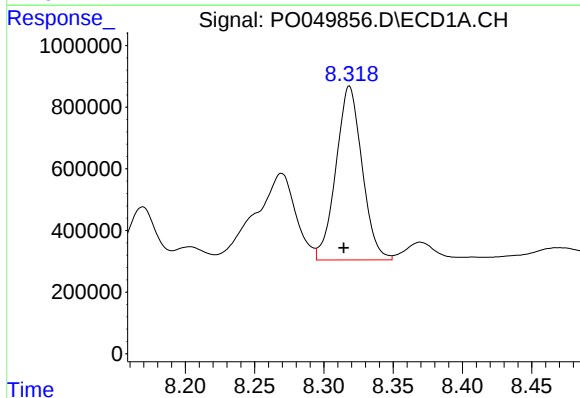

#35 AR-1260-5

R.T.: 8.318 min
Delta R.T.: 0.004 min
Response: 7395978
Conc: 174.83 ng/ml

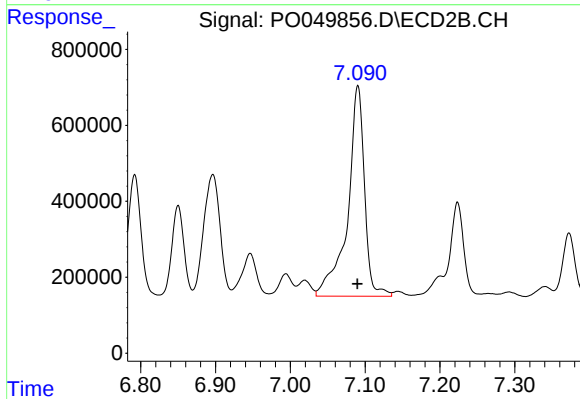

#35 AR-1260-5

R.T.: 7.090 min
Delta R.T.: 0.000 min
Response: 8700699
Conc: 169.71 ng/ml