

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101018\
 Data File : PO049882.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Oct 2018 3:02
 Operator : SM/SJ
 Sample : J5360-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 2-AVE-22

Manual Integrations
 APPROVED

Sohil
 10/11/2018 3:00:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 06:53:08 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 08 15:27:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.364	3.539	3516986	3288623	15.558m	13.635
2) SA Decachlor...	10.048	8.416	4307620	2877258	12.928	11.000

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101018\
Data File : P0049882.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Oct 2018 3:02
Operator : SM/SJ
Sample : J5360-01
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
2-AVE-22


Manual Integrations
APPROVED

Sohil
10/11/2018 3:00:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 06:53:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100818.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 08 15:27:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

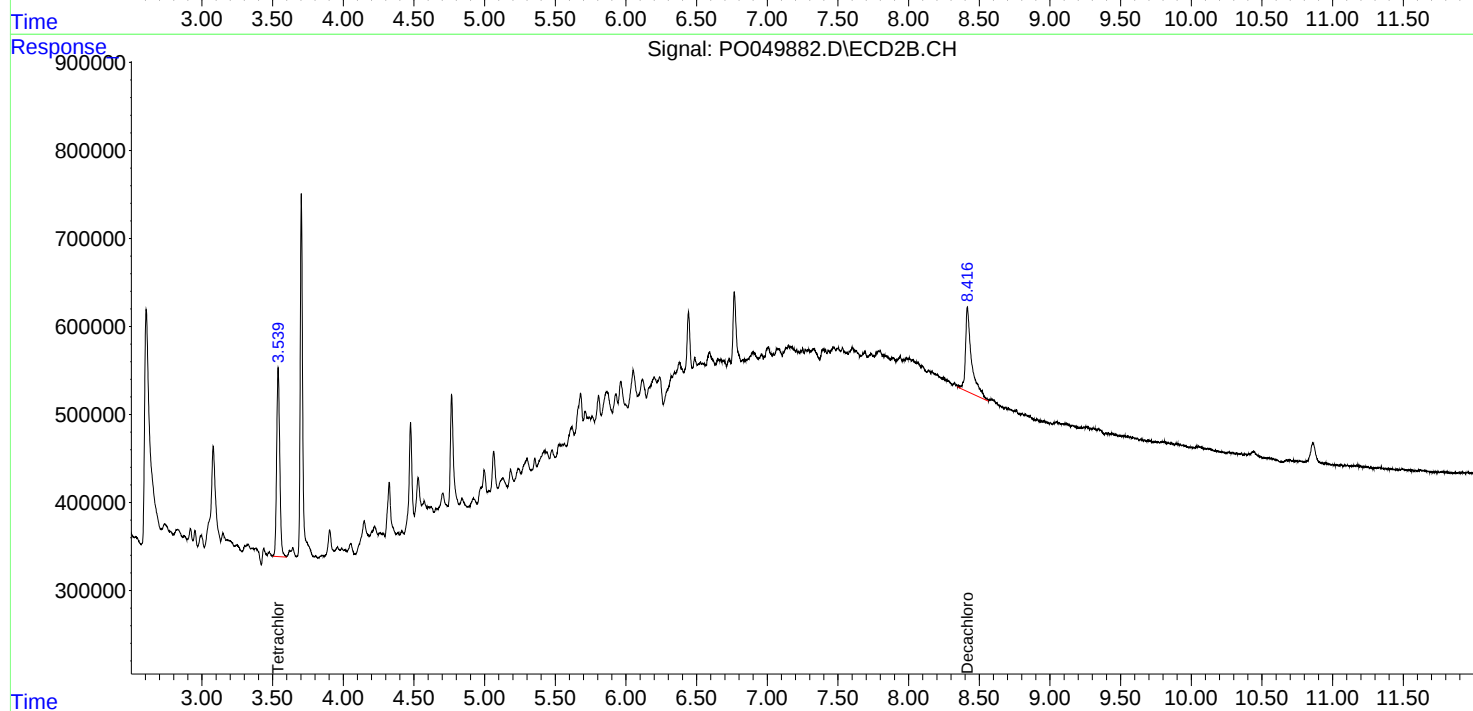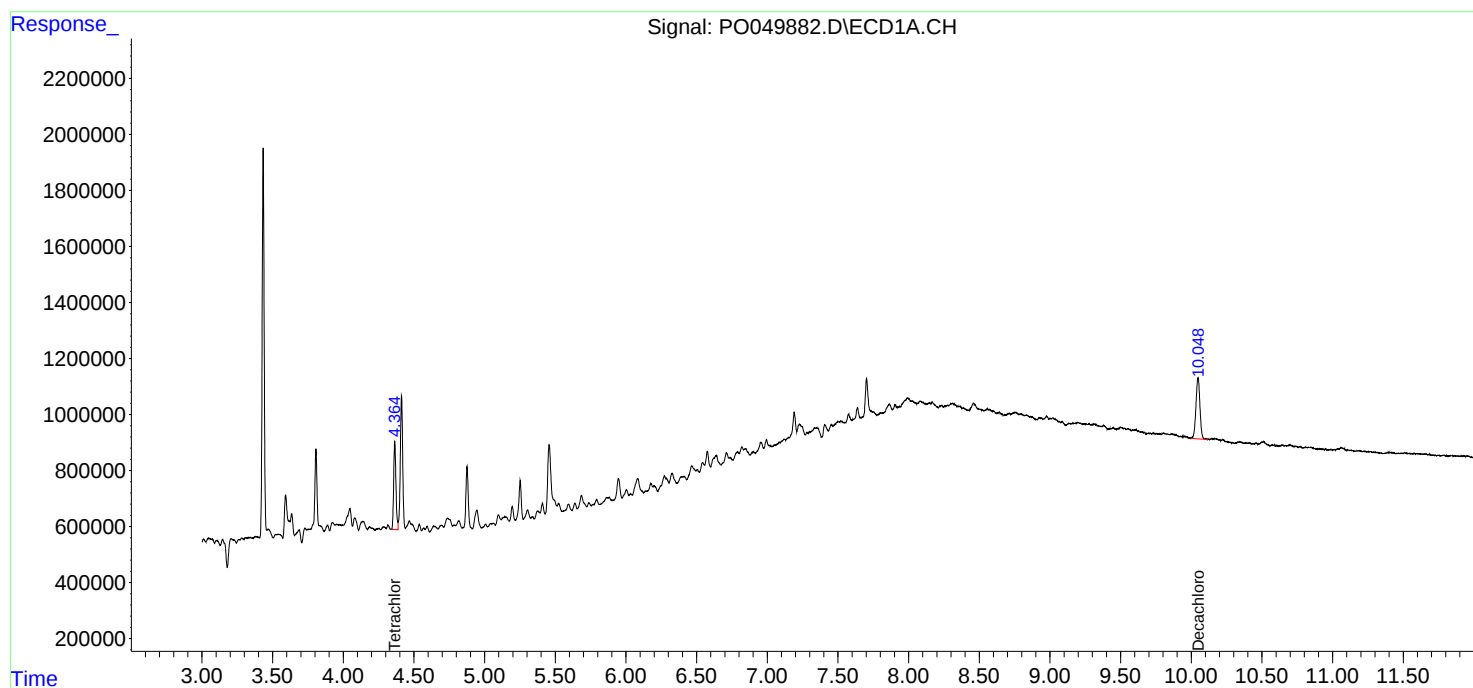

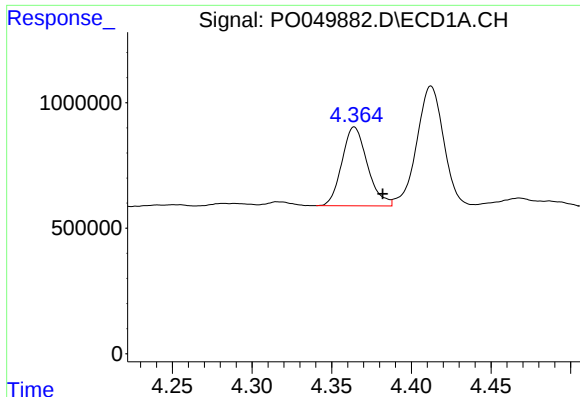


#1 Tetrachloro-m-xylene

R.T.: 4.364 min
Delta R.T.: -0.018 min
Response: 3516986
Conc: 15.56 ng/ml m

Instrument :
ECD_O
ClientSampleId :
2-AVE-22


Manual Integrations
APPROVED

Sohil
10/11/2018 3:00:47 PM

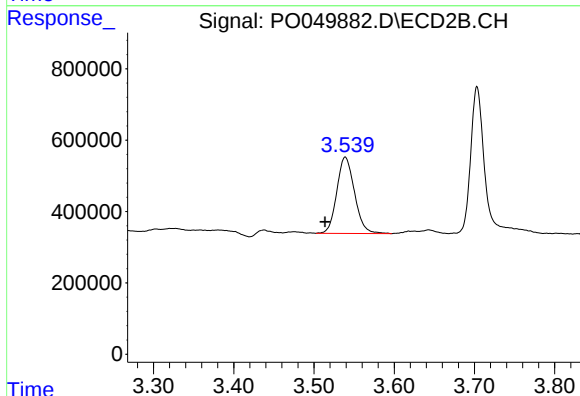


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: 0.025 min
Response: 3288623
Conc: 13.63 ng/ml

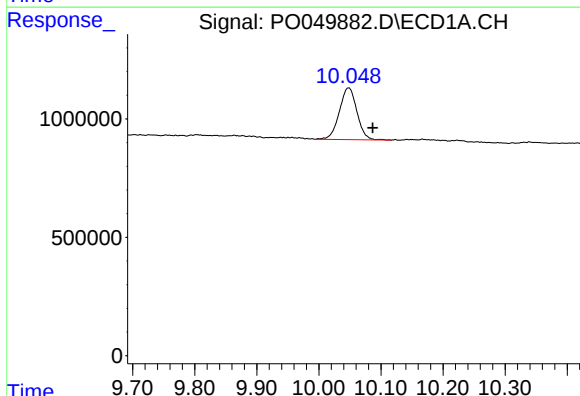

#2 Decachlorobiphenyl

R.T.: 10.048 min
Delta R.T.: -0.039 min
Response: 4307620
Conc: 12.93 ng/ml

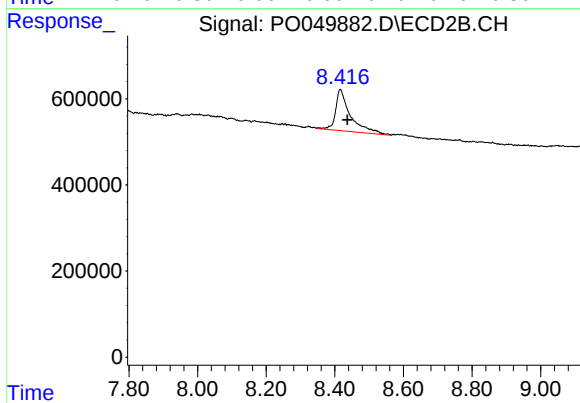

#2 Decachlorobiphenyl

R.T.: 8.416 min
Delta R.T.: -0.021 min
Response: 2877258
Conc: 11.00 ng/ml