

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101019\
 Data File : P0061853.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Oct 2019 13:17
 Operator : HP/AJ
 Sample : K5292-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20190850-COMPOSITE-B

Manual Integrations
 APPROVED

Ankita
 10/11/2019 2:10:19 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 13:38:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 10 11:46:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.355	3.513	758701	561025	18.498	17.348
2) SA Decachlor...	10.014	8.373	435270	307030	9.346	9.483m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101019\
Data File : PO061853.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Oct 2019 13:17
Operator : HP/AJ
Sample : K5292-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
20190850-COMPOSITE-B


Manual Integrations
APPROVED

Ankita
10/11/2019 2:10:19 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 13:38:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 10 11:46:12 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

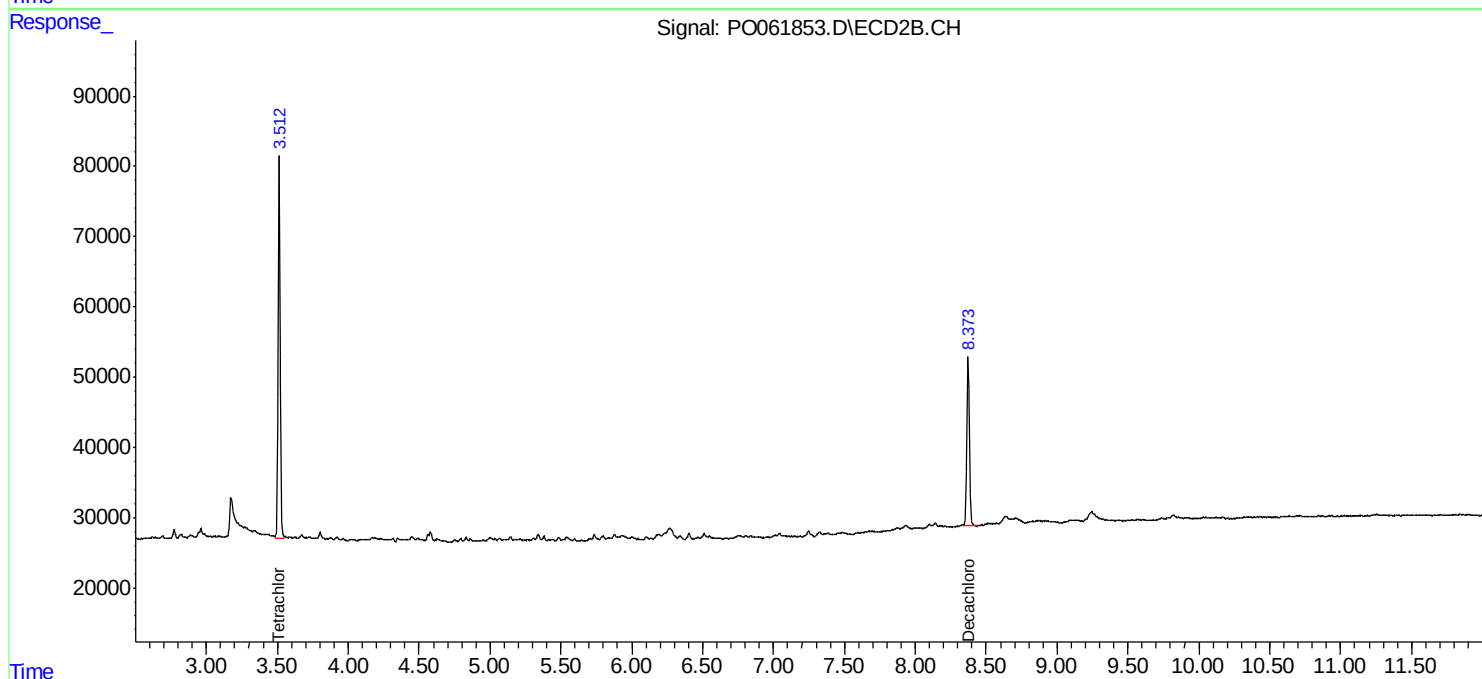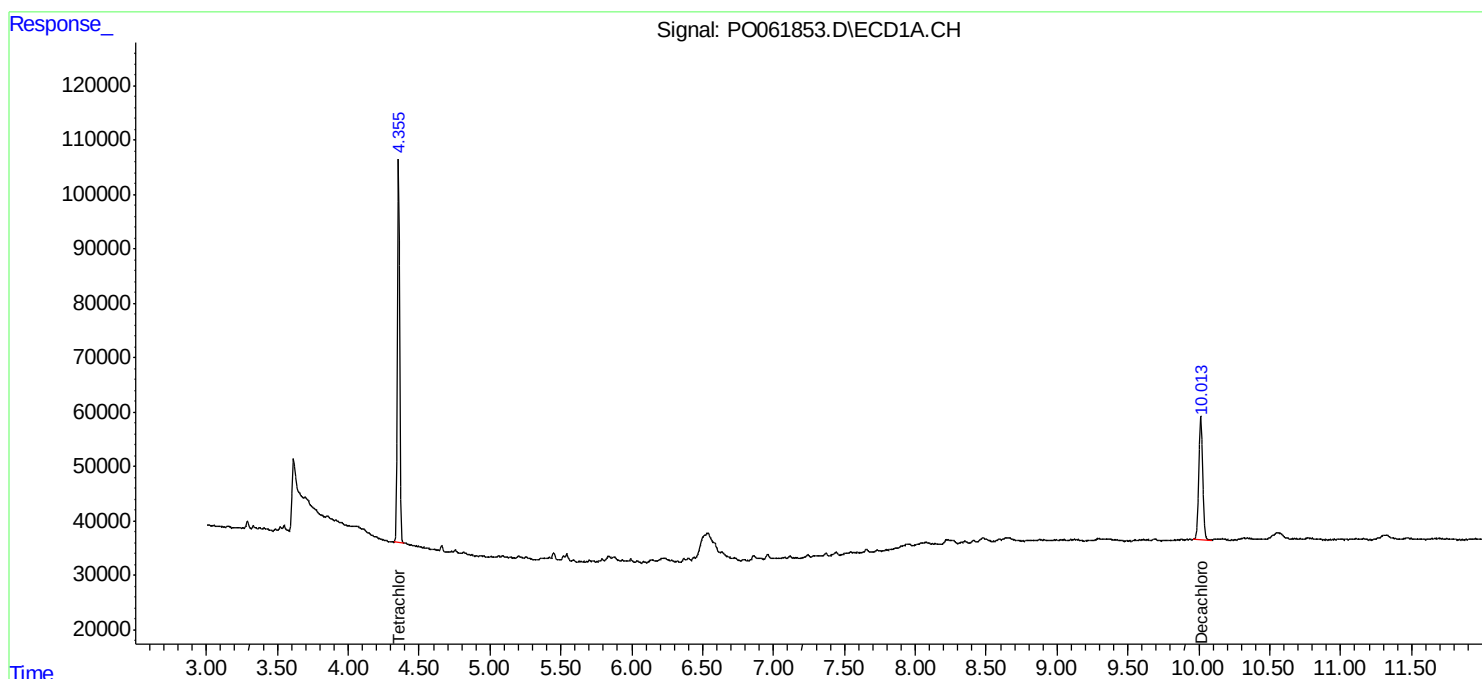

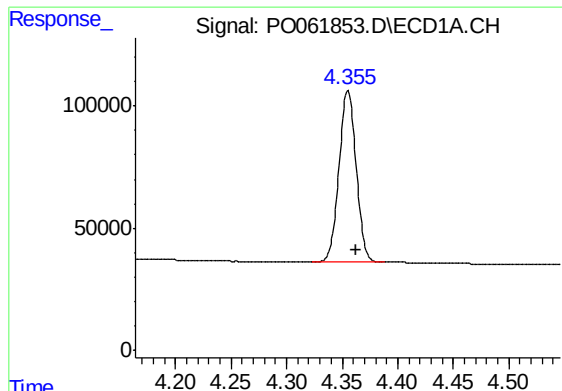


#1 Tetrachloro-m-xylene

R.T.: 4.355 min
Delta R.T.: -0.008 min
Response: 758701
Conc: 18.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
20190850-COMPOSITE-B


Manual Integrations
APPROVED

Ankita
10/11/2019 2:10:19 PM

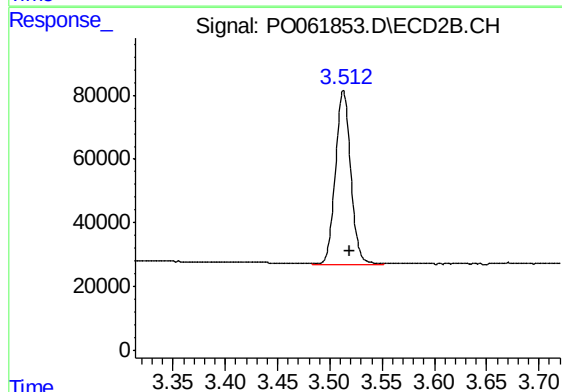


#1 Tetrachloro-m-xylene

R.T.: 3.513 min
Delta R.T.: -0.006 min
Response: 561025
Conc: 17.35 ng/ml

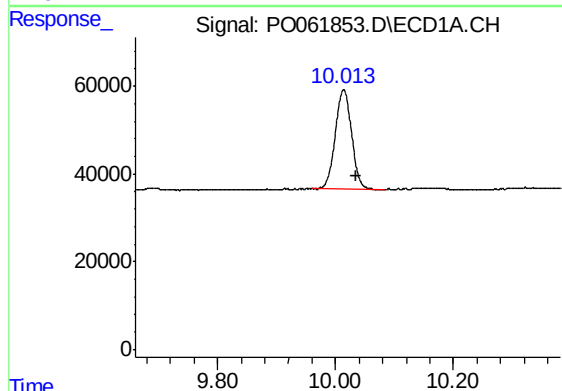

#2 Decachlorobiphenyl

R.T.: 10.014 min
Delta R.T.: -0.022 min
Response: 435270
Conc: 9.35 ng/ml

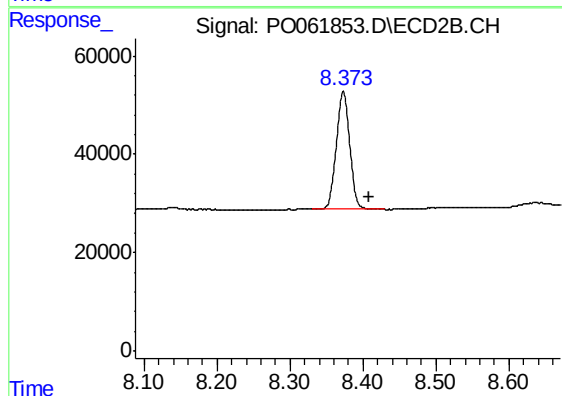

#2 Decachlorobiphenyl

R.T.: 8.373 min
Delta R.T.: -0.036 min
Response: 307030
Conc: 9.48 ng/ml m